

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
 Data File : PL074348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2022 18:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 02:05:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.489	7769074	40830616	24.045	22.900
28)	SA Decachlor...	10.404	11.331	11787707	43097910	22.667	24.400
Target Compounds							
2)	A alpha-BHC	5.364f	0.000	103692	0	0.247	N.D. #
6)	B beta-BHC	0.000	6.678	0	502296	N.D.	0.446 #
7)	B delta-BHC	0.000	6.940	0	1349097	N.D.	0.552 #
9)	A Endosulfan I	0.000	8.324	0	29973	N.D.	0.015 #
10)	B gamma-Chl...	0.000	8.198	0	172382	N.D.	0.077 #
11)	B alpha-Chl...	0.000	8.285	0	72627	N.D.	0.034 #
14)	MA Endrin	8.081f	8.873f	85444	241863	0.210	0.143 #
21)	B Endrin ke...	0.000	9.922	0	94875	N.D.	0.055 #
23)	Chlordane-1	0.000	6.848f	0	1159042	N.D.	14.524 #
25)	Chlordane-3	0.000	8.198	0	172382	N.D.	0.510 #
26)	Chlordane-4	0.000	8.285	0	72627	N.D.	0.183 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
Data File : PL074348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2022 18:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 02:05:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

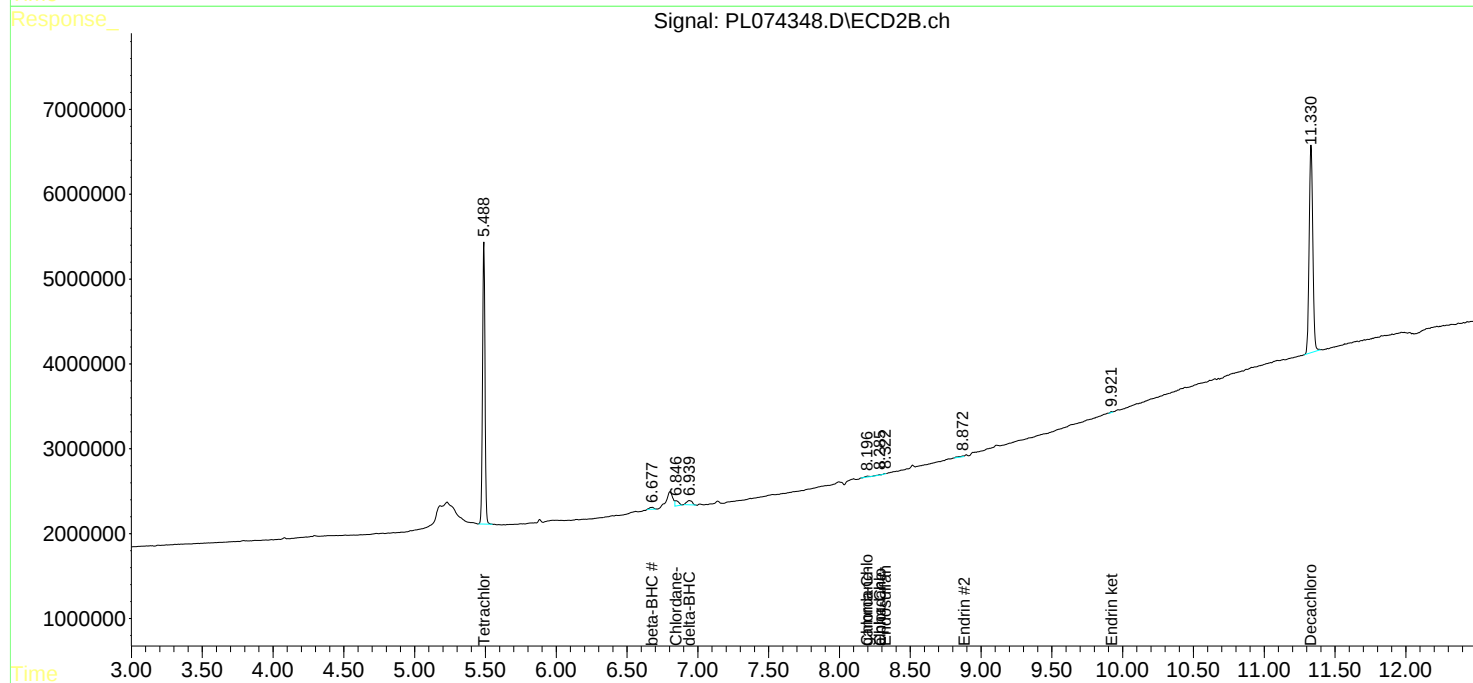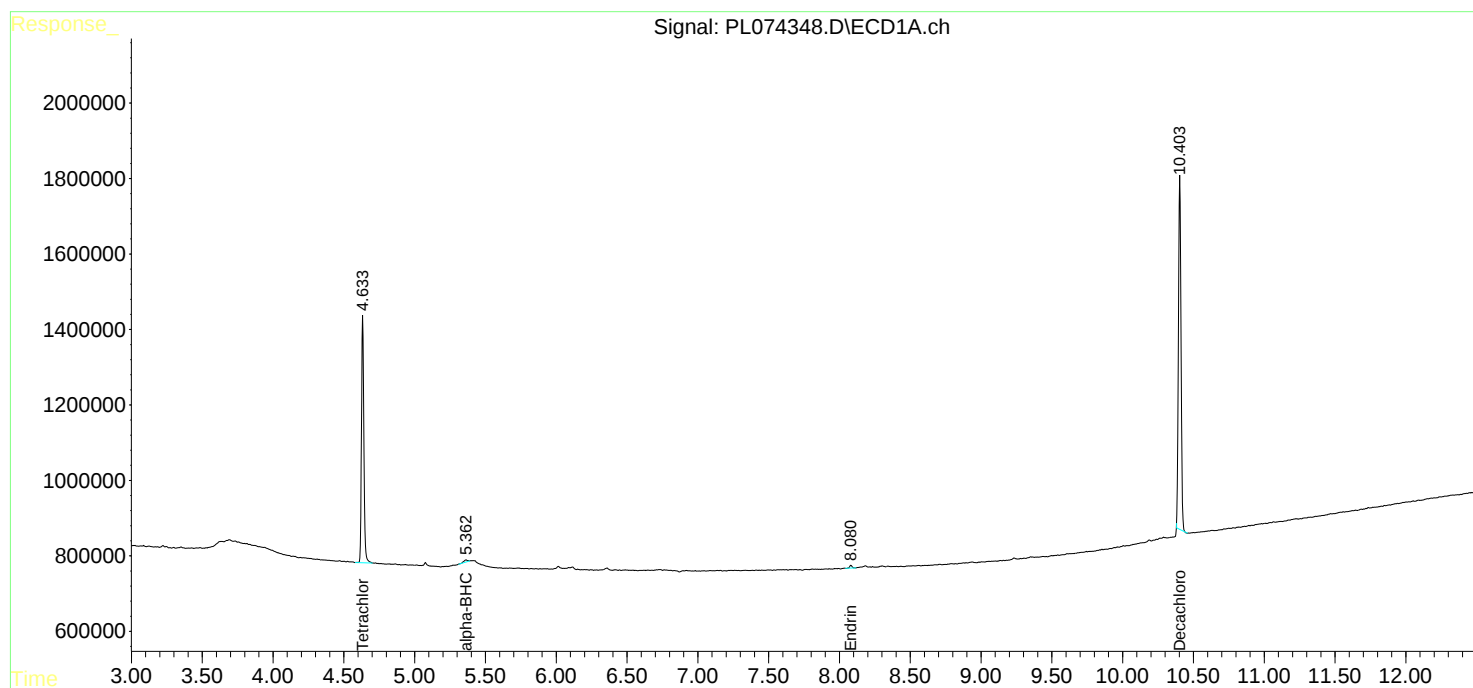


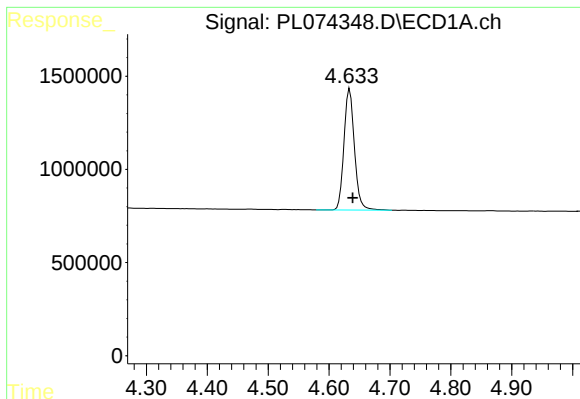

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: -0.005 min
Response: 7769074
Conc: 24.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

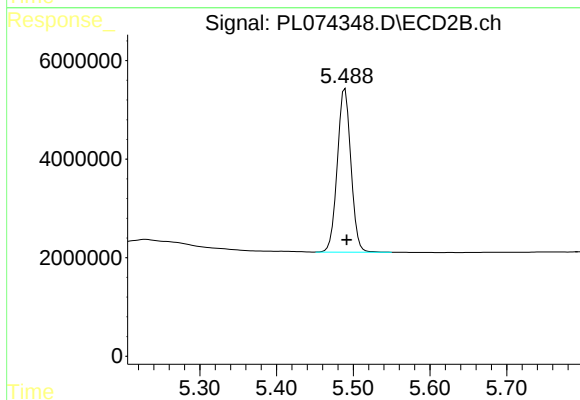


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 40830616
Conc: 22.90 ng/ml

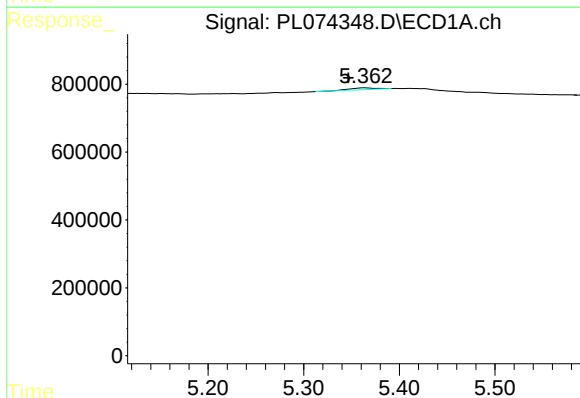


#2 alpha-BHC

R.T.: 5.364 min
Delta R.T.: 0.017 min
Response: 103692
Conc: 0.25 ng/ml

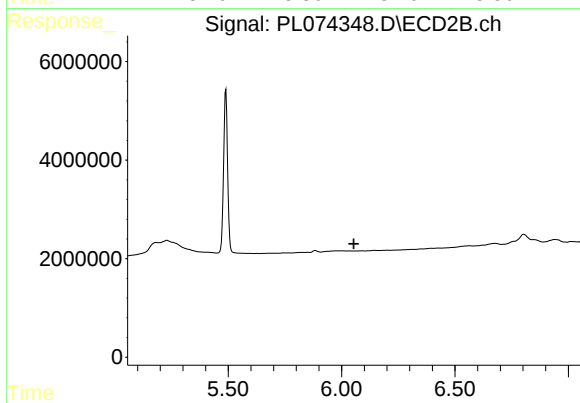

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

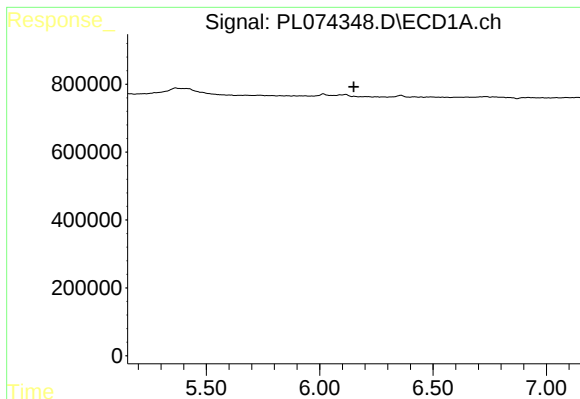

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

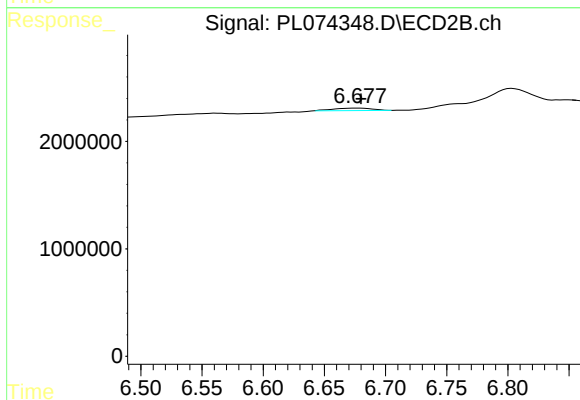


#6 beta-BHC

R.T.: 6.678 min
Delta R.T.: -0.001 min
Response: 502296
Conc: 0.45 ng/ml

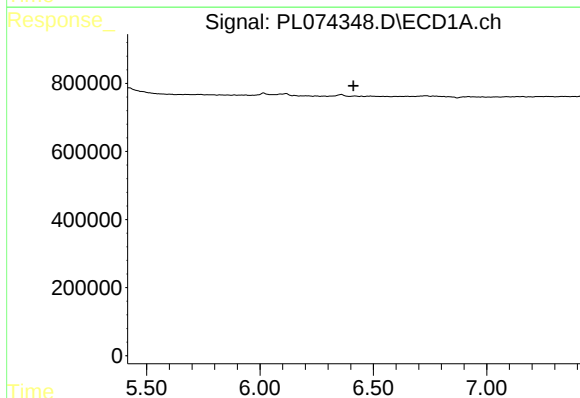


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

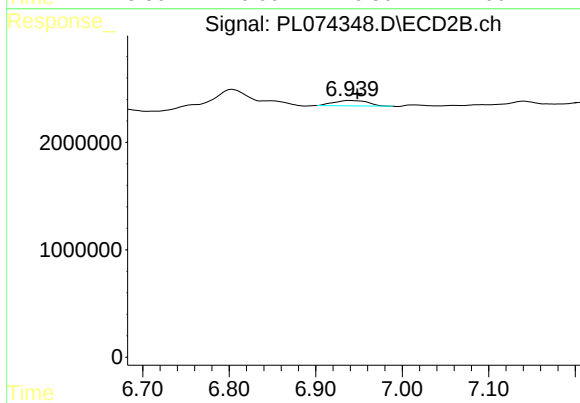

#7 delta-BHC


R.T.: 6.940 min
Delta R.T.: -0.008 min
Response: 1349097
Conc: 0.55 ng/ml

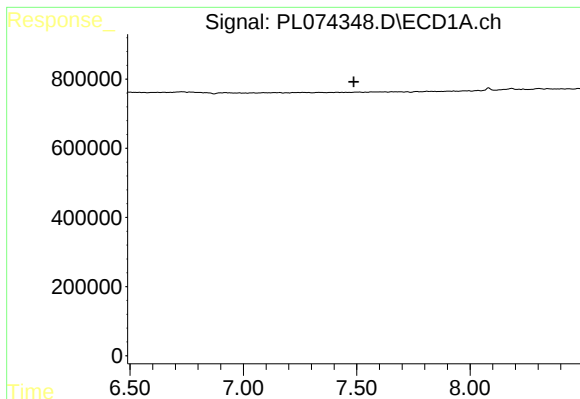

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

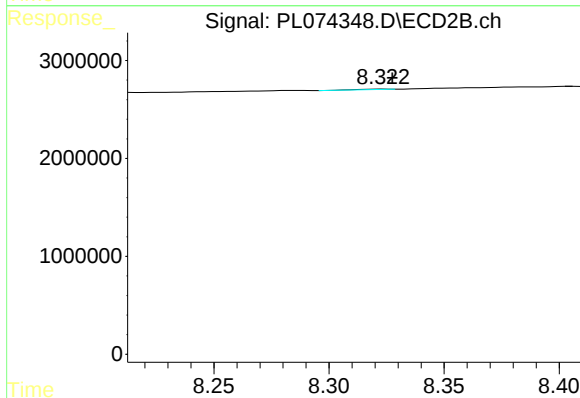


#9 Endosulfan I

R.T.: 8.324 min
Delta R.T.: -0.004 min
Response: 29973
Conc: 0.02 ng/ml

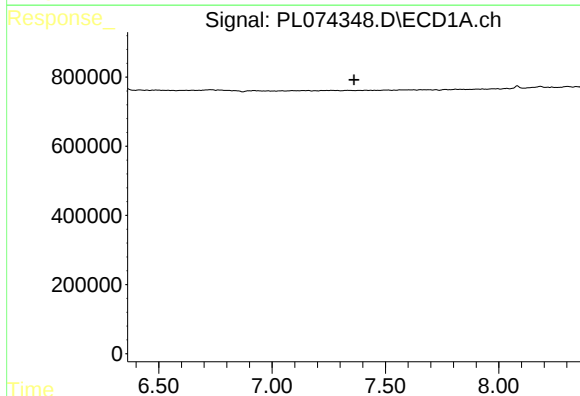


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

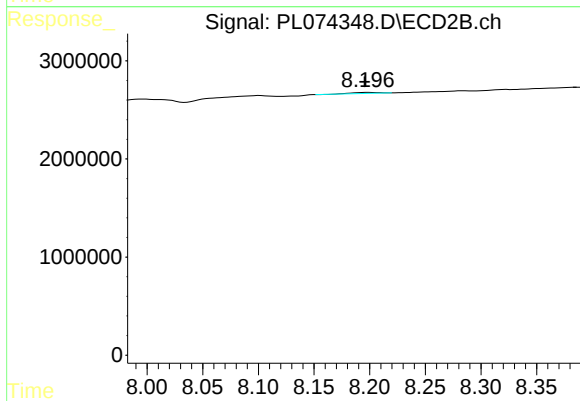

#10 gamma-Chlordane


R.T.: 8.198 min
Delta R.T.: 0.003 min
Response: 172382
Conc: 0.08 ng/ml

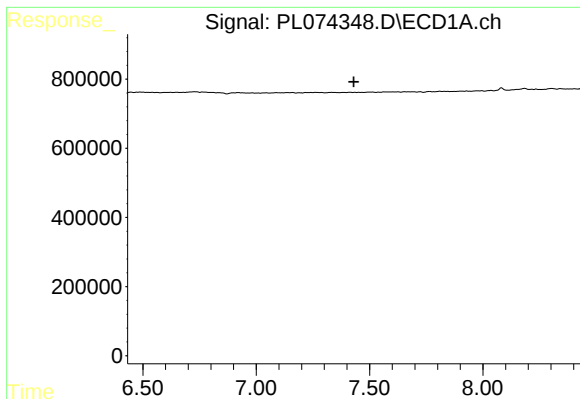

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

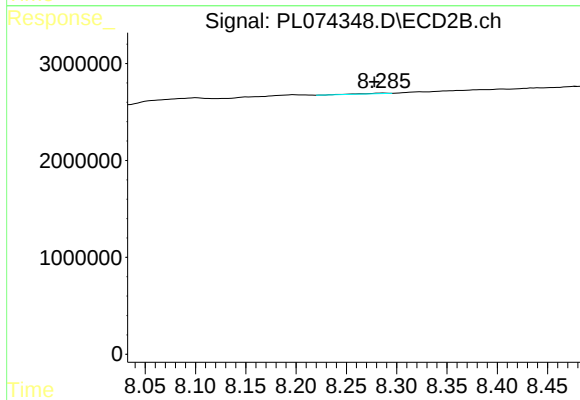


#11 alpha-Chlordane

R.T.: 8.285 min
Delta R.T.: 0.007 min
Response: 72627
Conc: 0.03 ng/ml

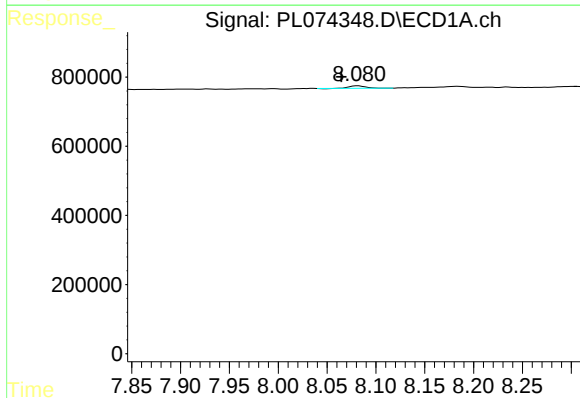


#14 Endrin

R.T.: 8.081 min
Delta R.T.: 0.017 min
Response: 85444
Conc: 0.21 ng/ml

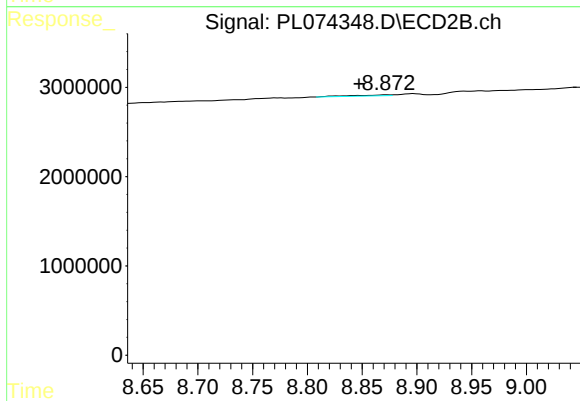

#14 Endrin


R.T.: 8.873 min
Delta R.T.: 0.026 min
Response: 241863
Conc: 0.14 ng/ml

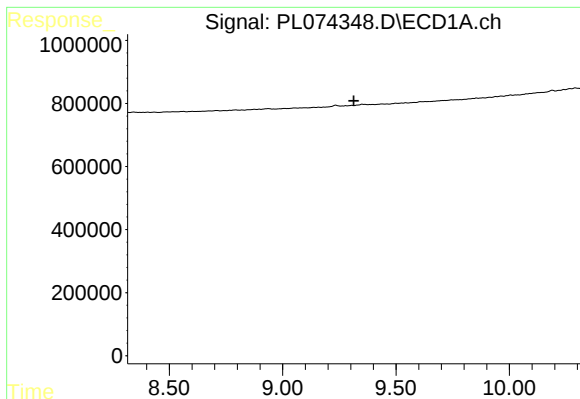

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

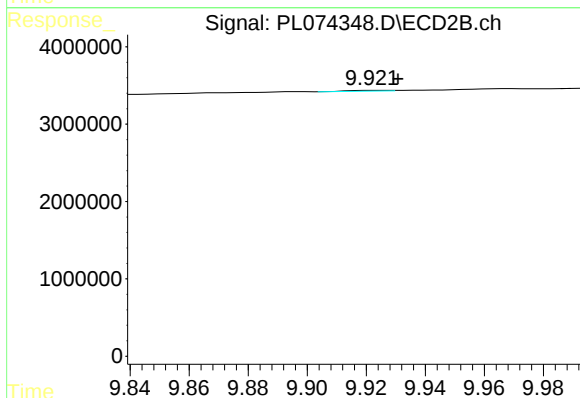


#21 Endrin ketone

R.T.: 9.922 min
Delta R.T.: -0.008 min
Response: 94875
Conc: 0.05 ng/ml

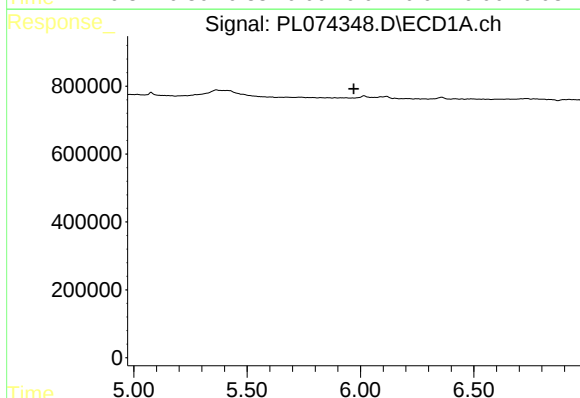


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

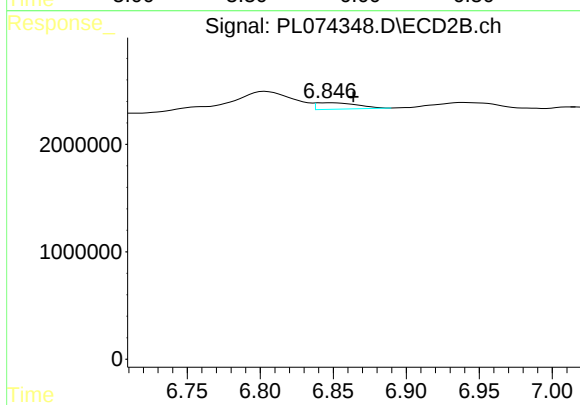

#23 Chlordane-1


R.T.: 6.848 min
Delta R.T.: -0.016 min
Response: 1159042
Conc: 14.52 ng/ml

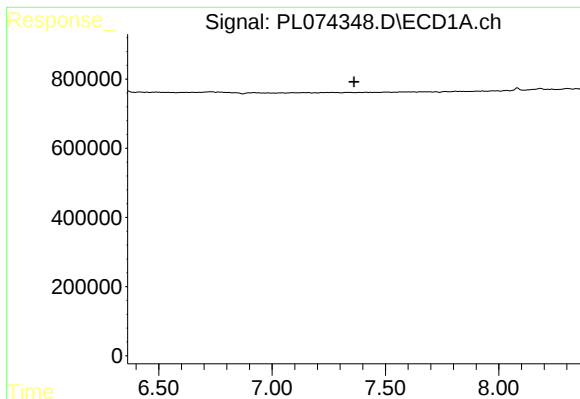

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

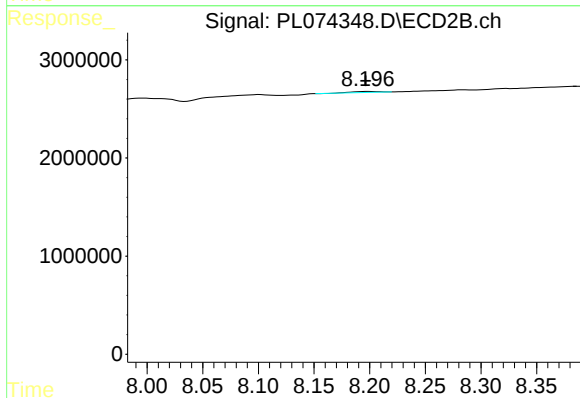


#25 Chlordane-3

R.T.: 8.198 min
Delta R.T.: 0.002 min
Response: 172382
Conc: 0.51 ng/ml

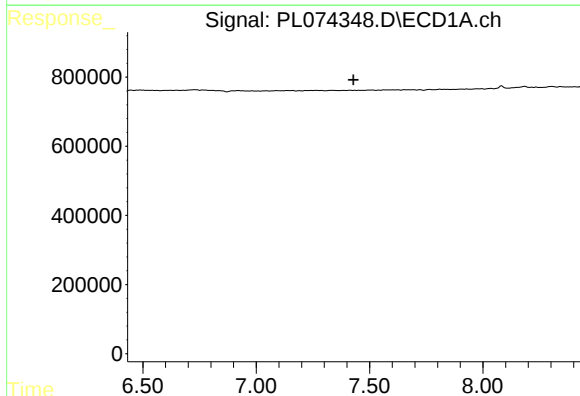


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

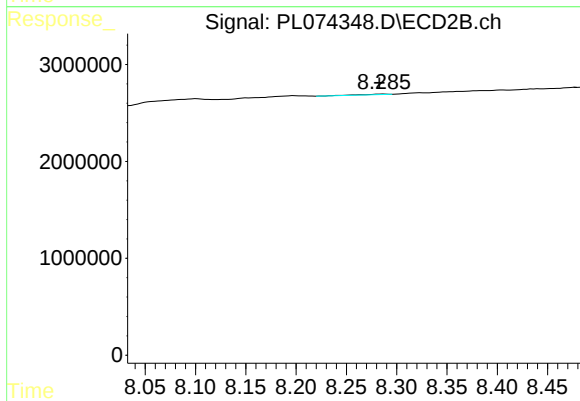

#26 Chlordane-4


R.T.: 8.285 min
Delta R.T.: 0.003 min
Response: 72627
Conc: 0.18 ng/ml

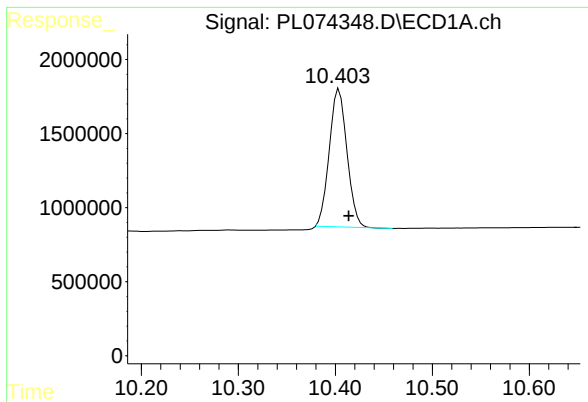

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 11787707
Conc: 22.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

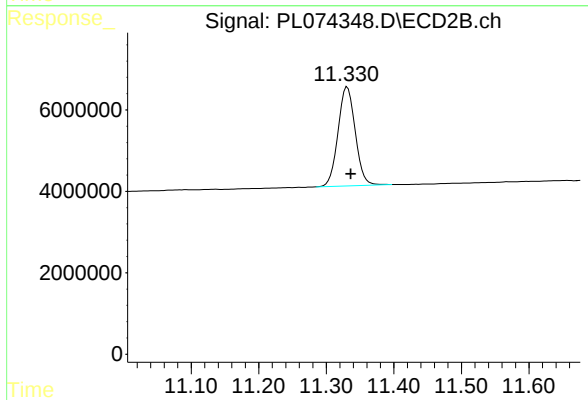

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: -0.005 min
Response: 43097910
Conc: 24.40 ng/ml