

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
 Data File : PL074358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 00:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 02:09:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.490	7937886	41661281	24.567	23.366
28)	SA Decachlor...	10.405	11.332	11896672	43594250	22.877	24.681
Target Compounds							
2)	A alpha-BHC	5.364f	0.000	9830	0	0.023	N.D. #
6)	B beta-BHC	0.000	6.678	0	710963	N.D.	0.631 #
7)	B delta-BHC	0.000	6.938	0	1394026	N.D.	0.571 #
10)	B gamma-Chl...	0.000	8.196	0	277304	N.D.	0.124 #
12)	B 4,4'-DDE	0.000	8.479f	0	69625	N.D.	0.035 #
14)	MA Endrin	8.082f	8.853	72915	208246	0.179	0.123 #
19)	B Endosulfa...	0.000	9.443	0	67184	N.D.	0.040 #
20)	A Methoxychlor	9.068f	0.000	28902	0	0.116	N.D. #
21)	B Endrin ke...	0.000	9.923	0	127804	N.D.	0.074 #
23)	Chlordane-1	0.000	6.855	0	772139	N.D.	9.676 #
24)	Chlordane-2	0.000	7.437	0	196438	N.D.	2.377 #
25)	Chlordane-3	0.000	8.196	0	277304	N.D.	0.820 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
Data File : PL074358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 00:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 02:09:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

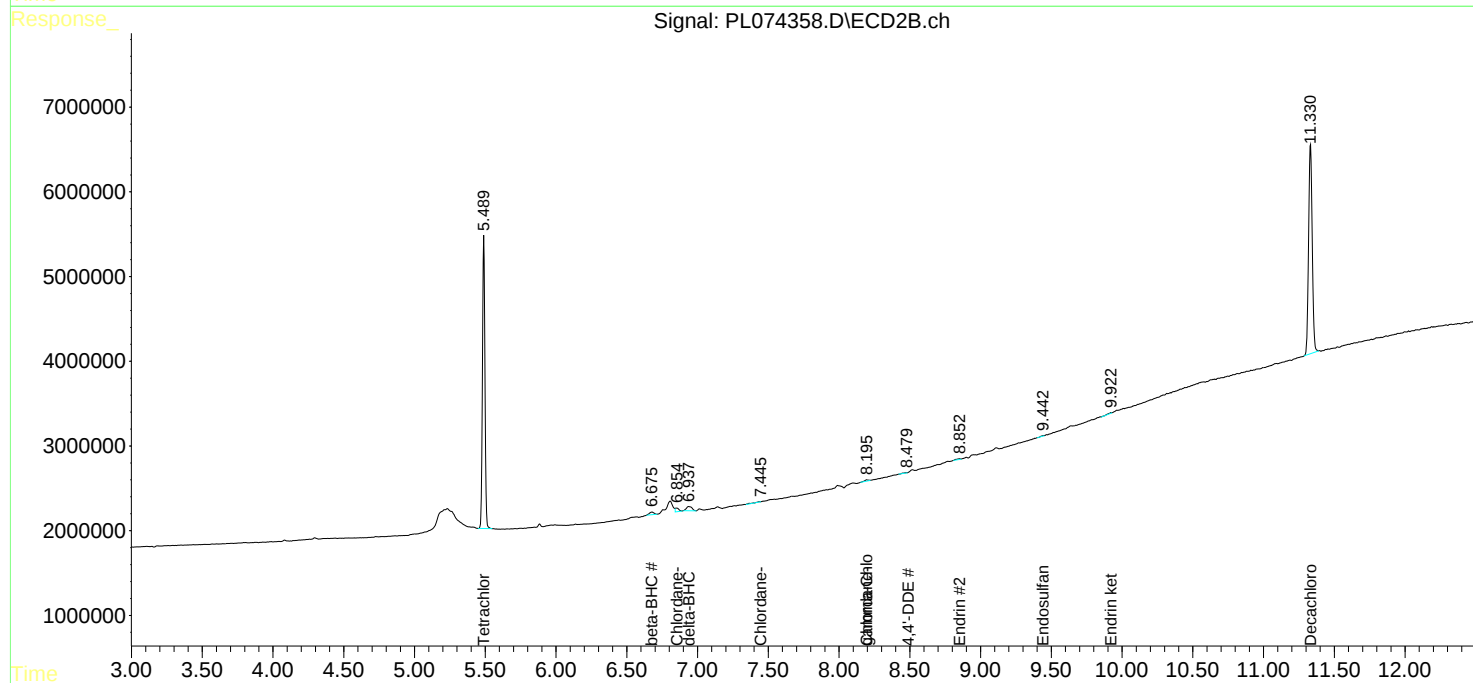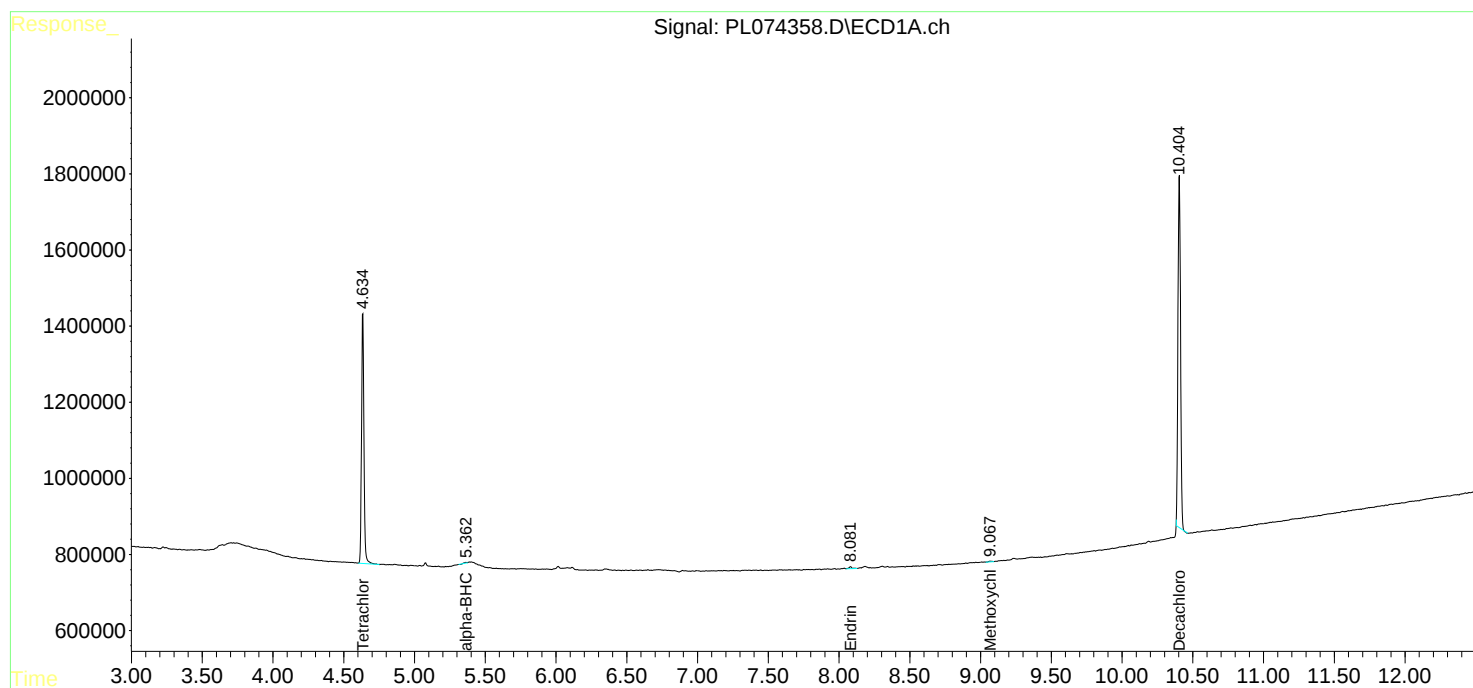


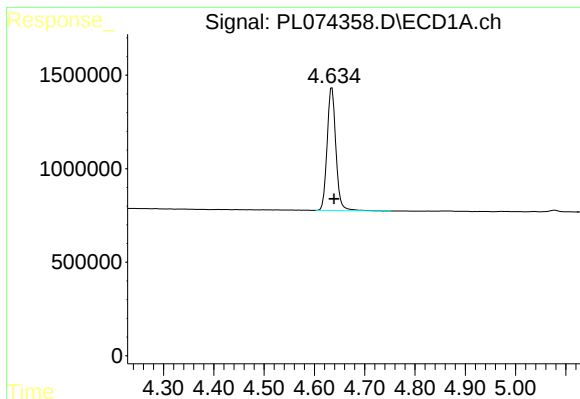

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 7937886
Conc: 24.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

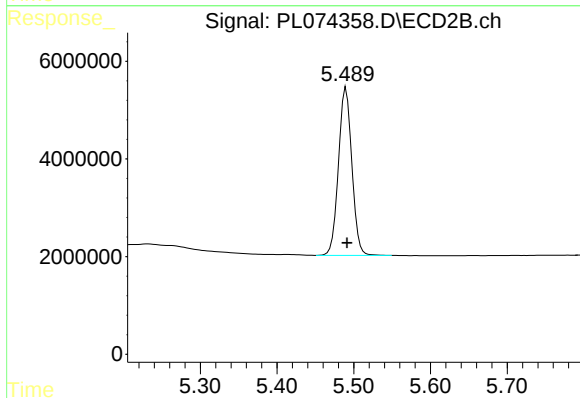


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.002 min
Response: 41661281
Conc: 23.37 ng/ml

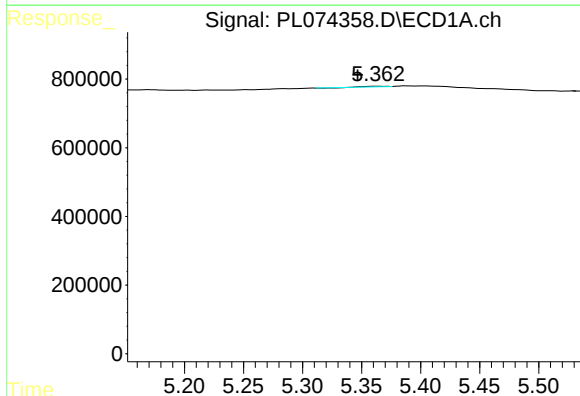


#2 alpha-BHC

R.T.: 5.364 min
Delta R.T.: 0.017 min
Response: 9830
Conc: 0.02 ng/ml

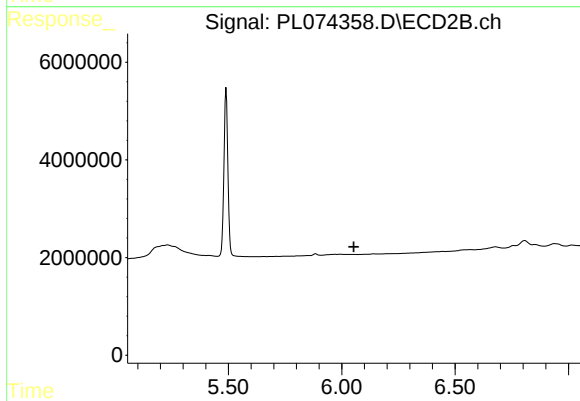

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

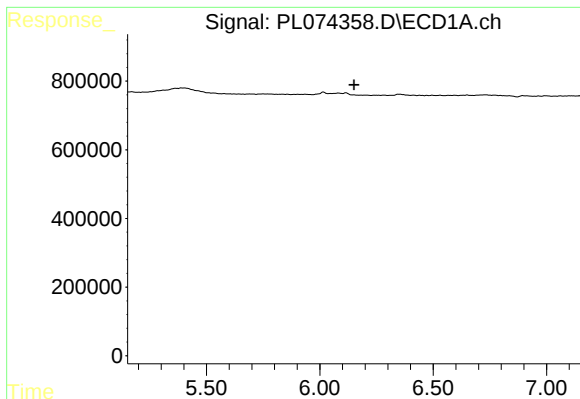

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

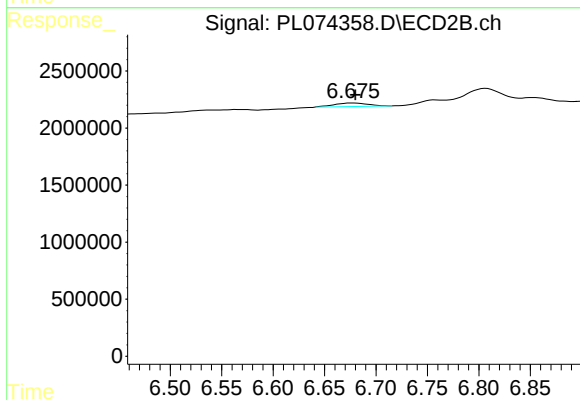


#6 beta-BHC

R.T.: 6.678 min
Delta R.T.: -0.002 min
Response: 710963
Conc: 0.63 ng/ml

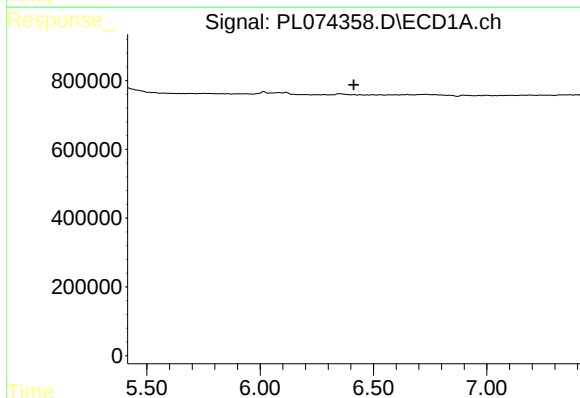


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

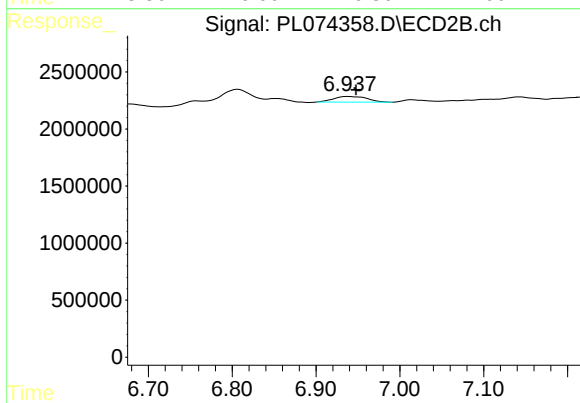

#7 delta-BHC


R.T.: 6.938 min
Delta R.T.: -0.010 min
Response: 1394026
Conc: 0.57 ng/ml

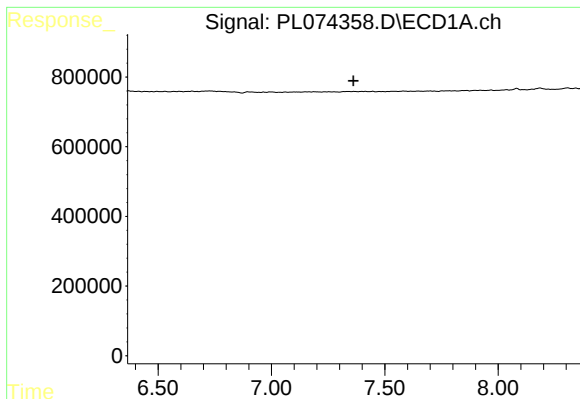

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

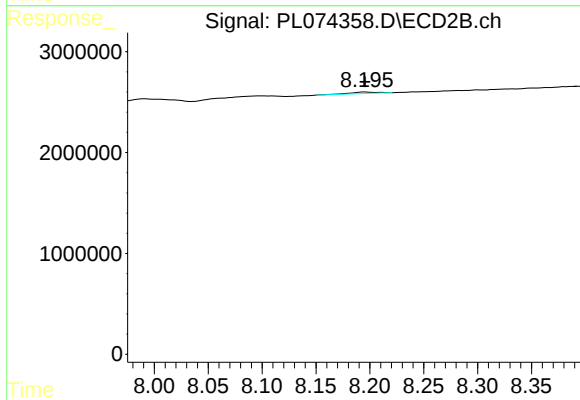


#10 gamma-Chlordane

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 277304
Conc: 0.12 ng/ml

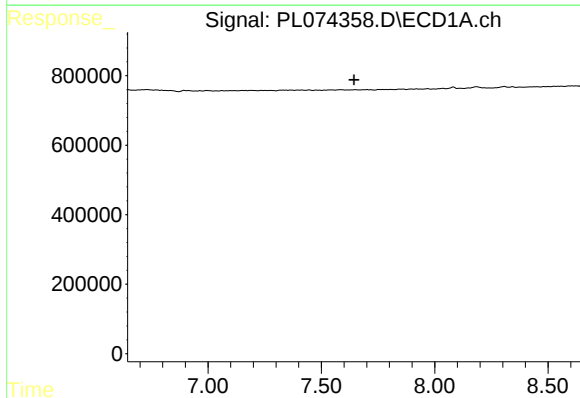


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

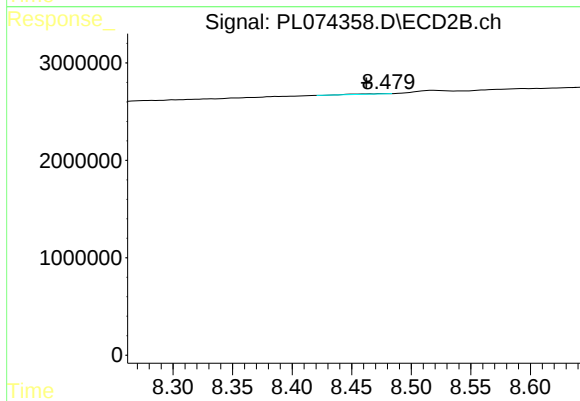

#12 4,4'-DDE


R.T.: 8.479 min
Delta R.T.: 0.017 min
Response: 69625
Conc: 0.03 ng/ml

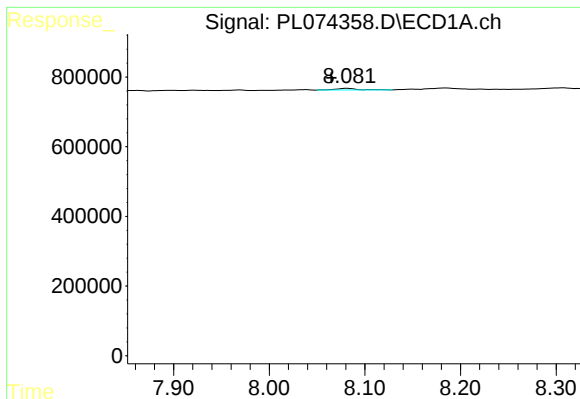

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 72915
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

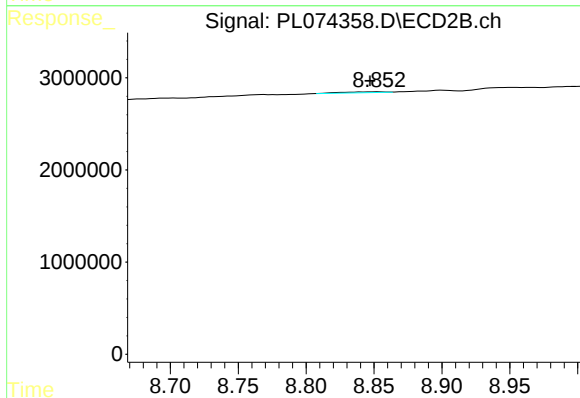


#14 Endrin

R.T.: 8.853 min
Delta R.T.: 0.006 min
Response: 208246
Conc: 0.12 ng/ml

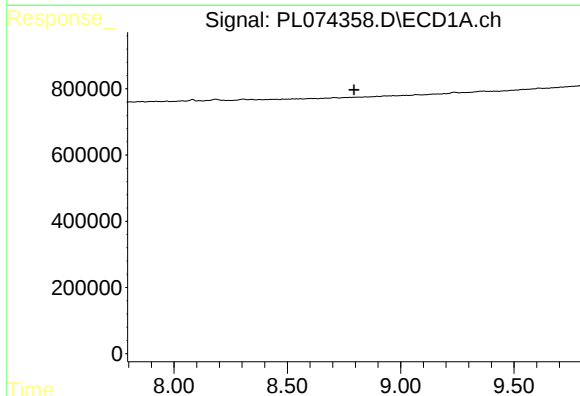


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

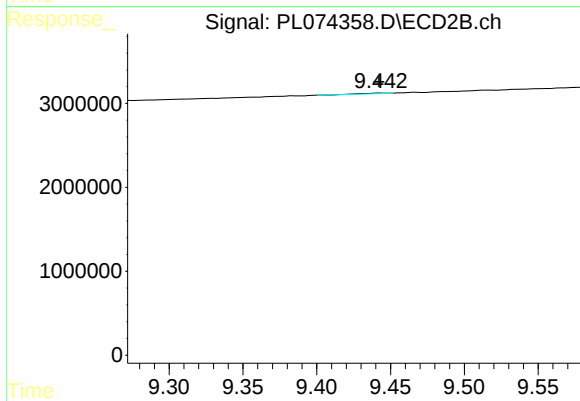

#19 Endosulfan Sulfate


R.T.: 9.443 min
Delta R.T.: 0.000 min
Response: 67184
Conc: 0.04 ng/ml

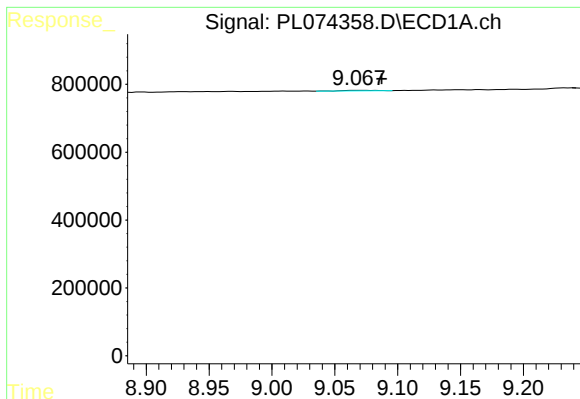

#20 Methoxychlor


R.T.: 9.068 min
Delta R.T.: -0.019 min
Response: 28902
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

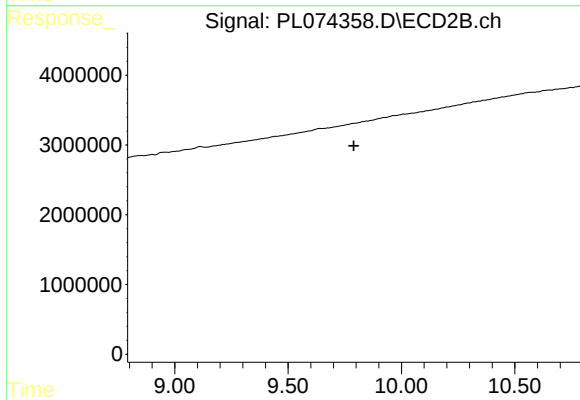


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.789 min
Response: 0
Conc: N.D.

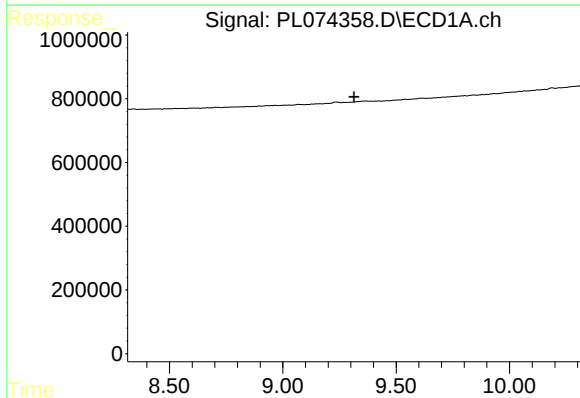


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.314 min
Response: 0
Conc: N.D.

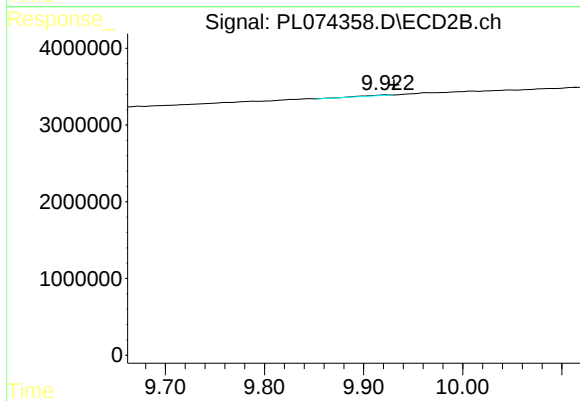

#21 Endrin ketone


R.T.: 9.923 min
Delta R.T.: -0.008 min
Response: 127804
Conc: 0.07 ng/ml

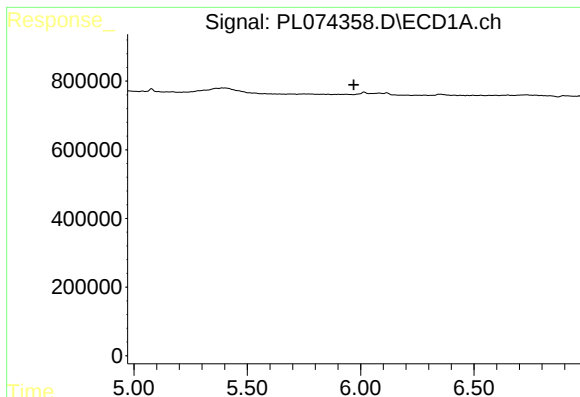

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

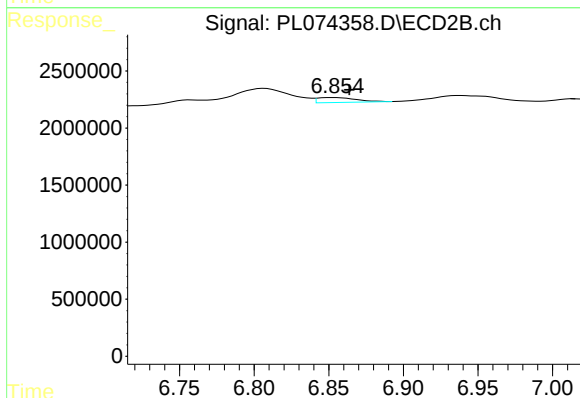


#23 Chlordane-1

R.T.: 6.855 min
Delta R.T.: -0.009 min
Response: 772139
Conc: 9.68 ng/ml

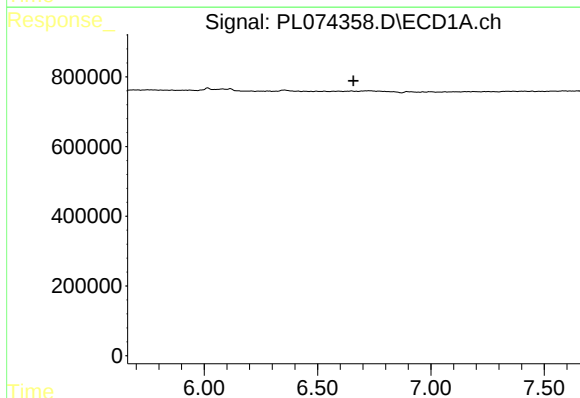


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.659 min
Response: 0
Conc: N.D.

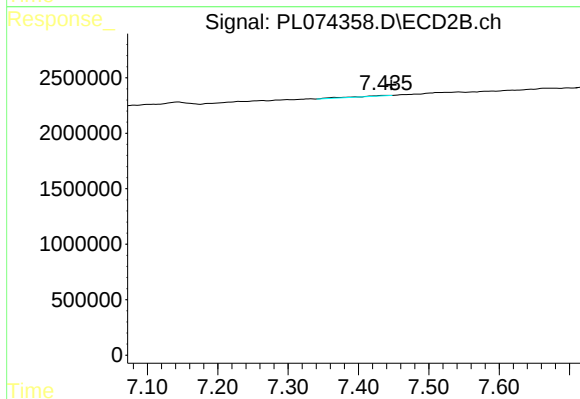

#24 Chlordane-2


R.T.: 7.437 min
Delta R.T.: -0.010 min
Response: 196438
Conc: 2.38 ng/ml

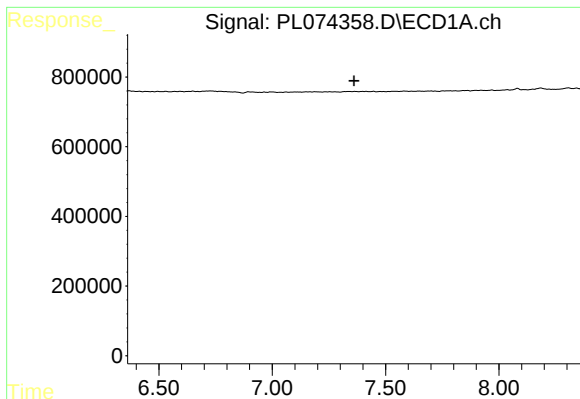

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

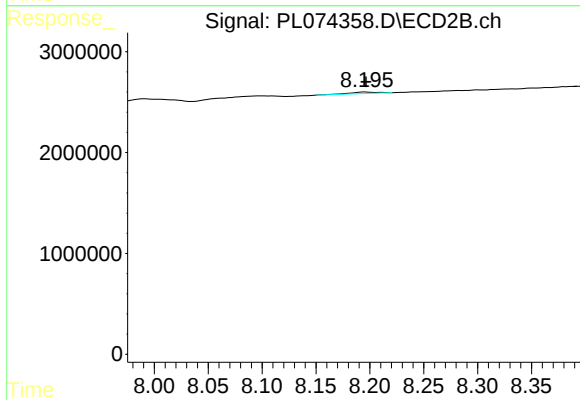


#25 Chlordane-3

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 277304
Conc: 0.82 ng/ml

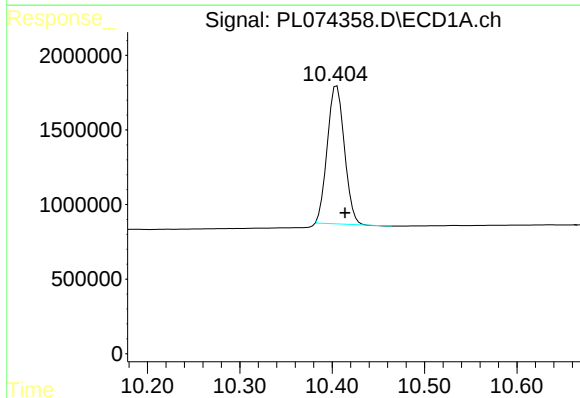

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 11896672
Conc: 22.88 ng/ml

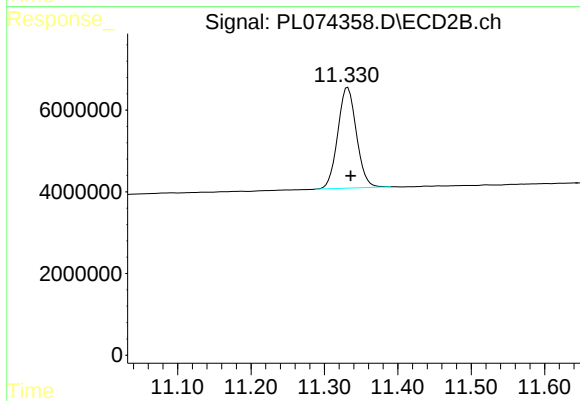

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: -0.004 min
Response: 43594250
Conc: 24.68 ng/ml