

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042523\
 Data File : PL082328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2023 14:47
 Operator : AR\AJ
 Sample : 02483-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S2S-TP2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 21:37:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.647	52912713	45685833	19.809	19.720
28) SA Decachlor...	8.740	7.758	37104602	39626176	19.436	17.361
Target Compounds						
17) MA 4,4'-DDT	6.778	5.884	2078394	2659429	0.909	1.259 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042523\
Data File : PL082328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2023 14:47
Operator : AR\AJ
Sample : 02483-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S2S-TP2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 21:37:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

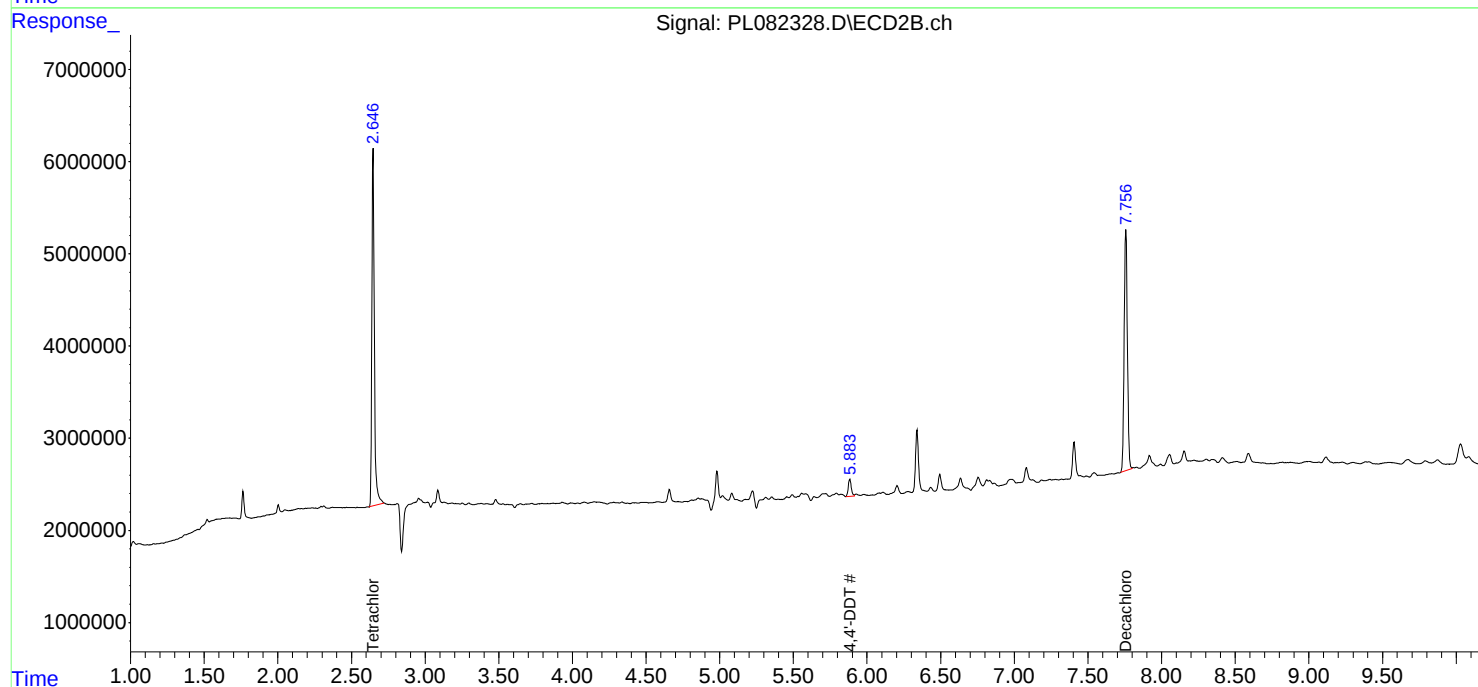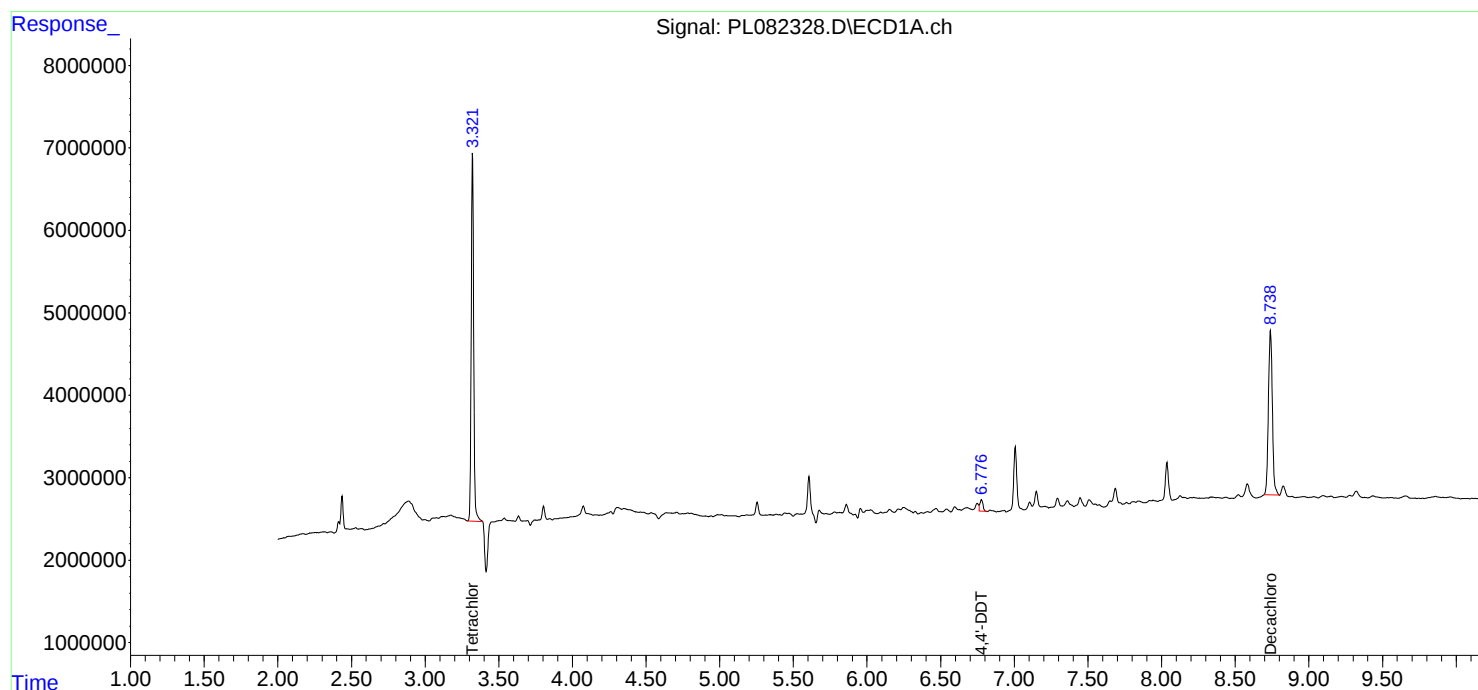


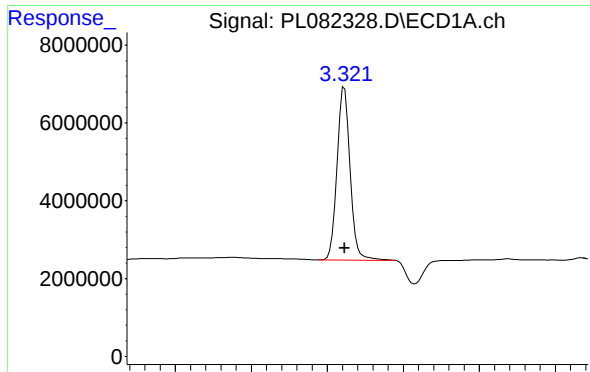

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 52912713
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2S-TP2

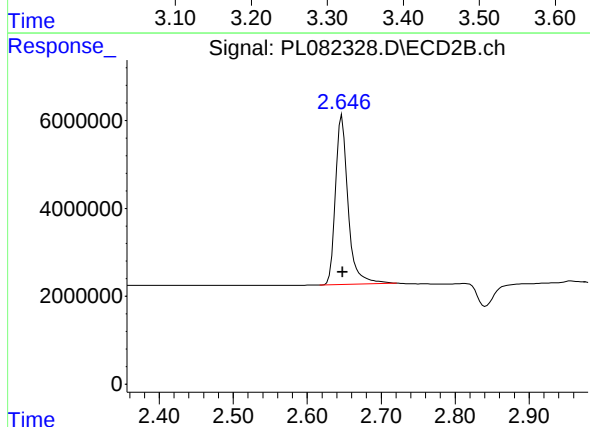


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: -0.001 min
Response: 45685833
Conc: 19.72 ng/ml

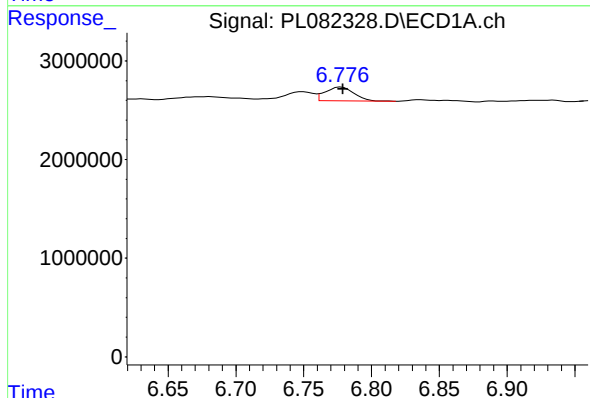


#17 4,4'-DDT

R.T.: 6.778 min
Delta R.T.: -0.001 min
Response: 2078394
Conc: 0.91 ng/ml

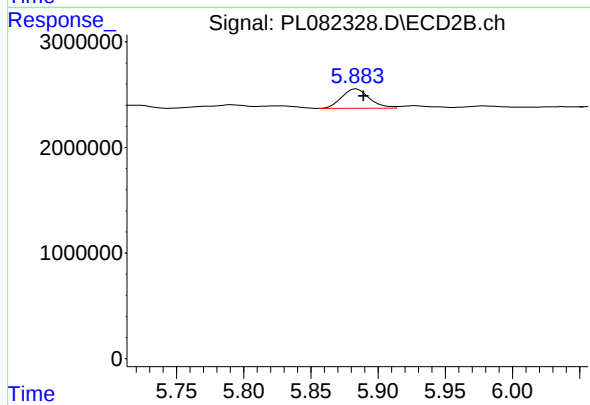

#17 4,4'-DDT


R.T.: 5.884 min
Delta R.T.: -0.005 min
Response: 2659429
Conc: 1.26 ng/ml

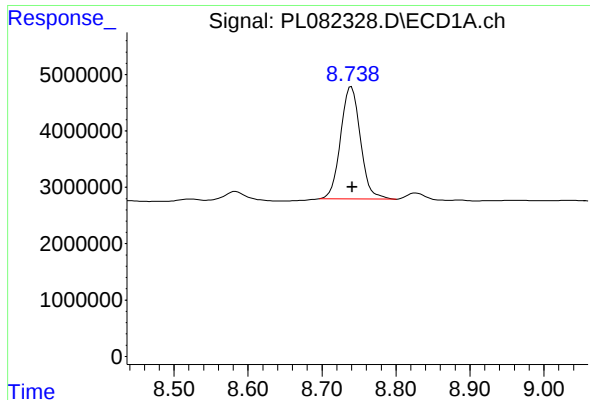

#28 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.001 min
Response: 37104602
Conc: 19.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2S-TP2

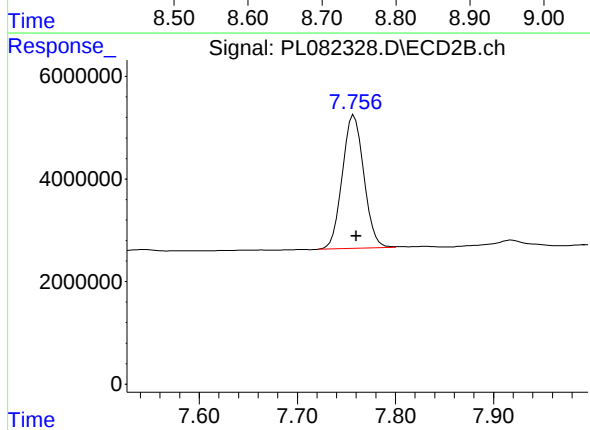

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 39626176
Conc: 17.36 ng/ml