

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
 Data File : PL047844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 10:18
 Operator : AJ\SJ
 Sample : K2569-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-004-SW021-042319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 23:06:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.943	196.7E6	48936087	21.274	20.499
28)	SA Decachlor...	8.004	8.984	161.4E6	43991584	14.417	15.411
Target Compounds							
20)	A Methoxychlor	0.000	7.549f	0	2646157	N.D.	1.887 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
Data File : PL047844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 10:18
Operator : AJ\SJ
Sample : K2569-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-004-SW021-042319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 23:06:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

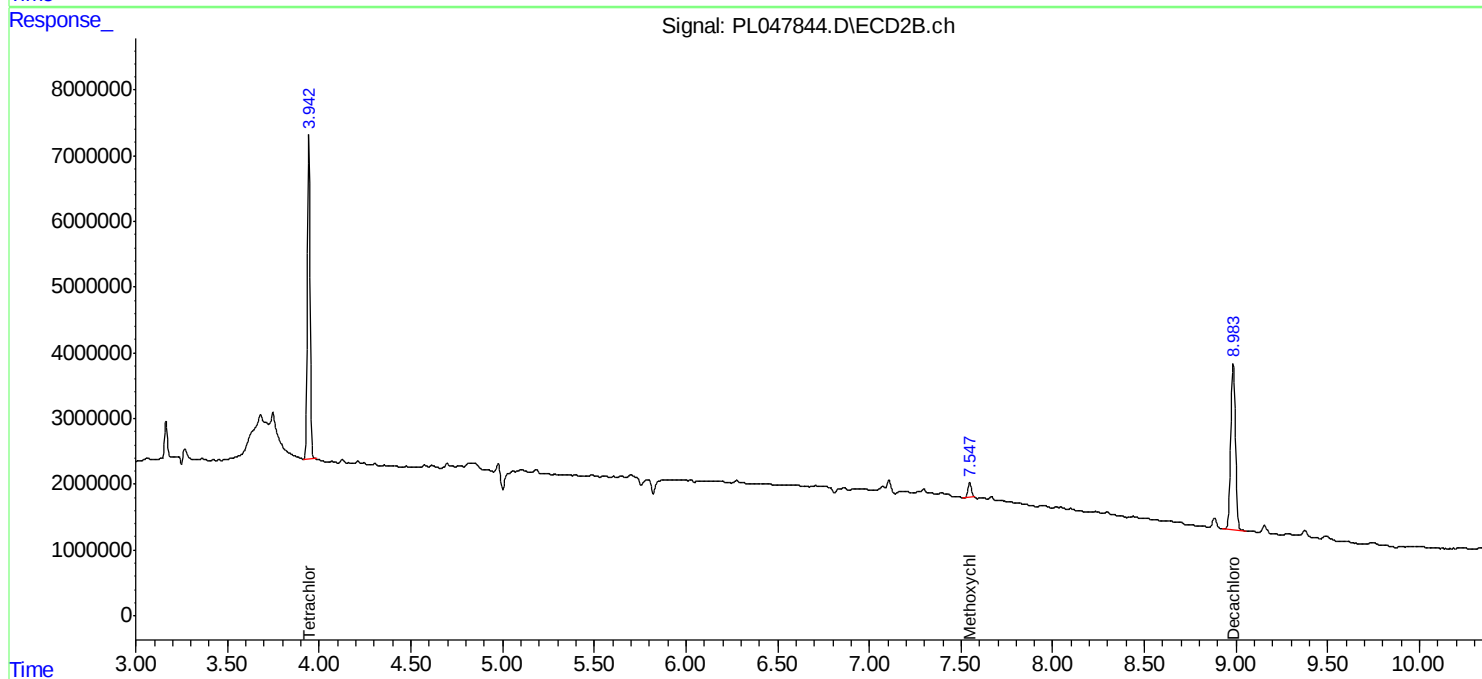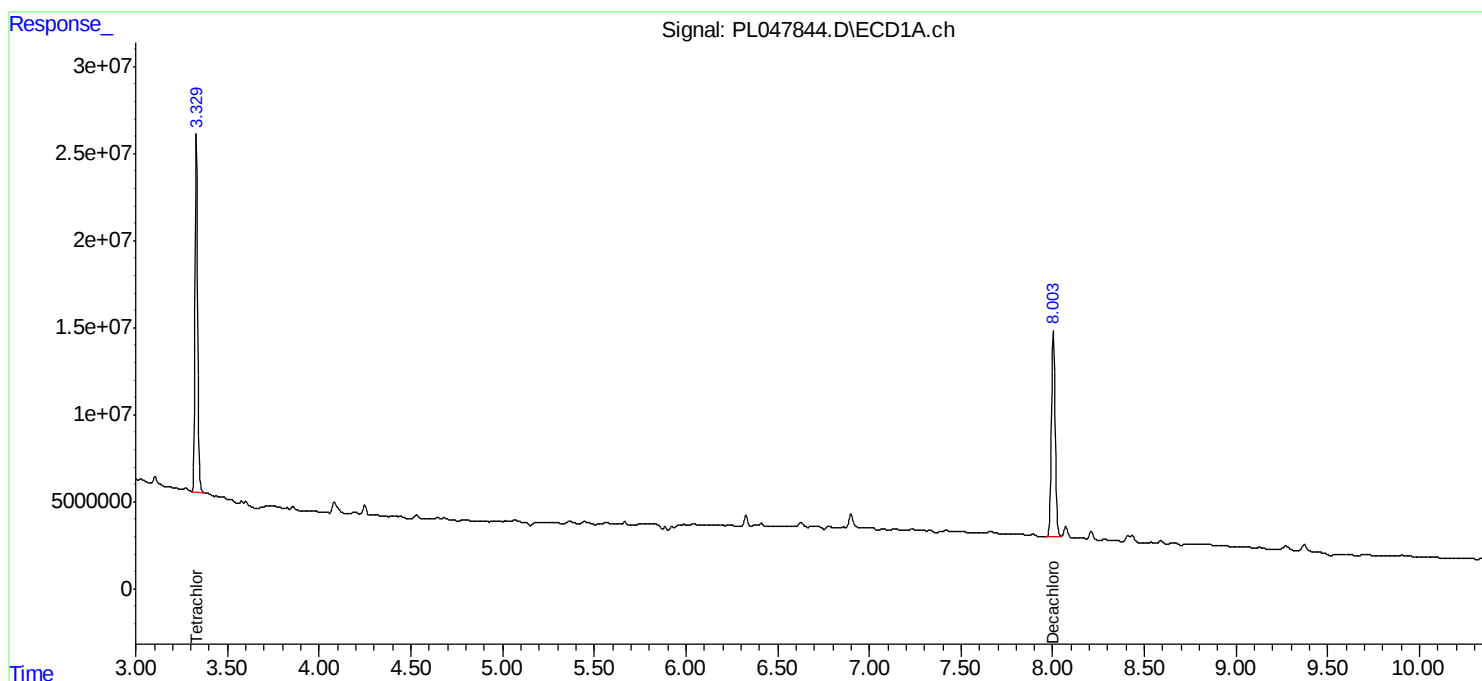


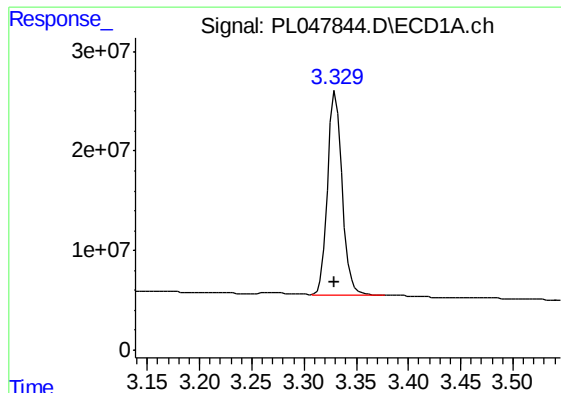

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 196743719
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-SW021-042319

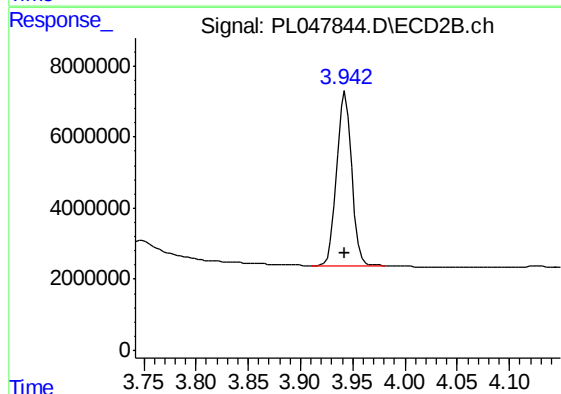


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.001 min
Response: 48936087
Conc: 20.50 ng/ml

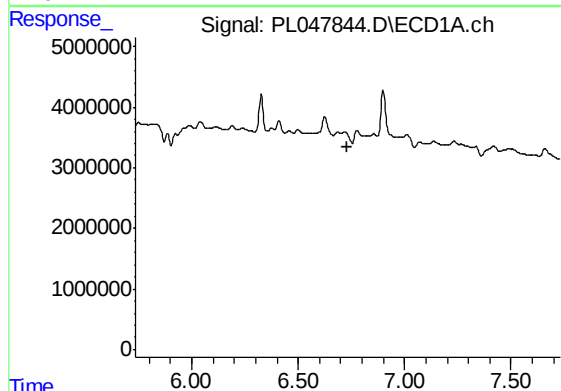


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

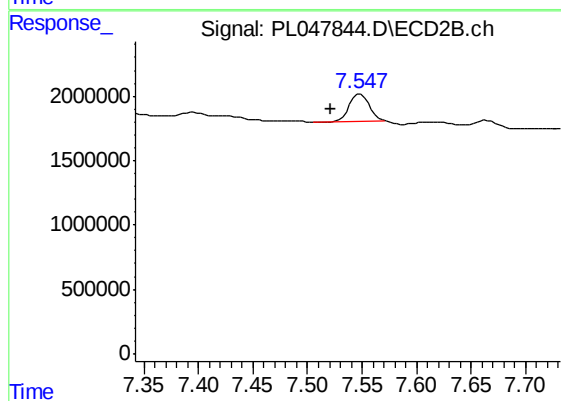

#20 Methoxychlor


R.T.: 7.549 min
Delta R.T.: 0.028 min
Response: 2646157
Conc: 1.89 ng/ml

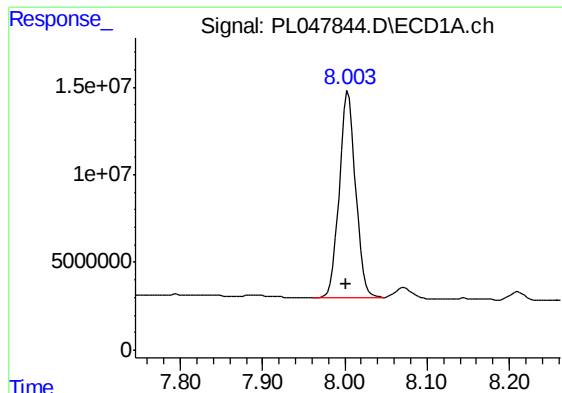

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.002 min
Response: 161384639
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-SW021-042319

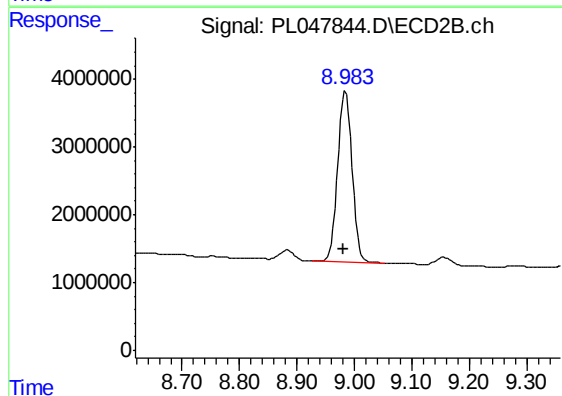

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.003 min
Response: 43991584
Conc: 15.41 ng/ml