

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
 Data File : PL047856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 13:21
 Operator : AJ\SJ
 Sample : K2569-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-003-SW024-042319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 23:09:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.942	210.4E6	54229543	22.748	22.716
28)	SA Decachlor...	8.003	8.984	200.2E6	54160554	17.880	18.973
Target Compounds							
8)	B Heptachlo...	5.006	5.803	5564820	3829249	0.434	1.370 #
10)	B gamma-Chl...	0.000	6.031	0	2082588	N.D.	0.688 #
12)	B 4,4'-DDE	5.442	6.274	43717318	16450239	3.515	5.957 #
13)	MA Dieldrin	5.556	0.000	14598683	0	1.125	N.D. #
14)	MA Endrin	5.823	0.000	11100071	0	0.934	N.D. #
15)	B Endosulfa...	0.000	6.868f	0	1655942	N.D.	0.631 #
17)	MA 4,4'-DDT	6.188	7.062	57588934	16148838	5.776	6.779
19)	B Endosulfa...	0.000	7.201	0	2110209	N.D.	0.771 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
Data File : PL047856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 13:21
Operator : AJ\SJ
Sample : K2569-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 23:09:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

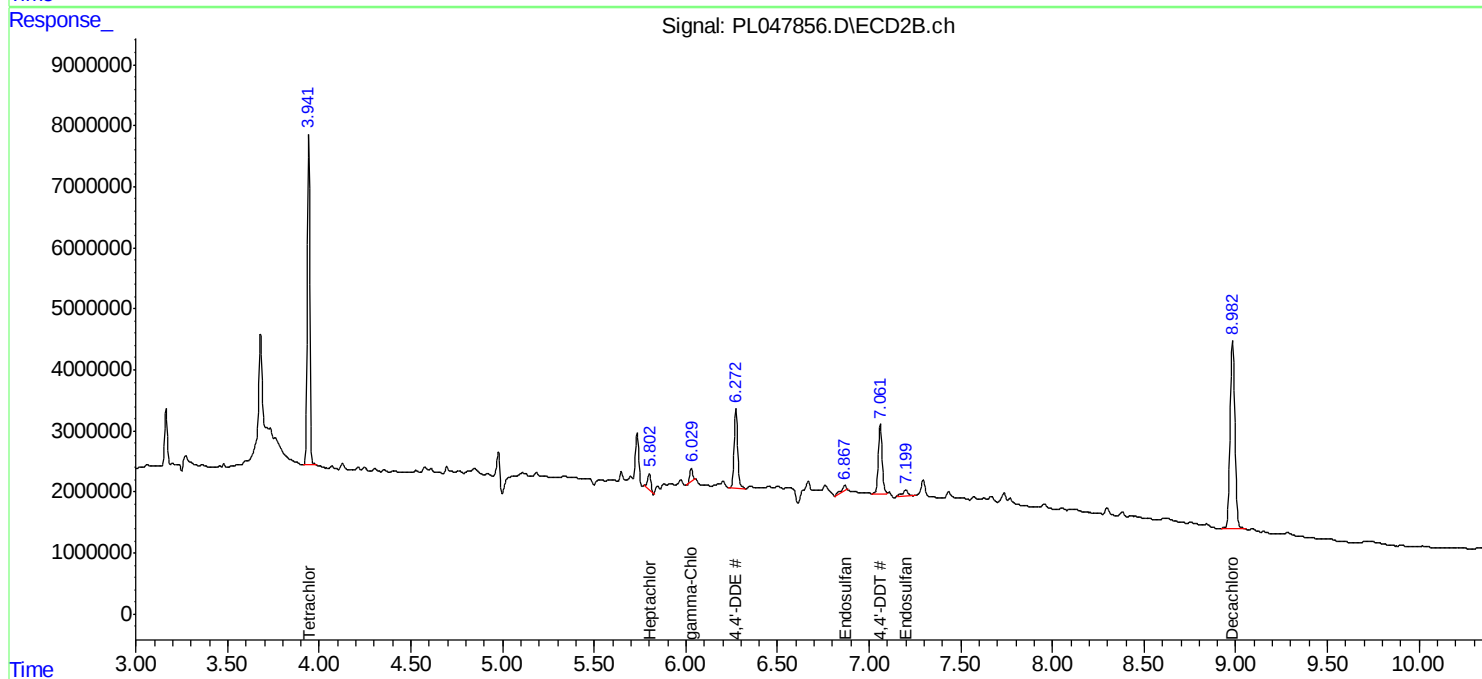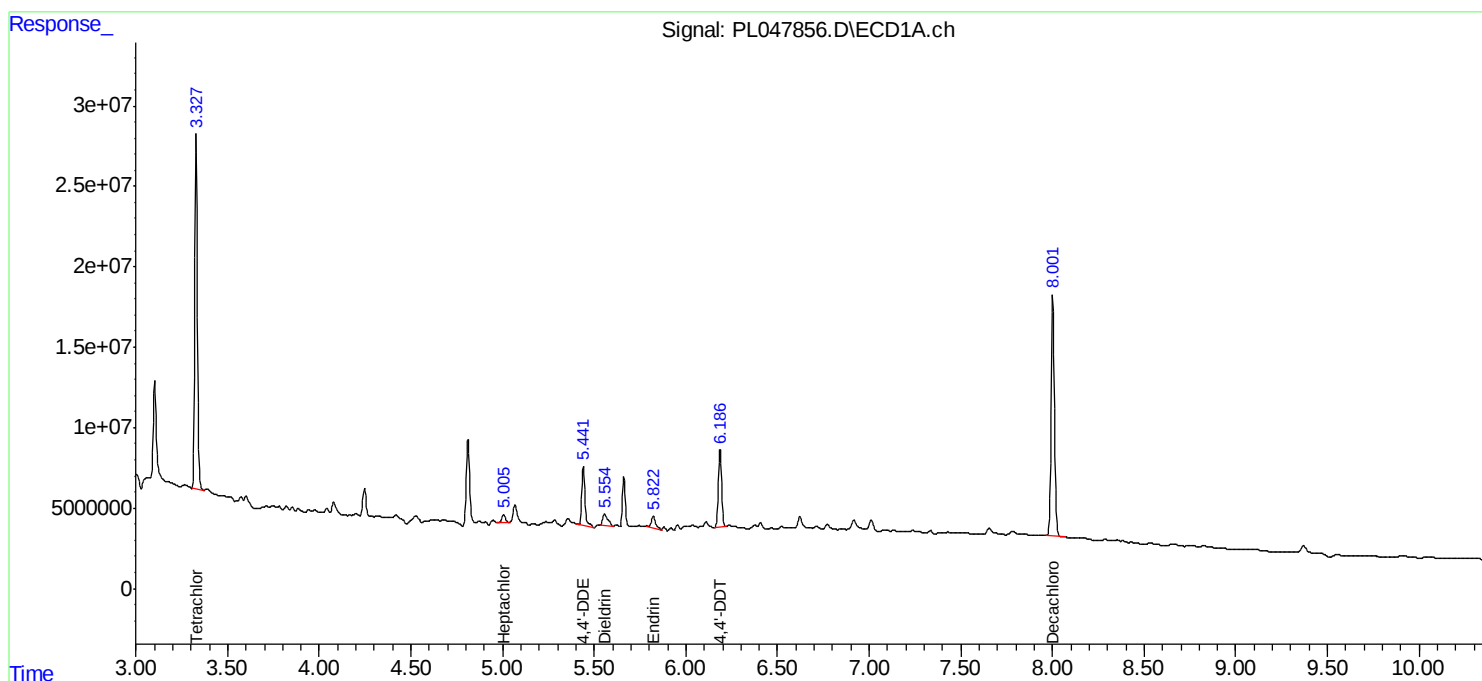


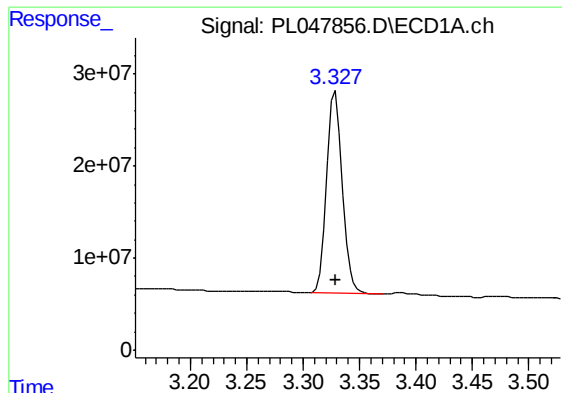

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 210376646
Conc: 22.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

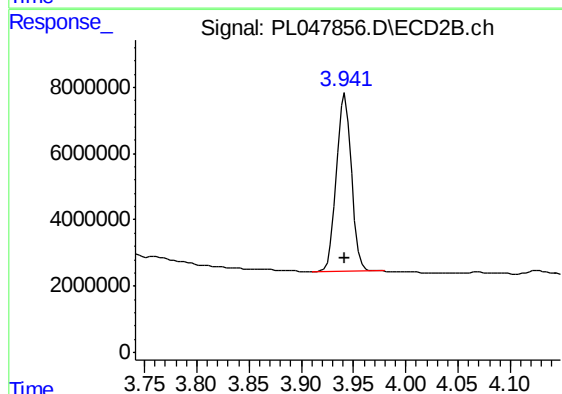


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 54229543
Conc: 22.72 ng/ml

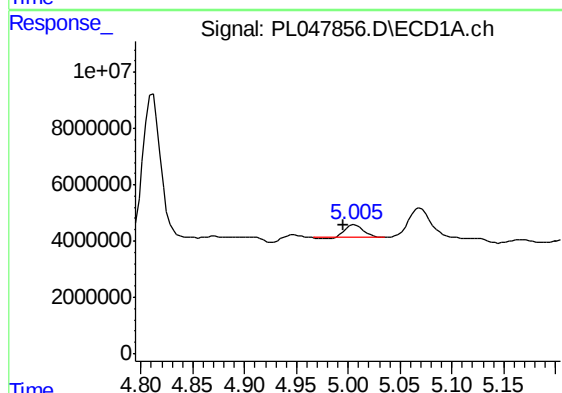


#8 Heptachlor epoxide

R.T.: 5.006 min
Delta R.T.: 0.011 min
Response: 5564820
Conc: 0.43 ng/ml

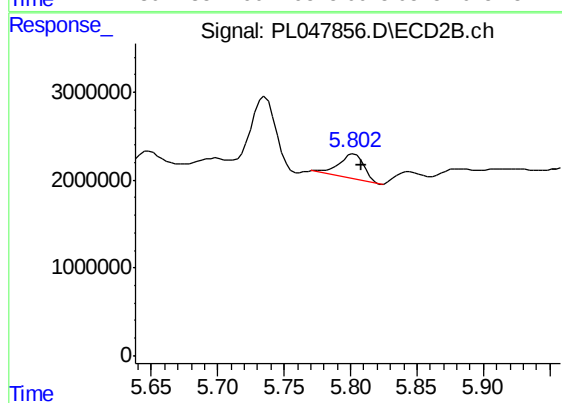

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: -0.005 min
Response: 3829249
Conc: 1.37 ng/ml

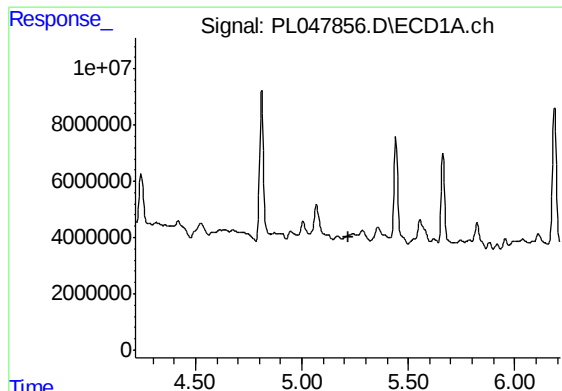

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

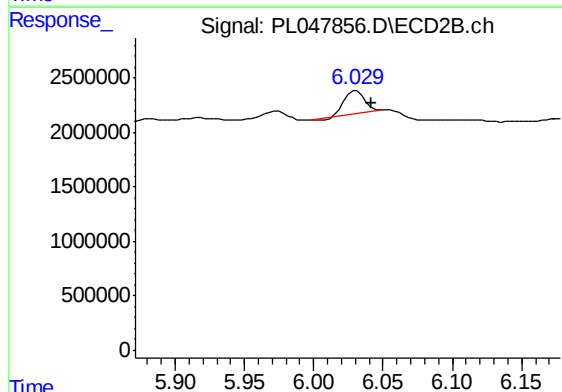


#10 gamma-Chlordane

R.T.: 6.031 min
Delta R.T.: -0.011 min
Response: 2082588
Conc: 0.69 ng/ml

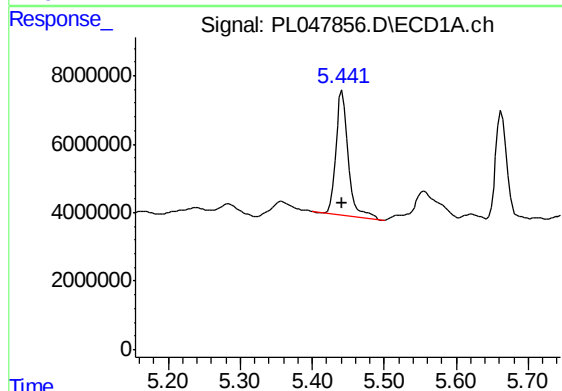


#12 4,4'-DDE

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 43717318
Conc: 3.51 ng/ml

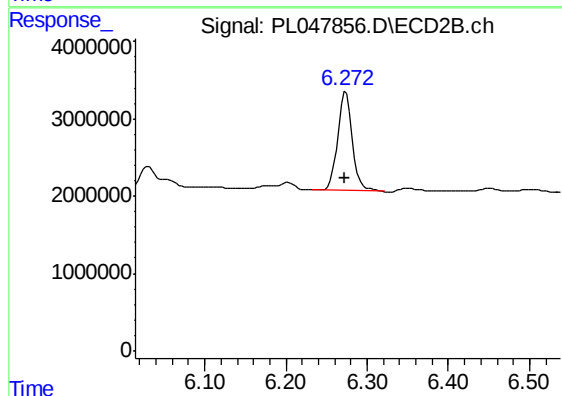

#12 4,4'-DDE


R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 16450239
Conc: 5.96 ng/ml

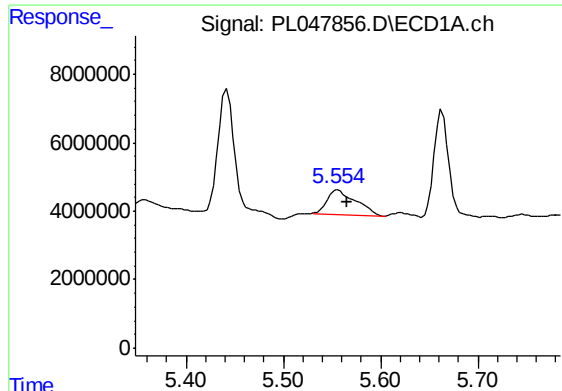

#13 Dieldrin


R.T.: 5.556 min
Delta R.T.: -0.010 min
Response: 14598683
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

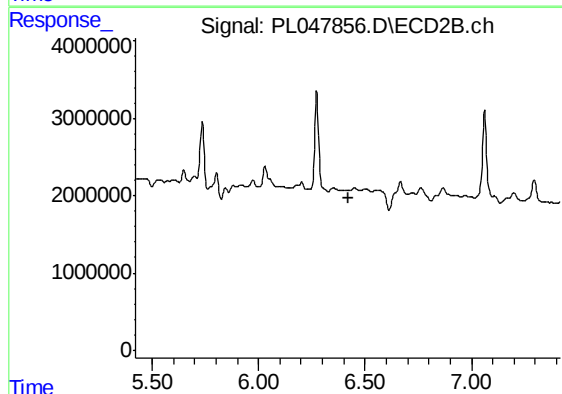


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.420 min
Response: 0
Conc: N.D.

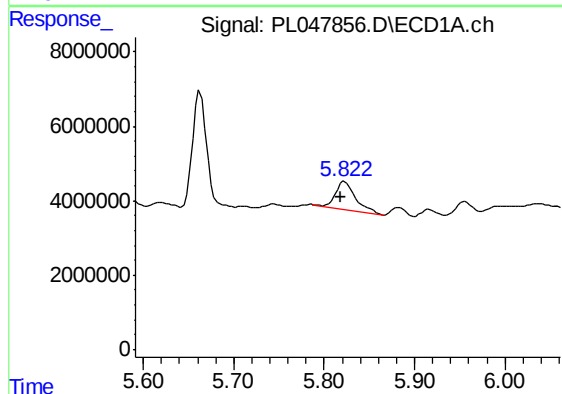


#14 Endrin

R.T.: 5.823 min
Delta R.T.: 0.005 min
Response: 11100071
Conc: 0.93 ng/ml

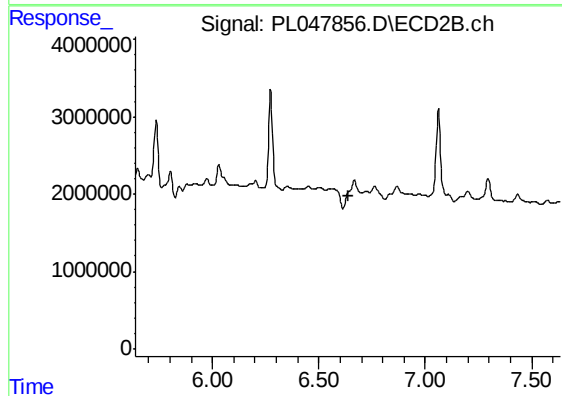

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

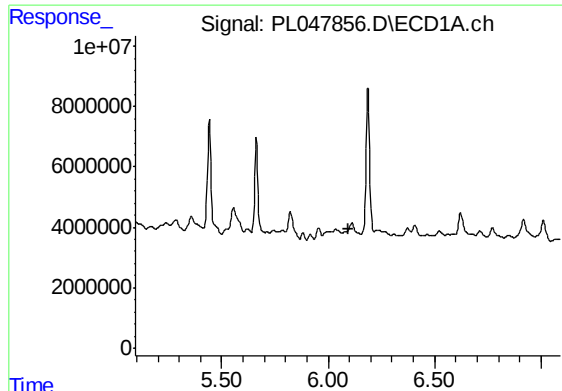

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

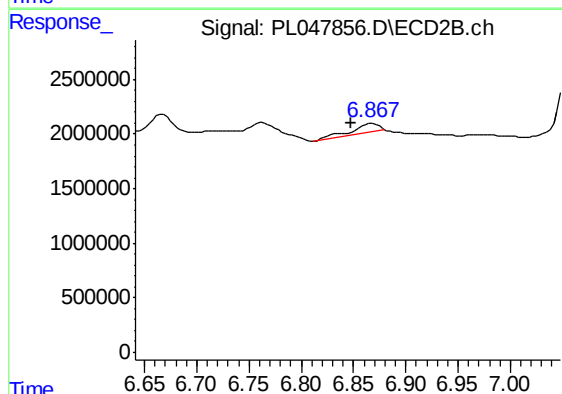


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.020 min
Response: 1655942
Conc: 0.63 ng/ml

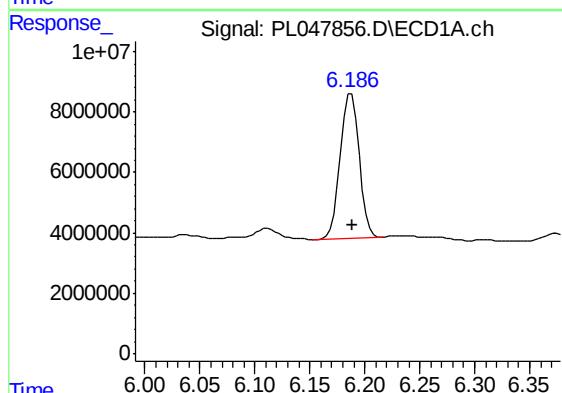


#17 4,4'-DDT

R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 57588934
Conc: 5.78 ng/ml

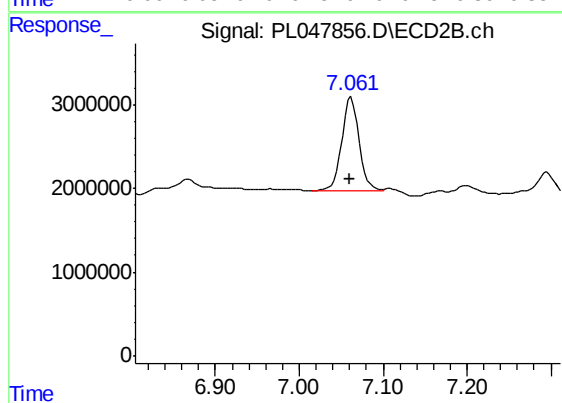

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.001 min
Response: 16148838
Conc: 6.78 ng/ml

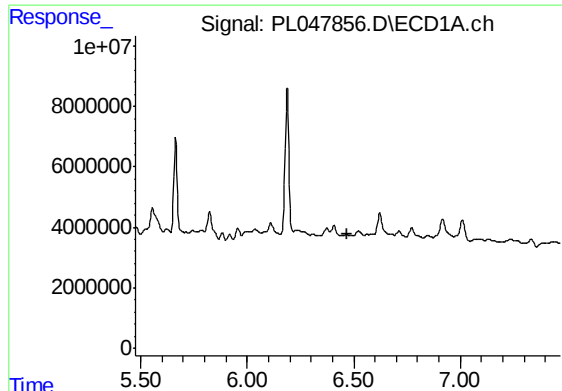

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-003-SW024-042319

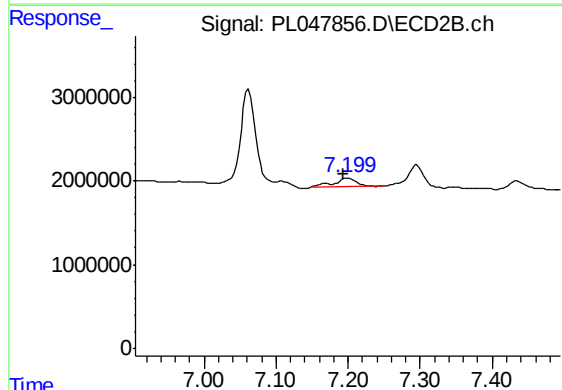


#19 Endosulfan Sulfate

R.T.: 7.201 min
Delta R.T.: 0.006 min
Response: 2110209
Conc: 0.77 ng/ml

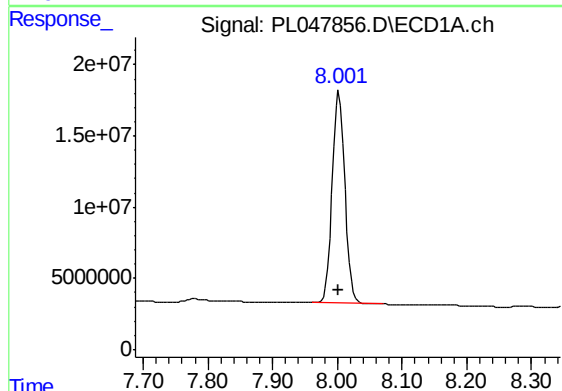

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.001 min
Response: 200151474
Conc: 17.88 ng/ml

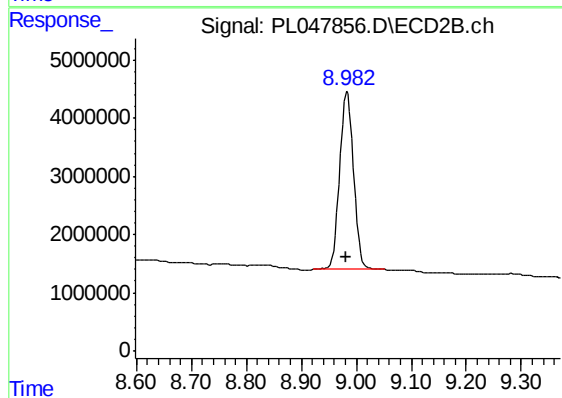

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.002 min
Response: 54160554
Conc: 18.97 ng/ml