

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
 Data File : PL047893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 23:15
 Operator : AJ\SJ
 Sample : K2571-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 114-PENNINGTON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:06:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.330	3.943	89261913	27231749	9.652	11.407
28) SA Decachlor...	8.005	8.987	111.1E6	31415599	9.925	11.005
Target Compounds						
10) B gamma-Chl...	5.220	6.041	5431185	2878792	0.408	0.951 #
11) B alpha-Chl...	5.276	6.117	7049237	3523184	0.540	1.165 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042619\
Data File : PL047893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 23:15
Operator : AJ\SJ
Sample : K2571-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
114-PENNINGTON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:06:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

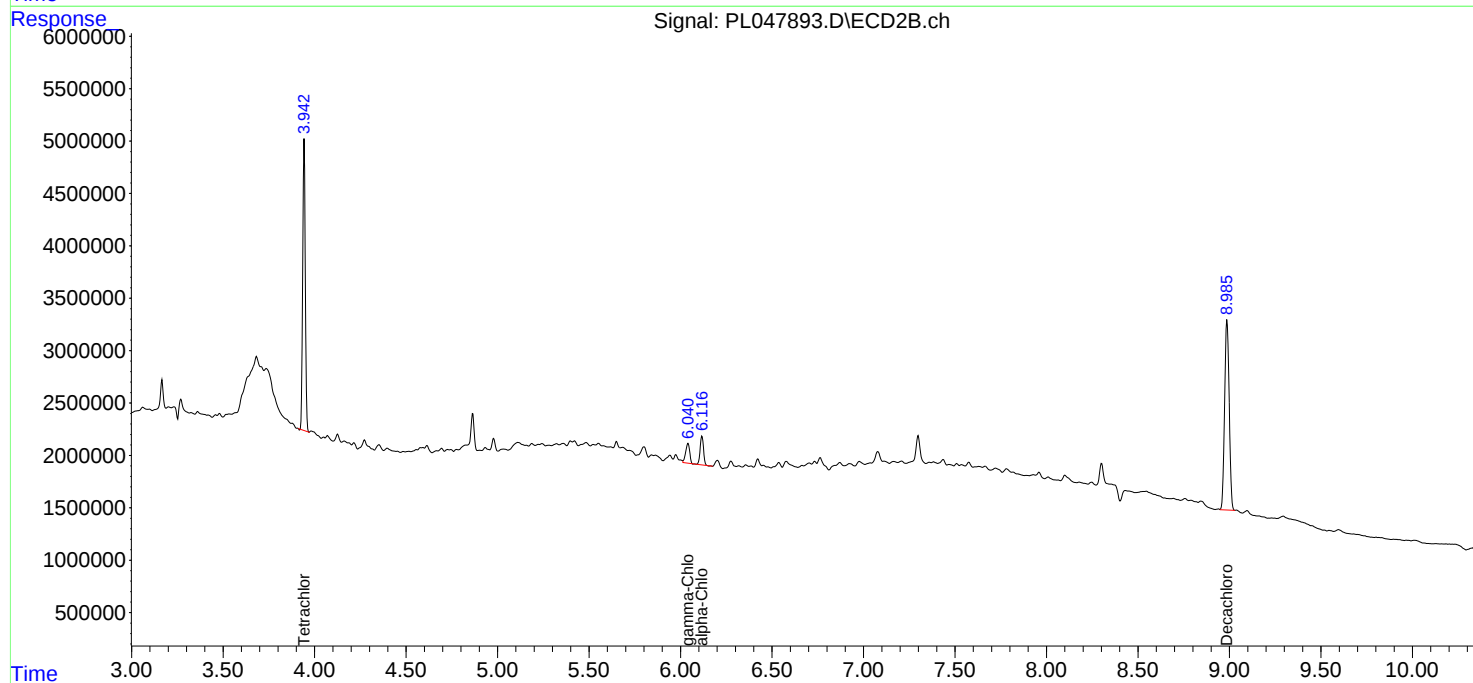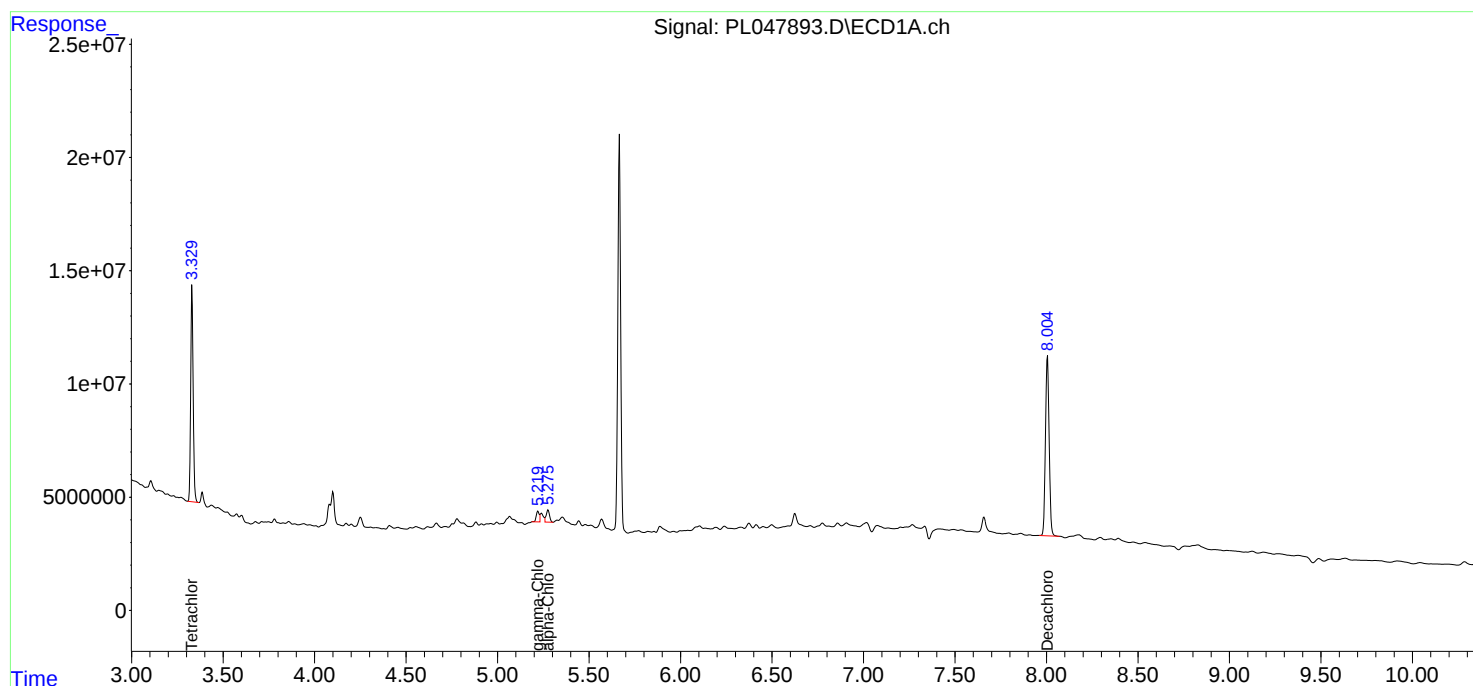


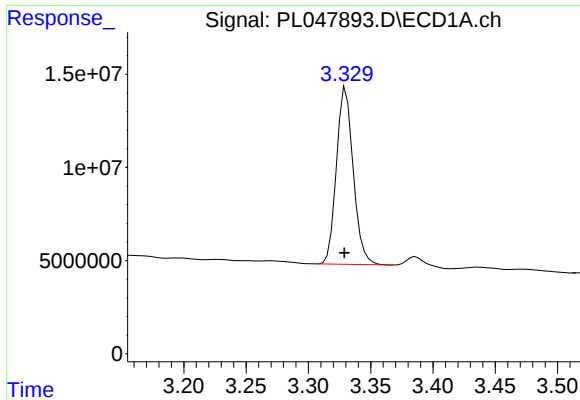

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 89261913
Conc: 9.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
114-PENNINGTON

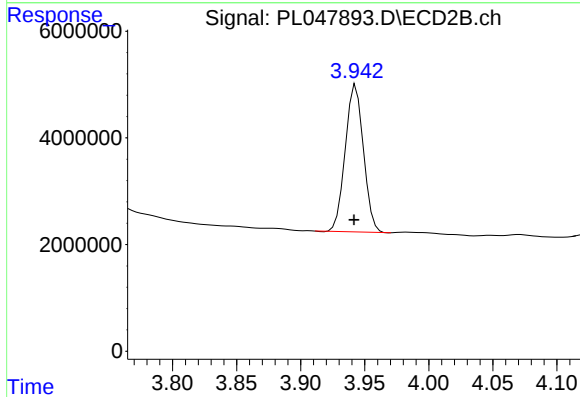


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.001 min
Response: 27231749
Conc: 11.41 ng/ml

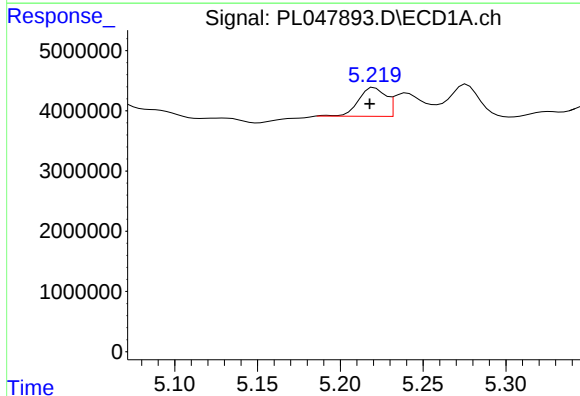


#10 gamma-Chlordane

R.T.: 5.220 min
Delta R.T.: 0.003 min
Response: 5431185
Conc: 0.41 ng/ml

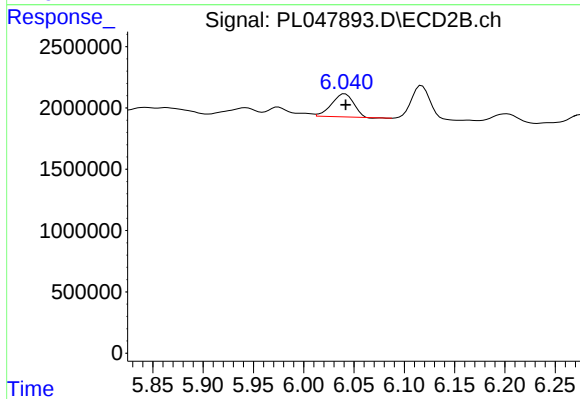

#10 gamma-Chlordane


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 2878792
Conc: 0.95 ng/ml

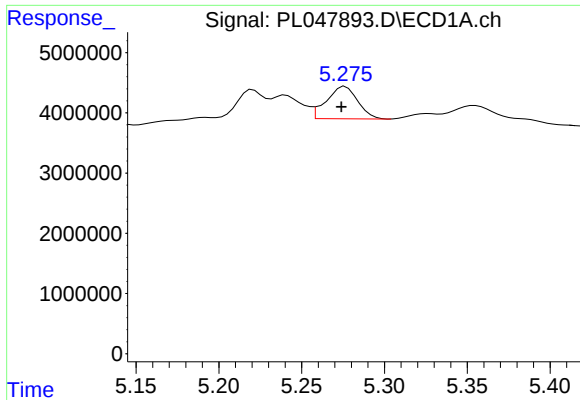

#11 alpha-Chlordane


R.T.: 5.276 min
Delta R.T.: 0.002 min
Response: 7049237
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
114-PENNINGTON

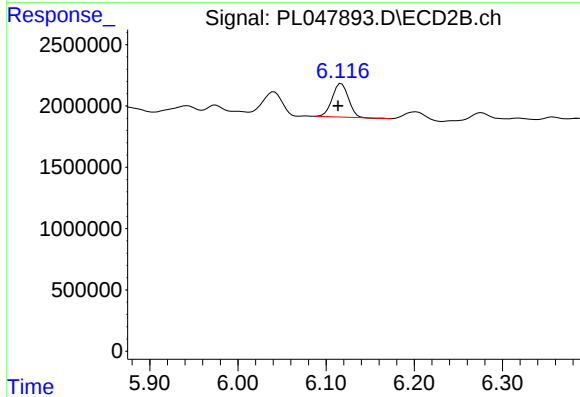


#11 alpha-Chlordane

R.T.: 6.117 min
Delta R.T.: 0.004 min
Response: 3523184
Conc: 1.16 ng/ml

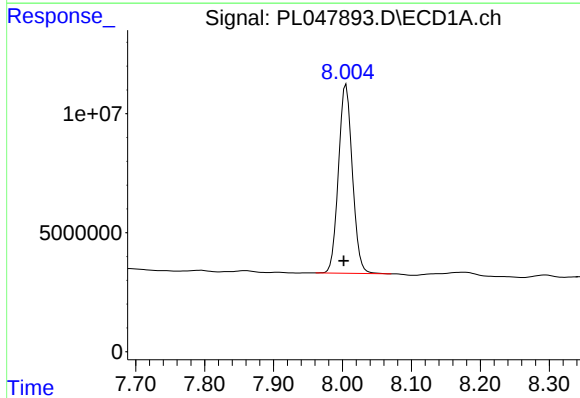

#28 Decachlorobiphenyl

R.T.: 8.005 min
Delta R.T.: 0.004 min
Response: 111107409
Conc: 9.93 ng/ml

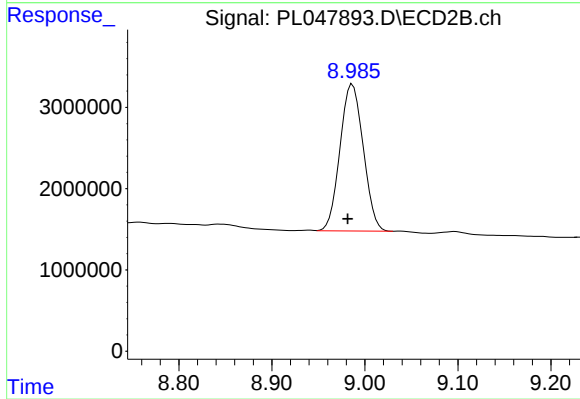

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: 0.005 min
Response: 31415599
Conc: 11.01 ng/ml