

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
 Data File : PL066465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 15:58
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:45:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 27 02:36:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.429	4.153	73438179	66995826	19.490	19.076
28) SA Decachlor...	8.159	9.351	76735706	60950134	20.013	19.702
Target Compounds						
14) MA Endrin	5.953	0.000	2547534	0	0.585	N.D. #
20) A Methoxychlor	6.872	7.799	1873228	1962424	0.954	1.094
24) Chlordane-2	0.000	5.647	0	18822924	N.D.	112.087 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
Data File : PL066465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 15:58
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:45:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Tue Apr 27 02:36:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

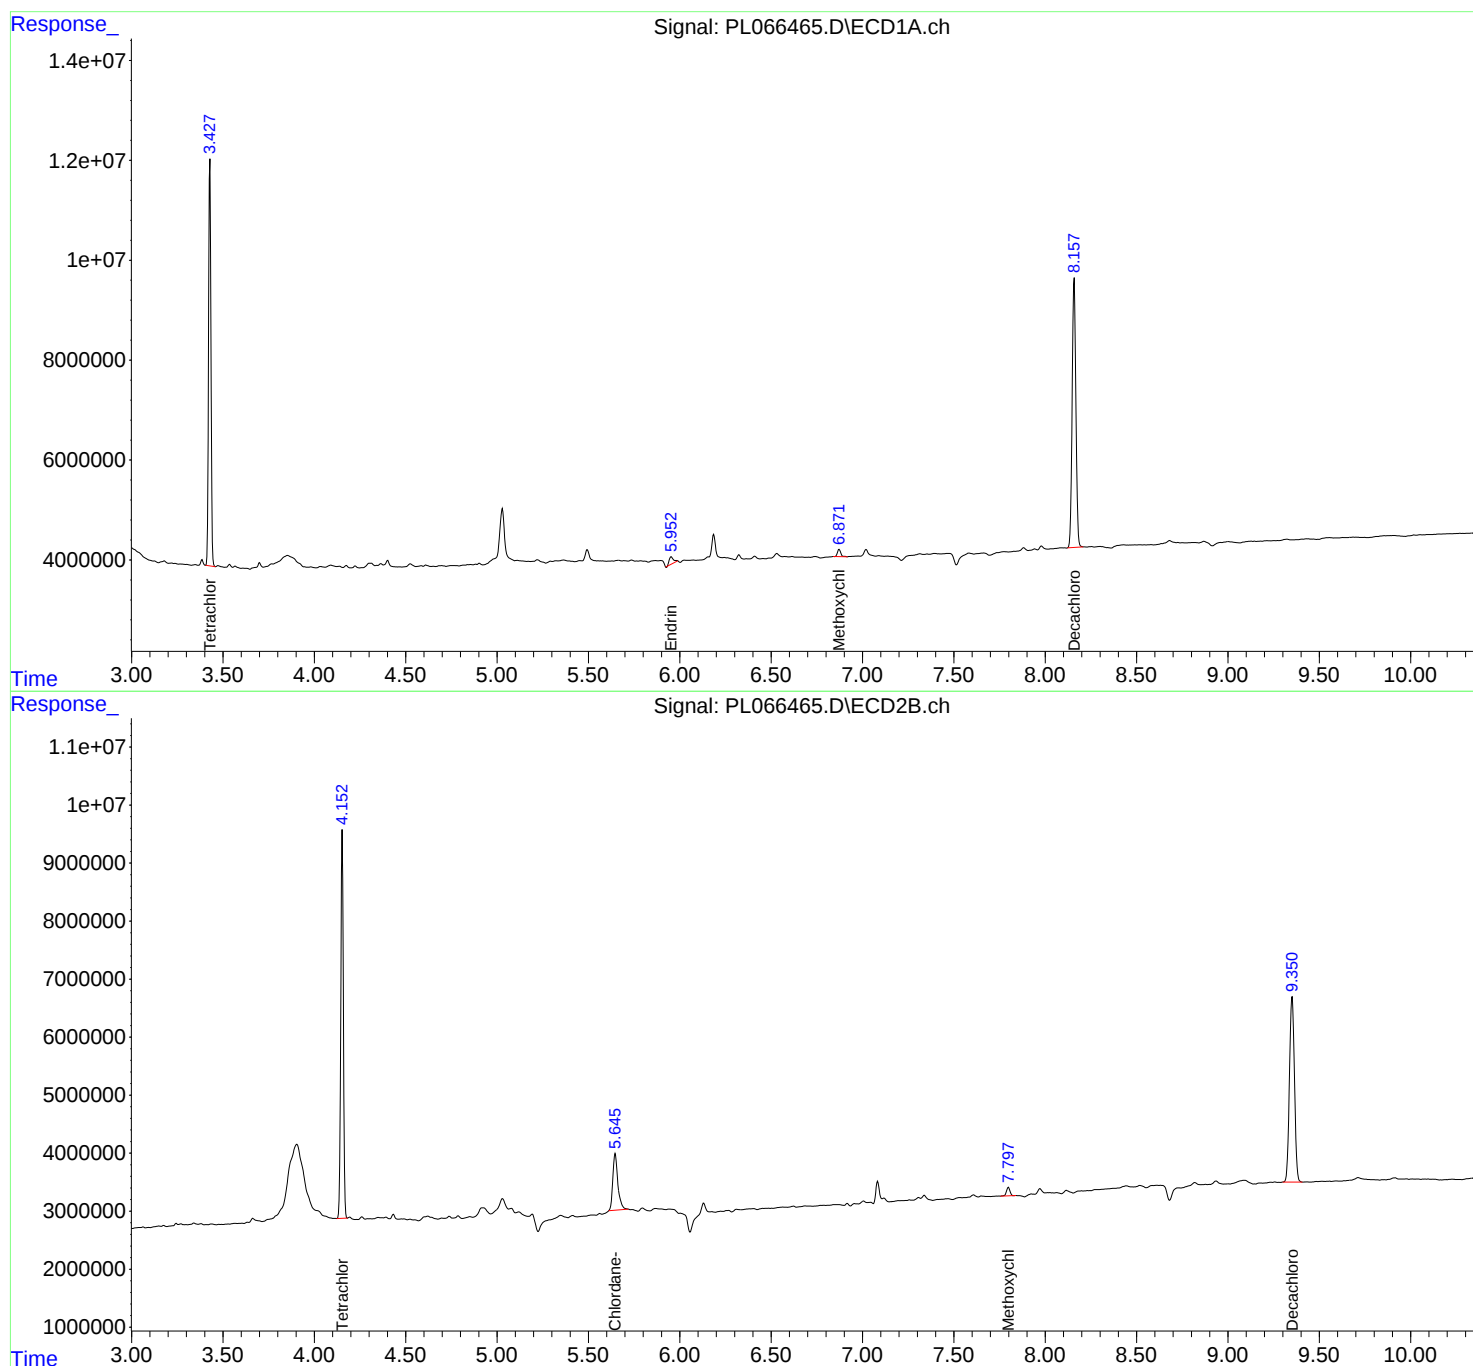


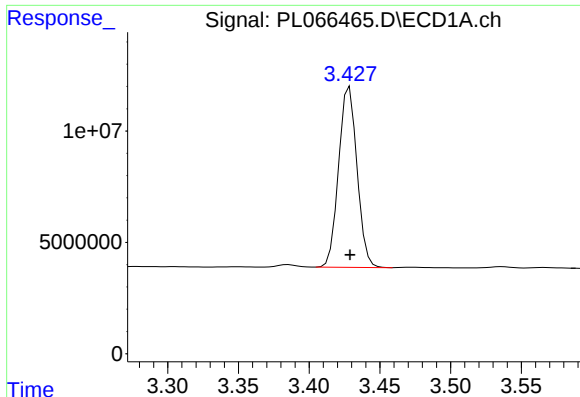

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 73438179
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

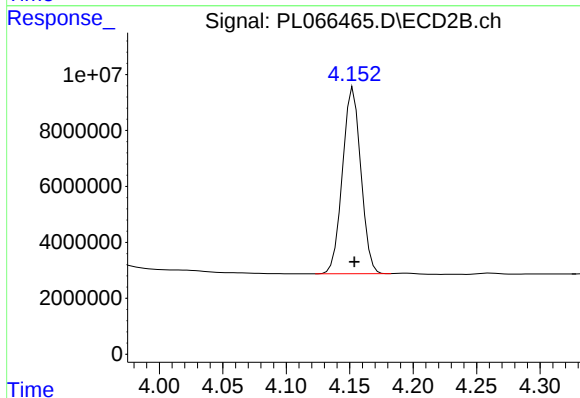


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 66995826
Conc: 19.08 ng/ml

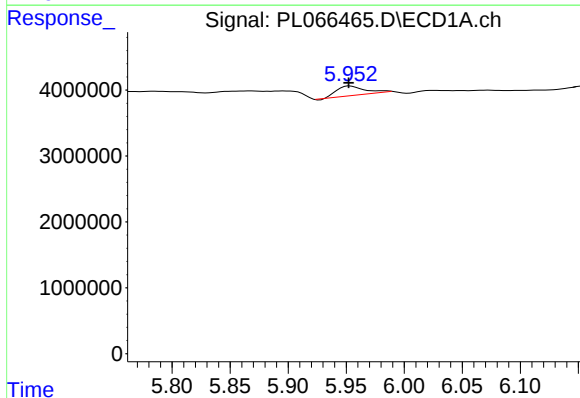


#14 Endrin

R.T.: 5.953 min
Delta R.T.: 0.001 min
Response: 2547534
Conc: 0.58 ng/ml

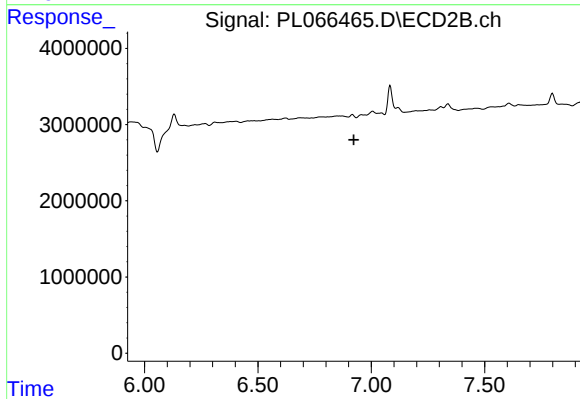

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

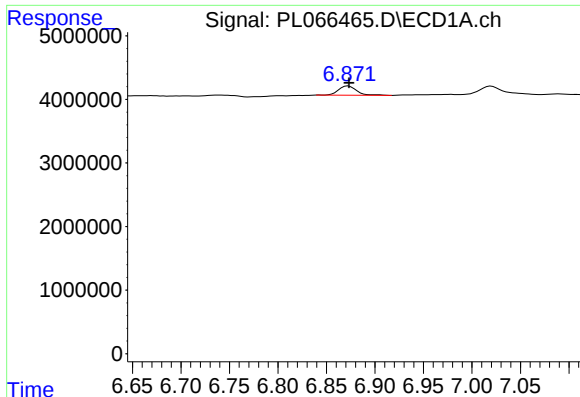

#20 Methoxychlor


R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 1873228
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

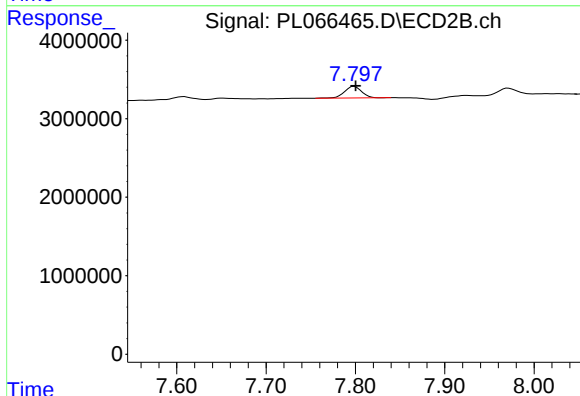


#20 Methoxychlor

R.T.: 7.799 min
Delta R.T.: -0.002 min
Response: 1962424
Conc: 1.09 ng/ml

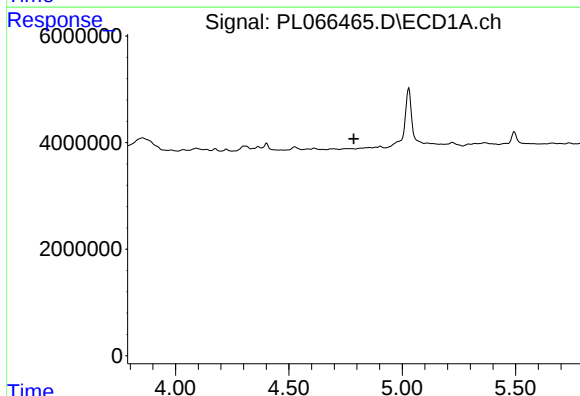


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

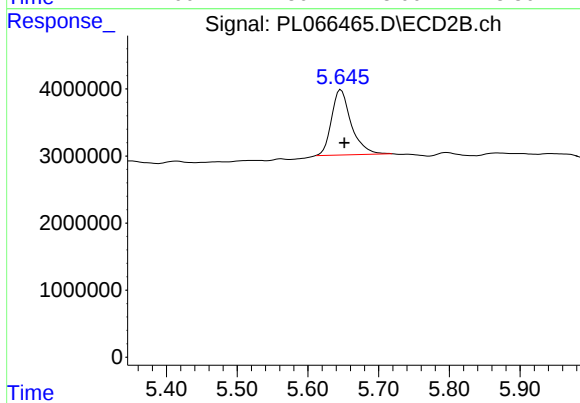

#24 Chlordane-2


R.T.: 5.647 min
Delta R.T.: -0.005 min
Response: 18822924
Conc: 112.09 ng/ml

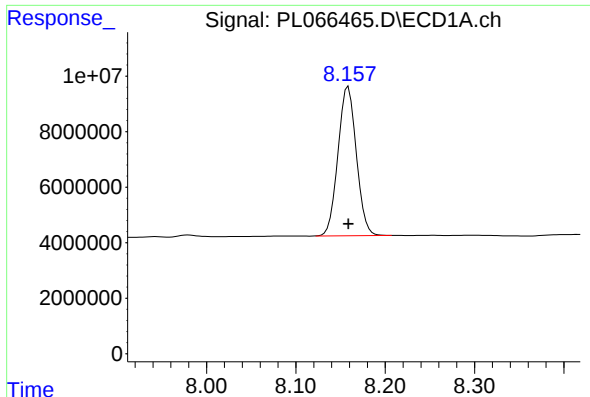

#28 Decachlorobiphenyl

R.T.: 8.159 min
Delta R.T.: 0.000 min
Response: 76735706
Conc: 20.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

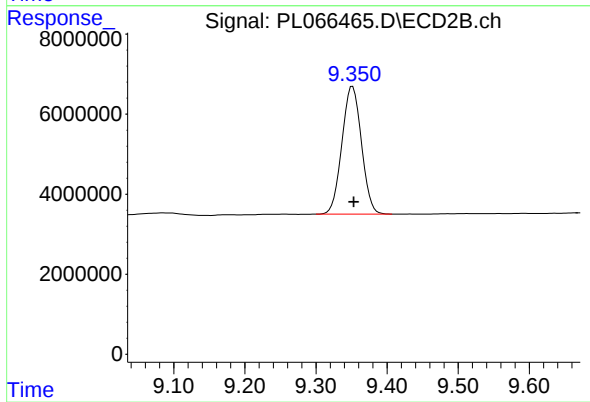

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: -0.002 min
Response: 60950134
Conc: 19.70 ng/ml