

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
 Data File : PL066474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 18:07
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:47:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 27 01:46:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.154	317.8E6	246.9E6	75.944	74.742
28)	SA Decachlor...	8.160	9.352	266.3E6	203.0E6	73.147	71.353
Target Compounds							
23)	Chlordane-1	4.290	5.174	106.3E6	107.0E6	750.257	729.578
24)	Chlordane-2	4.786	5.651	119.2E6	117.5E6	735.457	699.412
25)	Chlordane-3	5.349	6.310	360.2E6	409.7E6	763.982	756.801
26)	Chlordane-4	5.406	6.384	304.4E6	484.1E6	765.457	742.880
27)	Chlordane-5	6.233	7.206	121.9E6	87748677	756.310	747.629



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
Data File : PL066474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 18:07
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:47:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Tue Apr 27 01:46:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

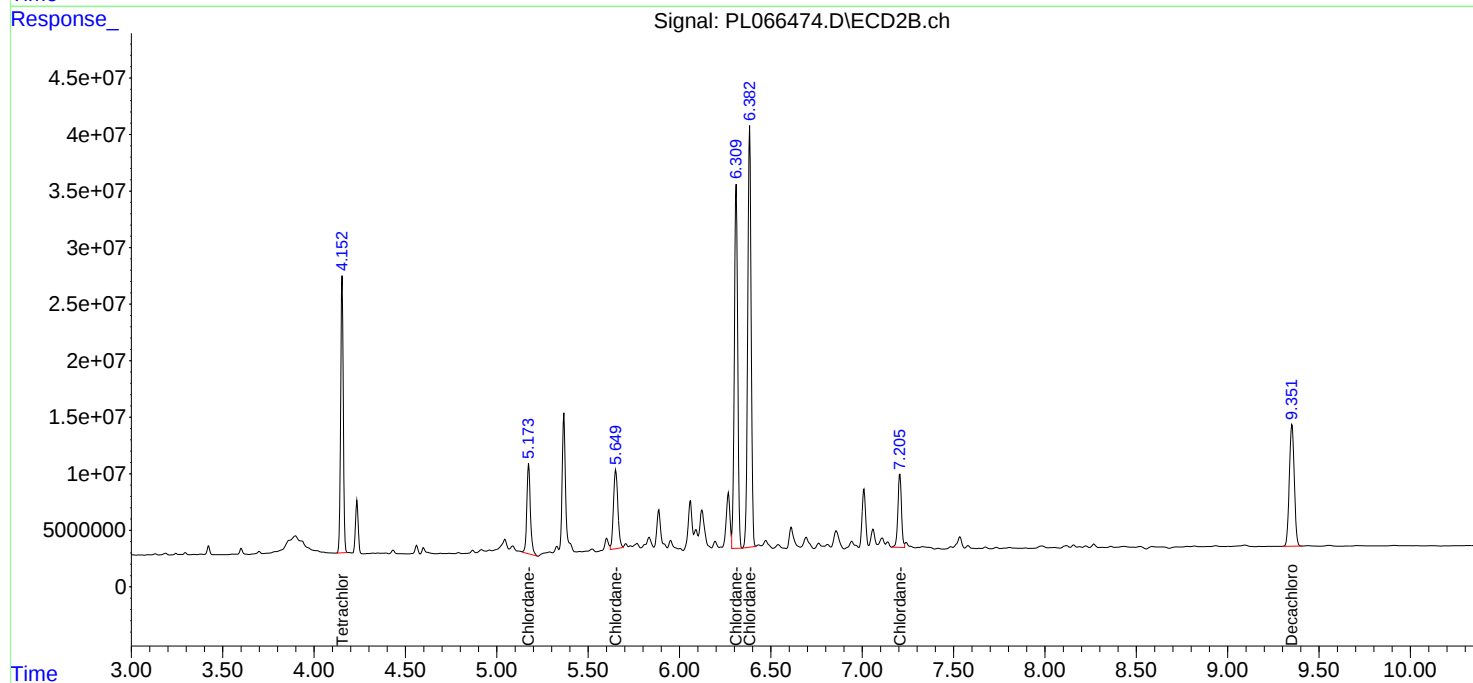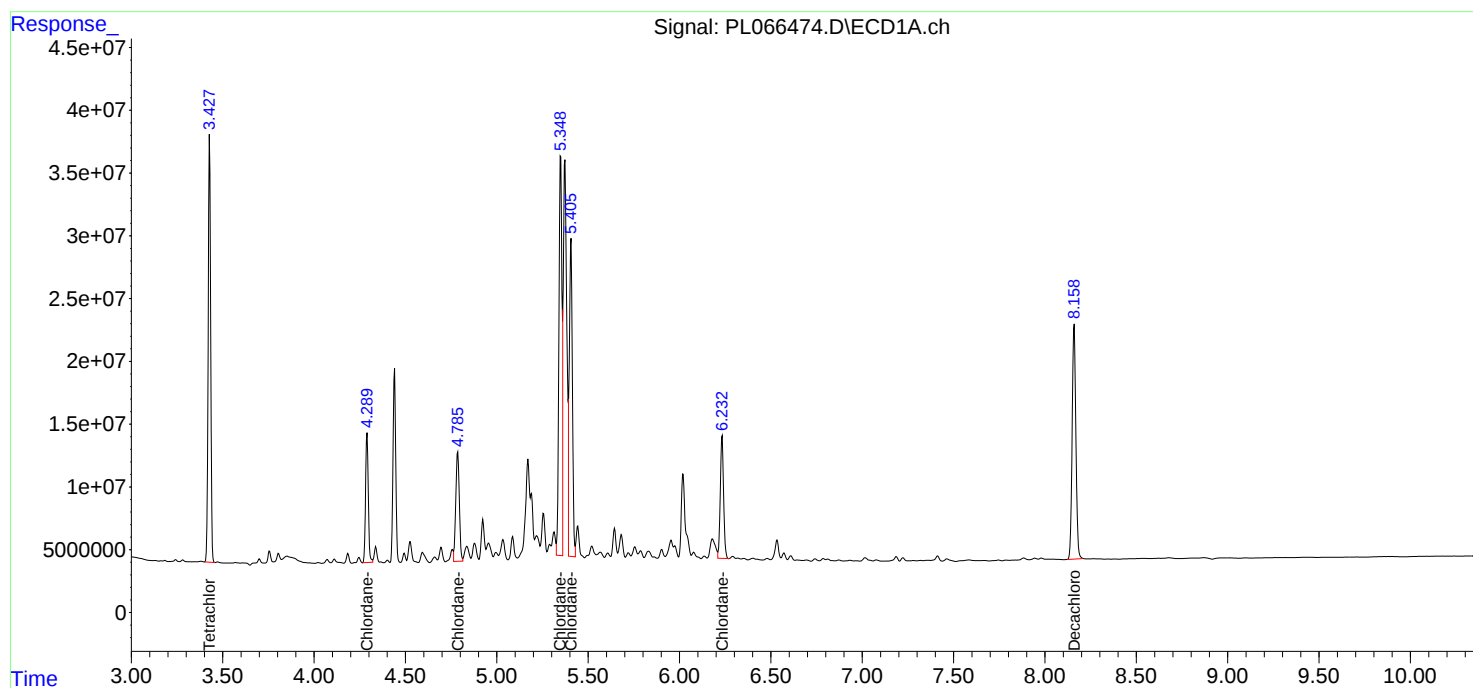


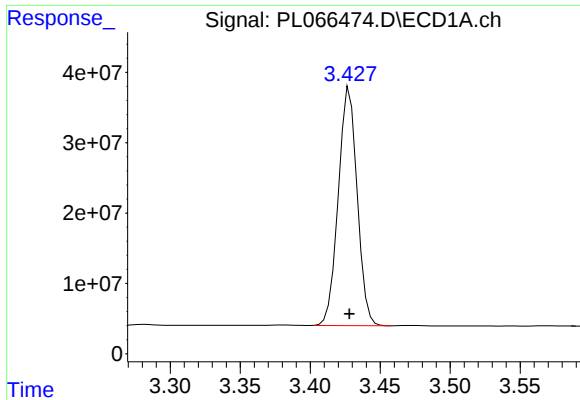

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 317841352
Conc: 75.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

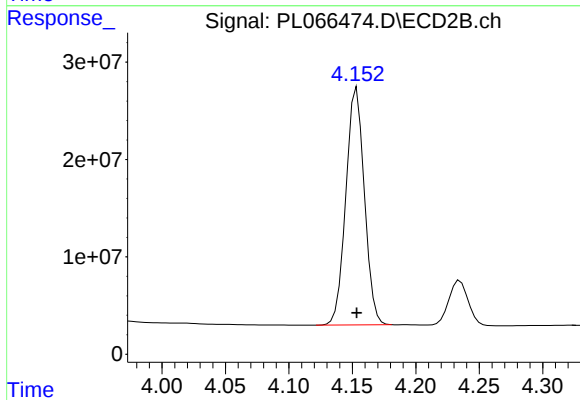


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 246903261
Conc: 74.74 ng/ml

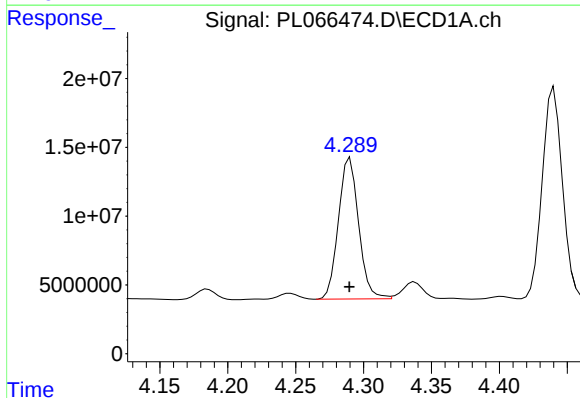


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 106336028
Conc: 750.26 ng/ml

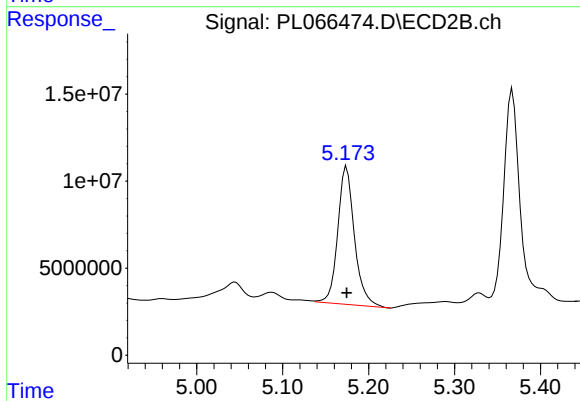

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 107038263
Conc: 729.58 ng/ml

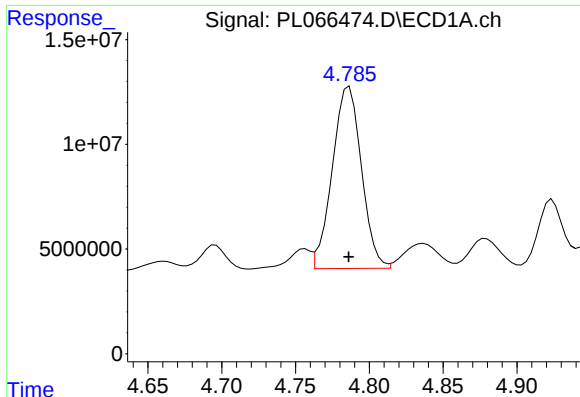

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 119241938
Conc: 735.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

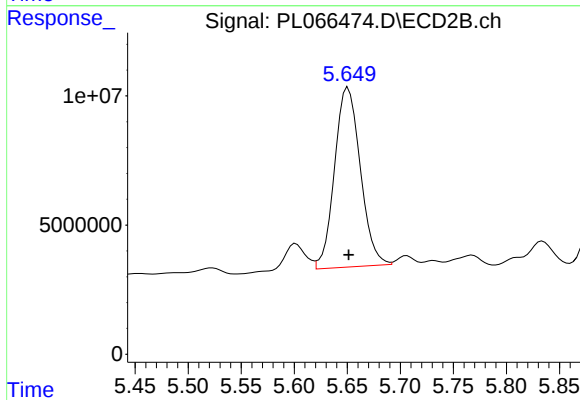


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 117453108
Conc: 699.41 ng/ml

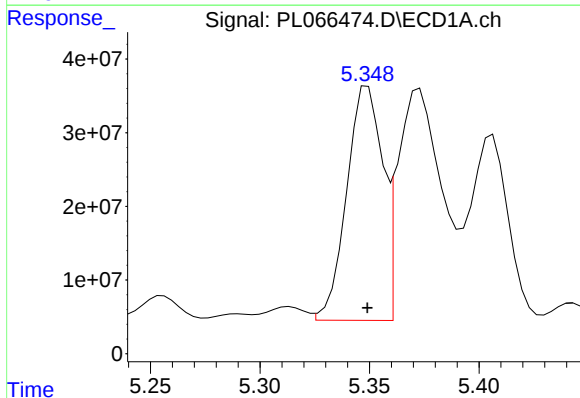


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 360175599
Conc: 763.98 ng/ml

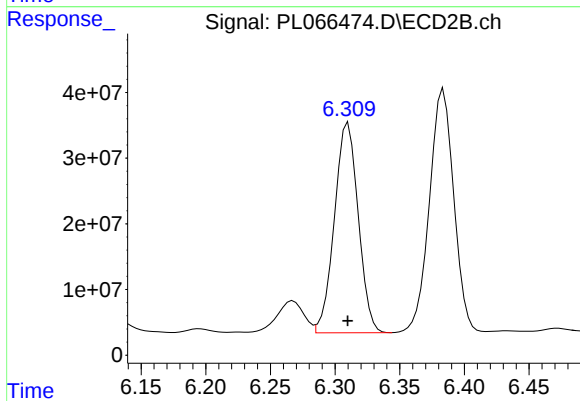

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 409651954
Conc: 756.80 ng/ml

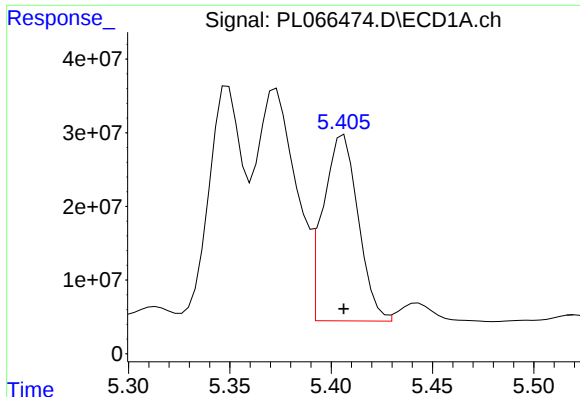

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 304407328
Conc: 765.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

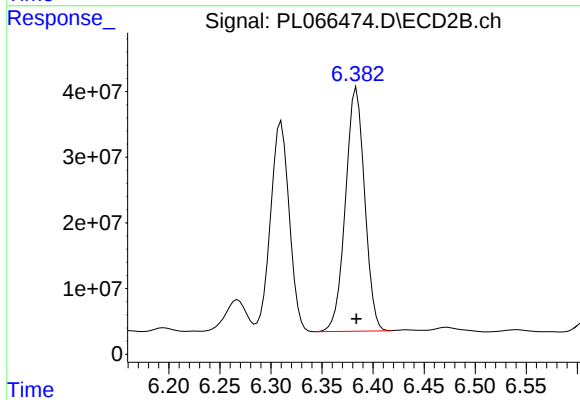


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 484148110
Conc: 742.88 ng/ml

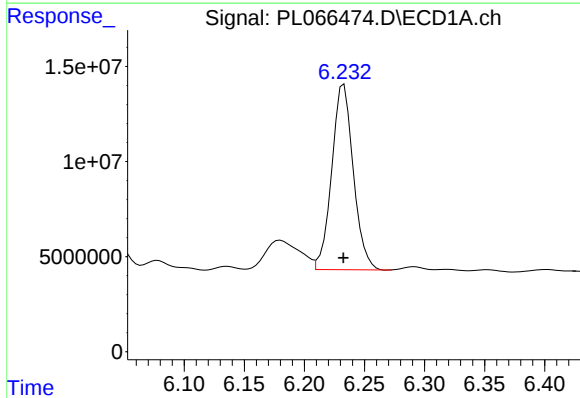


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 121935714
Conc: 756.31 ng/ml

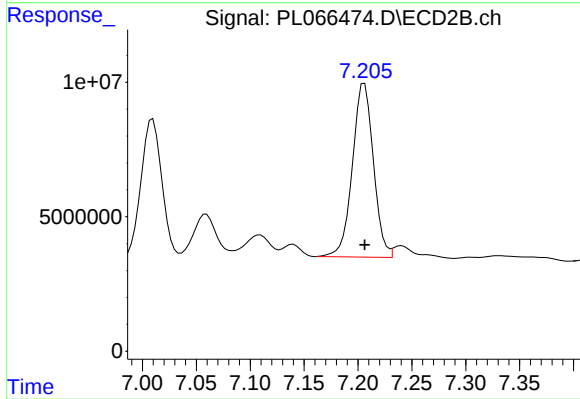

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 87748677
Conc: 747.63 ng/ml

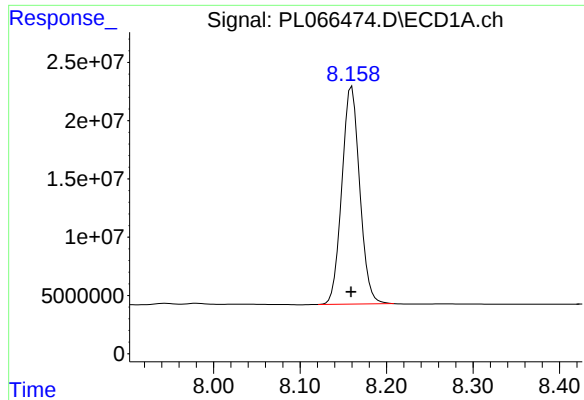

#28 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: 0.000 min
Response: 266294437
Conc: 73.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

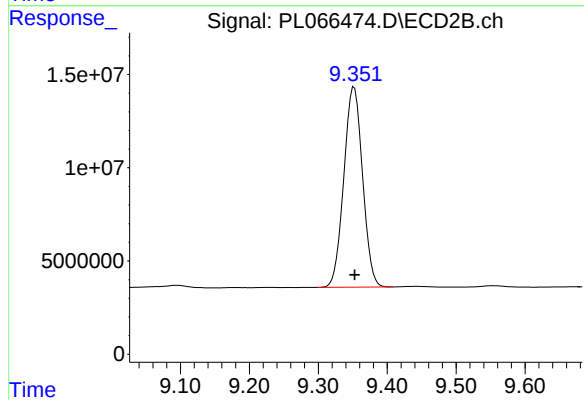

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 202980349
Conc: 71.35 ng/ml