

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
 Data File : PL066476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 18:35
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 01:47:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 27 01:46:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.153	104.1E6	85372500	24.863	25.844
28)	SA Decachlor...	8.160	9.352	93756571	71778188	25.753	25.232
Target Compounds							
23)	Chlordane-1	4.290	5.174	36595958	40745095	258.204	277.721
24)	Chlordane-2	4.787	5.650	41993771	51020970	259.008	303.821
25)	Chlordane-3	5.349	6.310	117.0E6	137.7E6	248.269	254.451
26)	Chlordane-4	5.407	6.384	97695121	167.0E6	245.662	256.237
27)	Chlordane-5	6.233	7.206	40474300	29679652	251.043	252.874



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
Data File : PL066476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 18:35
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 01:47:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Tue Apr 27 01:46:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

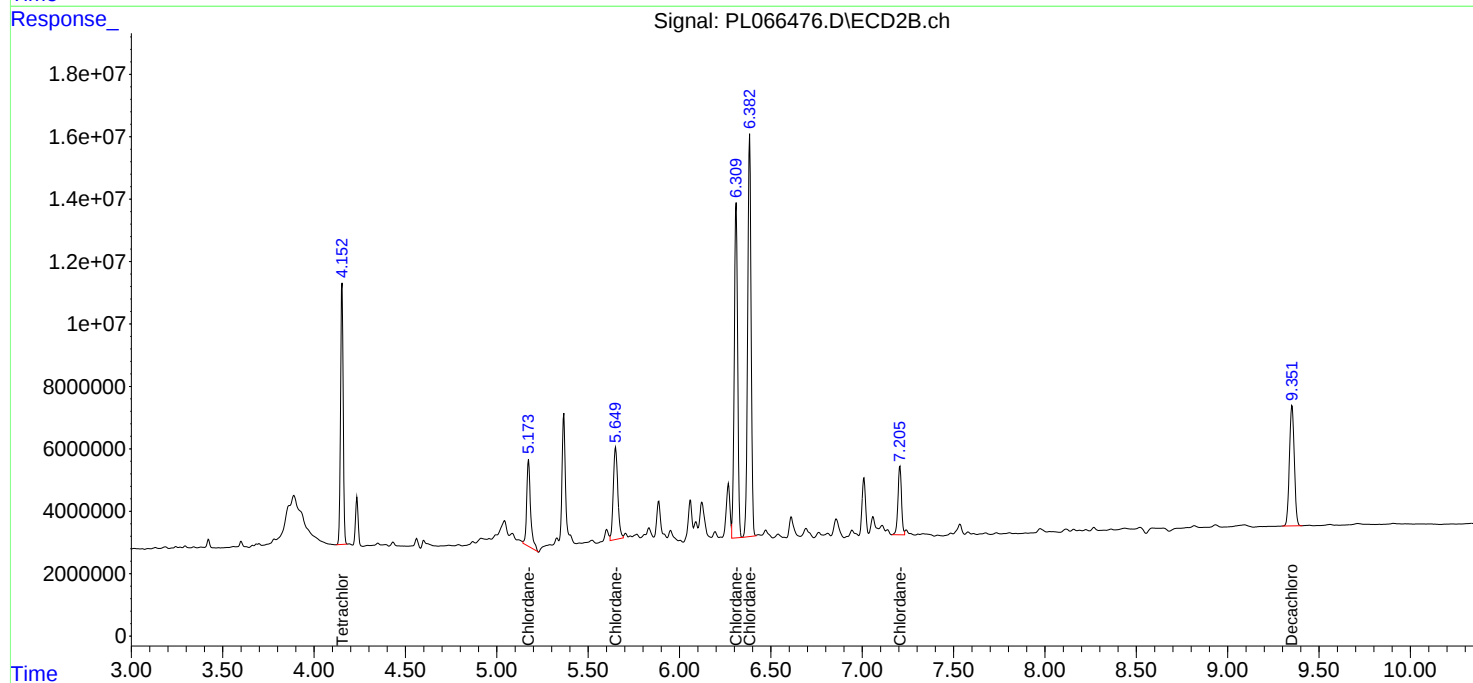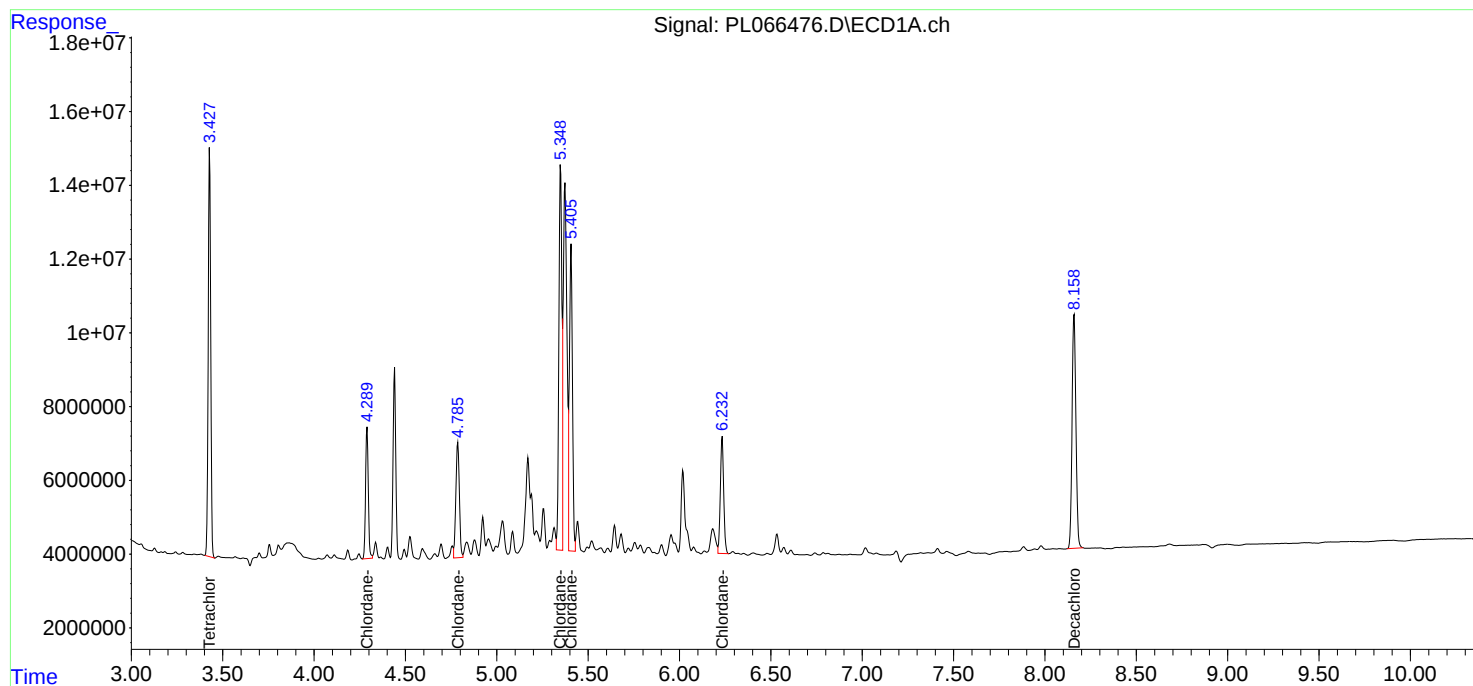


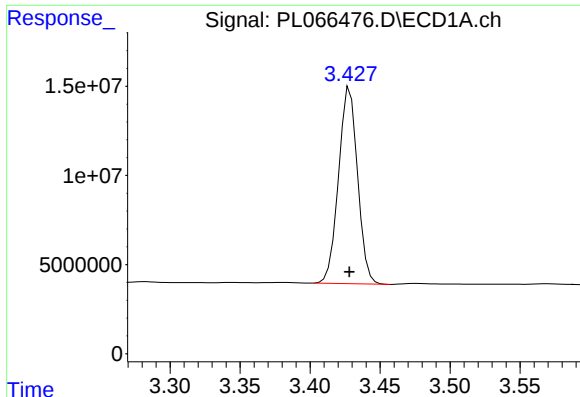

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 104056401
Conc: 24.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

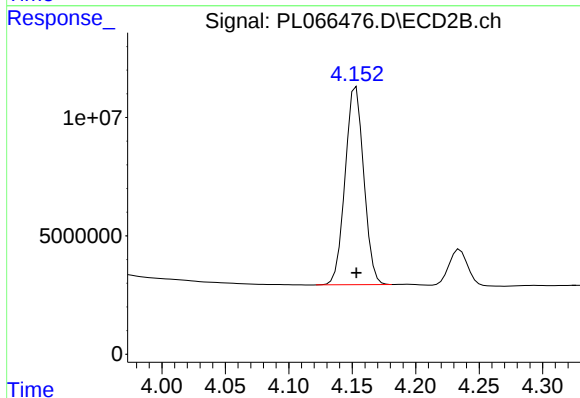


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 85372500
Conc: 25.84 ng/ml

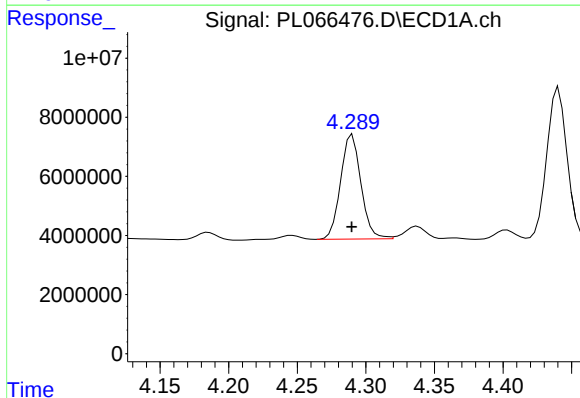


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 36595958
Conc: 258.20 ng/ml

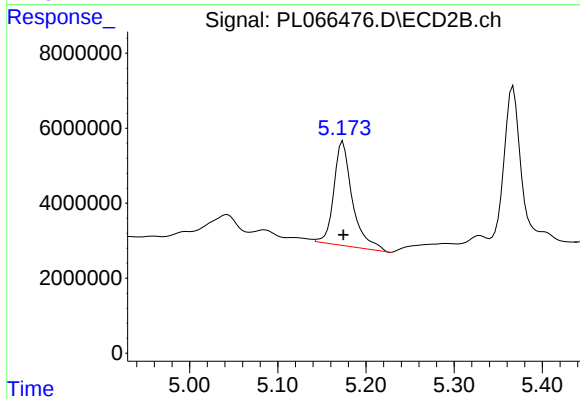

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 40745095
Conc: 277.72 ng/ml

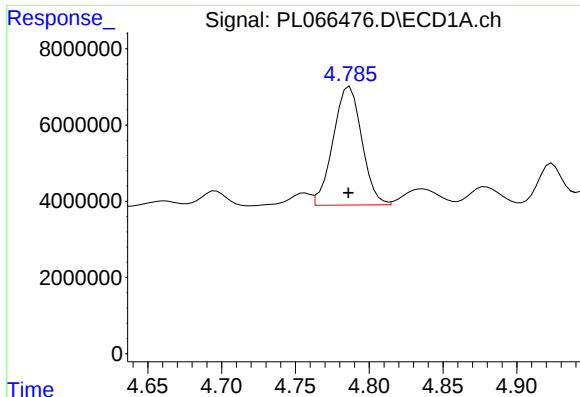

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 41993771
Conc: 259.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

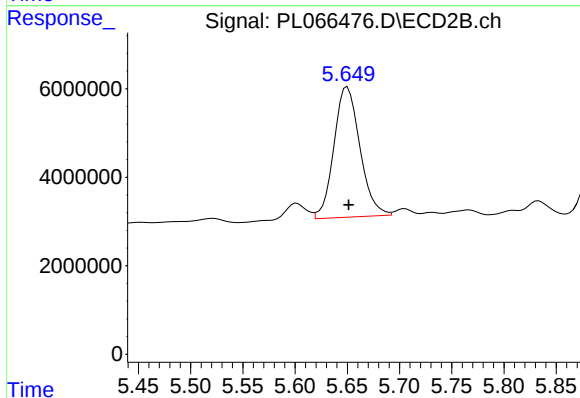


#24 Chlordane-2

R.T.: 5.650 min
Delta R.T.: -0.001 min
Response: 51020970
Conc: 303.82 ng/ml

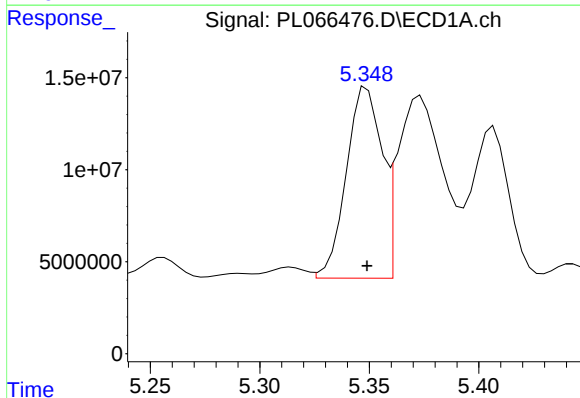


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 117045359
Conc: 248.27 ng/ml

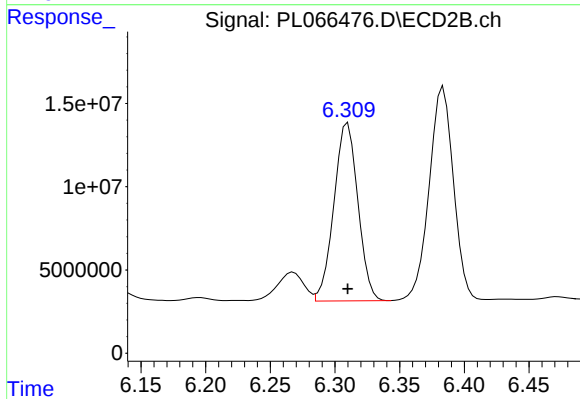

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 137732571
Conc: 254.45 ng/ml

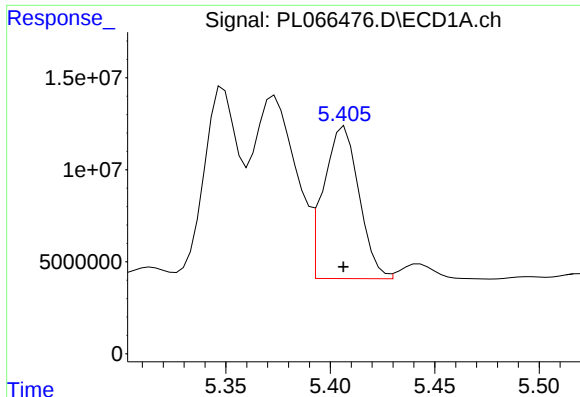

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 97695121
Conc: 245.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

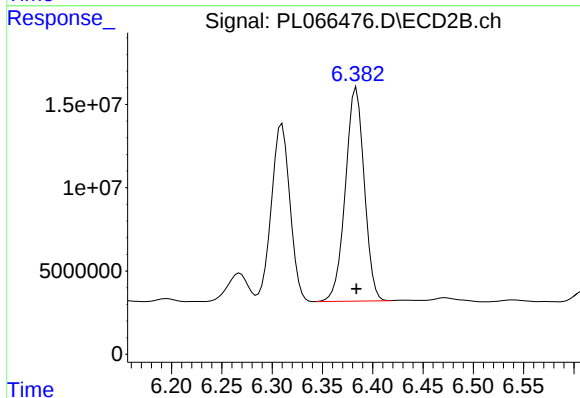


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 166994099
Conc: 256.24 ng/ml

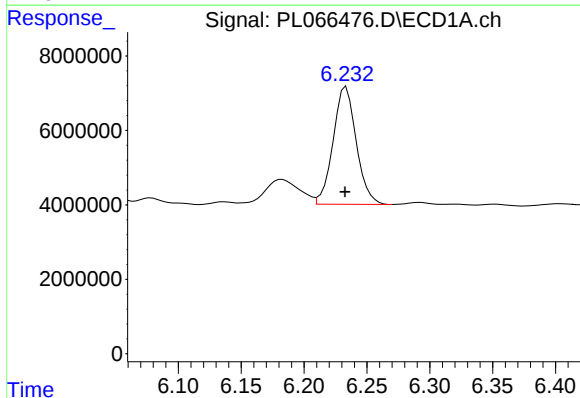


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 40474300
Conc: 251.04 ng/ml

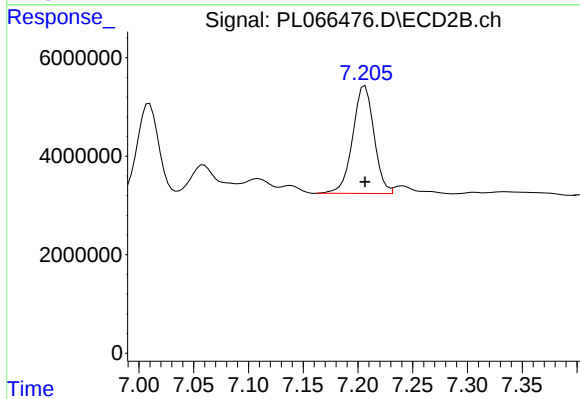

#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 29679652
Conc: 252.87 ng/ml

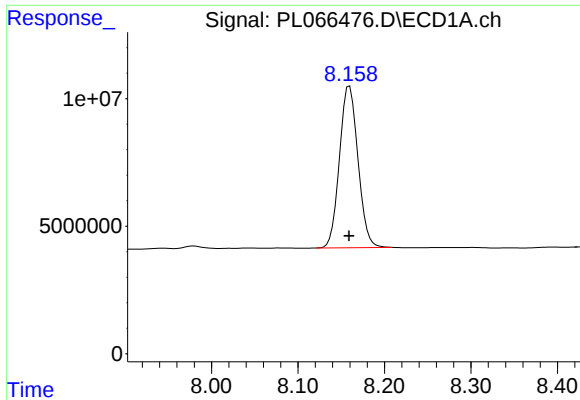

#28 Decachlorobiphenyl


R.T.: 8.160 min

Delta R.T.: 0.000 min

Response: 93756571

Conc: 25.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

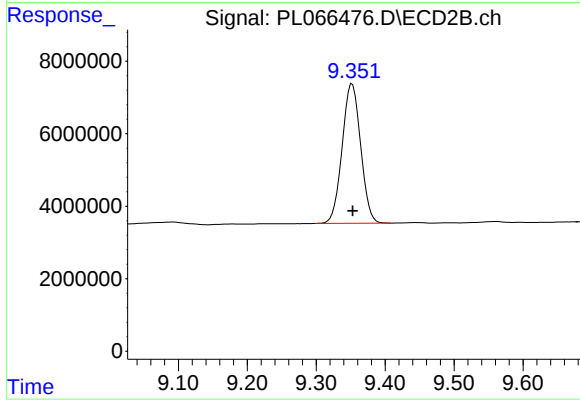

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 71778188

Conc: 25.23 ng/ml