

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
 Data File : PL066484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2021 20:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL042621CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 02:34:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 27 02:25:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.153	221.8E6	177.7E6	52.987	53.793
28)	SA Decachlor...	8.160	9.352	188.6E6	141.7E6	51.818	49.810
Target Compounds							
23)	Chlordane-1	4.290	5.174	76012541	78886136	536.309	537.692
24)	Chlordane-2	4.787	5.651	86460922	85168195	533.271	507.161
25)	Chlordane-3	5.350	6.310	252.6E6	300.1E6	535.775	554.460
26)	Chlordane-4	5.407	6.383	211.8E6	356.7E6	532.476	547.325
27)	Chlordane-5	6.233	7.206	86303425	61885101	535.300	527.268



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042621\
Data File : PL066484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2021 20:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL042621CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 02:34:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Tue Apr 27 02:25:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

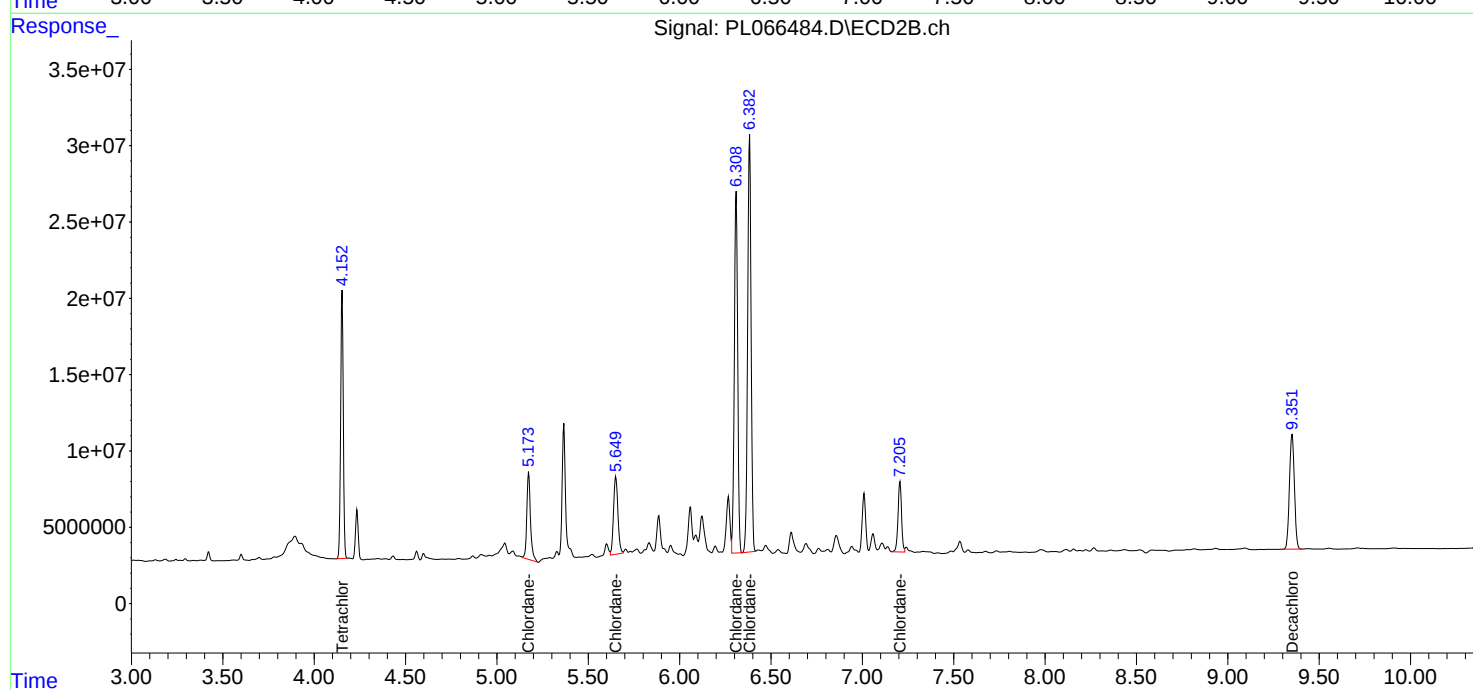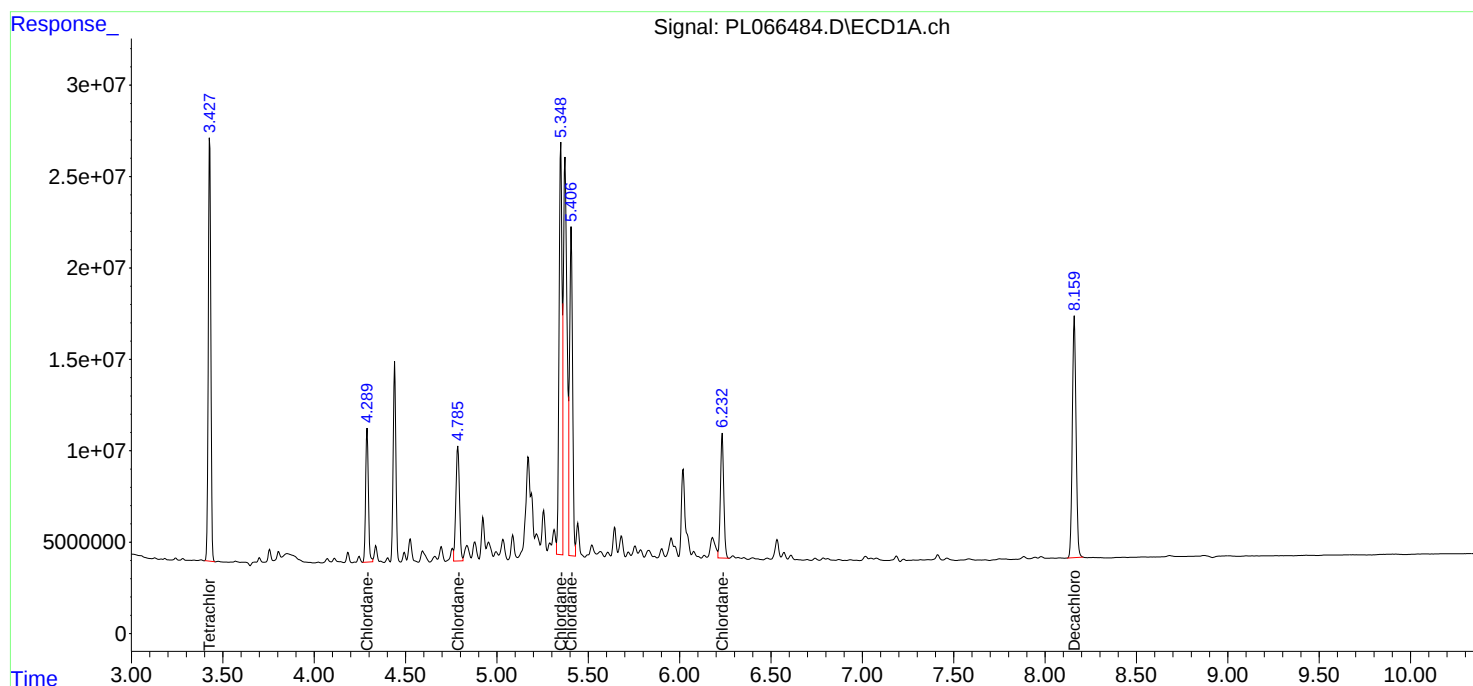


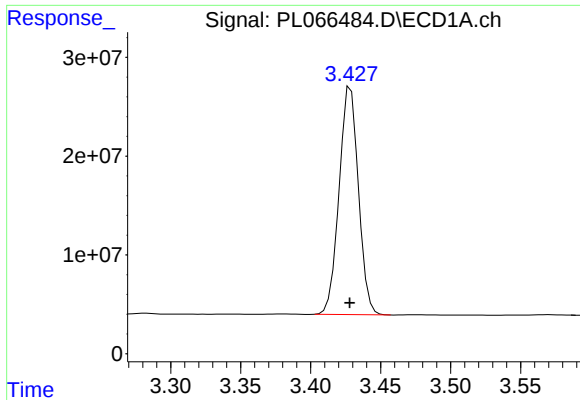

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 221760715
Conc: 52.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042621CHLOR

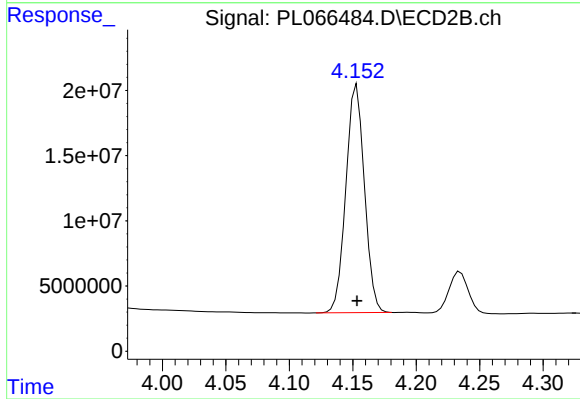


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 177699629
Conc: 53.79 ng/ml

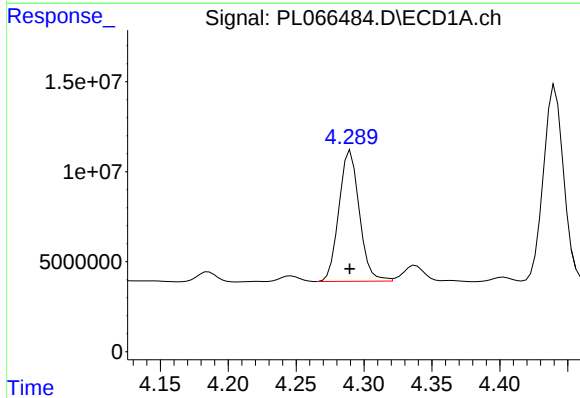


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 76012541
Conc: 536.31 ng/ml

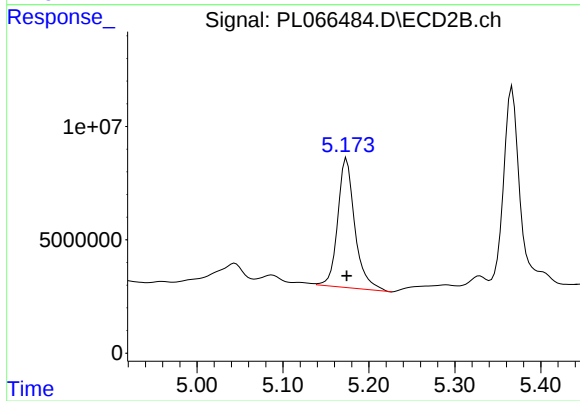

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 78886136
Conc: 537.69 ng/ml

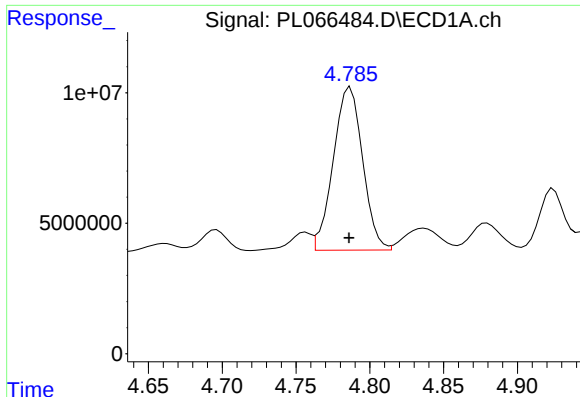

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 86460922
Conc: 533.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042621CHLOR

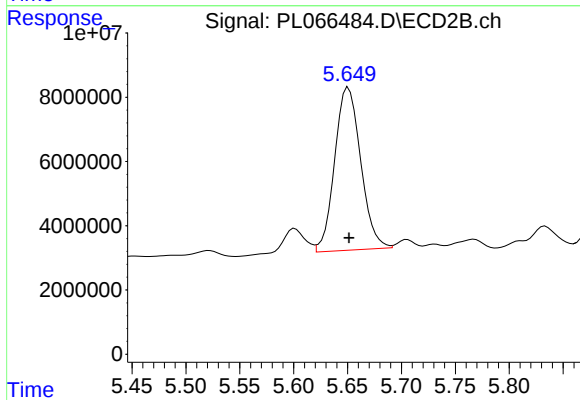


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 85168195
Conc: 507.16 ng/ml

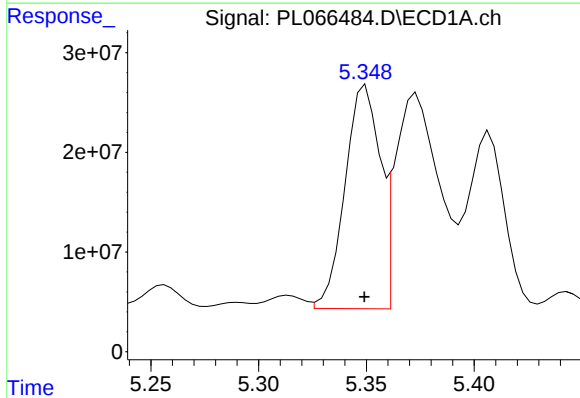


#25 Chlordane-3

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 252588264
Conc: 535.77 ng/ml

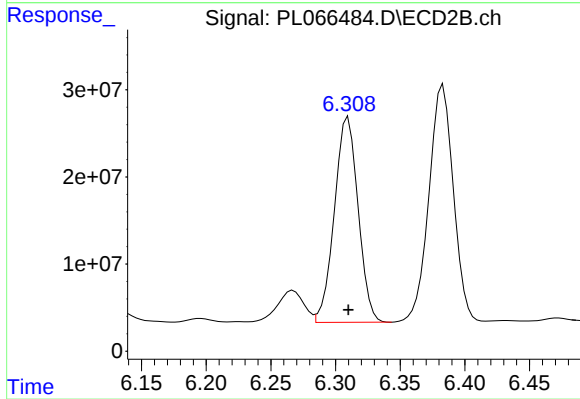

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 300125975
Conc: 554.46 ng/ml

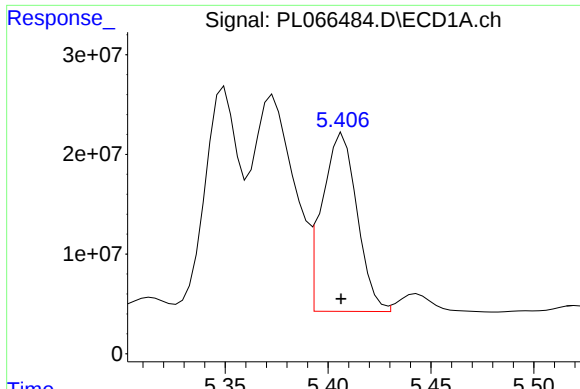

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 211755589
Conc: 532.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042621CHLOR

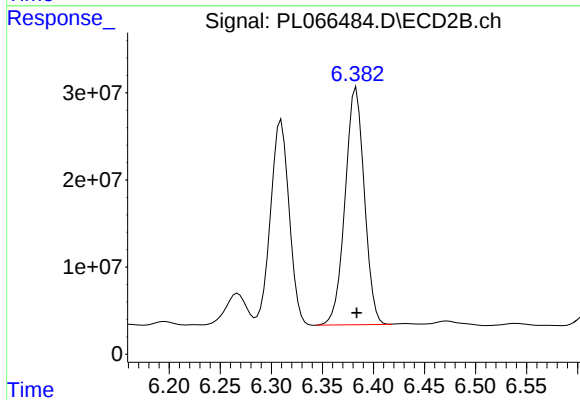


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 356701371
Conc: 547.33 ng/ml

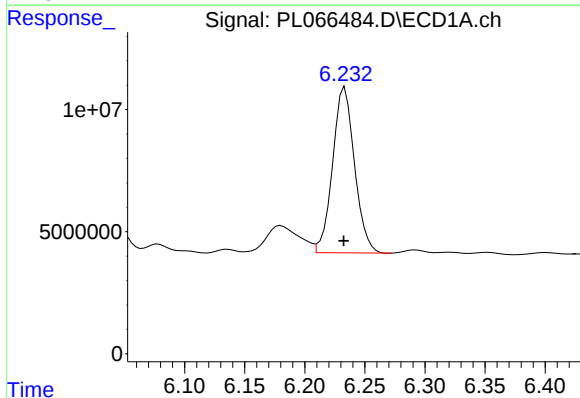


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 86303425
Conc: 535.30 ng/ml

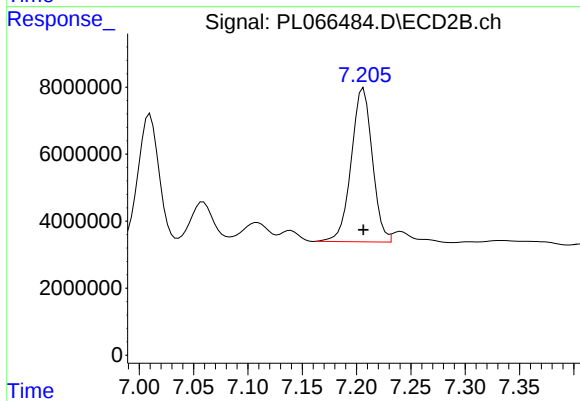

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 61885101
Conc: 527.27 ng/ml

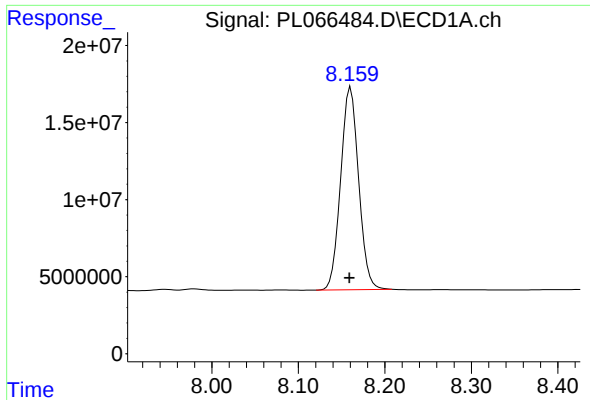

#28 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: 0.002 min
Response: 188645512
Conc: 51.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042621CHLOR

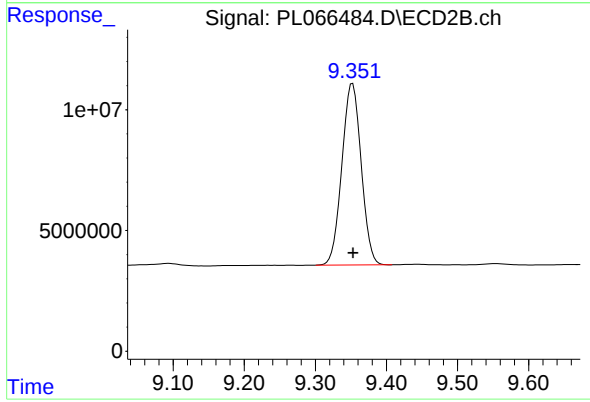

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 141695246
Conc: 49.81 ng/ml