

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
 Data File : PL074390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 23:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 00:29:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.490	8449143	45282431	26.149	25.397
28)	SA Decachlor...	10.405	11.334	13419904	46079171	25.806	26.088
Target Compounds							
6)	B beta-BHC	0.000	6.674	0	612733	N.D.	0.544 #
7)	B delta-BHC	0.000	6.938	0	1925841	N.D.	0.789 #
8)	B Heptachlo...	0.000	7.927	0	408710	N.D.	0.182 #
9)	A Endosulfan I	0.000	8.352f	0	1047960	N.D.	0.532 #
10)	B gamma-Chl...	0.000	8.209	0	234002	N.D.	0.105 #
13)	MA Dieldrin	7.771	0.000	138007	0	0.321	N.D. #
14)	MA Endrin	8.082f	8.843	142175	434457	0.350	0.257 #
15)	B Endosulfa...	0.000	9.074	0	664148	N.D.	0.382 #
16)	A 4,4'-DDD	0.000	9.018f	0	2905049	N.D.	1.888 #
18)	B Endrin al...	8.564	0.000	13716	0	0.042	N.D. #
20)	A Methoxychlor	9.068f	9.795	14774	11429390	0.060	11.883 #
22)	Mirex	9.512	0.000	27578	0	0.059	N.D. #
25)	Chlordane-3	0.000	8.209	0	234002	N.D.	0.692 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
Data File : PL074390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 23:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 00:29:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

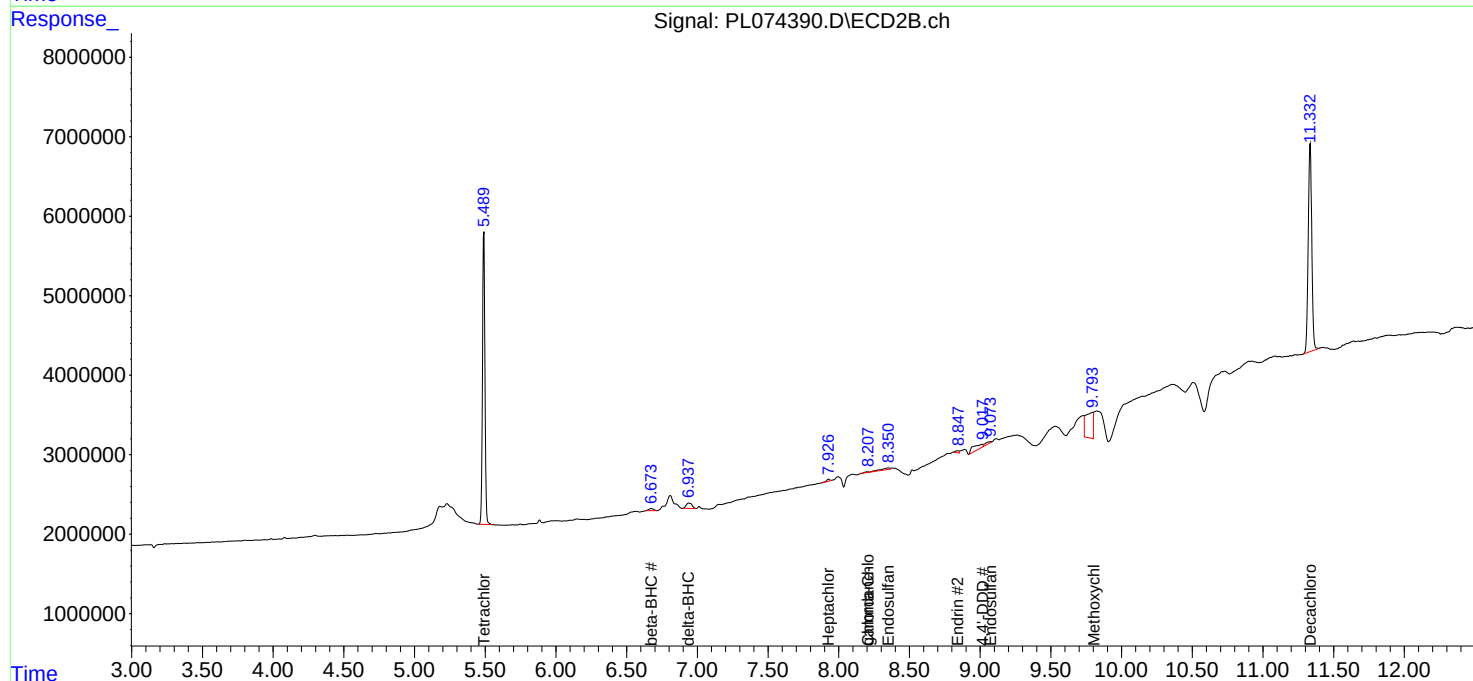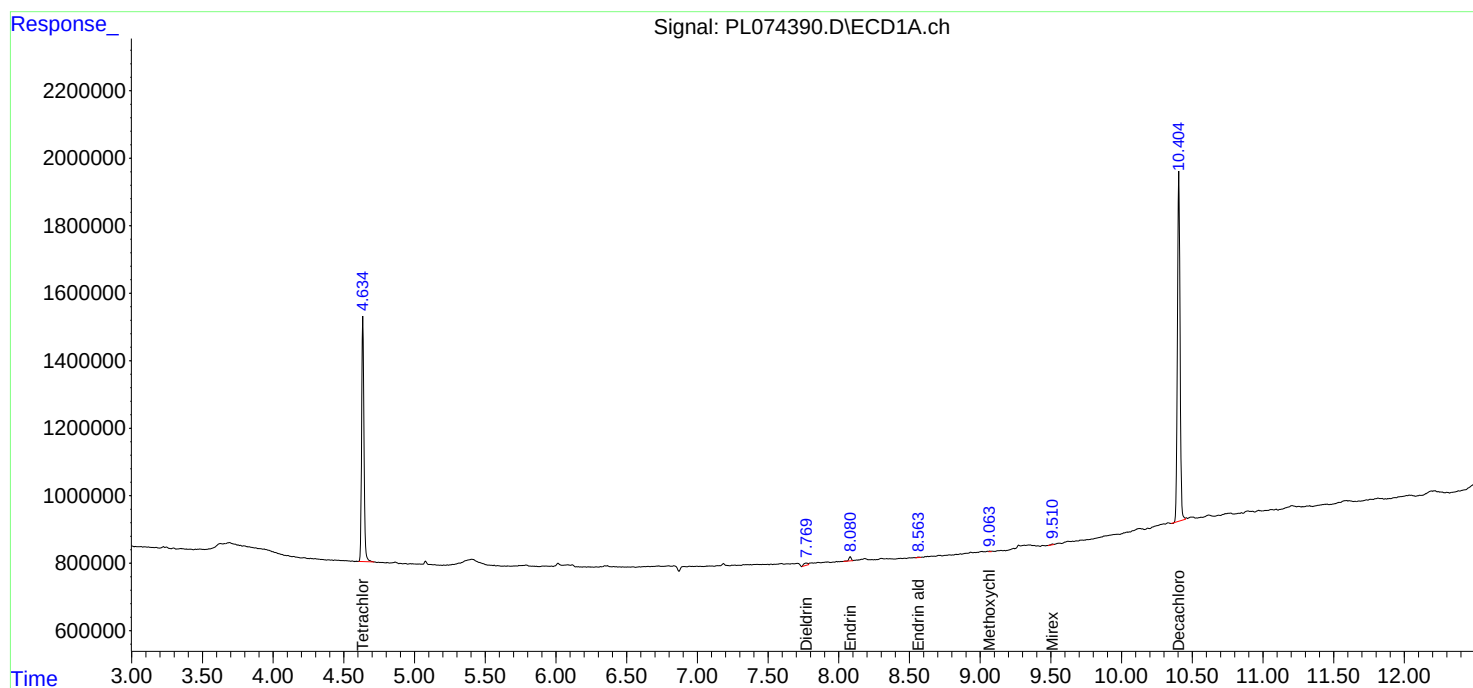


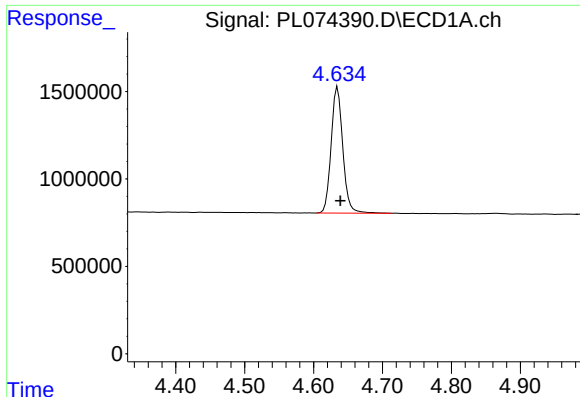

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 8449143
Conc: 26.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

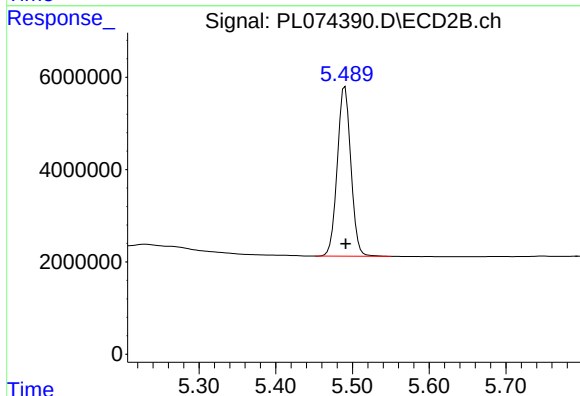


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 45282431
Conc: 25.40 ng/ml

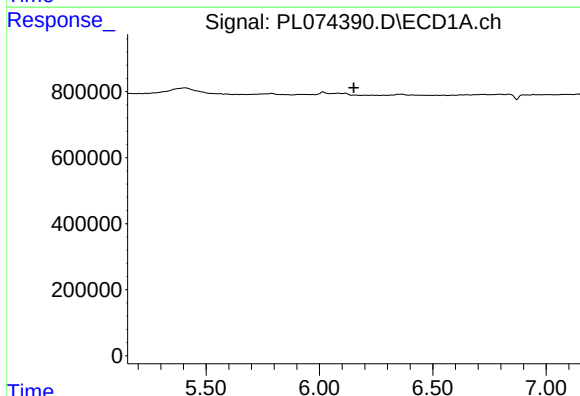


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

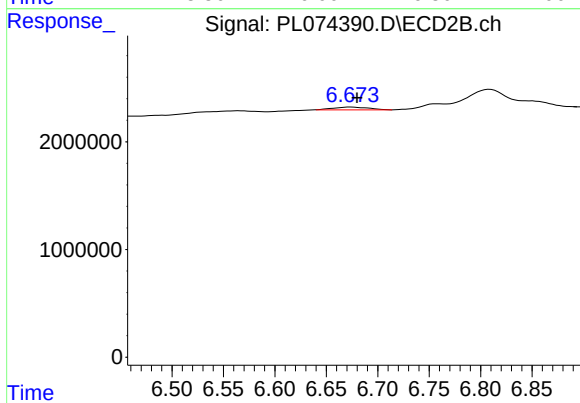

#6 beta-BHC


R.T.: 6.674 min
Delta R.T.: -0.006 min
Response: 612733
Conc: 0.54 ng/ml

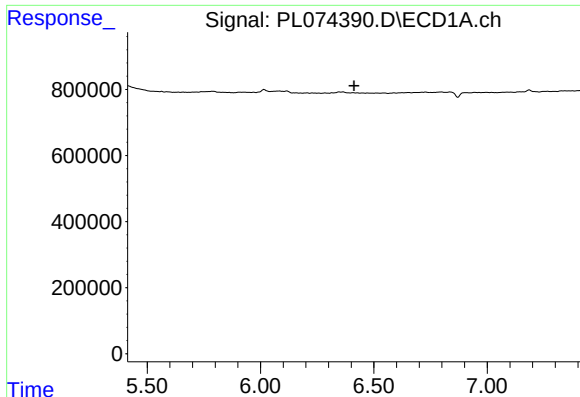

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

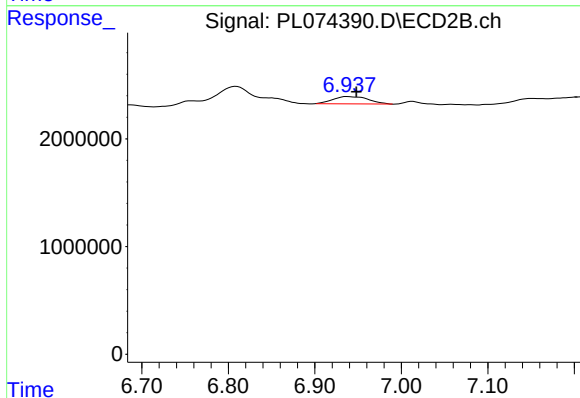


#7 delta-BHC

R.T.: 6.938 min
Delta R.T.: -0.010 min
Response: 1925841
Conc: 0.79 ng/ml

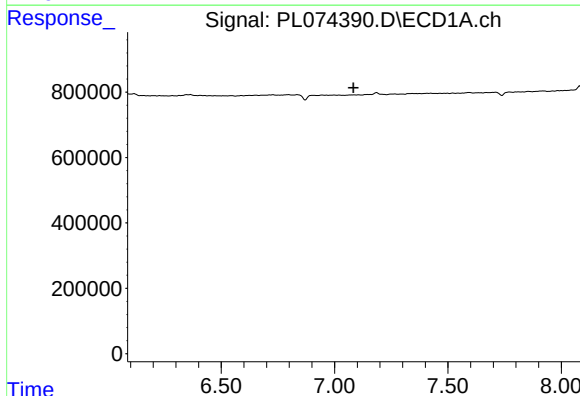


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

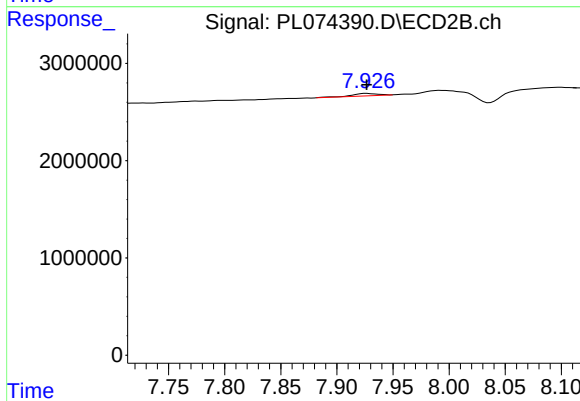

#8 Heptachlor epoxide


R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 408710
Conc: 0.18 ng/ml

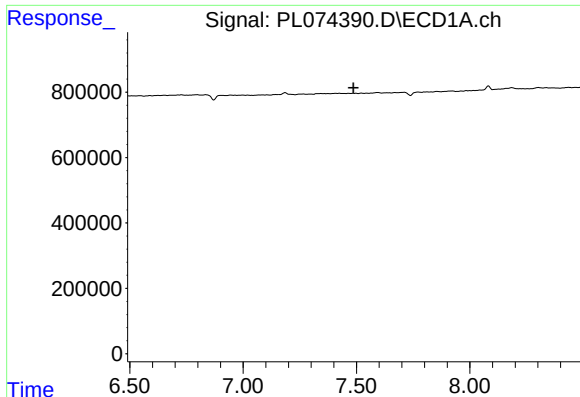

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

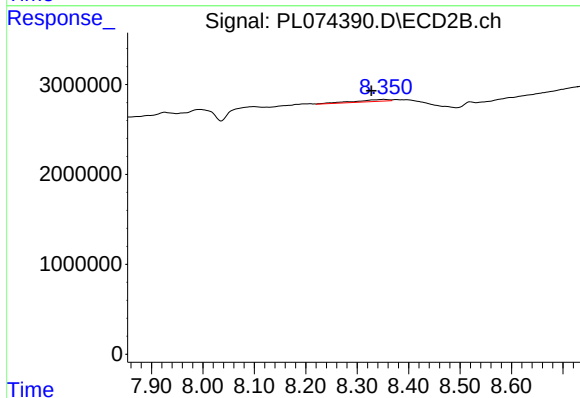


#9 Endosulfan I

R.T.: 8.352 min
Delta R.T.: 0.025 min
Response: 1047960
Conc: 0.53 ng/ml

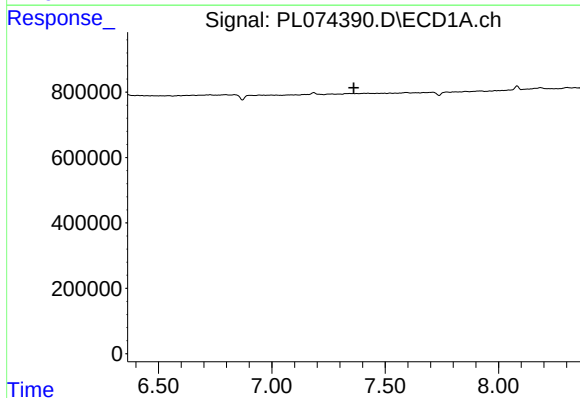


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

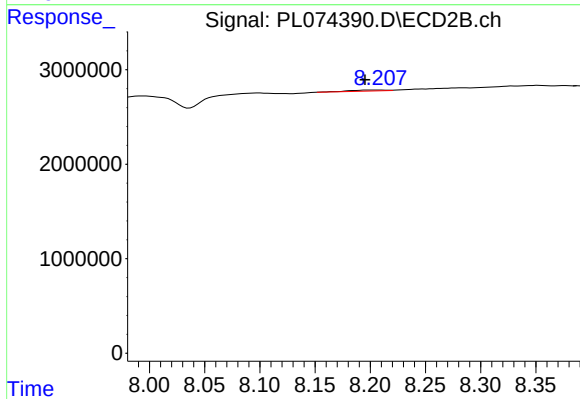

#10 gamma-Chlordane


R.T.: 8.209 min
Delta R.T.: 0.014 min
Response: 234002
Conc: 0.10 ng/ml

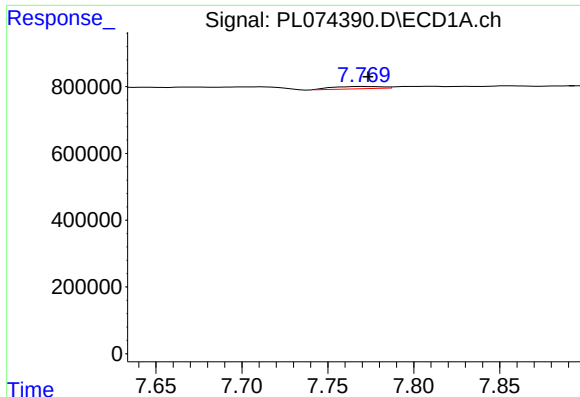

#13 Dieldrin


R.T.: 7.771 min
Delta R.T.: -0.003 min
Response: 138007
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

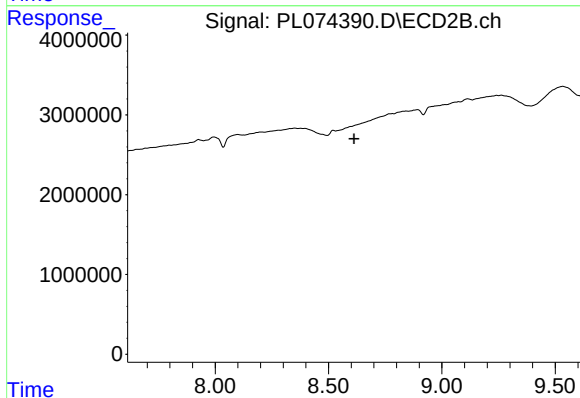


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.613 min
Response: 0
Conc: N.D.

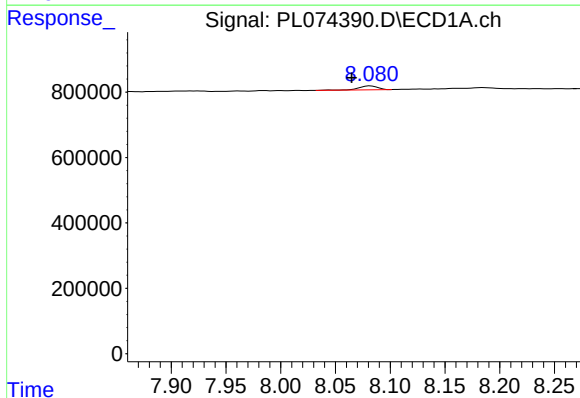


#14 Endrin

R.T.: 8.082 min
Delta R.T.: 0.017 min
Response: 142175
Conc: 0.35 ng/ml

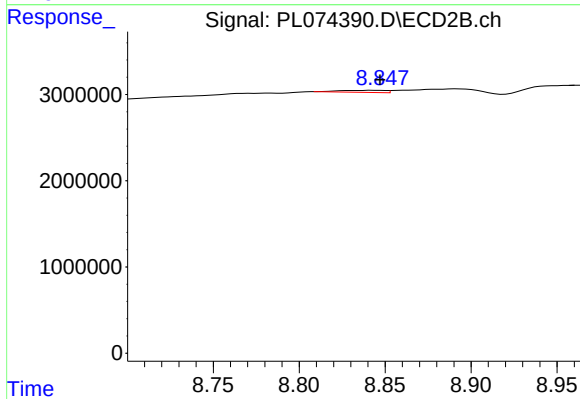

#14 Endrin


R.T.: 8.843 min
Delta R.T.: -0.004 min
Response: 434457
Conc: 0.26 ng/ml

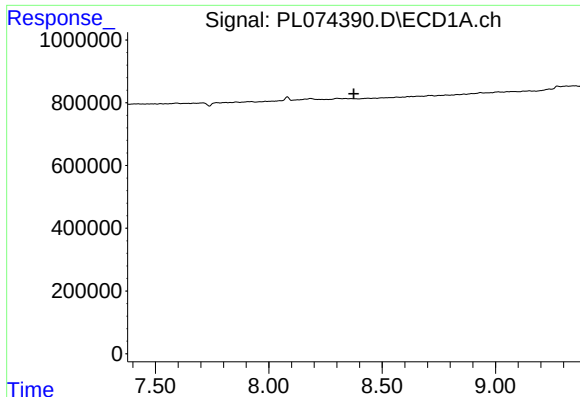

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

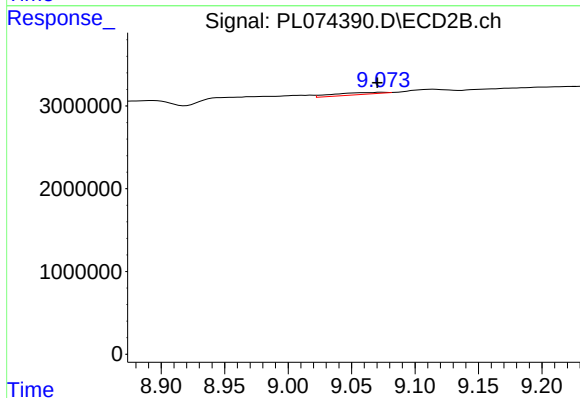


#15 Endosulfan II

R.T.: 9.074 min
Delta R.T.: 0.004 min
Response: 664148
Conc: 0.38 ng/ml

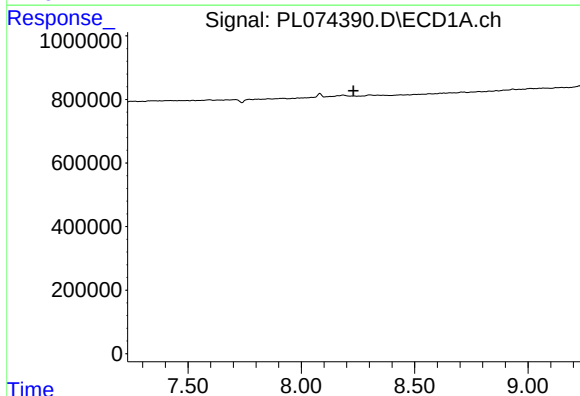


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

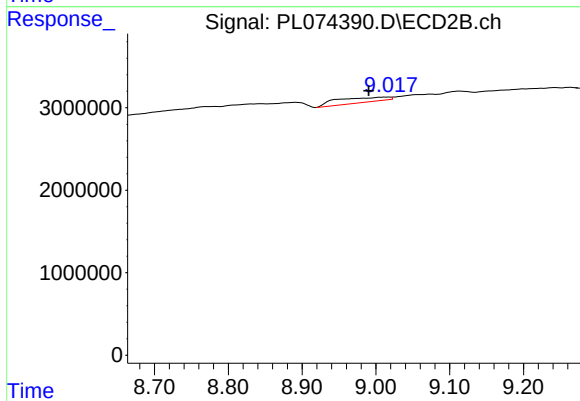

#16 4,4'-DDD


R.T.: 9.018 min
Delta R.T.: 0.028 min
Response: 2905049
Conc: 1.89 ng/ml

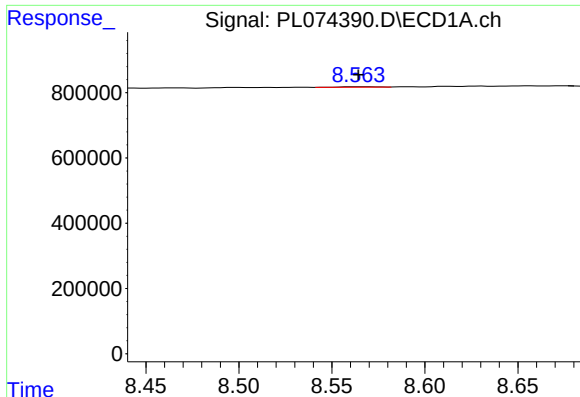

#18 Endrin aldehyde


R.T.: 8.564 min
Delta R.T.: 0.000 min
Response: 13716
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

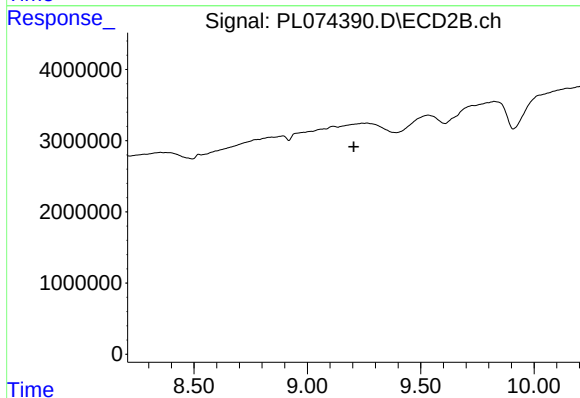


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.204 min
Response: 0
Conc: N.D.

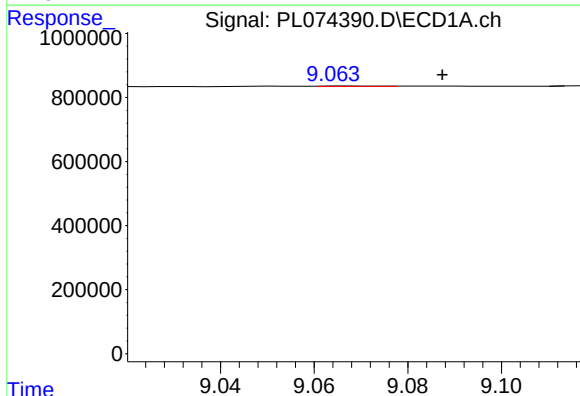


#20 Methoxychlor

R.T.: 9.068 min
Delta R.T.: -0.020 min
Response: 14774
Conc: 0.06 ng/ml

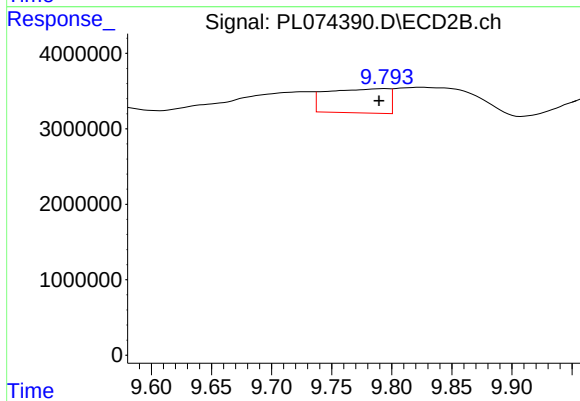

#20 Methoxychlor


R.T.: 9.795 min
Delta R.T.: 0.005 min
Response: 11429390
Conc: 11.88 ng/ml

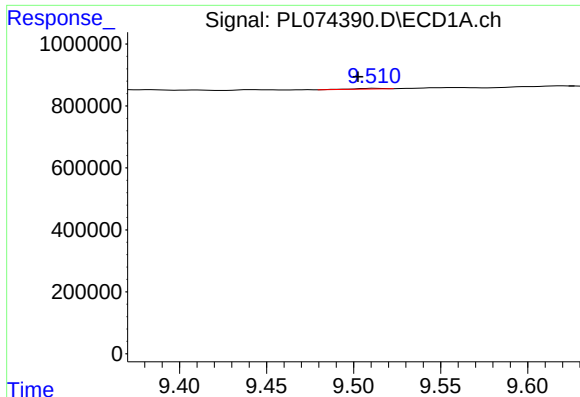

#22 Mirex


R.T.: 9.512 min
Delta R.T.: 0.010 min
Response: 27578
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

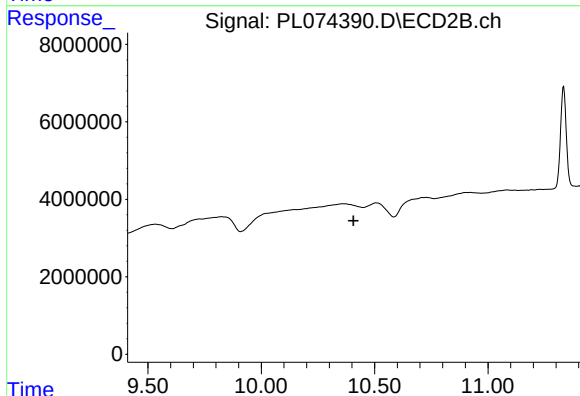


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.407 min
Response: 0
Conc: N.D.

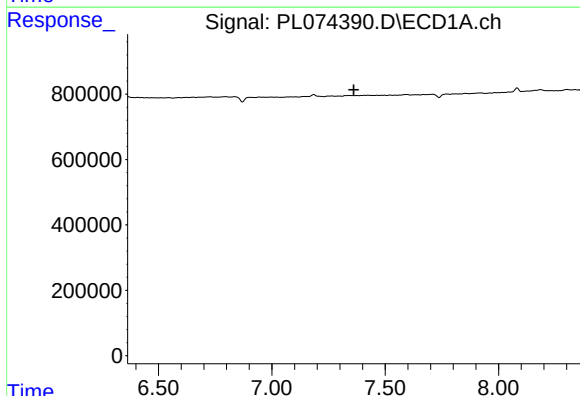


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

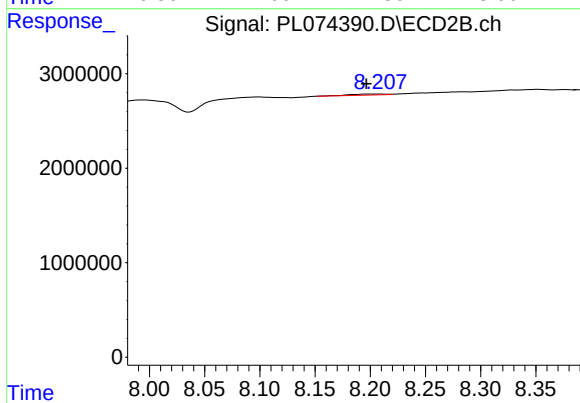

#25 Chlordane-3


R.T.: 8.209 min
Delta R.T.: 0.012 min
Response: 234002
Conc: 0.69 ng/ml

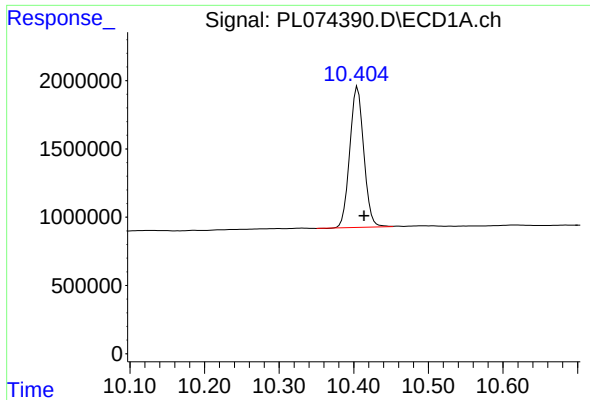

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 13419904
Conc: 25.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

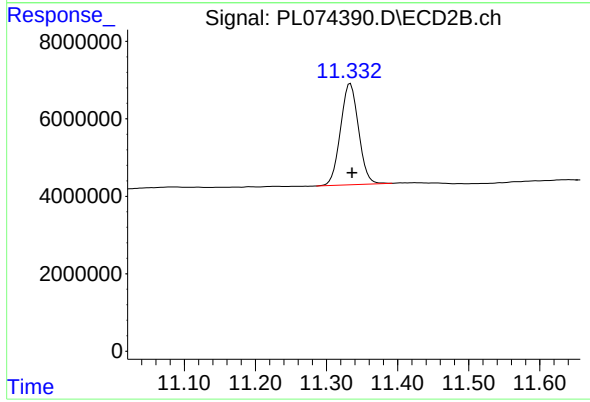

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: -0.002 min
Response: 46079171
Conc: 26.09 ng/ml