

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
 Data File : PL074373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 16:14
 Operator : AR\AJ
 Sample : N2502-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/27/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 20:49:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.490	6723284	33343594	20.808	18.701
28)	SA Decachlor...	10.404	11.333	10120687	32184997	19.462m	18.222
Target Compounds							
12)	B 4,4'-DDE	7.639	8.457	403851	7833582	1.107	3.933m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
Data File : PL074373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 16:14
Operator : AR\AJ
Sample : N2502-05
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
C3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/27/2022
Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 20:49:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

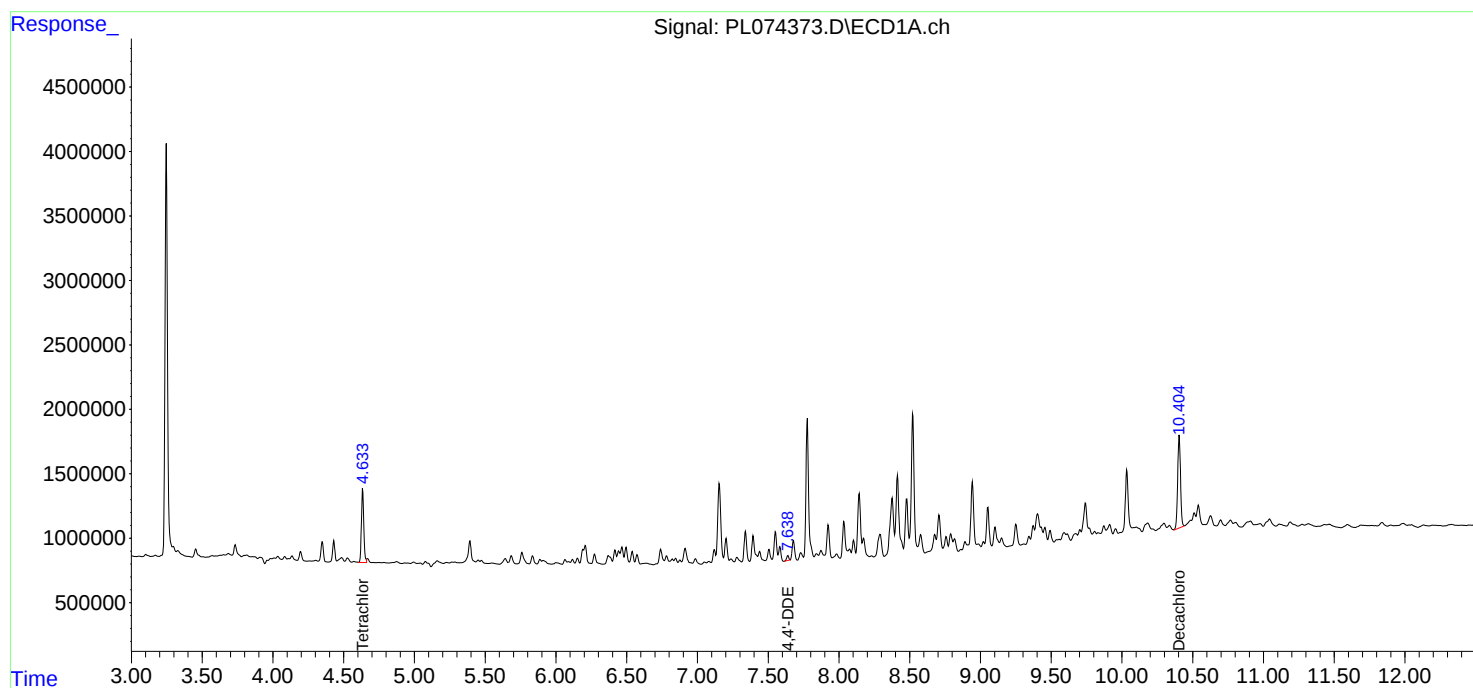

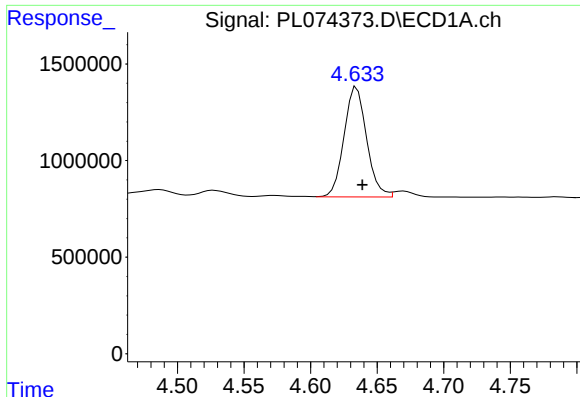


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 6723284
Conc: 20.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
C3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/27/2022
Supervised By :mohammad ahmed 04/28/2022

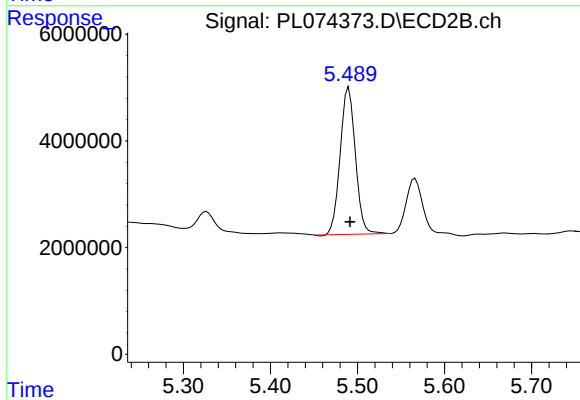


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 33343594
Conc: 18.70 ng/ml

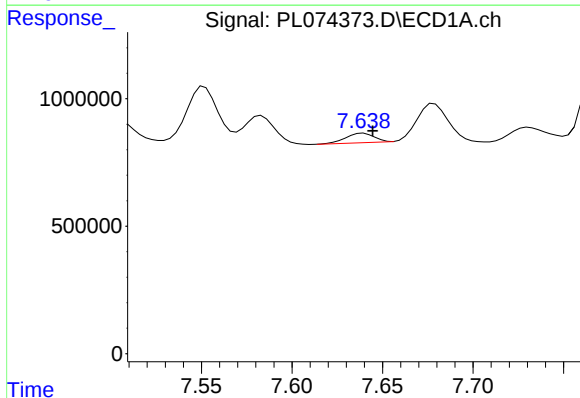


#12 4,4'-DDE

R.T.: 7.639 min
Delta R.T.: -0.005 min
Response: 403851
Conc: 1.11 ng/ml

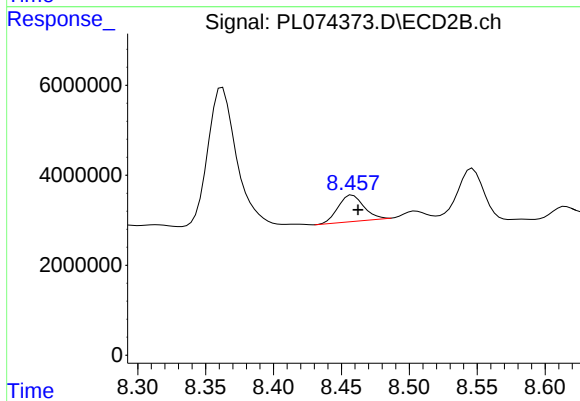

#12 4,4'-DDE

R.T.: 8.457 min
Delta R.T.: -0.006 min
Response: 7833582
Conc: 3.93 ng/ml m

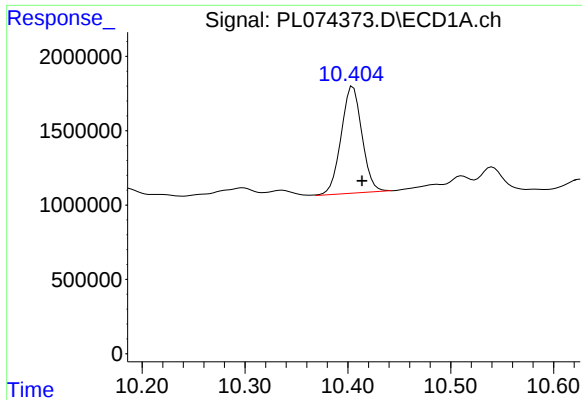


#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 10120687
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
C3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/27/2022
Supervised By :mohammad ahmed 04/28/2022

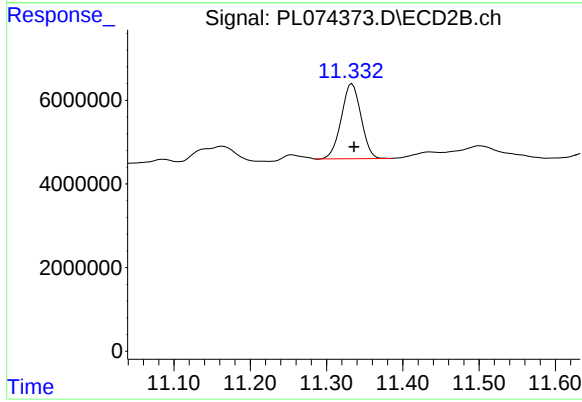

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 32184997
Conc: 18.22 ng/ml