

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
 Data File : PL074389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2022 23:23
 Operator : AR\AJ
 Sample : N2563-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 STORM-WATER-042622

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/27/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 00:28:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.488	6155852	48689767	19.052	27.308 #
2)	SA Decachlor...	10.404	11.334	7592271	27042521	14.600m	15.310

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042622\
Data File : PL074389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2022 23:23
Operator : AR\AJ
Sample : N2563-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
STORM-WATER-042622


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/27/2022
Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 00:28:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

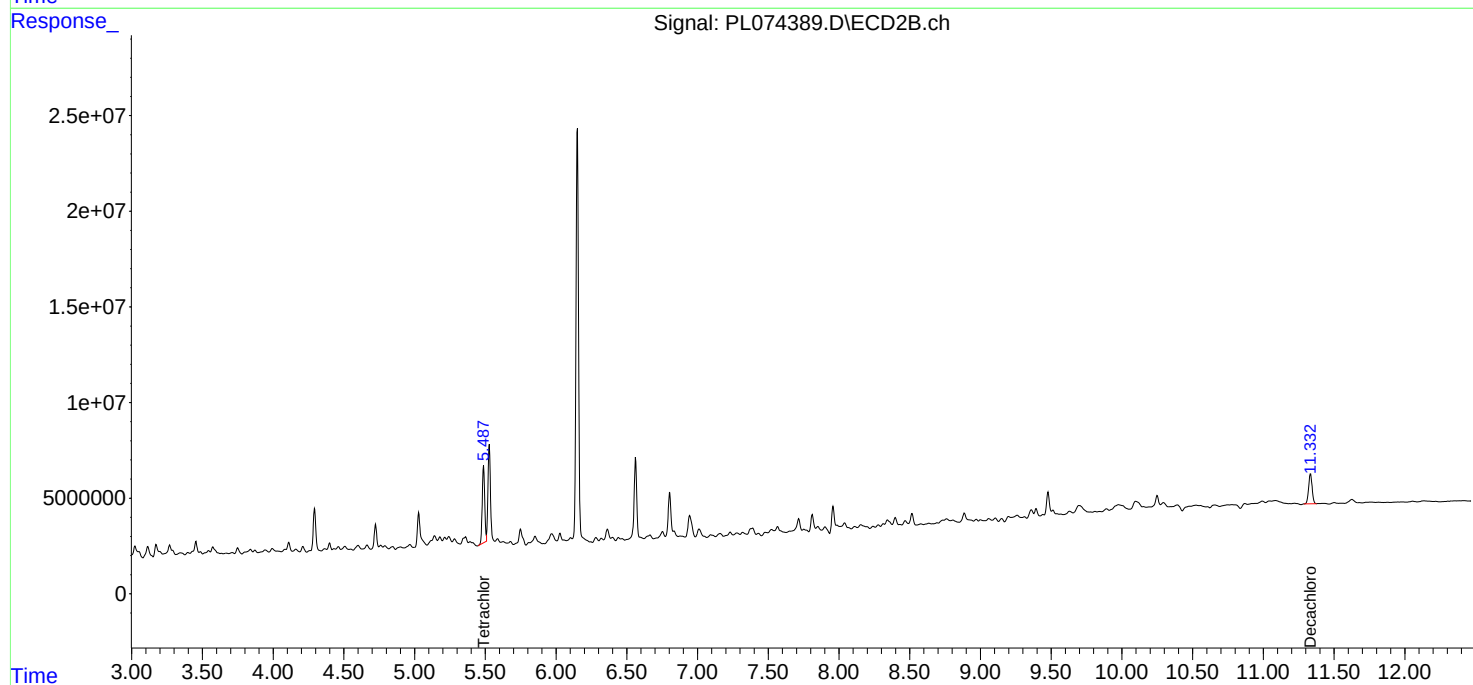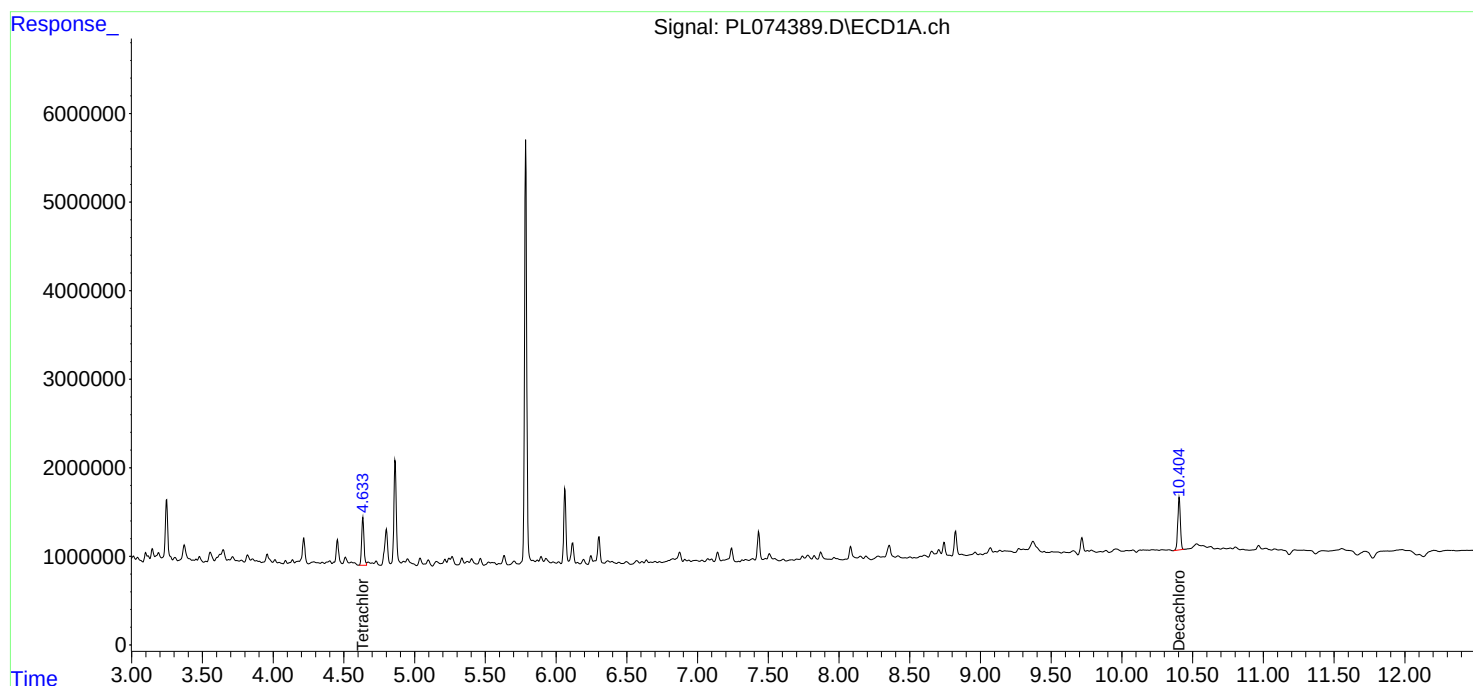

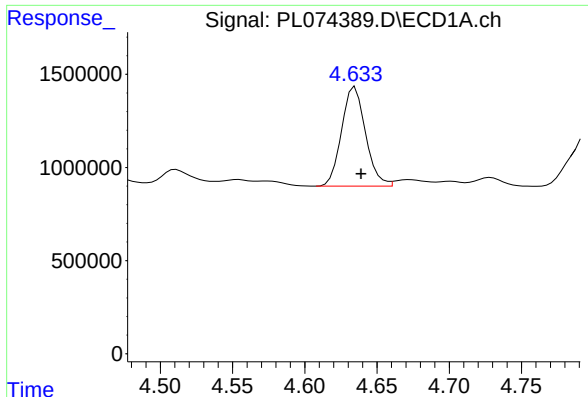


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 6155852
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
STORM-WATER-042622


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/27/2022
Supervised By :mohammad ahmed 04/28/2022

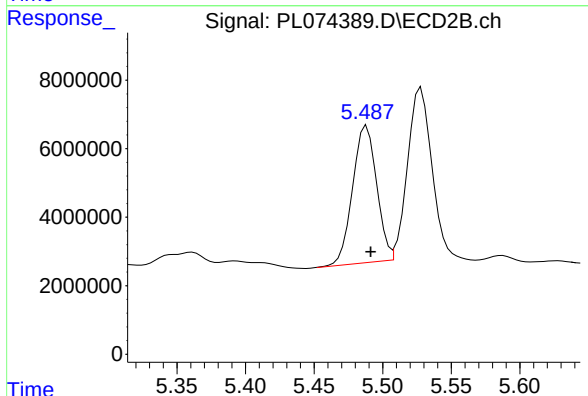


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 48689767
Conc: 27.31 ng/ml

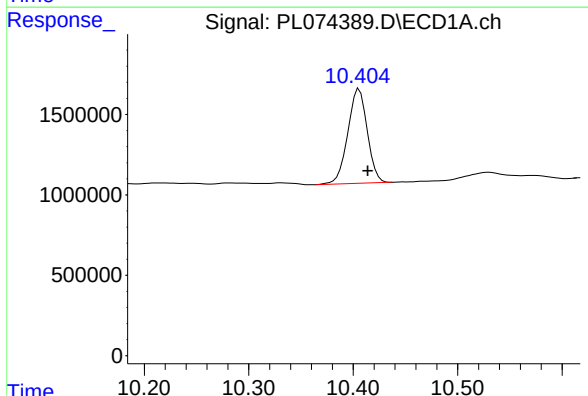

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 7592271
Conc: 14.60 ng/ml m

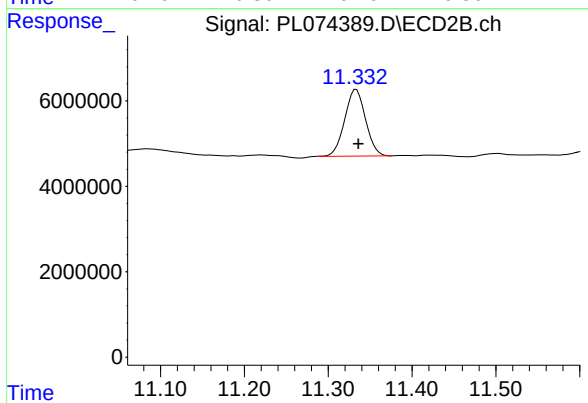

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: -0.003 min
Response: 27042521
Conc: 15.31 ng/ml