

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042623\
 Data File : PL082342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2023 14:37
 Operator : AR\AJ
 Sample : 02491-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S2S-TP4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 21:33:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	2.648	52962033	45815974	19.827	19.776
28) SA Decachlor...	8.740	7.758	34047747	35777213	17.835	15.675
Target Compounds						
13) MA Dieldrin	6.096	5.213	2958419	2995960	1.072	1.109



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042623\
Data File : PL082342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2023 14:37
Operator : AR\AJ
Sample : 02491-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S2S-TP4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 21:33:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

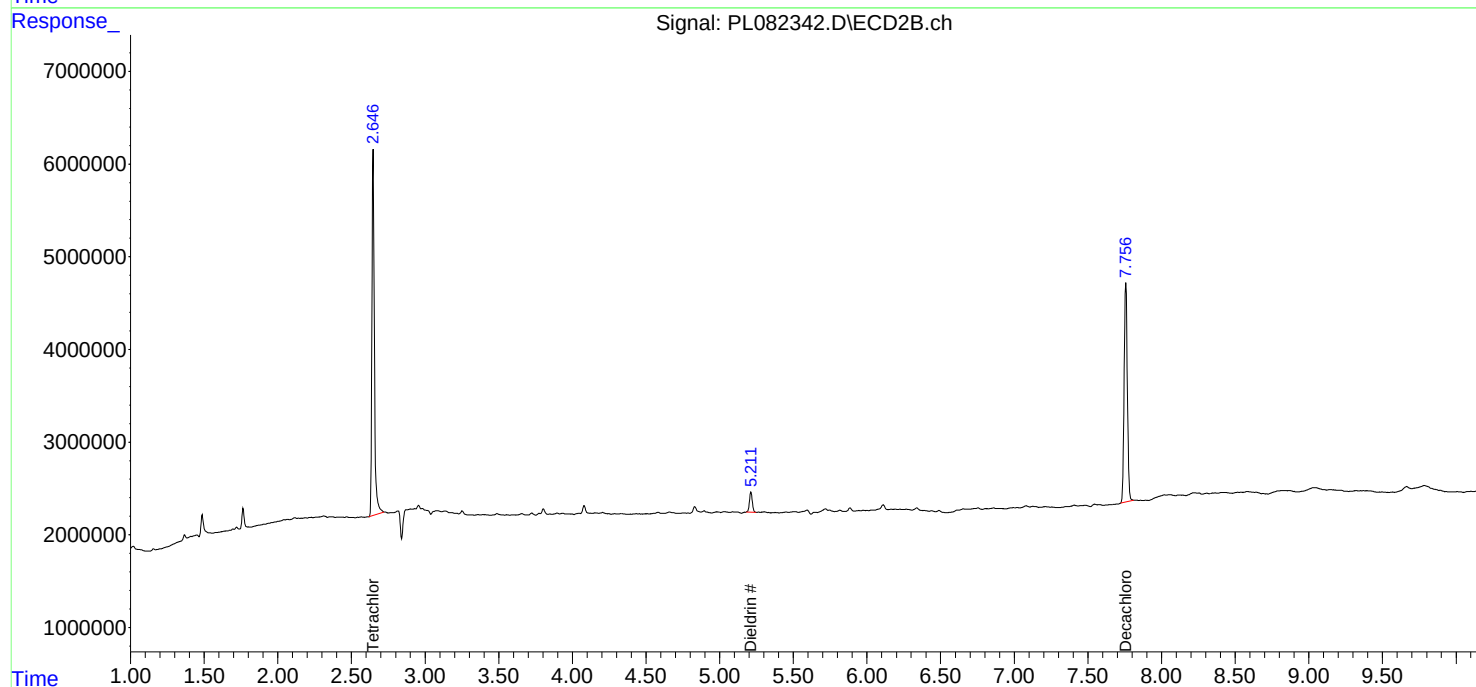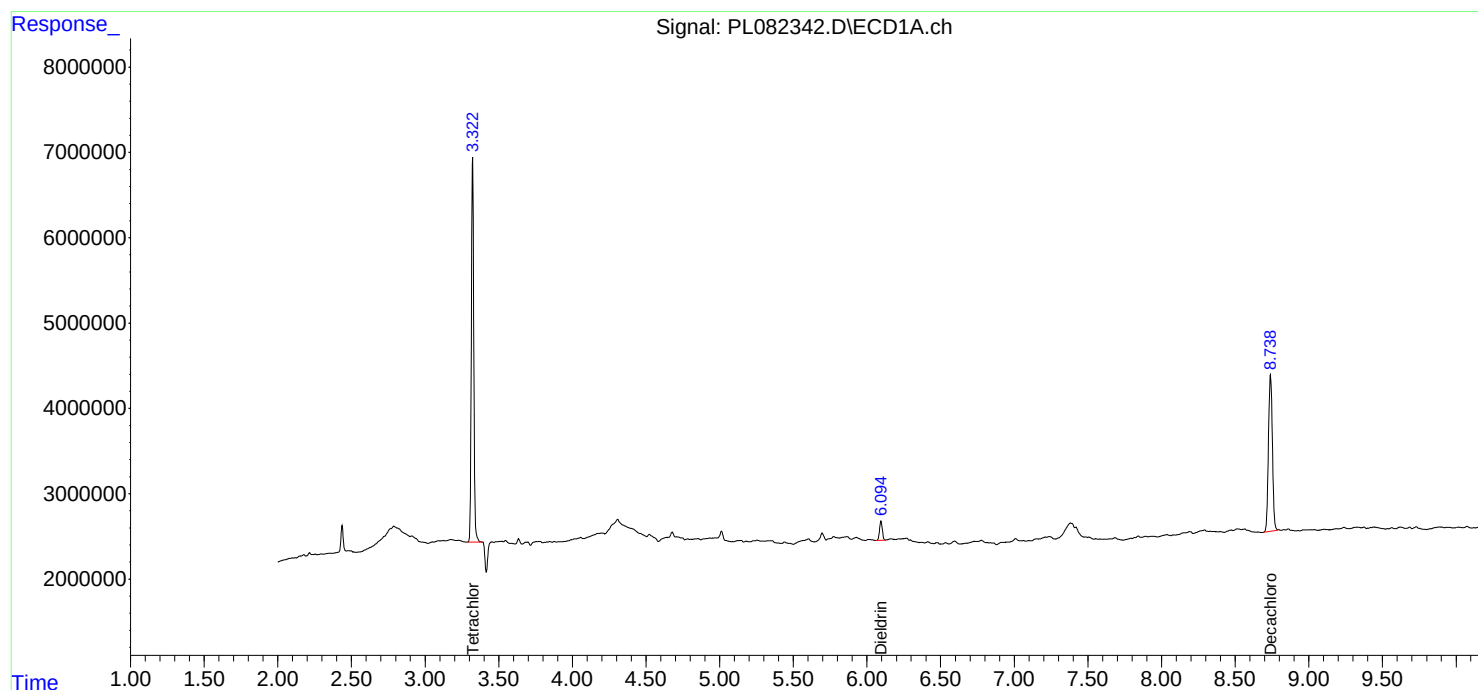


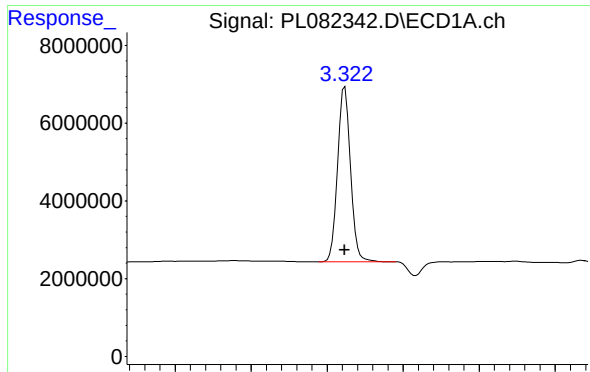

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 52962033
Conc: 19.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2S-TP4

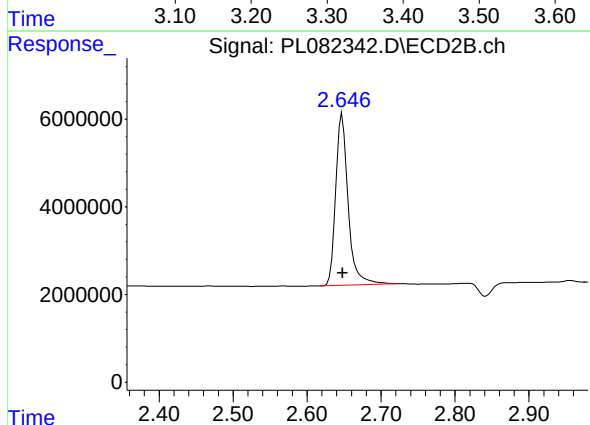


#1 Tetrachloro-m-xylene

R.T.: 2.648 min
Delta R.T.: 0.000 min
Response: 45815974
Conc: 19.78 ng/ml

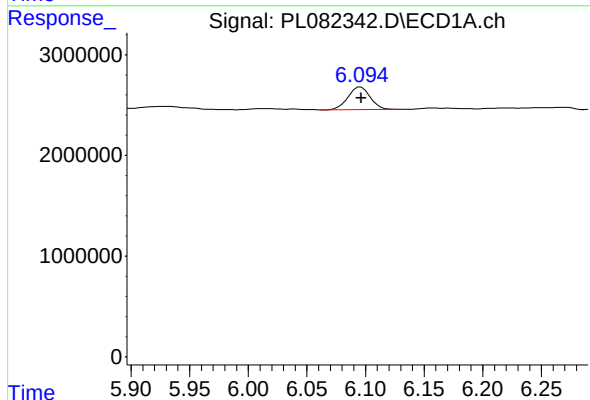


#13 Dieldrin

R.T.: 6.096 min
Delta R.T.: 0.000 min
Response: 2958419
Conc: 1.07 ng/ml

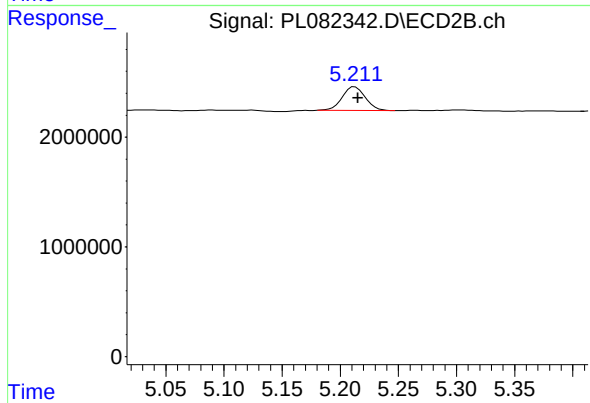

#13 Dieldrin


R.T.: 5.213 min
Delta R.T.: -0.003 min
Response: 2995960
Conc: 1.11 ng/ml

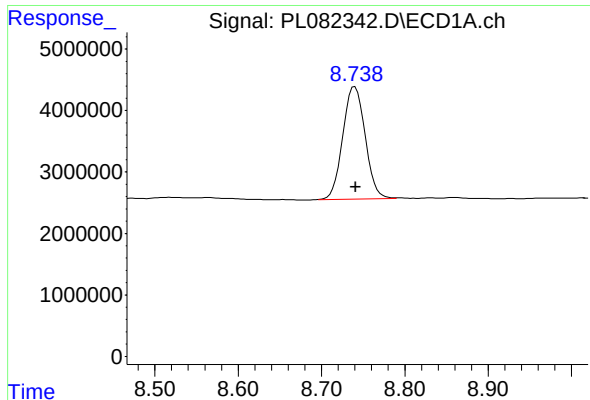

#28 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.001 min
Response: 34047747
Conc: 17.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2S-TP4

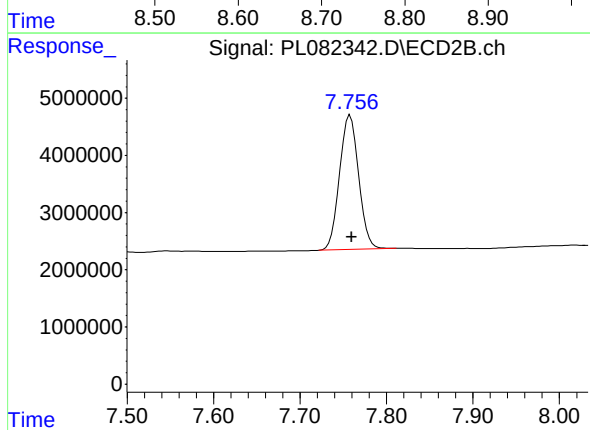

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 35777213
Conc: 15.67 ng/ml