

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
 Data File : PL089197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 14:51
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:53:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 15:50:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.796	186.3E6	161.7E6	98.264	101.213
28) SA Decachlor...	9.061	7.947	130.3E6	132.9E6	97.869	98.974
Target Compounds						
23) Chlordane-1	4.712	3.800	83435089	49210123	976.305	1008.624
24) Chlordane-2	5.240	4.378	91541700	59287117	963.558	984.682
25) Chlordane-3	5.950	5.009	303.4E6	174.7E6	994.259	1019.697
26) Chlordane-4	6.033	5.072	371.9E6	162.3E6	989.670	1012.908
27) Chlordane-5	6.880	5.738	76468373	48765660	976.459	996.832



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
Data File : PL089197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 14:51
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:53:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 15:50:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

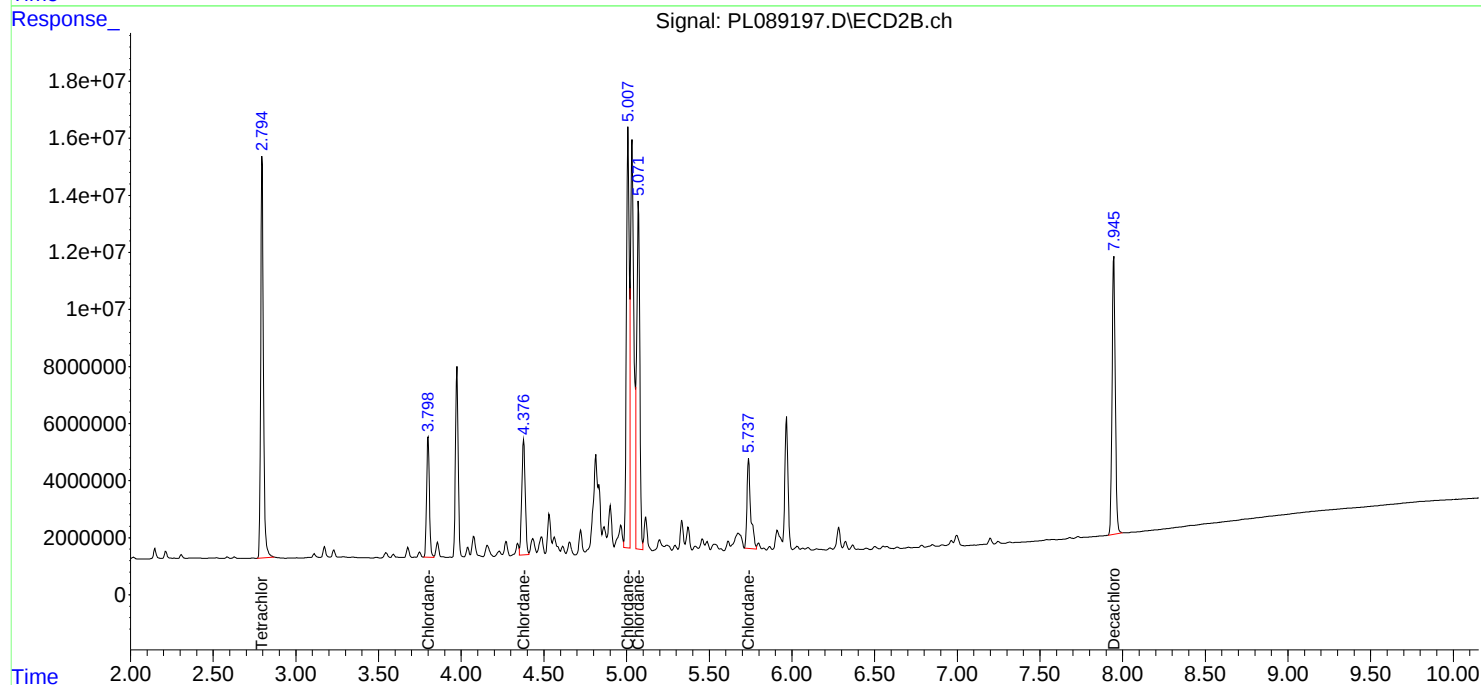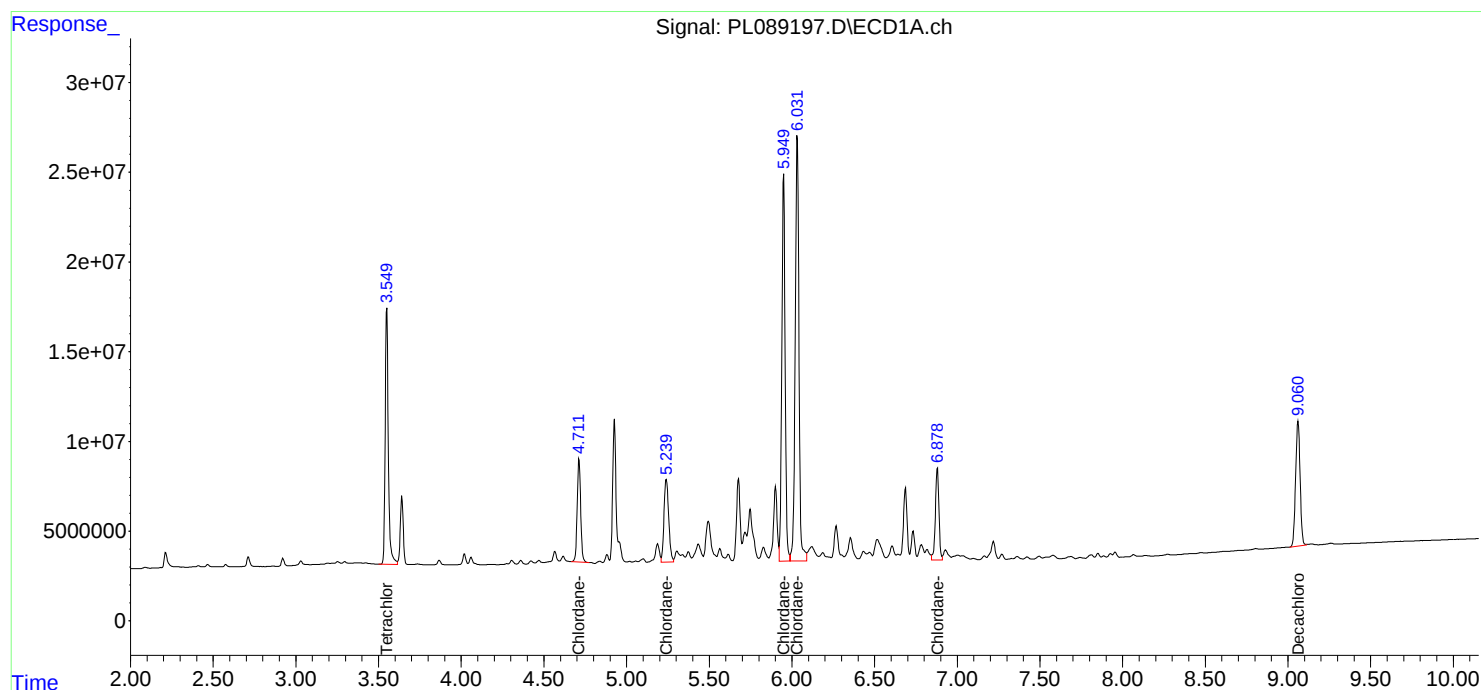


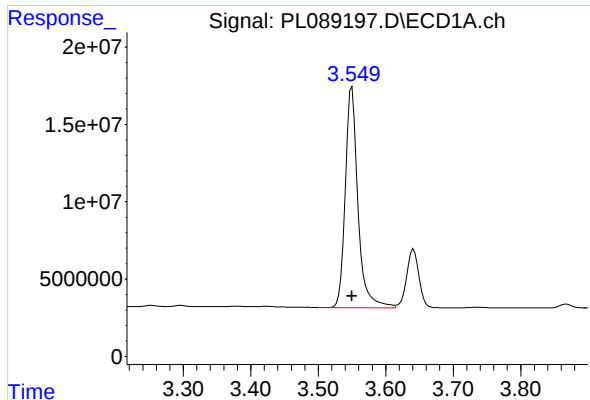

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 186250945
Conc: 98.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

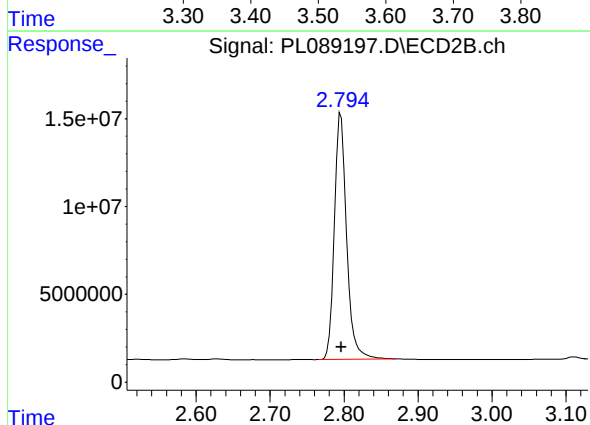


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 161736946
Conc: 101.21 ng/ml

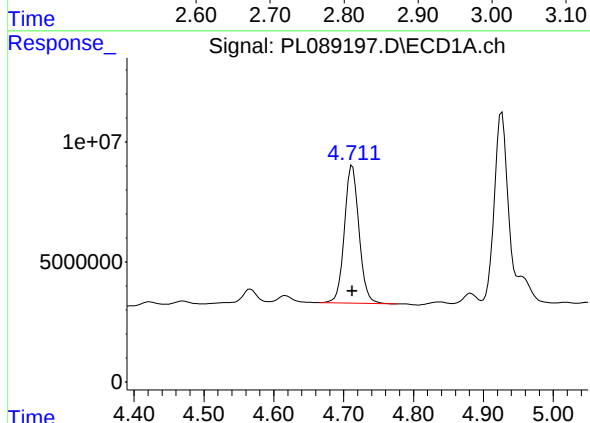


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 83435089
Conc: 976.31 ng/ml

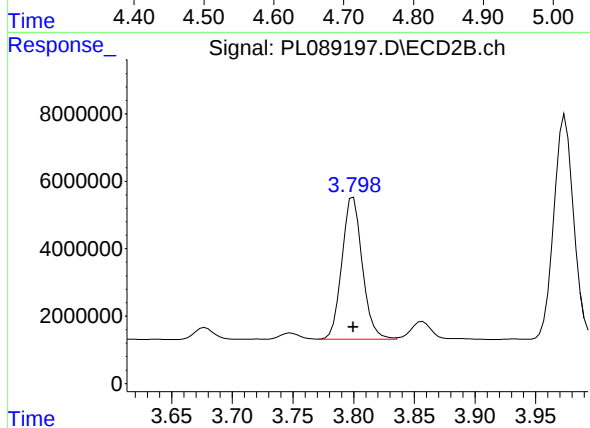

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 49210123
Conc: 1008.62 ng/ml

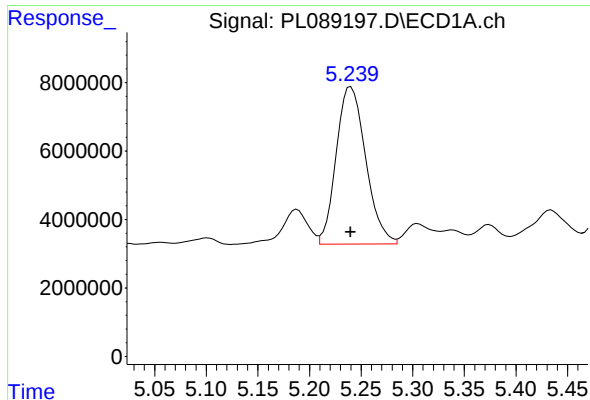

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 91541700
Conc: 963.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

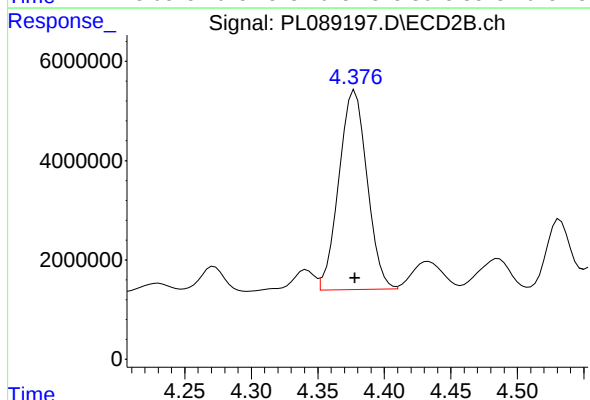


#24 Chlordane-2

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 59287117
Conc: 984.68 ng/ml

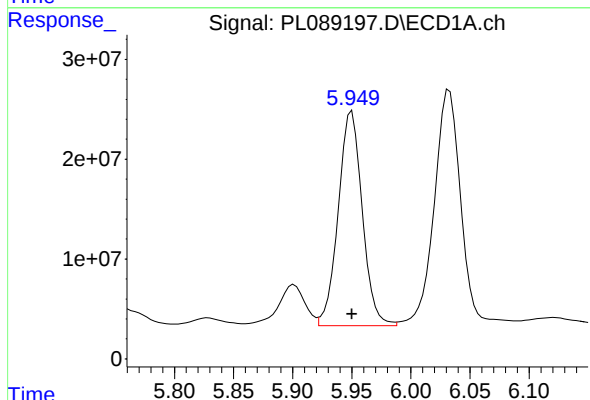


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 303392482
Conc: 994.26 ng/ml

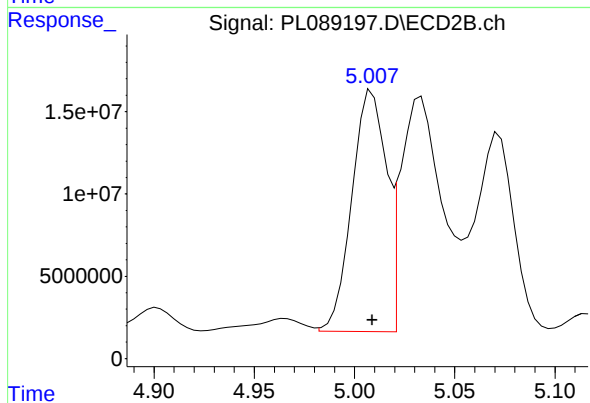

#25 Chlordane-3


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 174716440
Conc: 1019.70 ng/ml

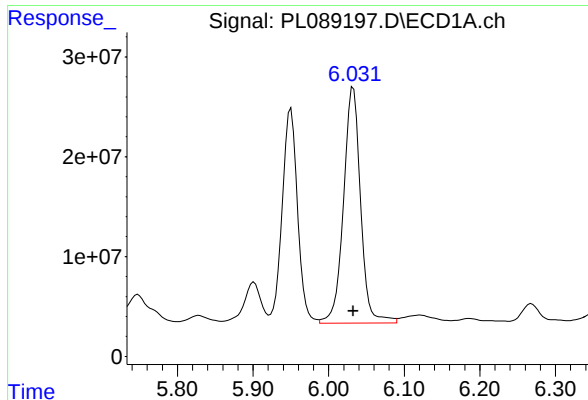

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 371891858
Conc: 989.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

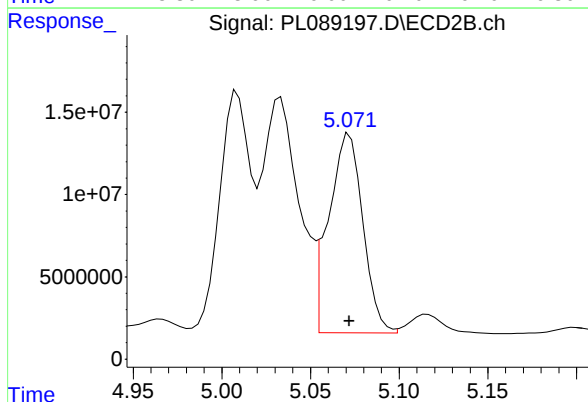


#26 Chlordane-4

R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 162325734
Conc: 1012.91 ng/ml

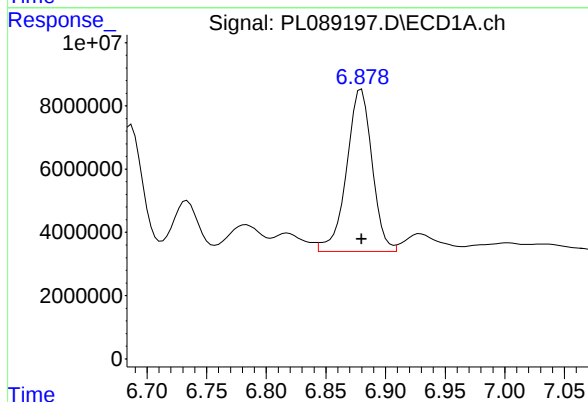


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 76468373
Conc: 976.46 ng/ml

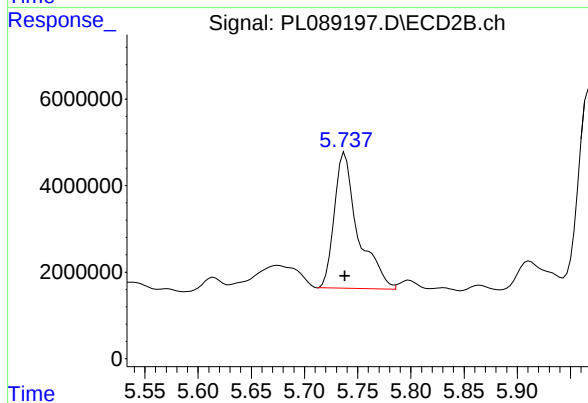

#27 Chlordane-5


R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 48765660
Conc: 996.83 ng/ml

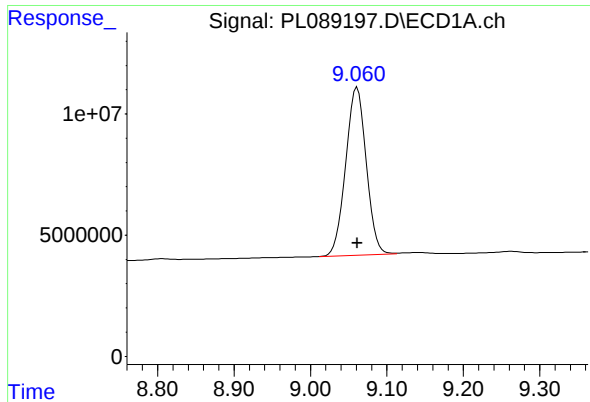

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 130345235
Conc: 97.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

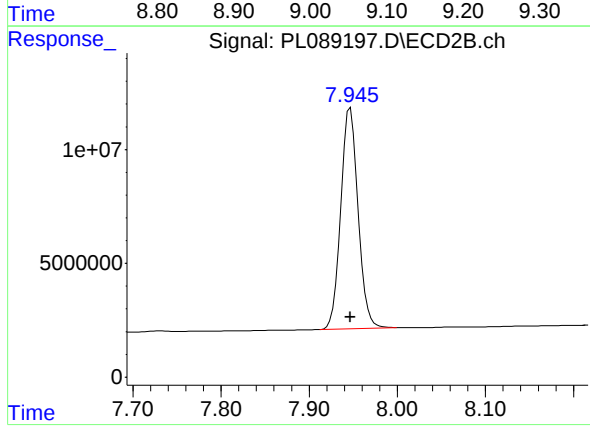

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 132894976
Conc: 98.97 ng/ml