

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
 Data File : PL089198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 15:05
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:55:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 15:50:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.796	136.7E6	115.6E6	73.042	73.221
28) SA Decachlor...	9.061	7.947	95424365	96774661	72.732	73.023
Target Compounds						
23) Chlordane-1	4.712	3.800	61831821	35285481	732.135	731.932
24) Chlordane-2	5.241	4.378	68666043	43741510	731.625	734.161
25) Chlordane-3	5.951	5.009	221.2E6	124.9E6	733.144	735.727
26) Chlordane-4	6.033	5.072	272.7E6	115.4E6	733.682	729.614
27) Chlordane-5	6.881	5.739	56701793	35725836	732.498	736.738



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
Data File : PL089198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 15:05
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:55:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 15:50:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

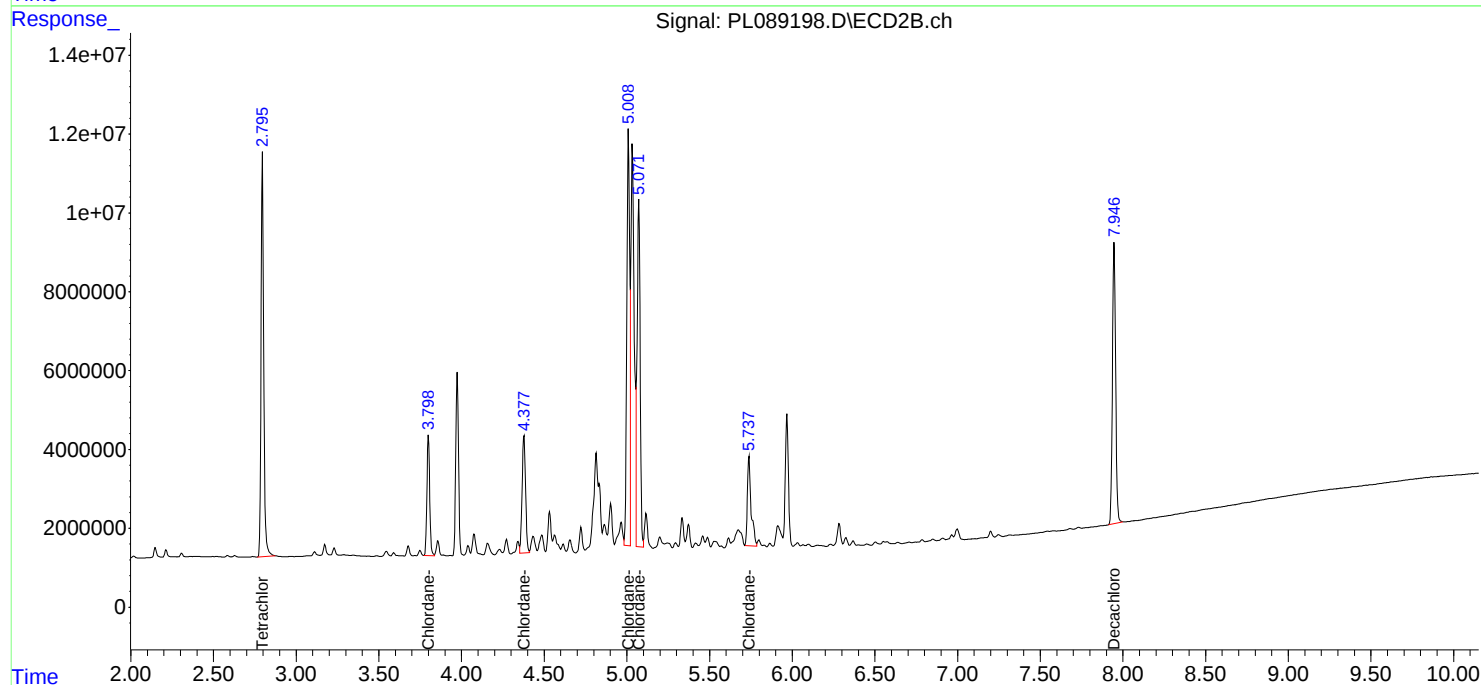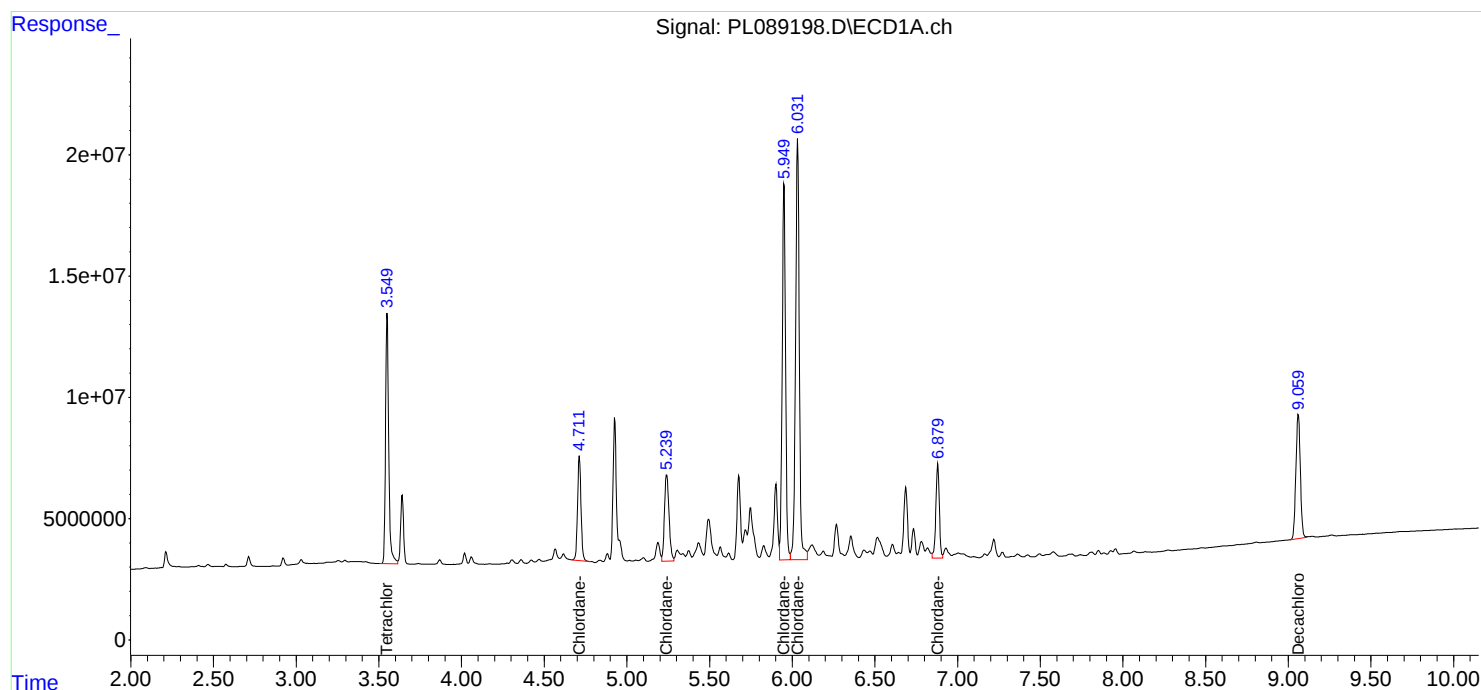


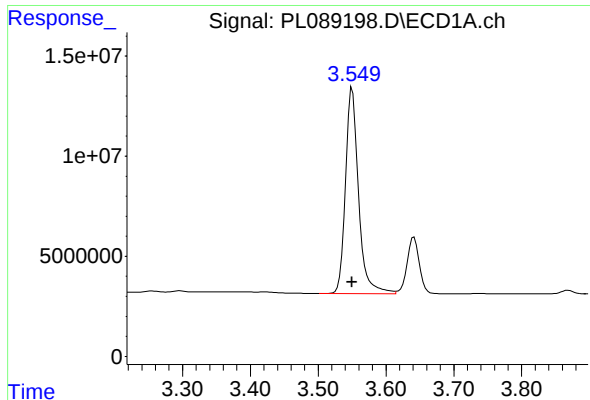

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 136662186
Conc: 73.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

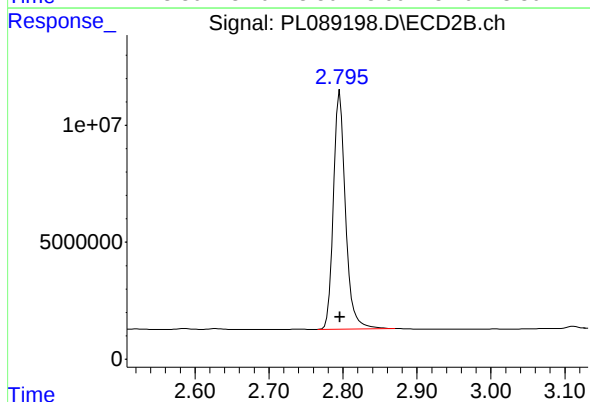


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 115634815
Conc: 73.22 ng/ml

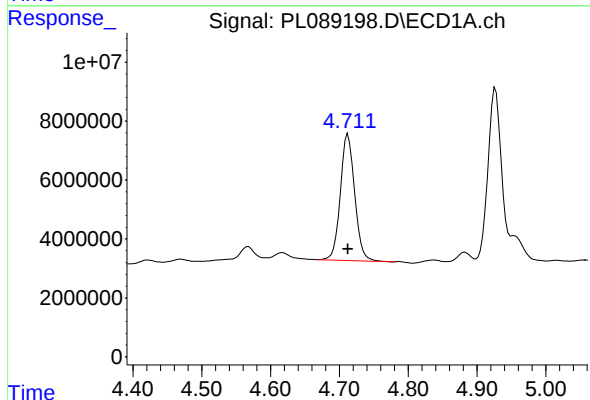


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 61831821
Conc: 732.13 ng/ml

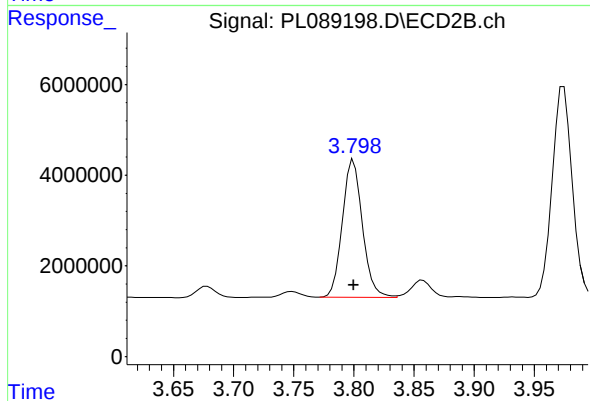

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 35285481
Conc: 731.93 ng/ml

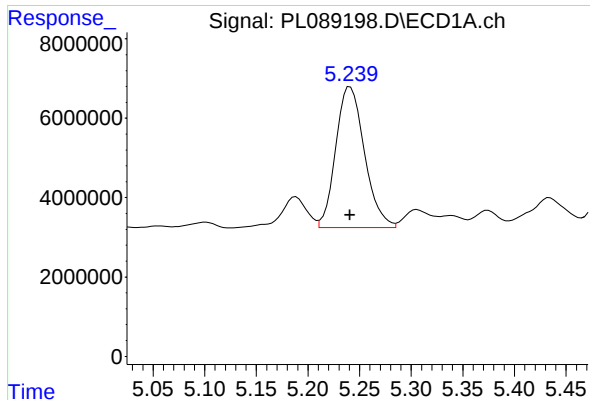

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 68666043
Conc: 731.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

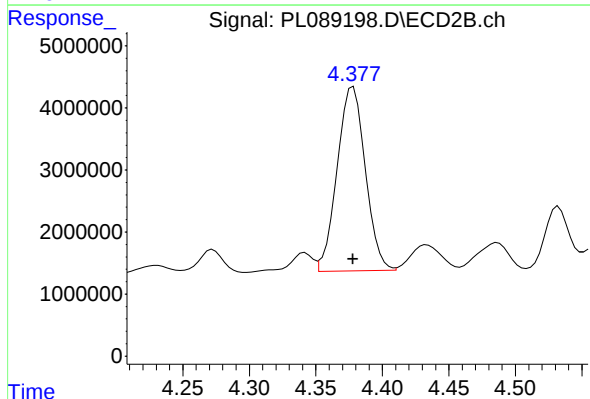


#24 Chlordane-2

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 43741510
Conc: 734.16 ng/ml

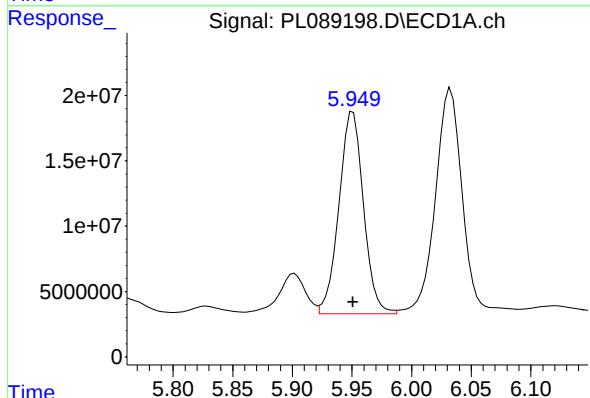


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 221228903
Conc: 733.14 ng/ml

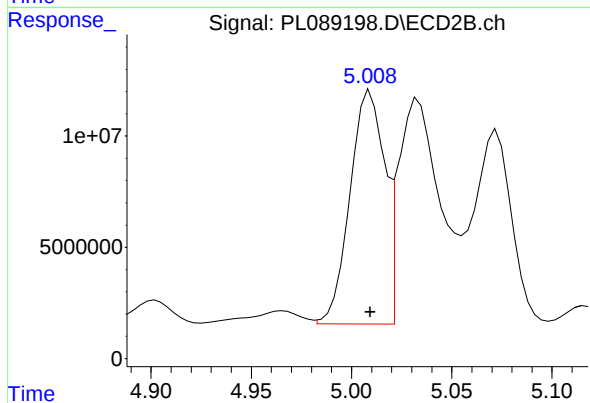

#25 Chlordane-3


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 124872497
Conc: 735.73 ng/ml

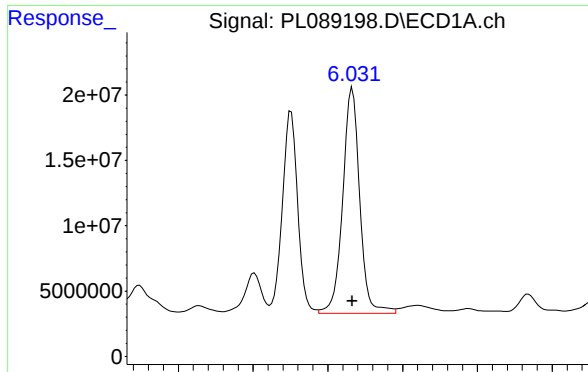

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 272730991
Conc: 733.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

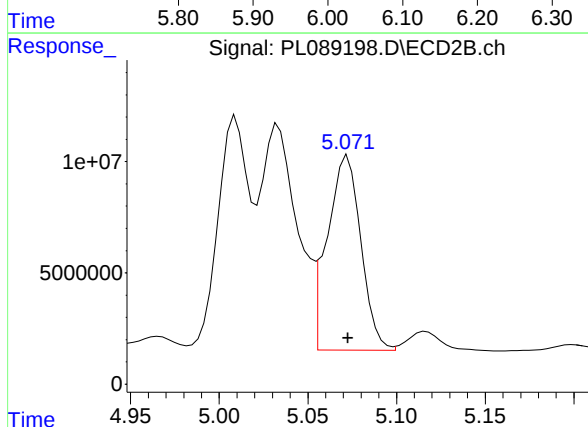


#26 Chlordane-4

R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 115357912
Conc: 729.61 ng/ml

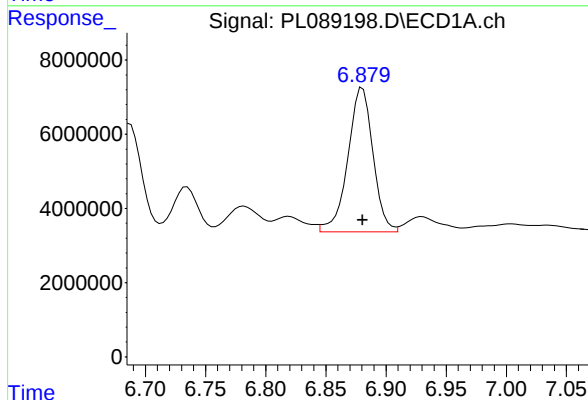


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 56701793
Conc: 732.50 ng/ml

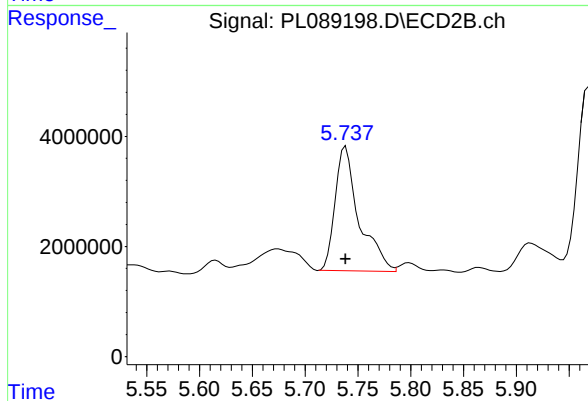

#27 Chlordane-5


R.T.: 5.739 min
Delta R.T.: 0.000 min
Response: 35725836
Conc: 736.74 ng/ml

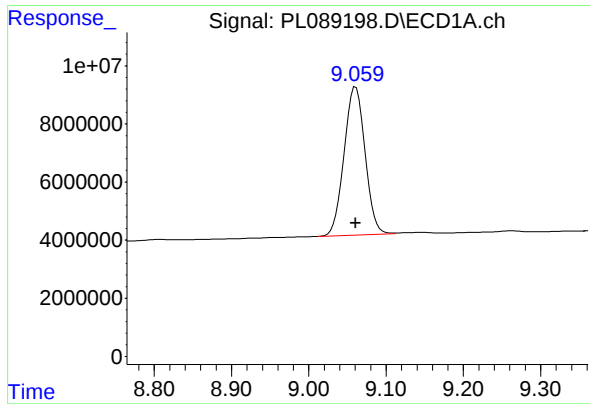

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 95424365
Conc: 72.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

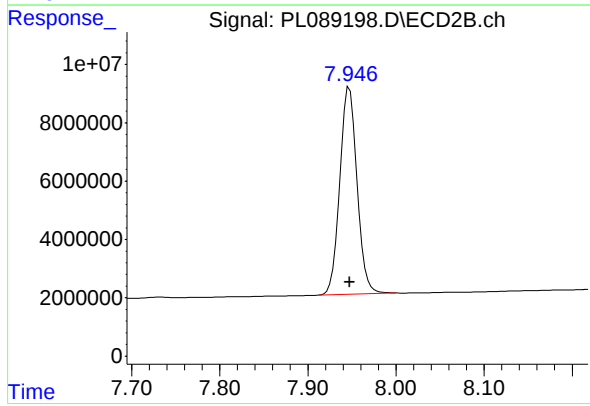

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 96774661
Conc: 73.02 ng/ml