

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
 Data File : PL089199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 15:19
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:51:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 15:50:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.796	96416417	78930365	50.000	50.000
28) SA Decachlor...	9.061	7.947	68011218	67824592	50.000	50.000
Target Compounds						
23) Chlordane-1	4.713	3.800	43742495	24184280	500.000	500.000
24) Chlordane-2	5.240	4.378	49232943	30565822	500.000	500.000
25) Chlordane-3	5.951	5.010	153.4E6	83983389	500.000	500.000
26) Chlordane-4	6.033	5.072	189.8E6	79094219	500.000	500.000
27) Chlordane-5	6.880	5.738	40077748	24537796	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
Data File : PL089199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 15:19
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:51:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 15:50:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

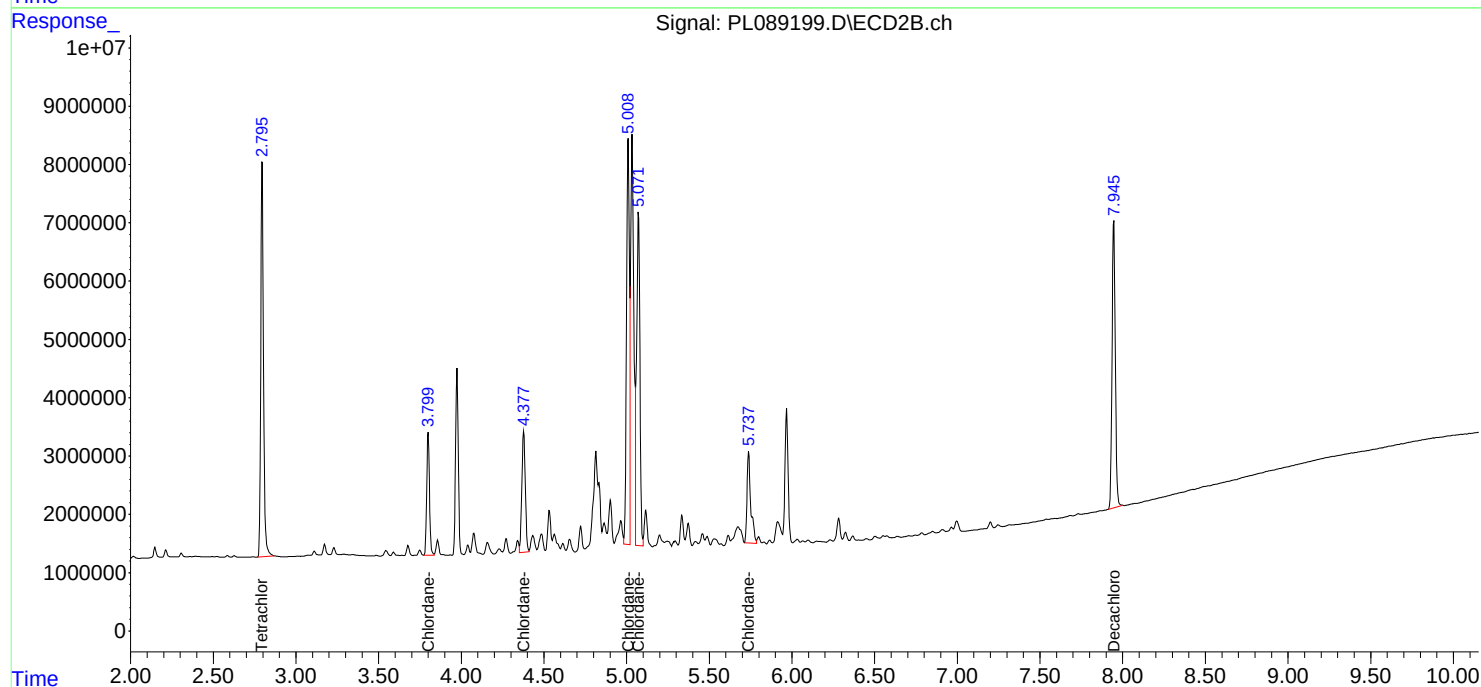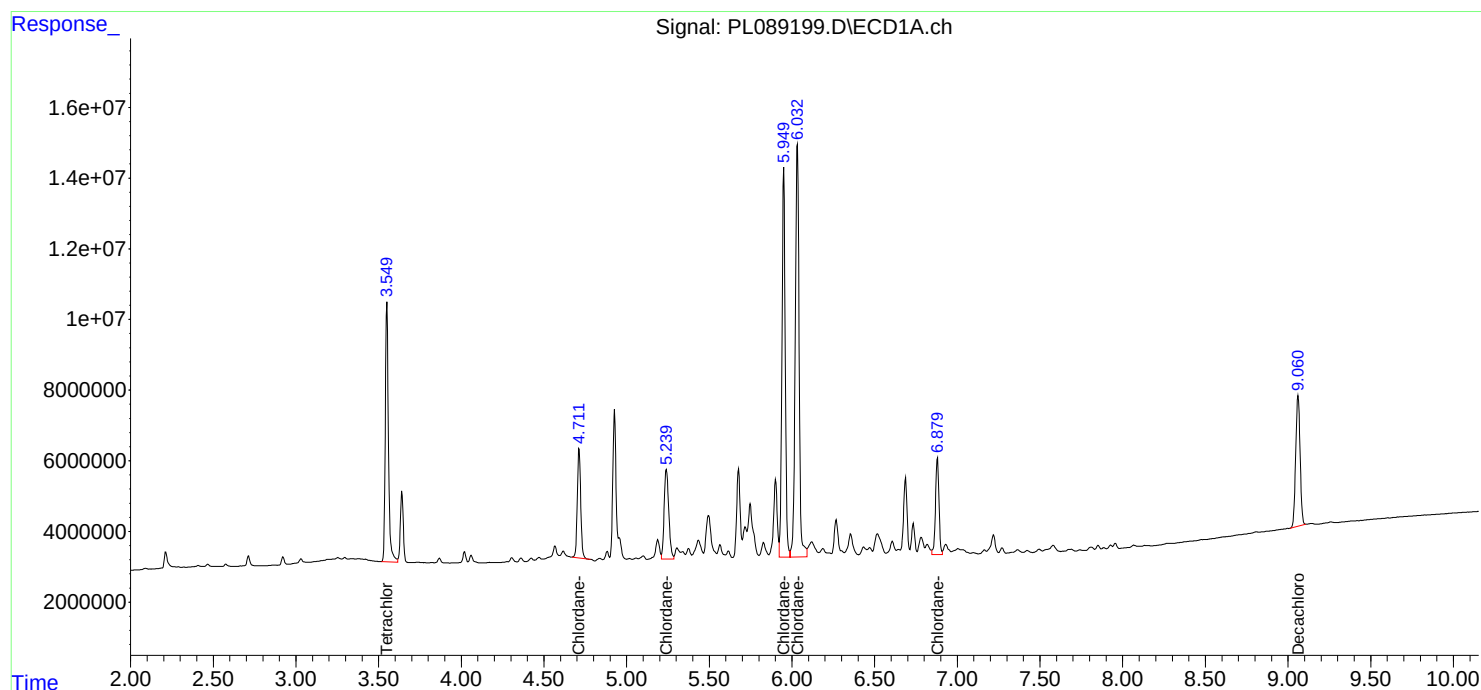


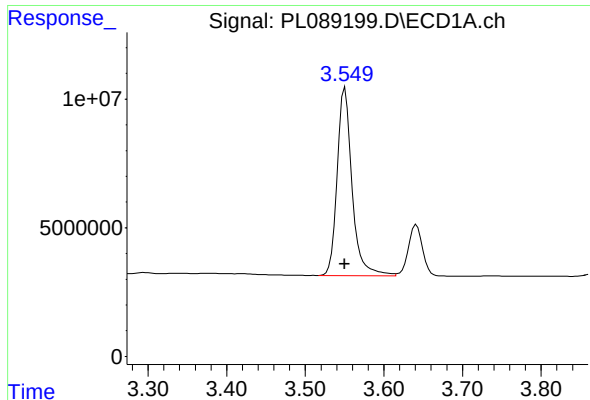

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 96416417
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

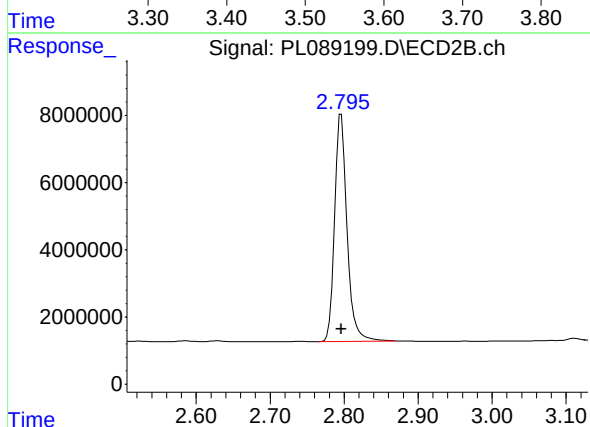


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 78930365
Conc: 50.00 ng/ml

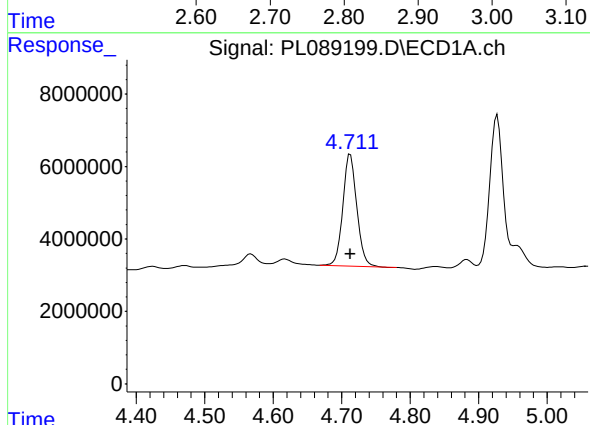


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 43742495
Conc: 500.00 ng/ml

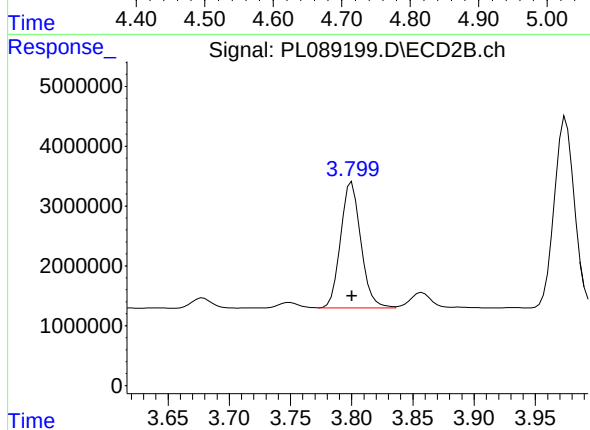

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 24184280
Conc: 500.00 ng/ml

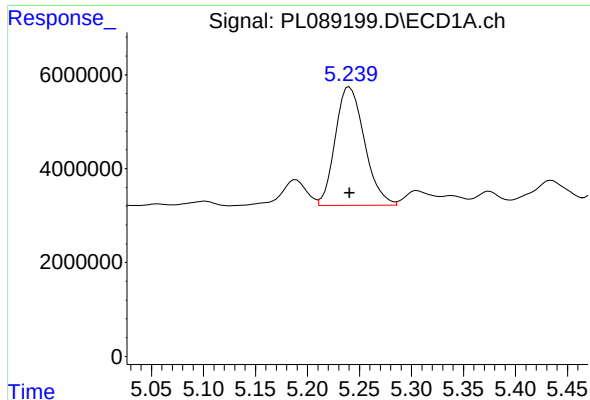

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 49232943
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

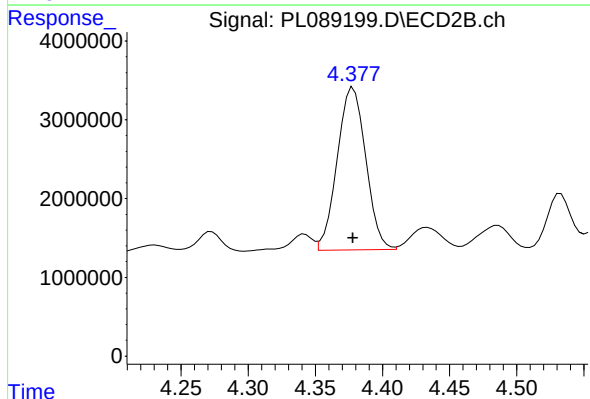


#24 Chlordane-2

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 30565822
Conc: 500.00 ng/ml

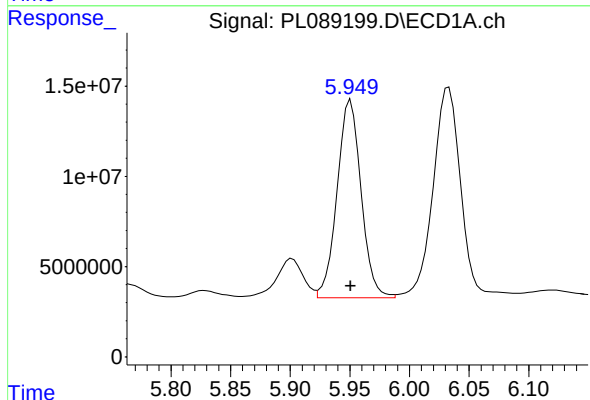


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 153448217
Conc: 500.00 ng/ml

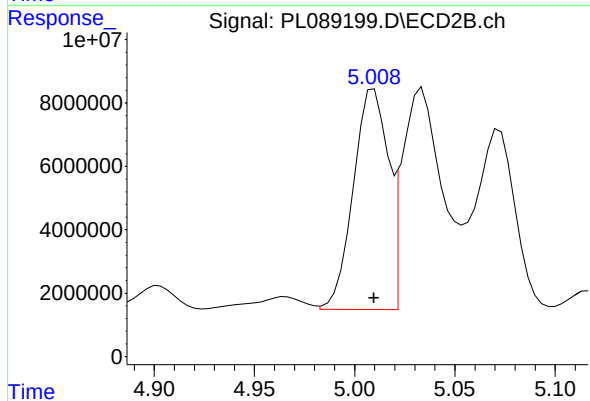

#25 Chlordane-3


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 83983389
Conc: 500.00 ng/ml

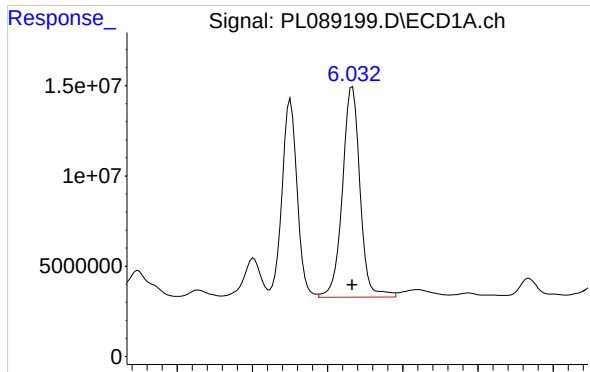

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 189827498
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

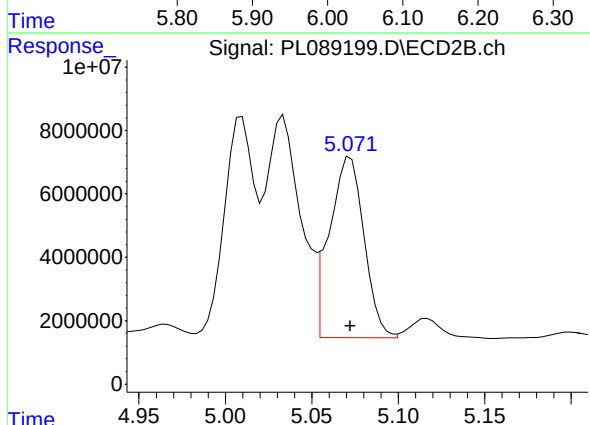


#26 Chlordane-4

R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 79094219
Conc: 500.00 ng/ml

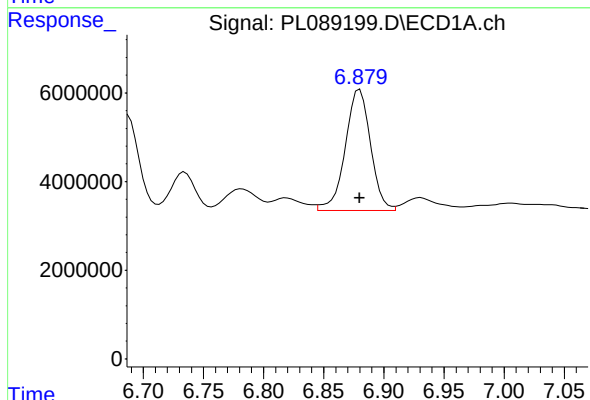


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 40077748
Conc: 500.00 ng/ml

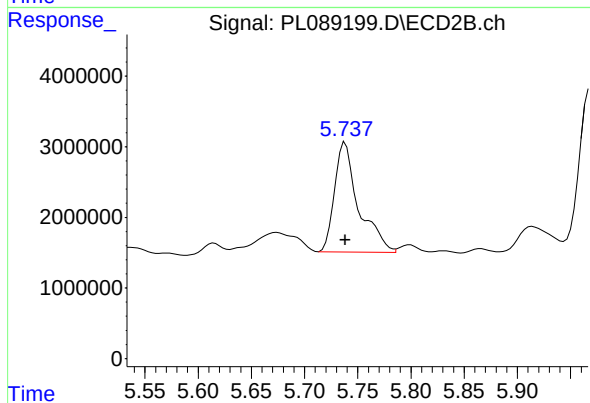

#27 Chlordane-5


R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 24537796
Conc: 500.00 ng/ml

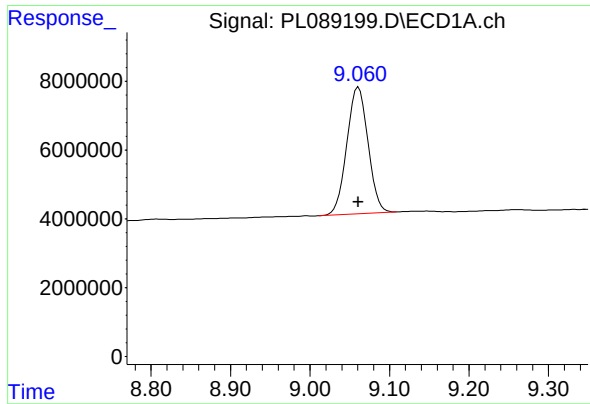

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 68011218
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

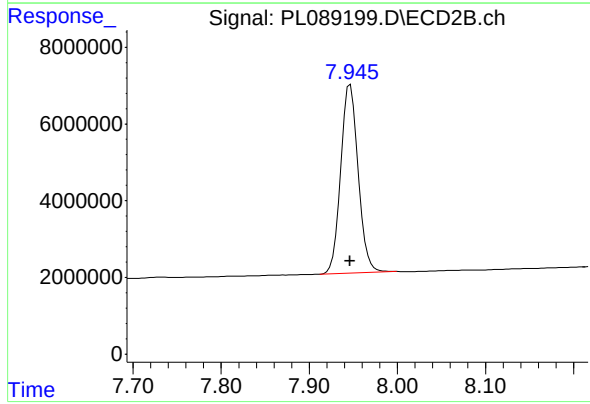

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 67824592
Conc: 50.00 ng/ml