

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
 Data File : PL089200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 15:33
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 15:57:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 15:50:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.796	51073267	39279922	26.684	24.904
28) SA Decachlor...	9.060	7.947	36615838	35665923	27.120	26.407
Target Compounds						
23) Chlordane-1	4.712	3.800	23627020	12414085	271.676	255.589
24) Chlordane-2	5.241	4.378	27013718	16329444	277.336	267.632
25) Chlordane-3	5.950	5.009	82526146	42042739	267.212	248.277
26) Chlordane-4	6.032	5.072	101.9E6	39257249	267.680	248.718
27) Chlordane-5	6.880	5.739	21708479	12997820	272.155	263.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042624\
Data File : PL089200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 15:33
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 15:57:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 15:50:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

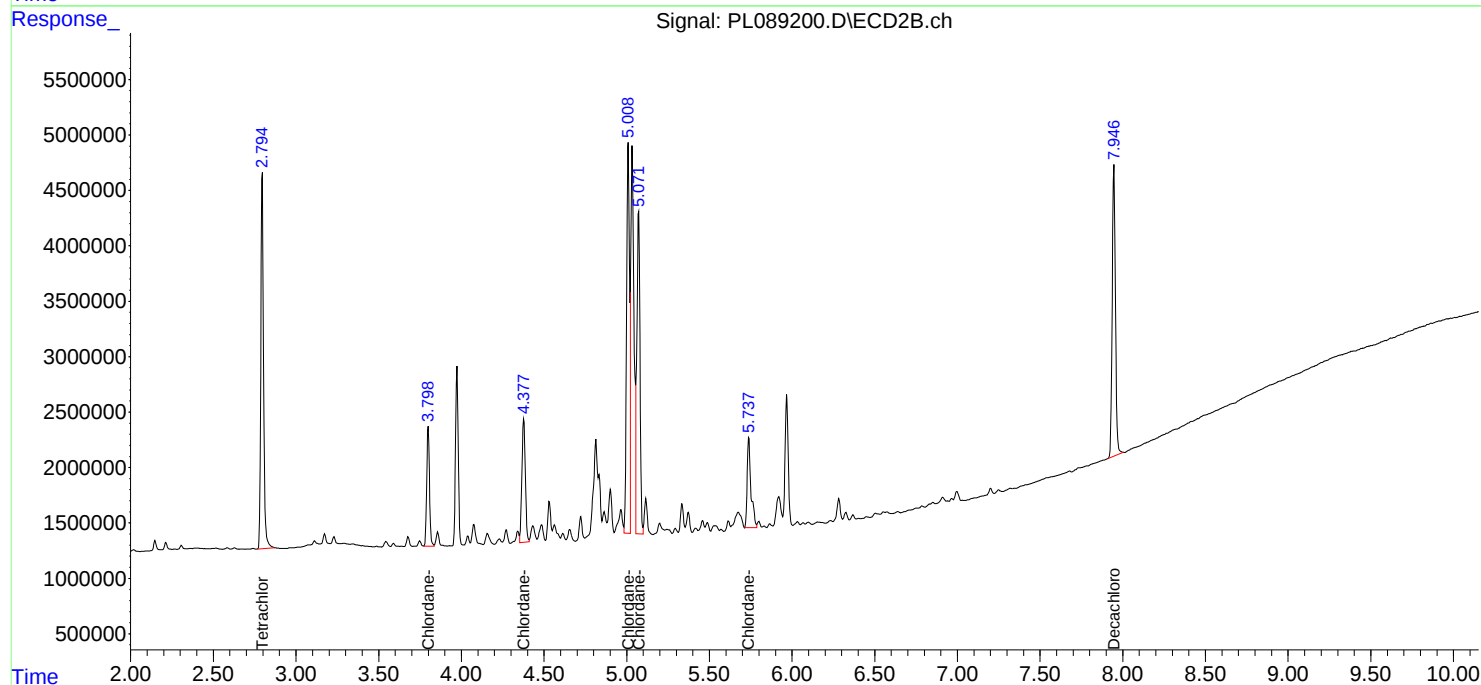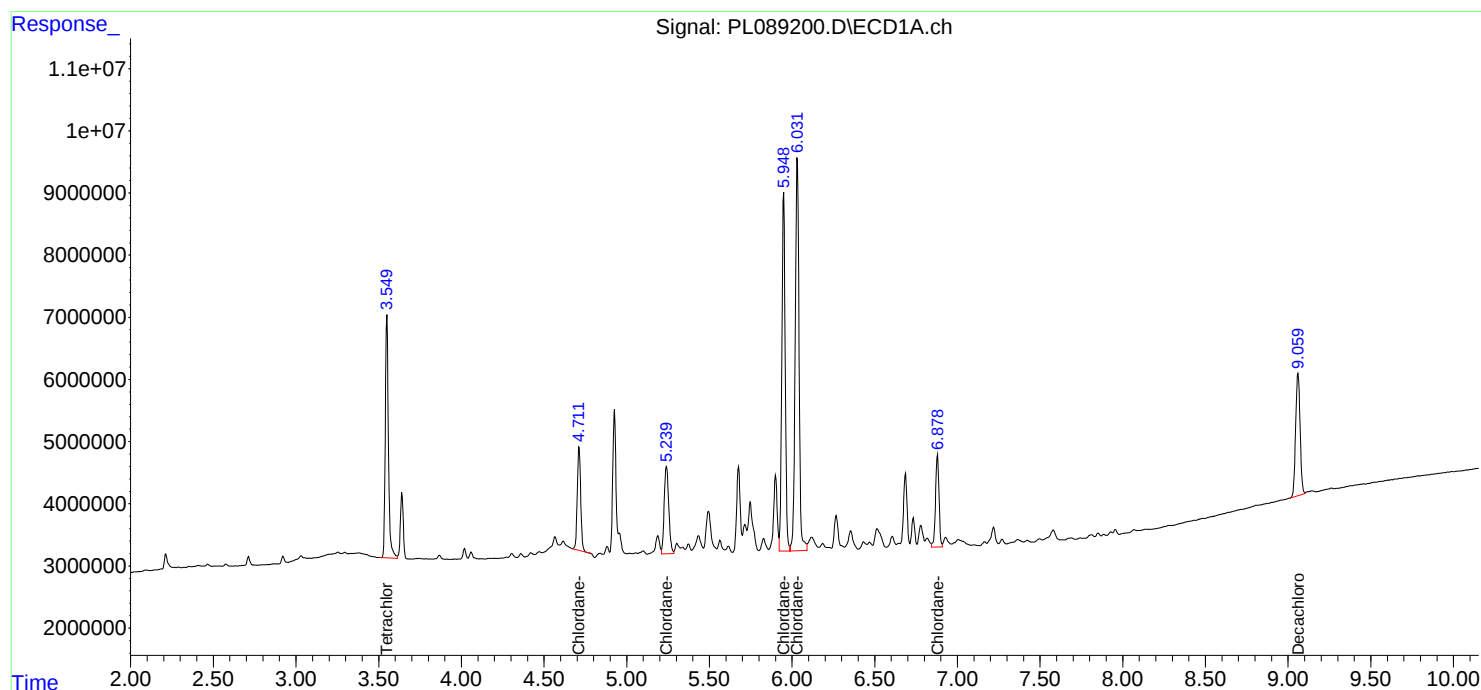


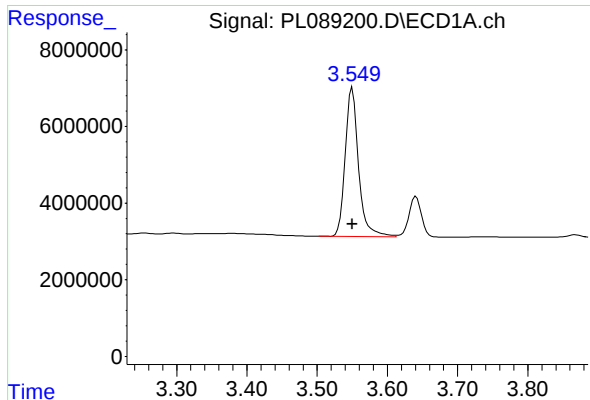

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 51073267
Conc: 26.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

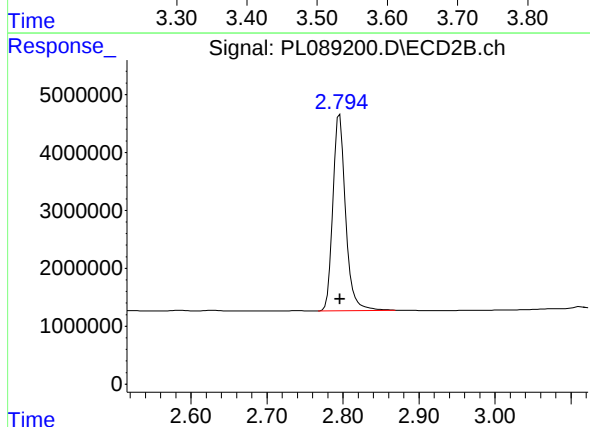


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 39279922
Conc: 24.90 ng/ml

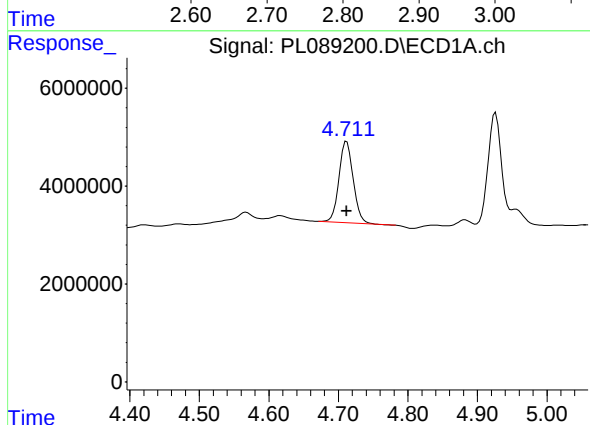


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 23627020
Conc: 271.68 ng/ml

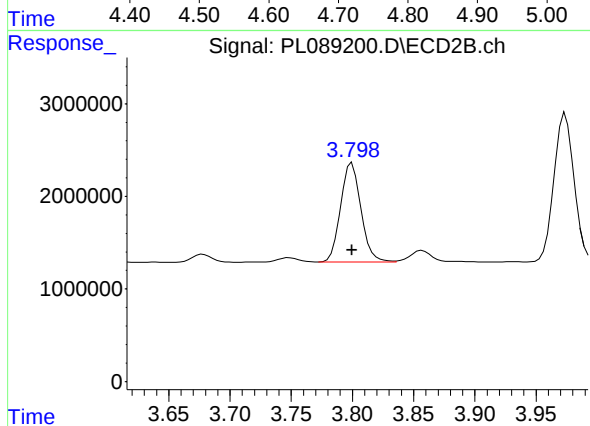

#23 Chlordane-1


R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 12414085
Conc: 255.59 ng/ml

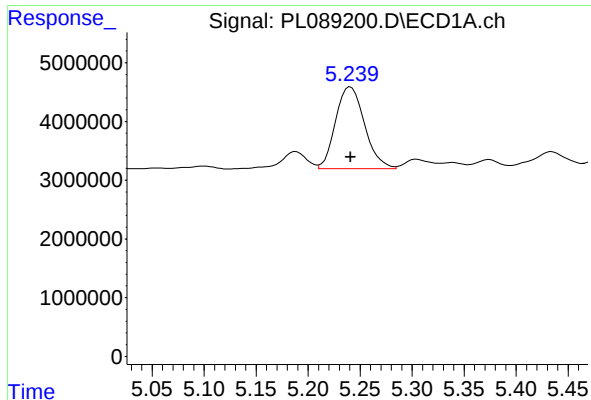

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 27013718
Conc: 277.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

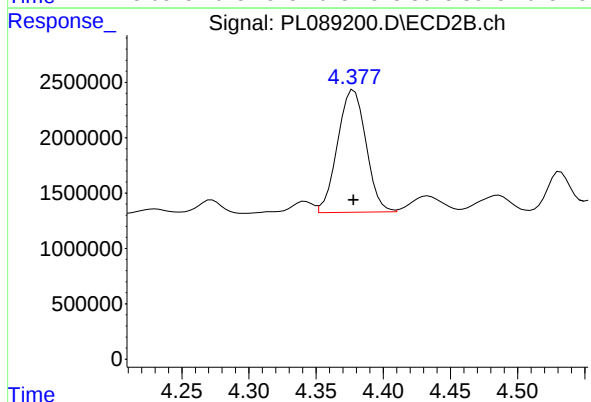


#24 Chlordane-2

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 16329444
Conc: 267.63 ng/ml

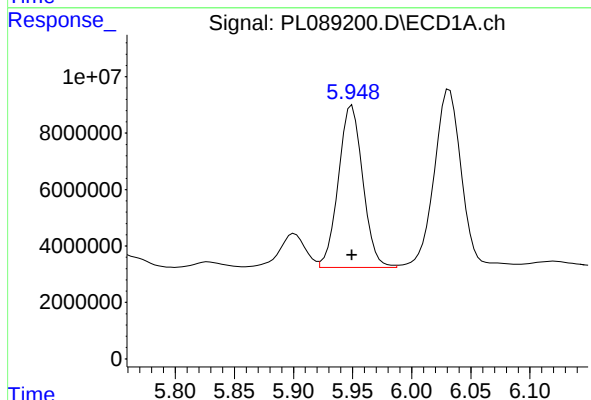


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 82526146
Conc: 267.21 ng/ml

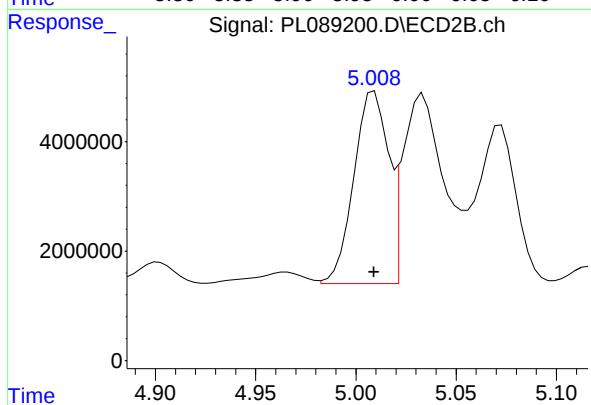

#25 Chlordane-3


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 42042739
Conc: 248.28 ng/ml

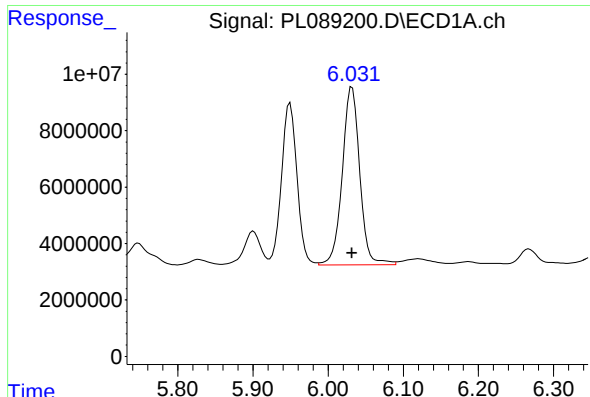

#26 Chlordane-4


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 101906677
Conc: 267.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

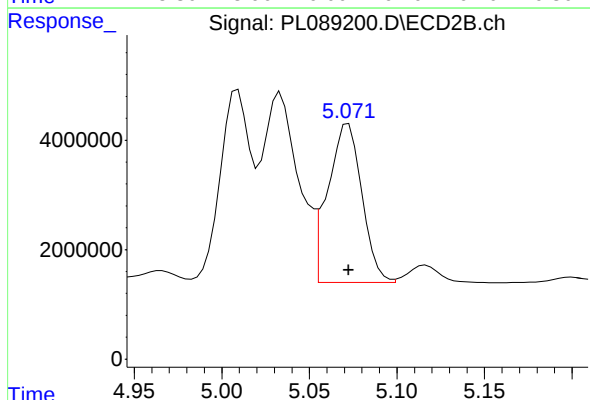


#26 Chlordane-4

R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 39257249
Conc: 248.72 ng/ml

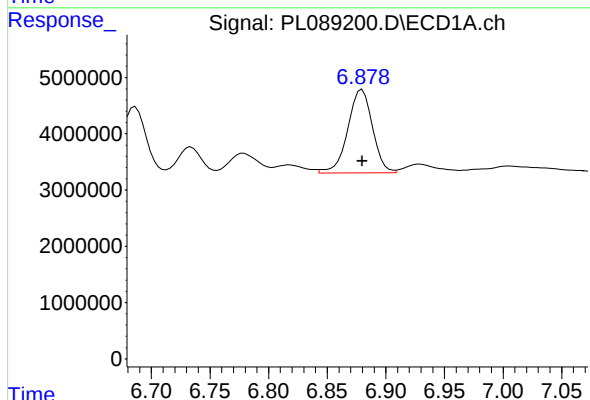


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 21708479
Conc: 272.16 ng/ml

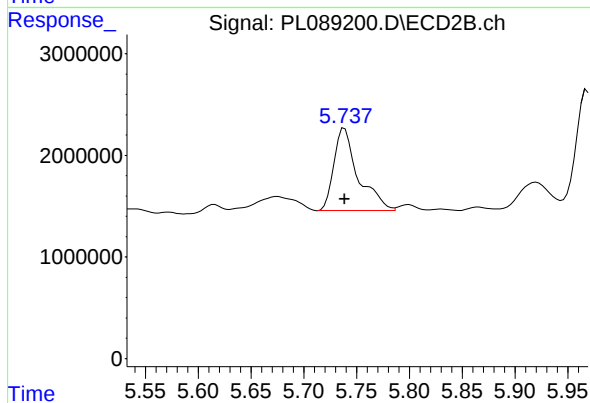

#27 Chlordane-5


R.T.: 5.739 min
Delta R.T.: 0.000 min
Response: 12997820
Conc: 263.29 ng/ml

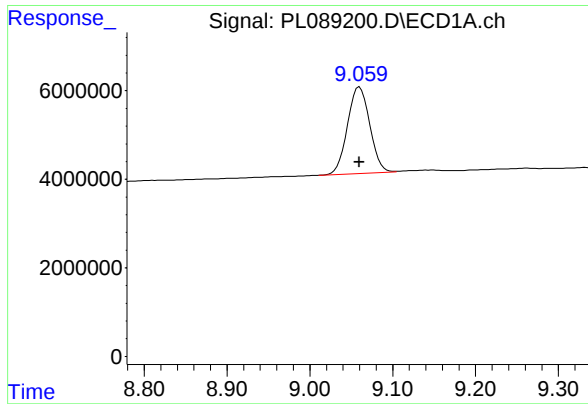

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 36615838
Conc: 27.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

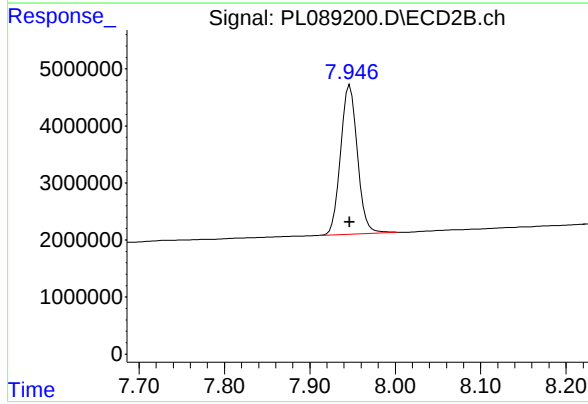

#28 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 35665923
Conc: 26.41 ng/ml