

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042719\
 Data File : PL047934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2019 12:33
 Operator : AJ\SJ
 Sample : K2588-01
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-004-B167-042319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: 01:09:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.943	191.6E6	49952717	20.721	20.925
28)	SA Decachlor...	8.004	8.986	123.3E6	36335908	11.018	12.729
Target Compounds							
2)	A alpha-BHC	0.000	4.304f	0	1600597	N.D.	0.482 #
5)	MB Aldrin	4.529f	0.000	15503965	0	1.113	N.D. #
6)	B beta-BHC	4.288	0.000	6889344	0	1.219	N.D. #
10)	B gamma-Chl...	0.000	6.032	0	3124441	N.D.	1.032 #
12)	B 4,4'-DDE	5.444	6.275	21042840	4673608	1.692	1.692
13)	MA Dieldrin	5.559	0.000	14747919	0	1.136	N.D. #
15)	B Endosulfa...	0.000	6.870f	0	1726889	N.D.	0.658 #
17)	MA 4,4'-DDT	6.190	7.064	9555176	3688180	0.958	1.548 #
20)	A Methoxychlor	0.000	7.550f	0	2458031	N.D.	1.753 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042719\
Data File : PL047934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2019 12:33
Operator : AJ\SJ
Sample : K2588-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PST-004-B167-042319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:09:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

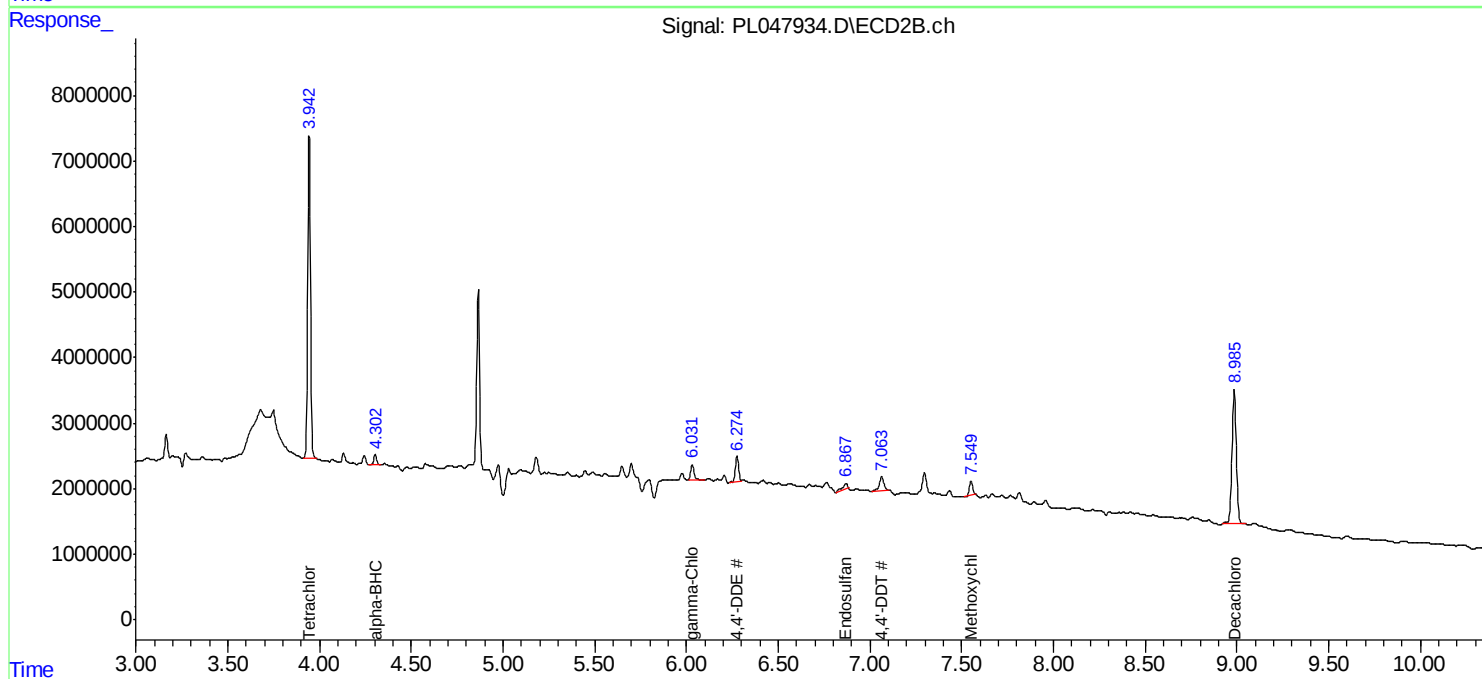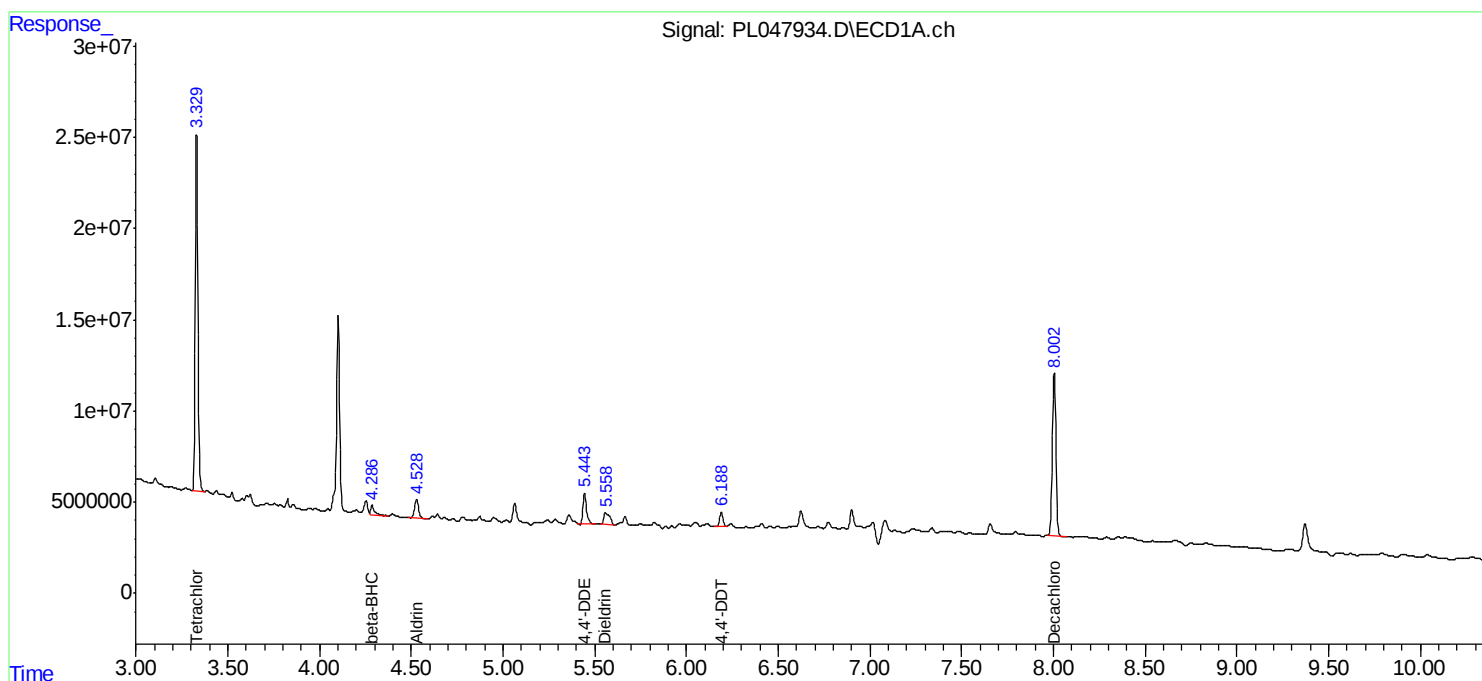


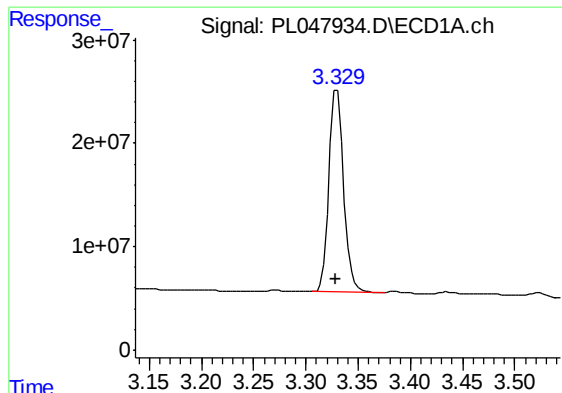

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 191635490
Conc: 20.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

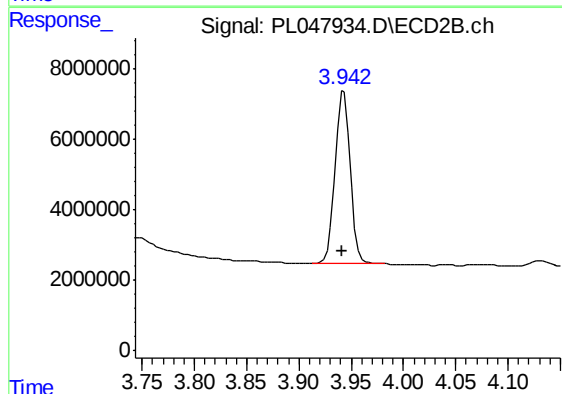


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.001 min
Response: 49952717
Conc: 20.92 ng/ml

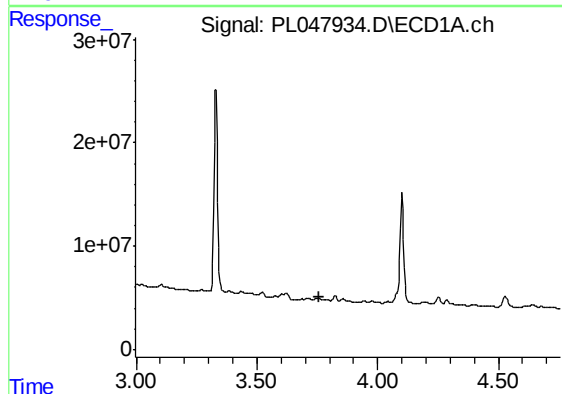


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.757 min
Response: 0
Conc: N.D.

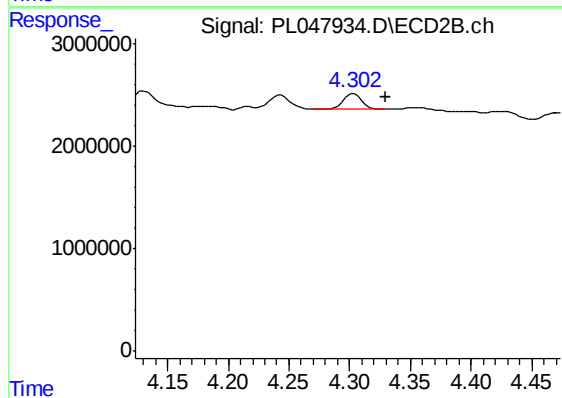

#2 alpha-BHC


R.T.: 4.304 min
Delta R.T.: -0.026 min
Response: 1600597
Conc: 0.48 ng/ml

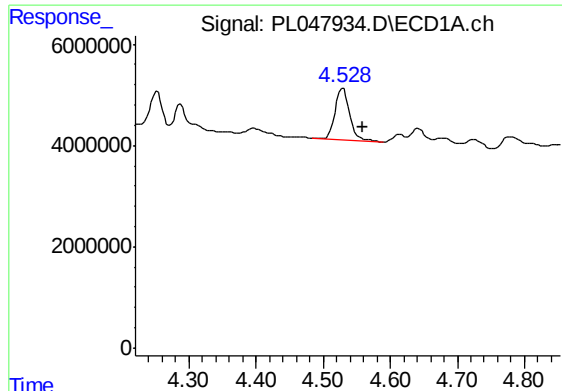

#5 Aldrin


R.T.: 4.529 min
Delta R.T.: -0.029 min
Response: 15503965
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

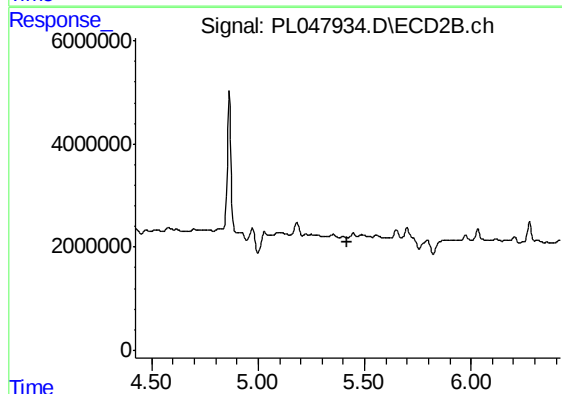


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.421 min
Response: 0
Conc: N.D.

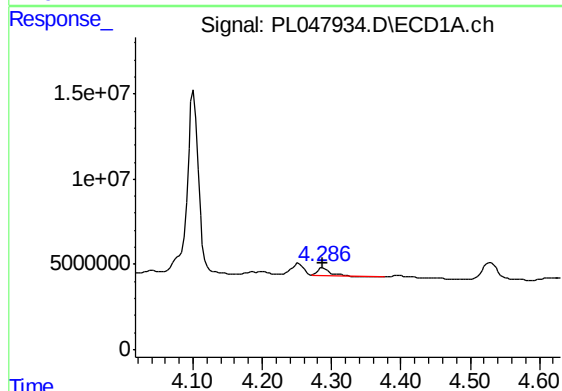


#6 beta-BHC

R.T.: 4.288 min
Delta R.T.: 0.000 min
Response: 6889344
Conc: 1.22 ng/ml

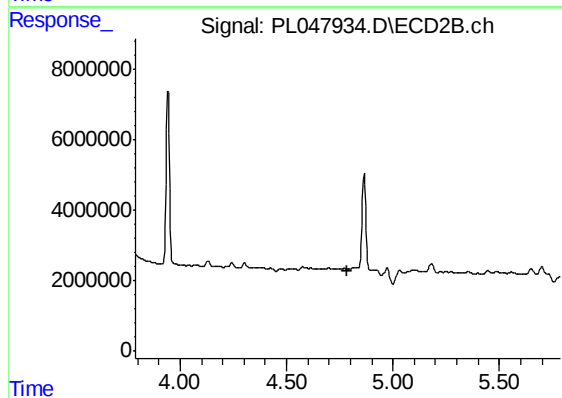

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

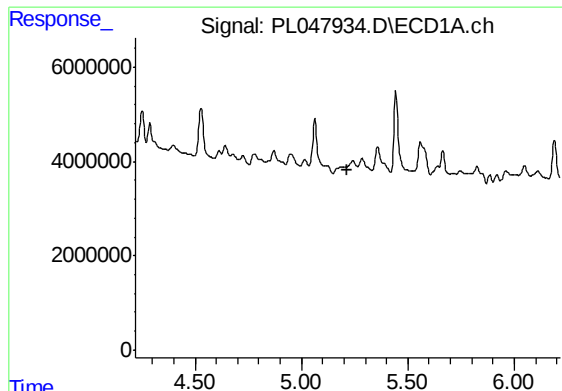

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

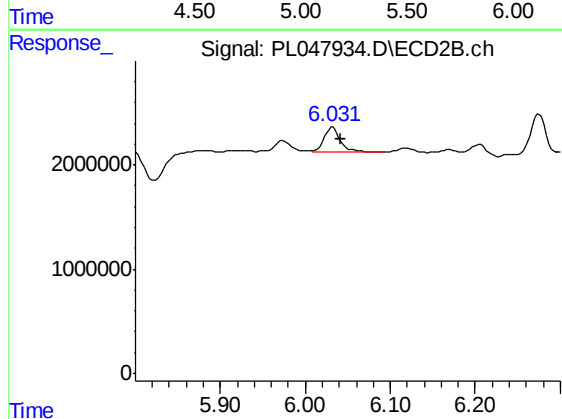


#10 gamma-Chlordane

R.T.: 6.032 min
Delta R.T.: -0.010 min
Response: 3124441
Conc: 1.03 ng/ml

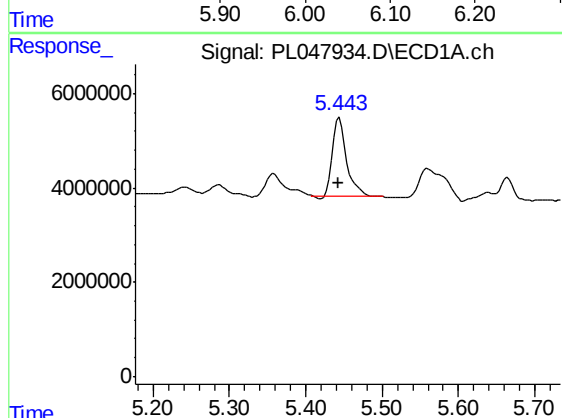


#12 4,4'-DDE

R.T.: 5.444 min
Delta R.T.: 0.002 min
Response: 21042840
Conc: 1.69 ng/ml

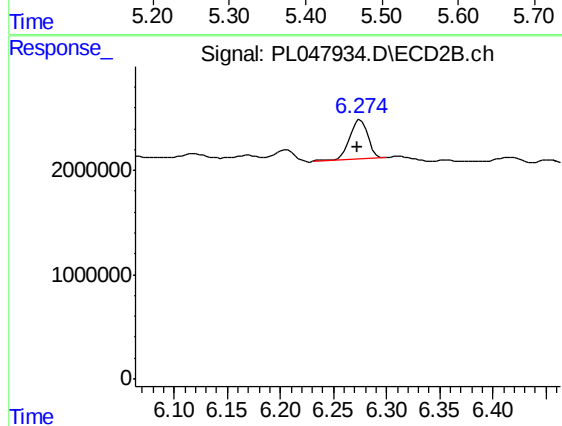

#12 4,4'-DDE


R.T.: 6.275 min
Delta R.T.: 0.002 min
Response: 4673608
Conc: 1.69 ng/ml

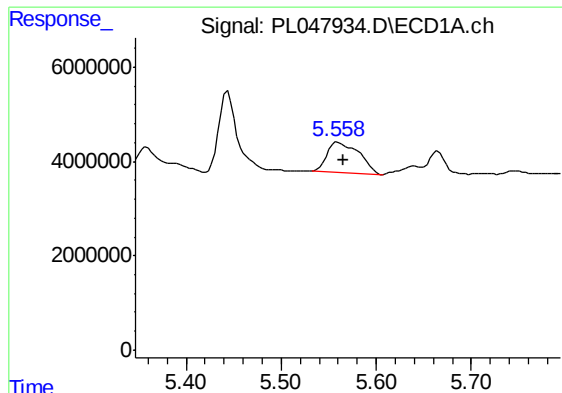

#13 Dieldrin


R.T.: 5.559 min
Delta R.T.: -0.007 min
Response: 14747919
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

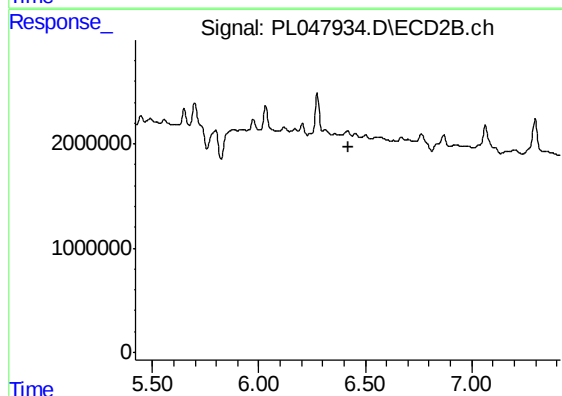


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.420 min
Response: 0
Conc: N.D.

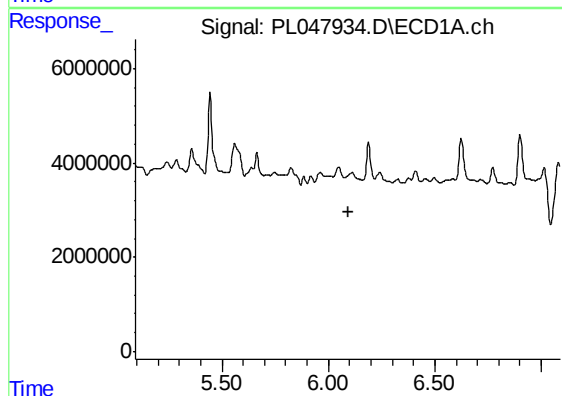


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

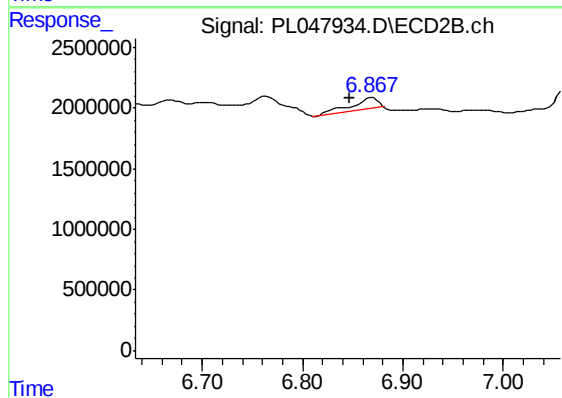

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.022 min
Response: 1726889
Conc: 0.66 ng/ml

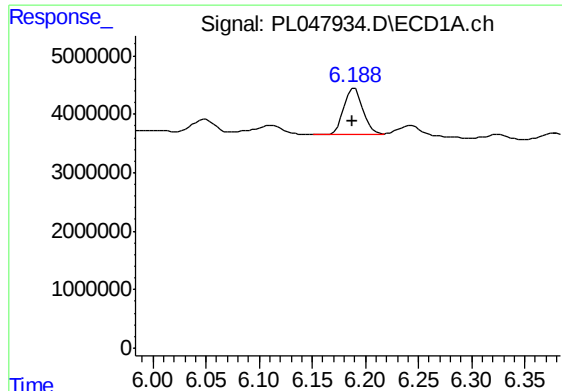

#17 4,4'-DDT


R.T.: 6.190 min
Delta R.T.: 0.001 min
Response: 9555176
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

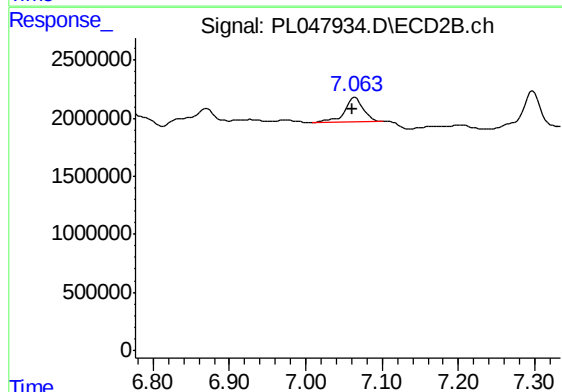


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: 0.004 min
Response: 3688180
Conc: 1.55 ng/ml

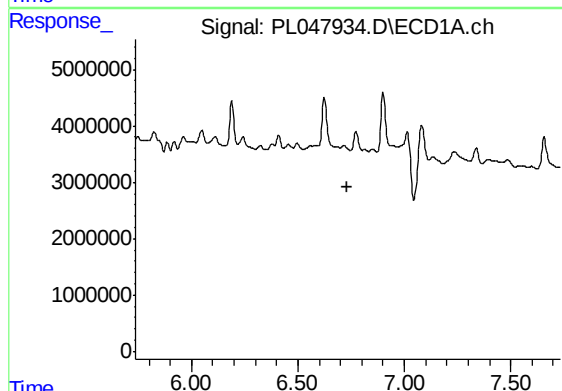


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.734 min
Response: 0
Conc: N.D.

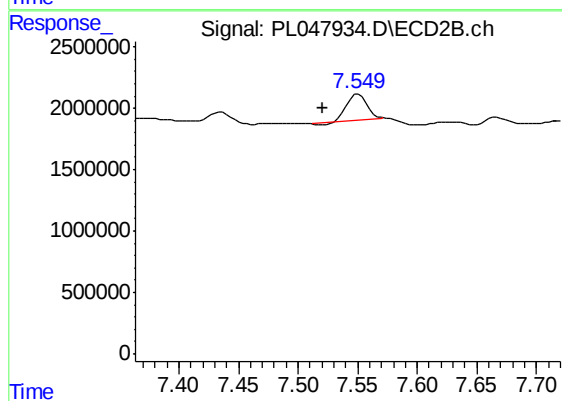

#20 Methoxychlor


R.T.: 7.550 min
Delta R.T.: 0.029 min
Response: 2458031
Conc: 1.75 ng/ml

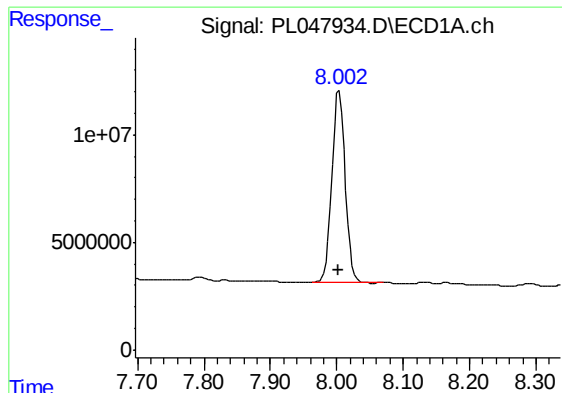

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.002 min
Response: 123337872
Conc: 11.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B167-042319

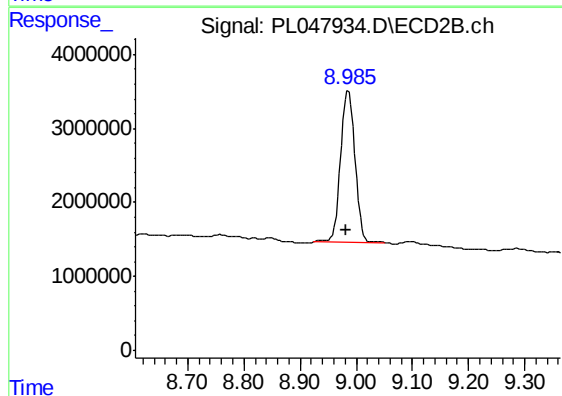

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.005 min
Response: 36335908
Conc: 12.73 ng/ml