

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042719\
 Data File : PL047935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2019 12:48
 Operator : AJ\SJ
 Sample : K2588-02
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-004-B170-042319

Manual Integrations
 APPROVED

mohammad
 4/29/2019 4:33:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 01:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.943	157.5E6	35799010	17.026	14.996
28)	SA Decachlor...	8.004	8.986	61863636	17868267	5.526	6.259
Target Compounds							
12)	B 4,4'-DDE	5.442	6.275	7619487	1731925	0.613m	0.627

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042719\
Data File : PL047935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2019 12:48
Operator : AJ\SJ
Sample : K2588-02
Misc :
ALS Vial : 81 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-004-B170-042319


Manual Integrations
APPROVED

mohammad
4/29/2019 4:33:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 01:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

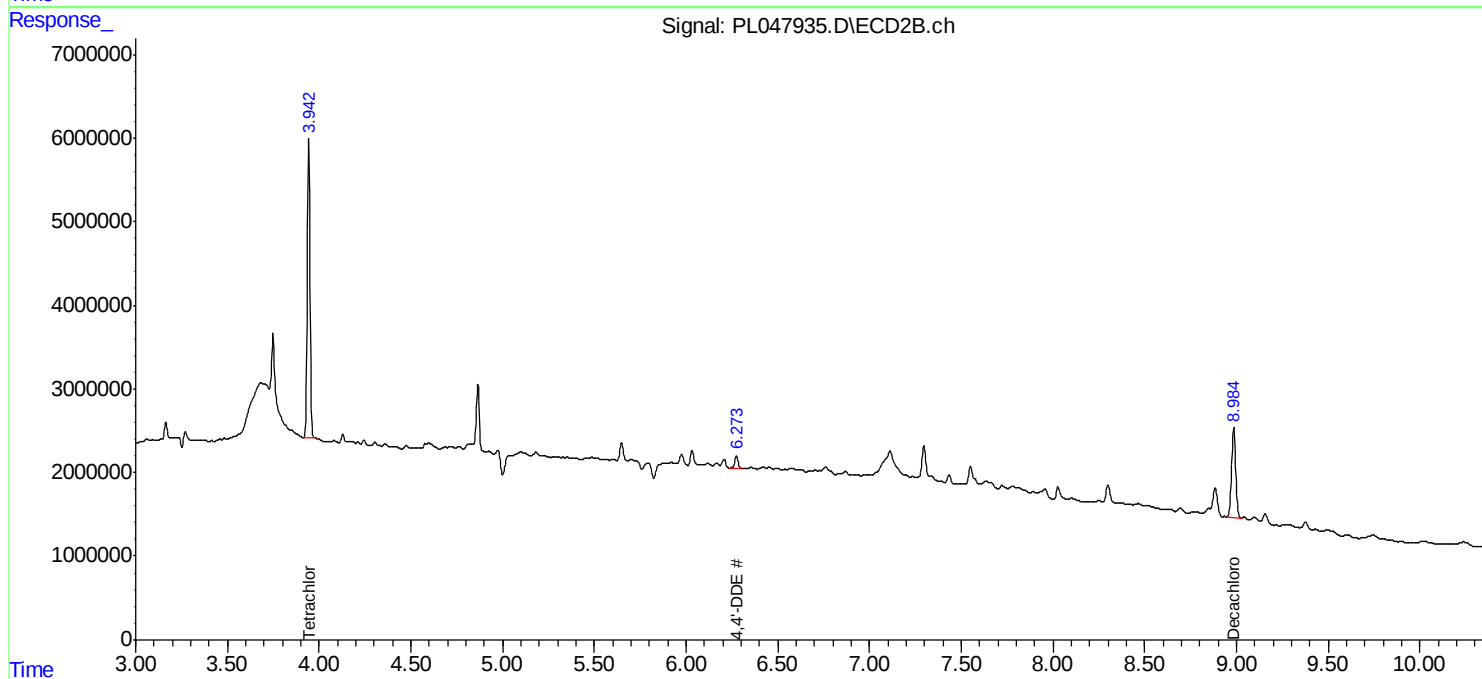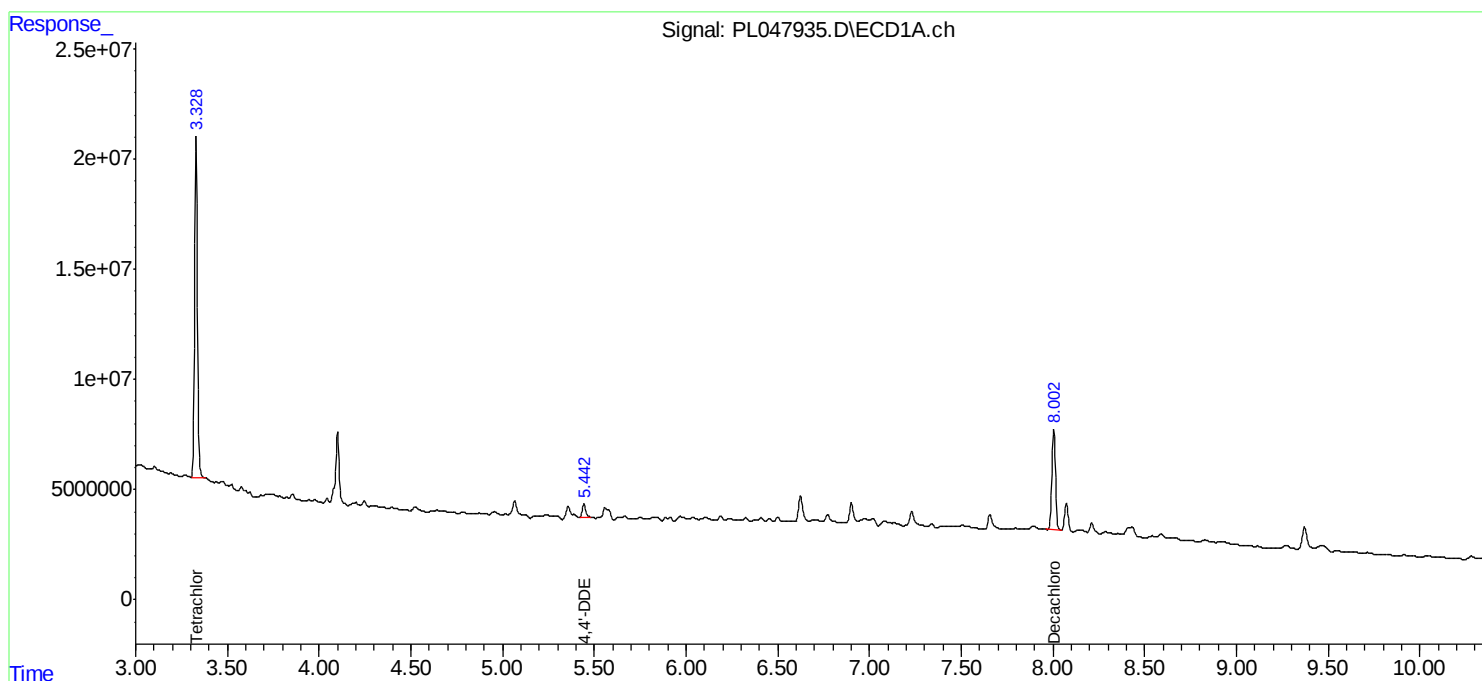

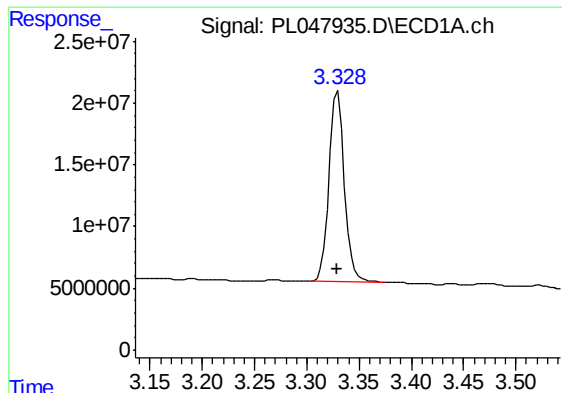


#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 157464289
Conc: 17.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B170-042319


Manual Integrations
APPROVED

mohammad
4/29/2019 4:33:48 PM

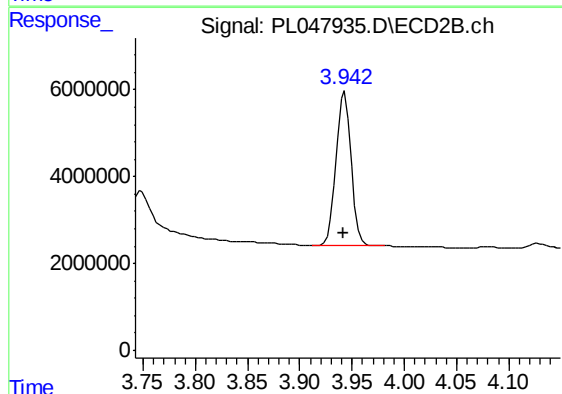


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.001 min
Response: 35799010
Conc: 15.00 ng/ml

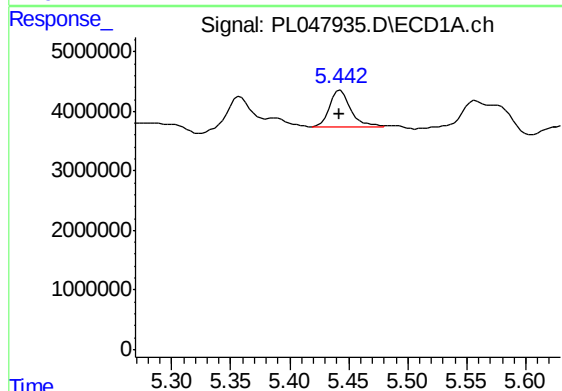


#12 4,4'-DDE

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 7619487
Conc: 0.61 ng/ml m

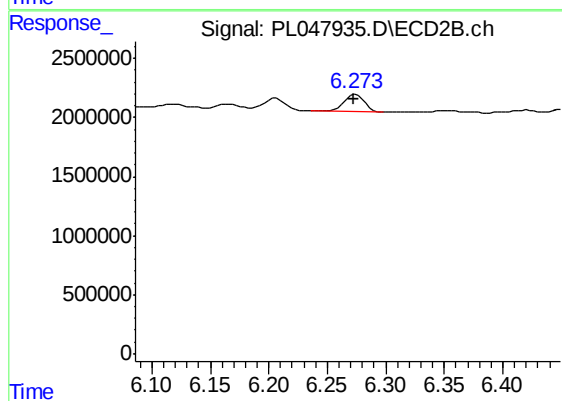

#12 4,4'-DDE

R.T.: 6.275 min
Delta R.T.: 0.002 min
Response: 1731925
Conc: 0.63 ng/ml

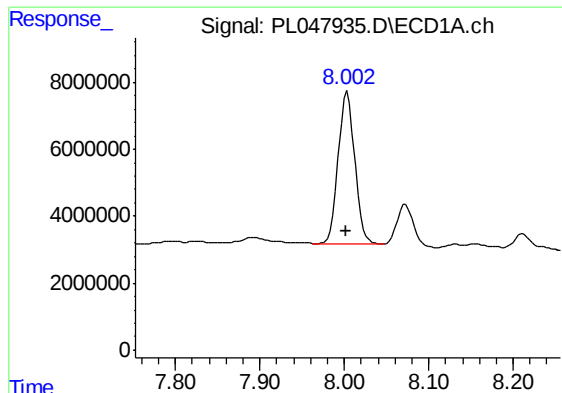


#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.002 min
Response: 61863636
Conc: 5.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-004-B170-042319

Manual Integrations
APPROVED

mohammad
4/29/2019 4:33:48 PM

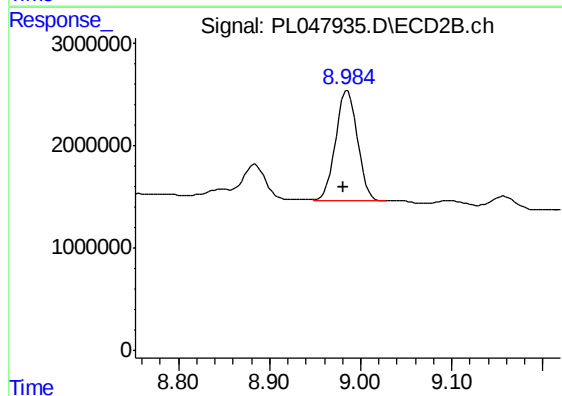

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 17868267
Conc: 6.26 ng/ml