

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042720\
 Data File : PL058390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2020 13:40
 Operator : AJ\MA
 Sample : L2408-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

mohammad
 4/29/2020 8:12:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 01:12:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.951	1209.8E6	40931548	120.011	18.861m#
28)	SA Decachlor...	8.205	8.972	35396661	5712898	3.434m	2.558m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042720\
Data File : PL058390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2020 13:40
Operator : AJ\MA
Sample : L2408-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

mohammad
4/29/2020 8:12:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 01:12:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

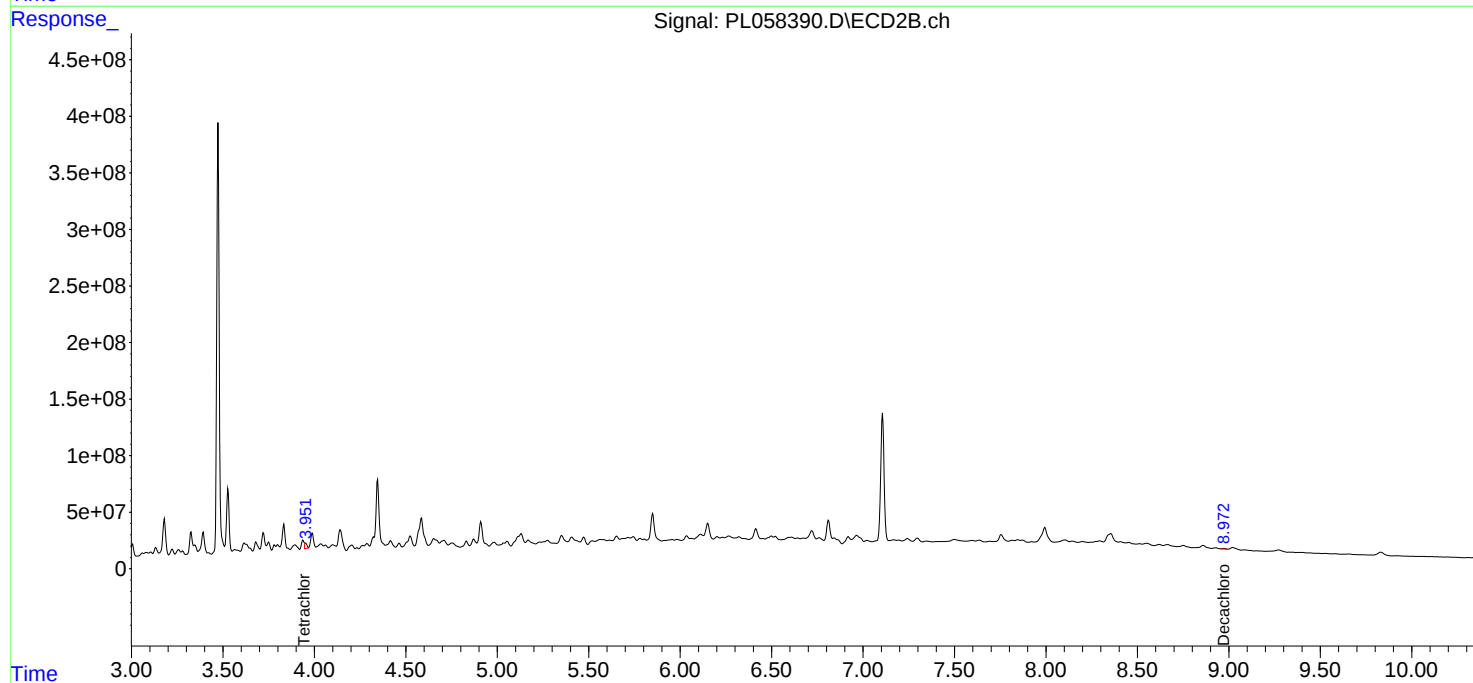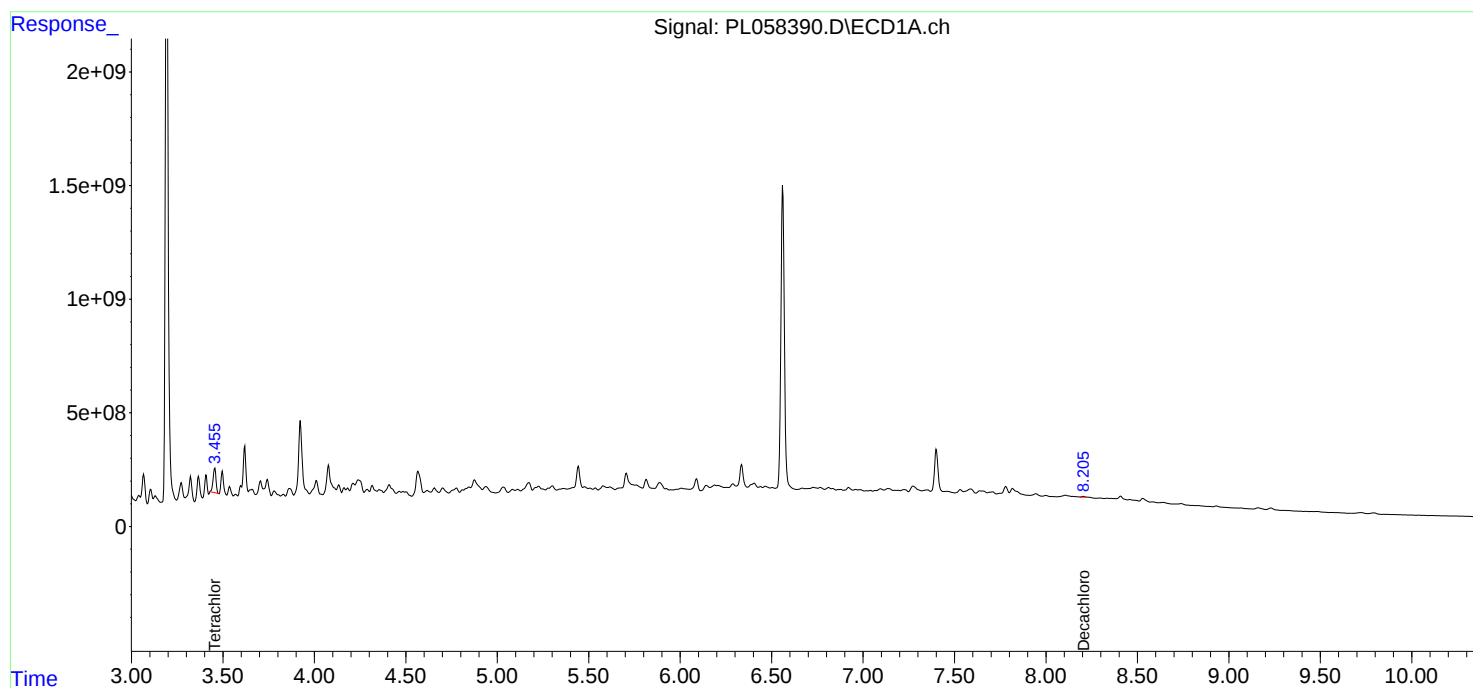

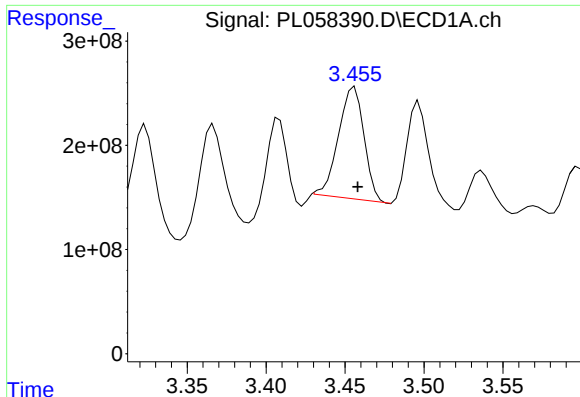


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 1209836707
Conc: 120.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

mohammad
4/29/2020 8:12:11 AM

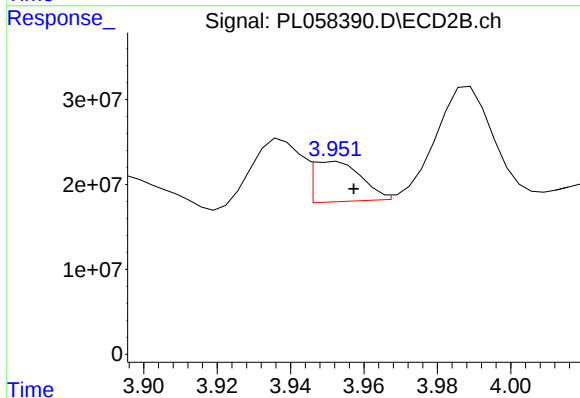


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: -0.006 min
Response: 40931548
Conc: 18.86 ng/ml m

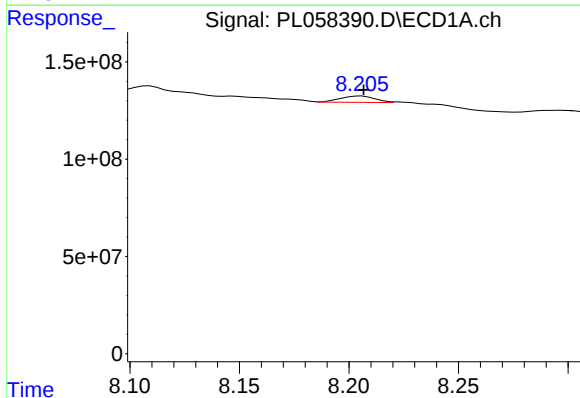

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 35396661
Conc: 3.43 ng/ml m

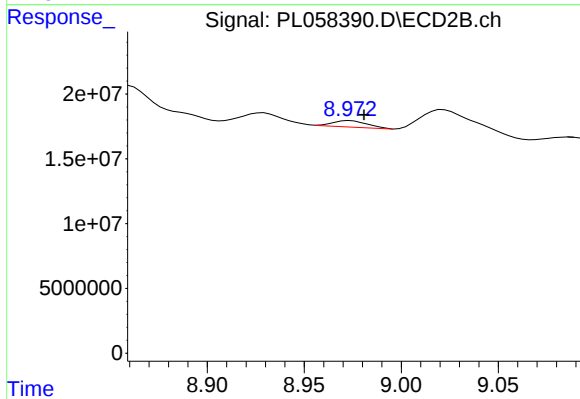

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: -0.009 min
Response: 5712898
Conc: 2.56 ng/ml m