

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042720\
 Data File : PL058402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2020 18:16
 Operator : AJ\MA
 Sample : L2422-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUCK-ISLAND-ROLLOFF

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 01:15:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.954	94561045	20123444	9.380	9.273
28)	SA Decachlor...	8.200	8.973	92785179	21735968	9.001	9.731

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042720\
Data File : PL058402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2020 18:16
Operator : AJ\MA
Sample : L2422-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DUCK-ISLAND-ROLLOFF

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 01:15:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

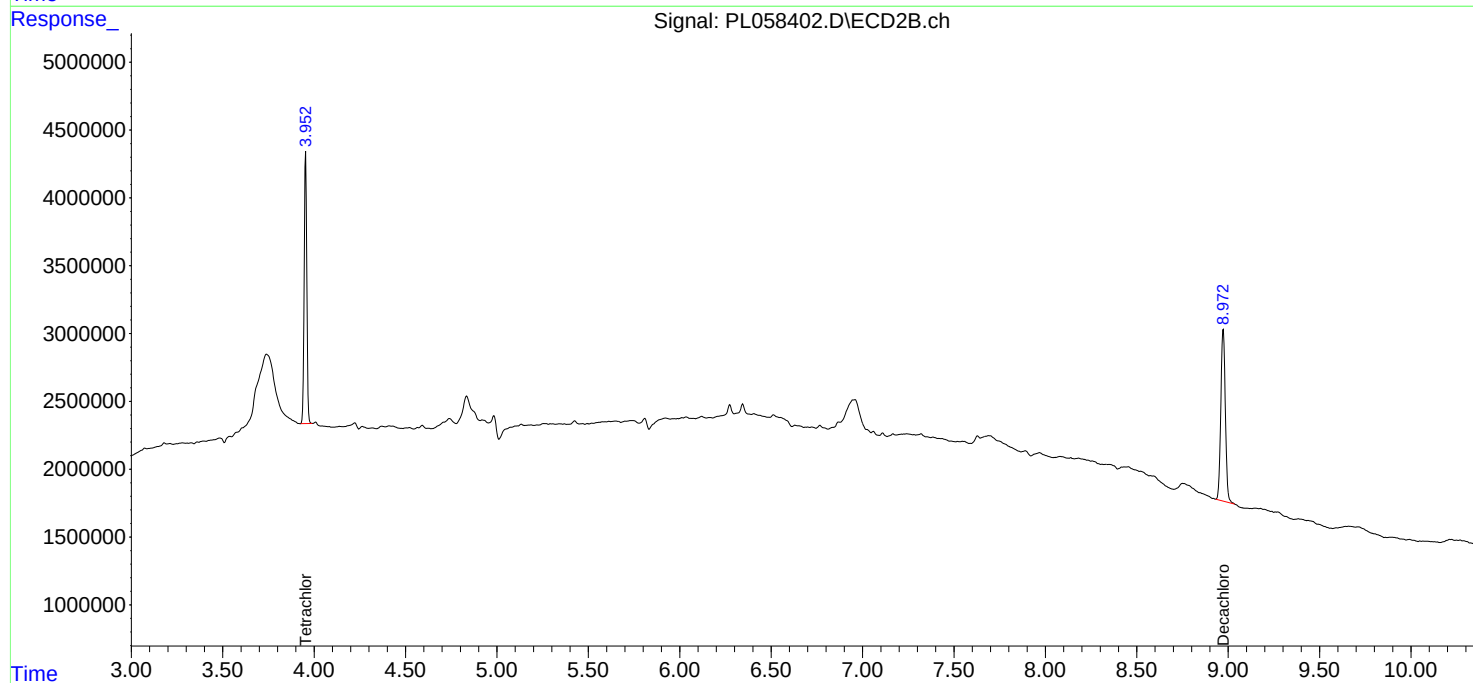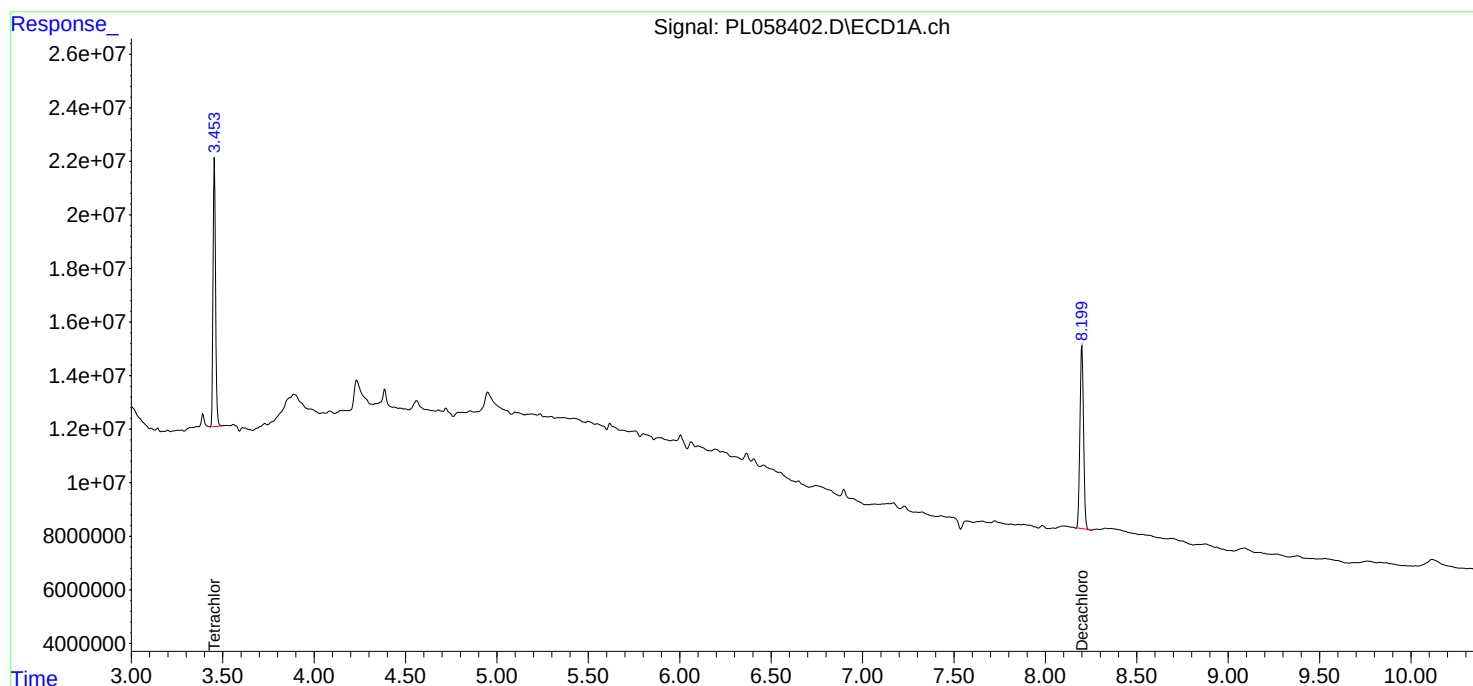


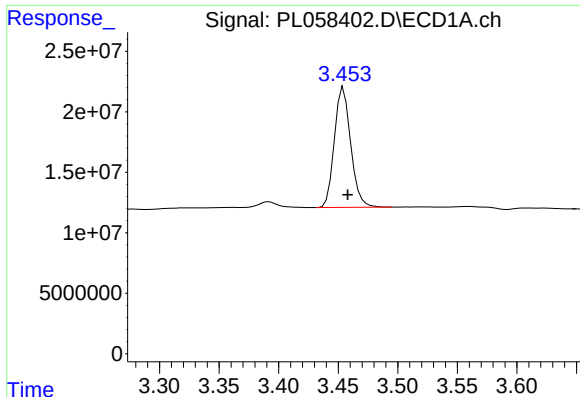

#1 Tetrachloro-m-xylene


R.T.: 3.454 min
Delta R.T.: -0.004 min
Response: 94561045
Conc: 9.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUCK-ISLAND-ROLLOFF

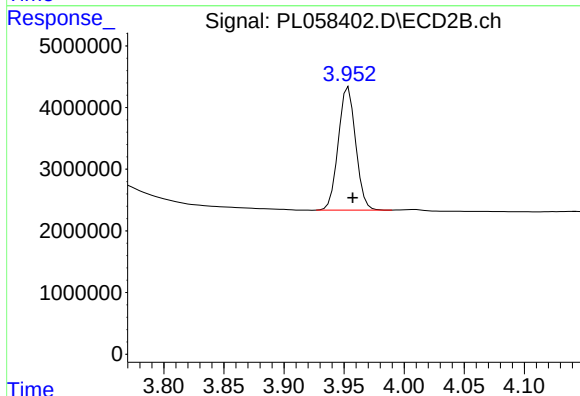


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.004 min
Response: 20123444
Conc: 9.27 ng/ml

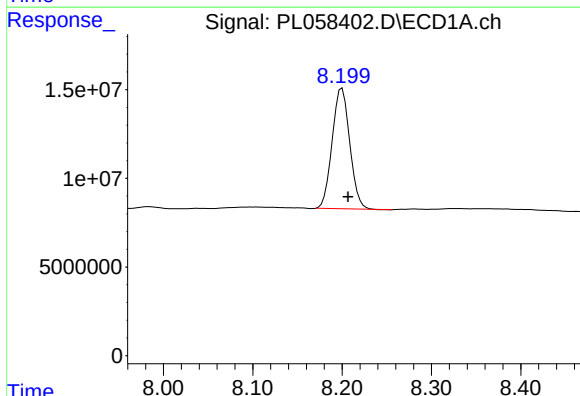

#28 Decachlorobiphenyl

R.T.: 8.200 min
Delta R.T.: -0.007 min
Response: 92785179
Conc: 9.00 ng/ml

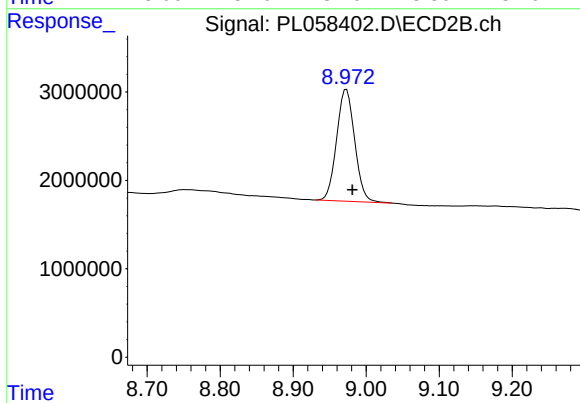

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.008 min
Response: 21735968
Conc: 9.73 ng/ml