

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
 Data File : PL066490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 09:49
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 08:43:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:43:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	443.0E6	336.1E6	100.892	98.277
28)	SA Decachlor...	8.160	9.352	344.5E6	256.6E6	91.393	91.185
Target Compounds							
23)	Chlordane-1	4.290	5.173	149.3E6	138.9E6	952.990	987.142
24)	Chlordane-2	4.786	5.651	162.4E6	141.5E6	939.434	916.478
25)	Chlordane-3	5.349	6.310	504.0E6	560.1E6	987.990	989.720
26)	Chlordane-4	5.407	6.383	418.7E6	660.4E6	977.598	982.455
27)	Chlordane-5	6.233	7.206	165.1E6	116.0E6	963.445	948.504



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
Data File : PL066490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 09:49
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 08:43:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:43:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

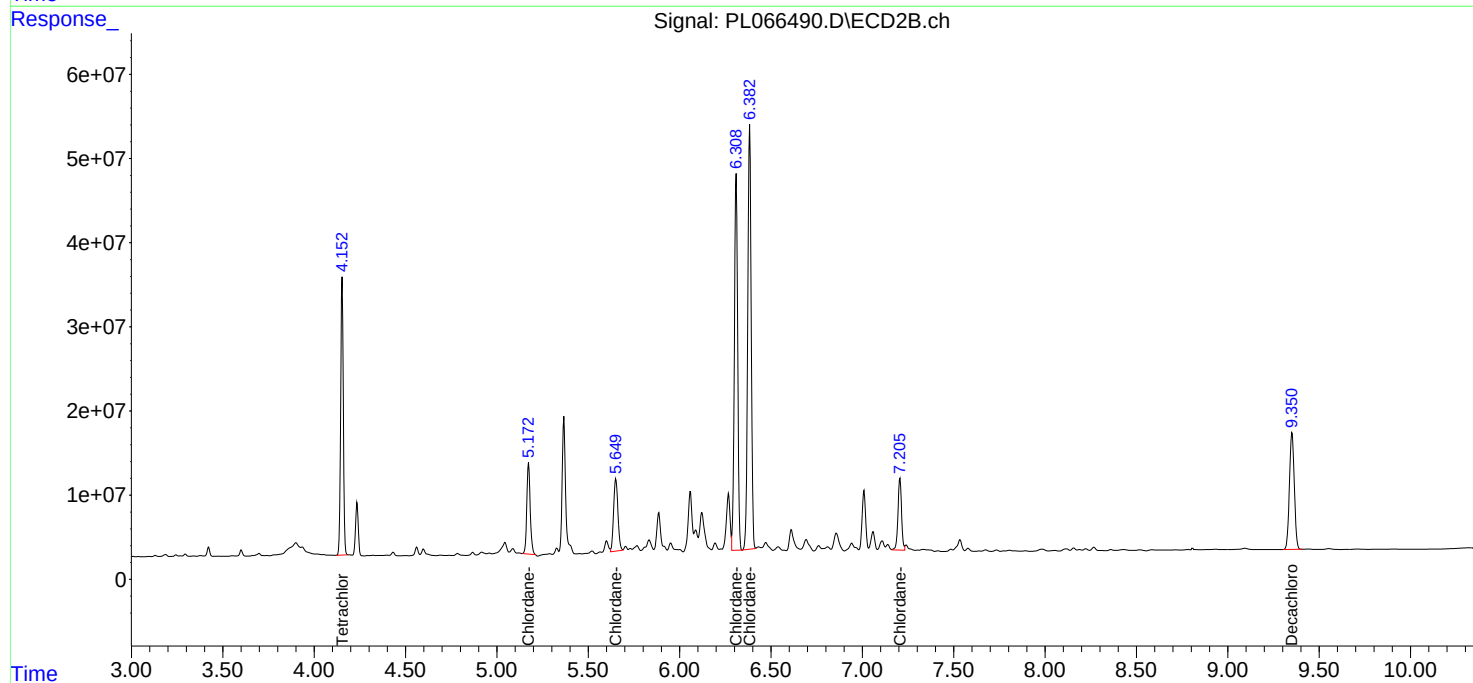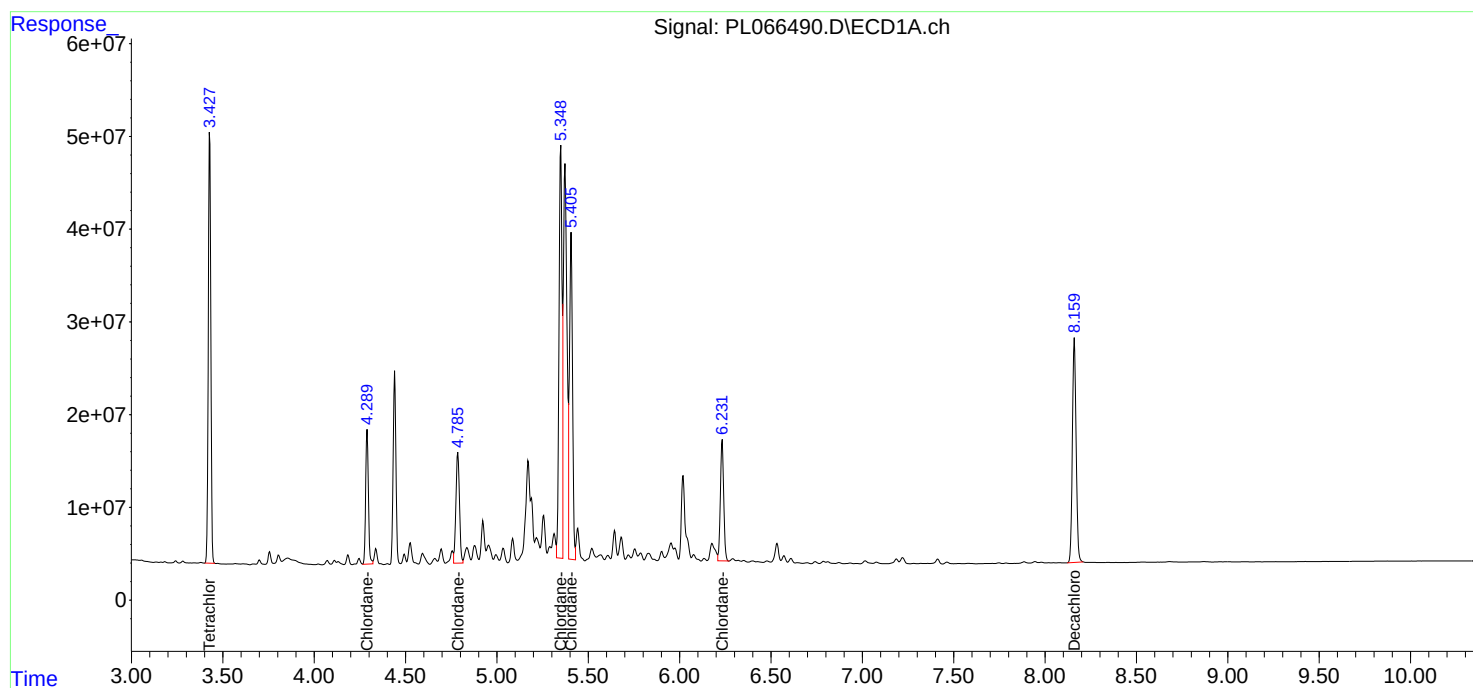


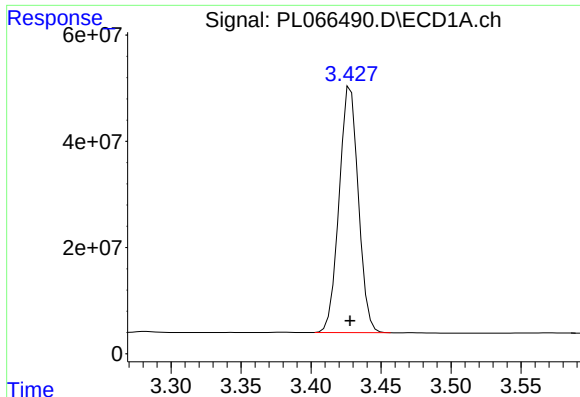

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 442984838
Conc: 100.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

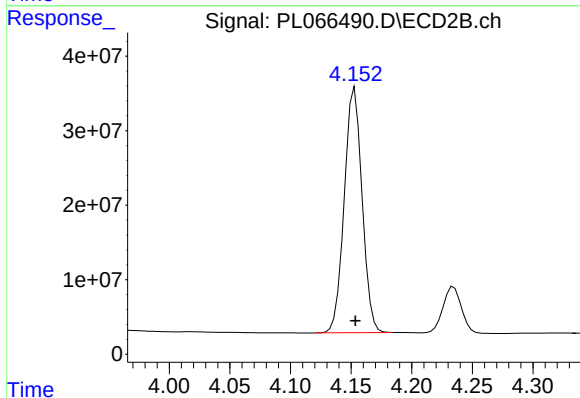


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 336112226
Conc: 98.28 ng/ml

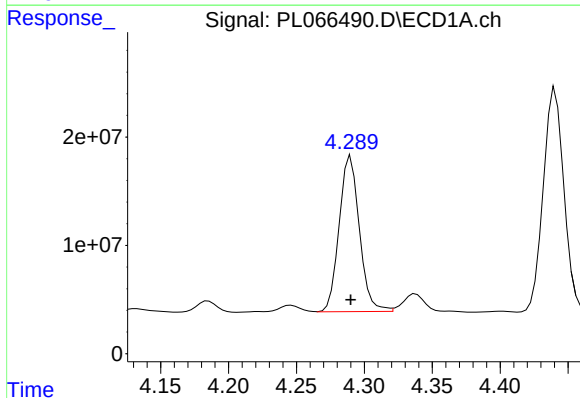


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 149252964
Conc: 952.99 ng/ml

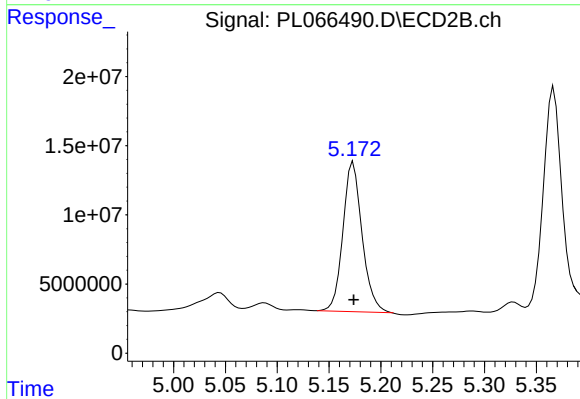

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 138916207
Conc: 987.14 ng/ml

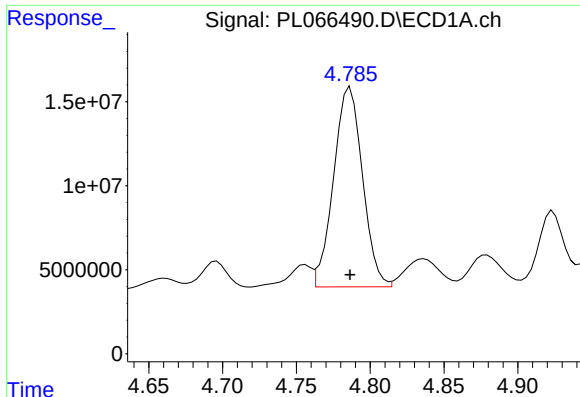

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 162377226
Conc: 939.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

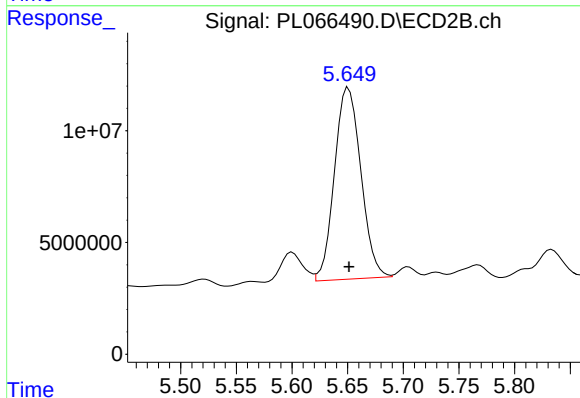


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 141537563
Conc: 916.48 ng/ml

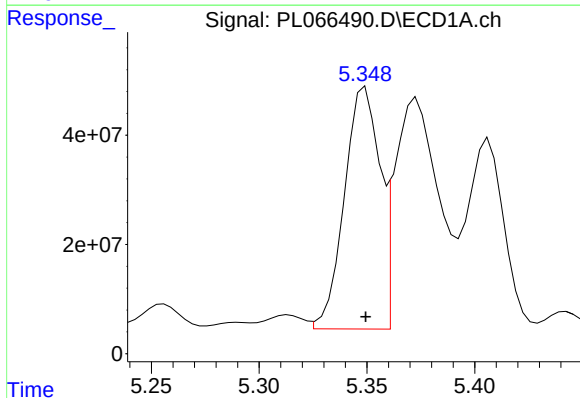


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 503997905
Conc: 987.99 ng/ml

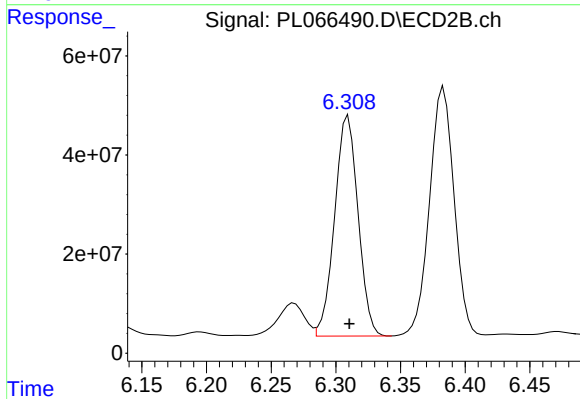

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 560096831
Conc: 989.72 ng/ml

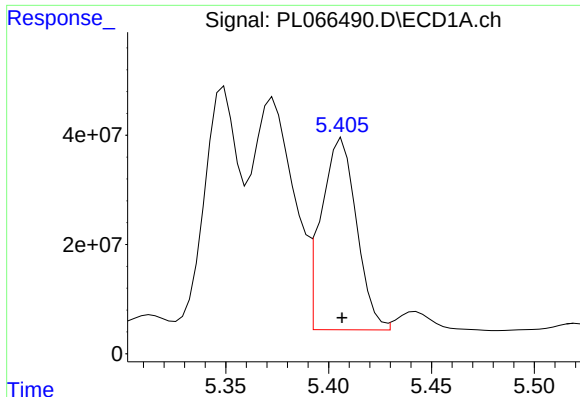

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 418652922
Conc: 977.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

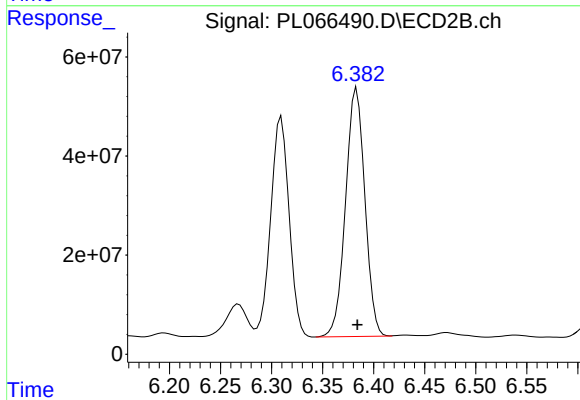


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 660424572
Conc: 982.45 ng/ml

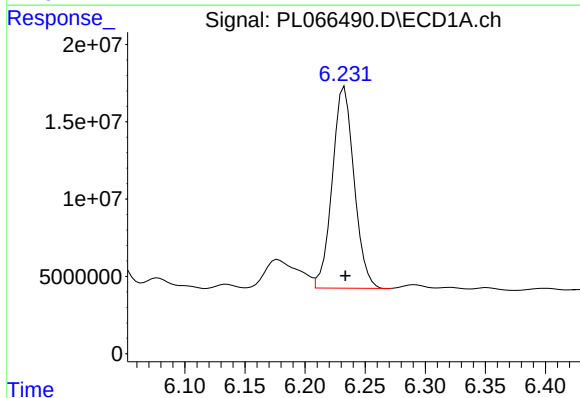


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 165132930
Conc: 963.44 ng/ml

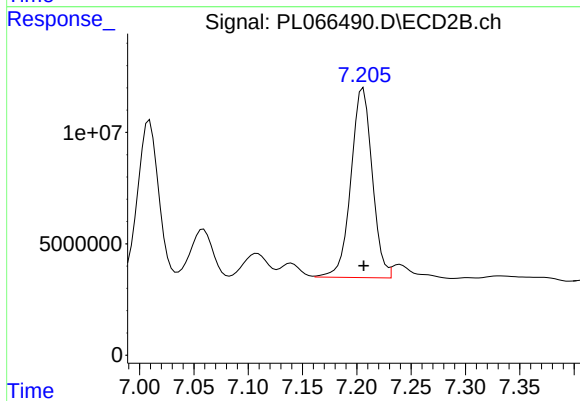

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 115985251
Conc: 948.50 ng/ml

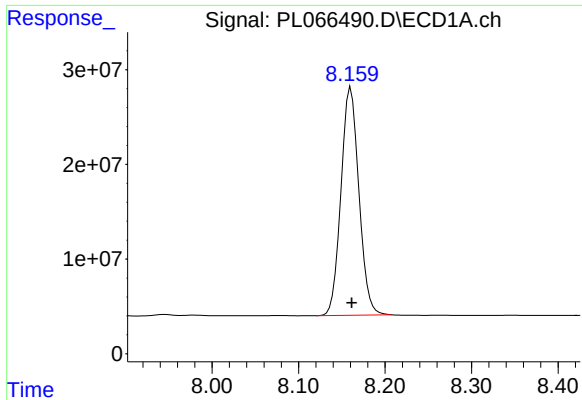

#28 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: 0.000 min
Response: 344526085
Conc: 91.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

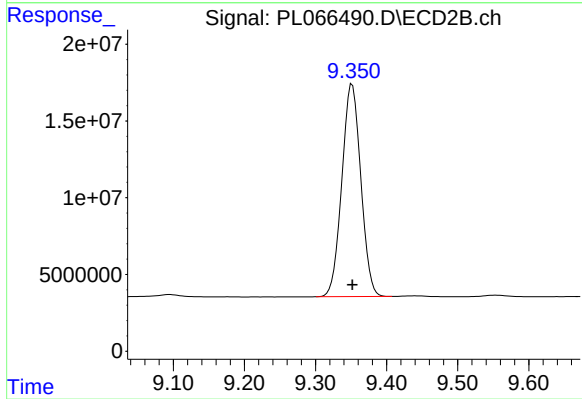

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 256628054
Conc: 91.19 ng/ml