

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
 Data File : PL066491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 10:03
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 08:43:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:43:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	335.6E6	262.5E6	76.446	76.762
28)	SA Decachlor...	8.162	9.351	269.5E6	207.4E6	71.481	73.709
Target Compounds							
23)	Chlordane-1	4.290	5.174	115.9E6	109.6E6	739.990	778.934
24)	Chlordane-2	4.786	5.651	127.8E6	113.5E6	739.118	735.035
25)	Chlordane-3	5.349	6.310	382.2E6	438.5E6	749.230	774.827
26)	Chlordane-4	5.406	6.383	325.1E6	518.0E6	759.098	770.588
27)	Chlordane-5	6.233	7.206	129.5E6	92182674	755.417	753.852



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
Data File : PL066491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 10:03
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 08:43:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:43:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

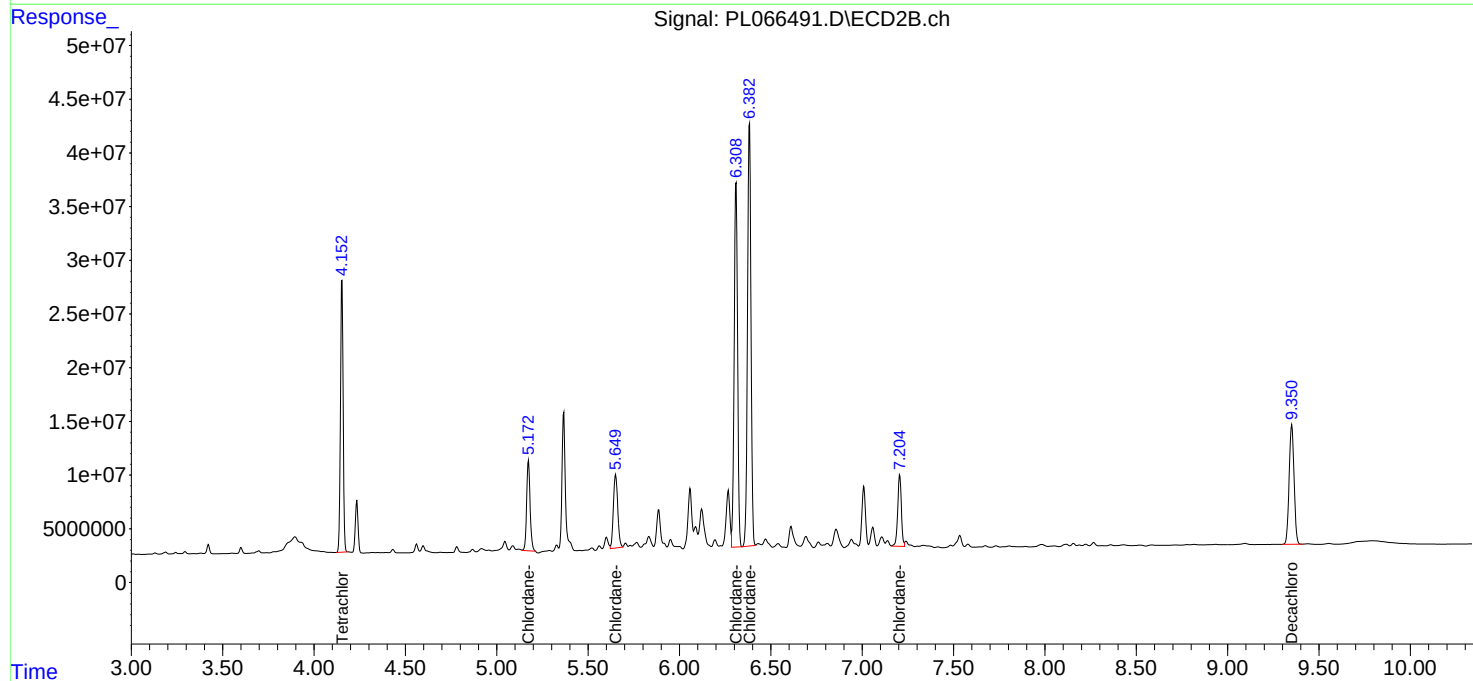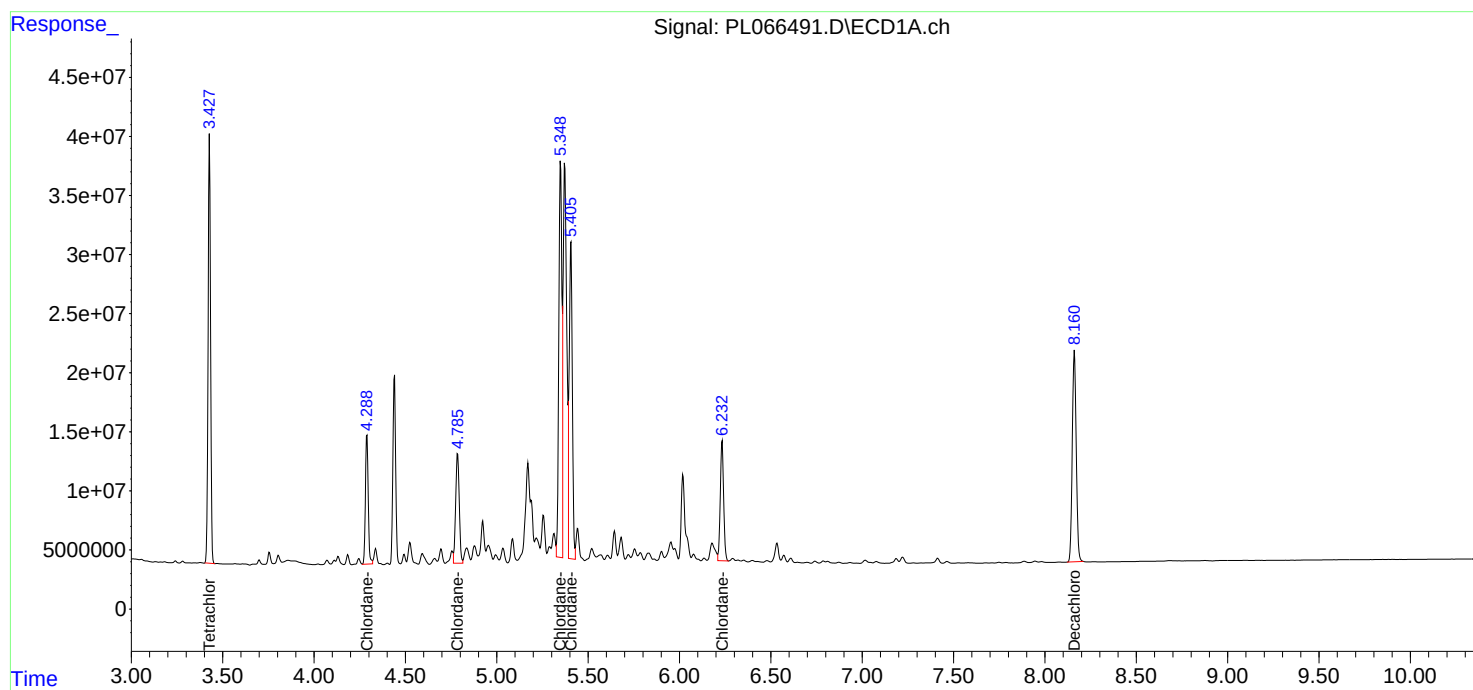


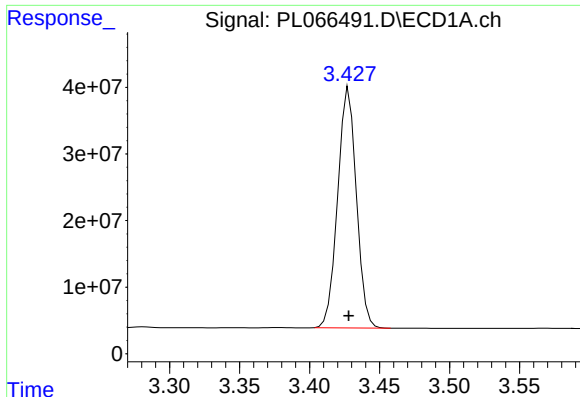

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 335649577
Conc: 76.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

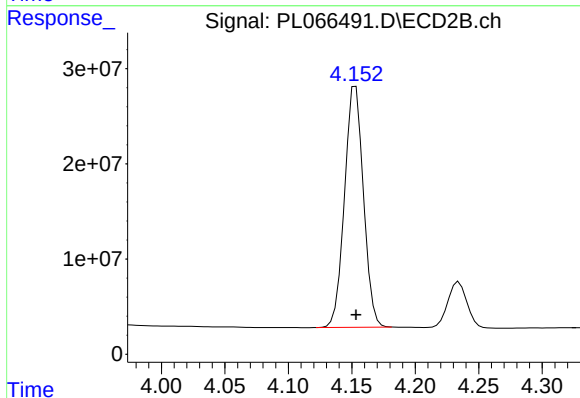


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 262528251
Conc: 76.76 ng/ml

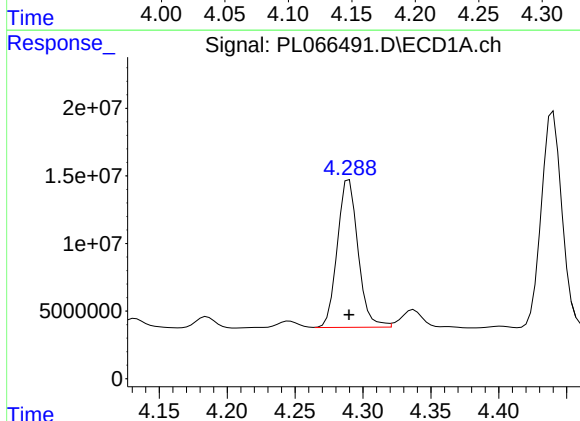


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 115893903
Conc: 739.99 ng/ml

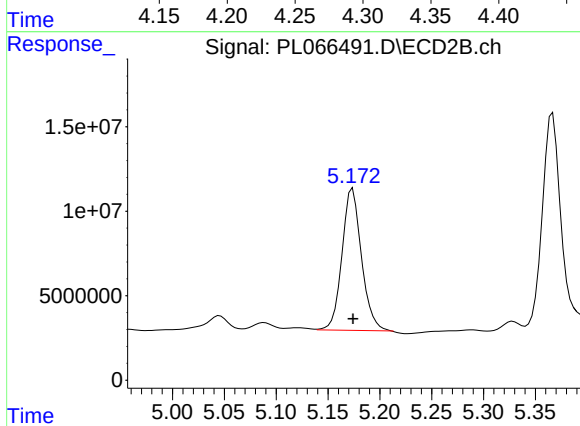

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 109616116
Conc: 778.93 ng/ml

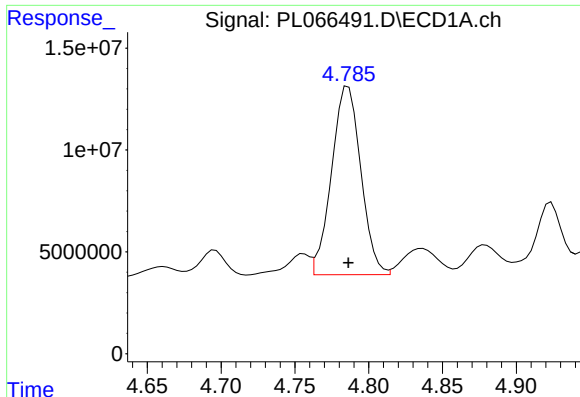

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 127753387
Conc: 739.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

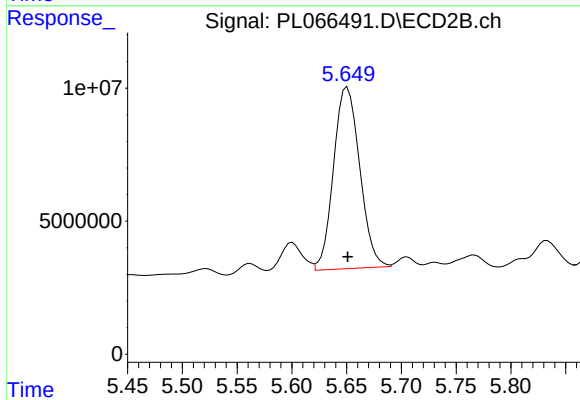


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 113516250
Conc: 735.04 ng/ml

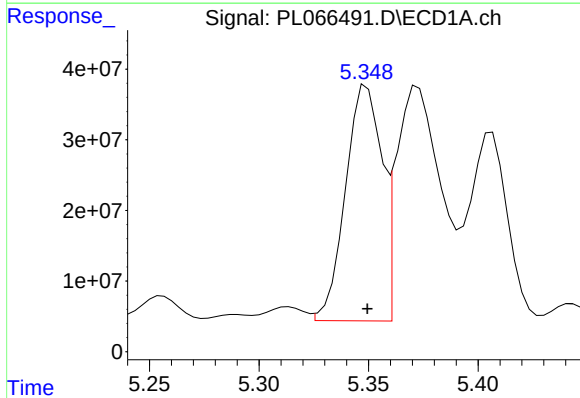


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 382200996
Conc: 749.23 ng/ml

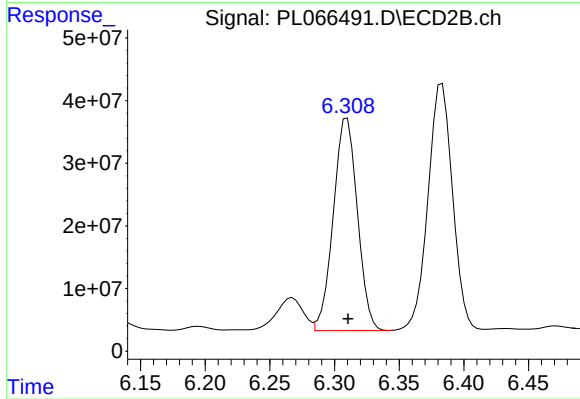

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 438485860
Conc: 774.83 ng/ml

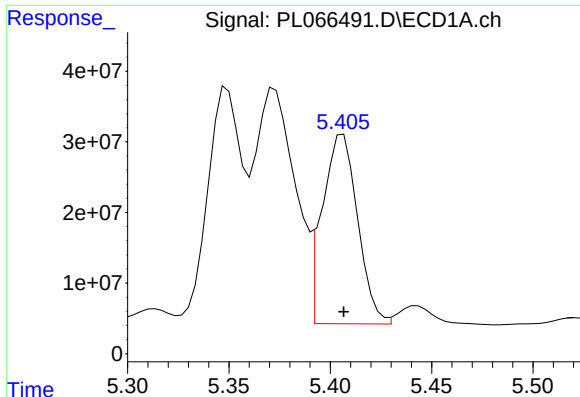

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 325080919
Conc: 759.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

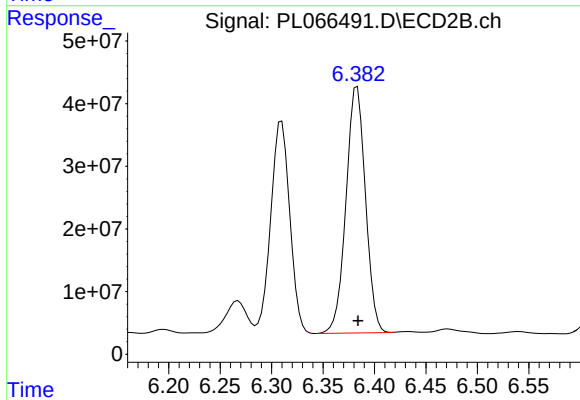


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: -0.001 min
Response: 518003545
Conc: 770.59 ng/ml

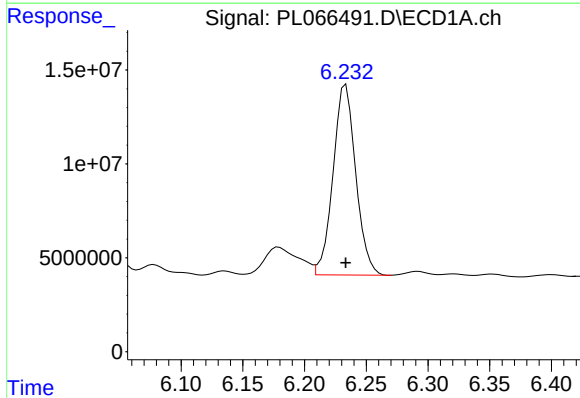


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 129477390
Conc: 755.42 ng/ml

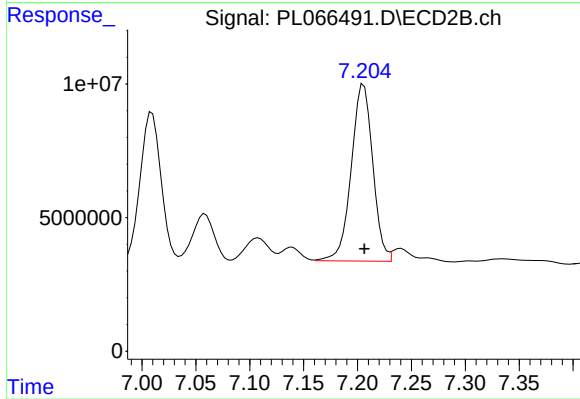

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 92182674
Conc: 753.85 ng/ml

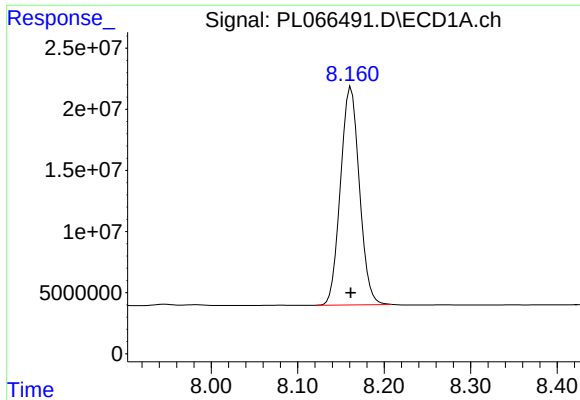

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 269462369
Conc: 71.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

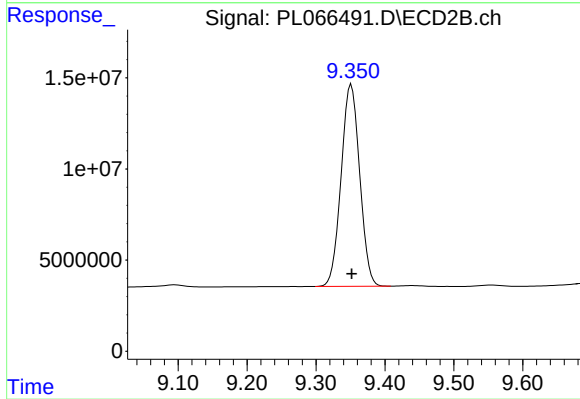

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 207443183
Conc: 73.71 ng/ml