

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
 Data File : PL066493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 10:32
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 08:44:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:43:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	107.5E6	87152798	24.484	25.483
28)	SA Decachlor...	8.161	9.353	96385799	72013045	25.568	25.588
Target Compounds							
23)	Chlordane-1	4.290	5.174	40533010	35913641	258.806	255.203
24)	Chlordane-2	4.786	5.651	44354320	41423221	256.612	268.222
25)	Chlordane-3	5.350	6.310	122.0E6	137.4E6	239.146	242.765
26)	Chlordane-4	5.407	6.383	104.4E6	166.3E6	243.816	247.340
27)	Chlordane-5	6.233	7.206	41985542	29651525	244.959	242.484


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
Data File : PL066493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 10:32
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 08:44:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:43:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

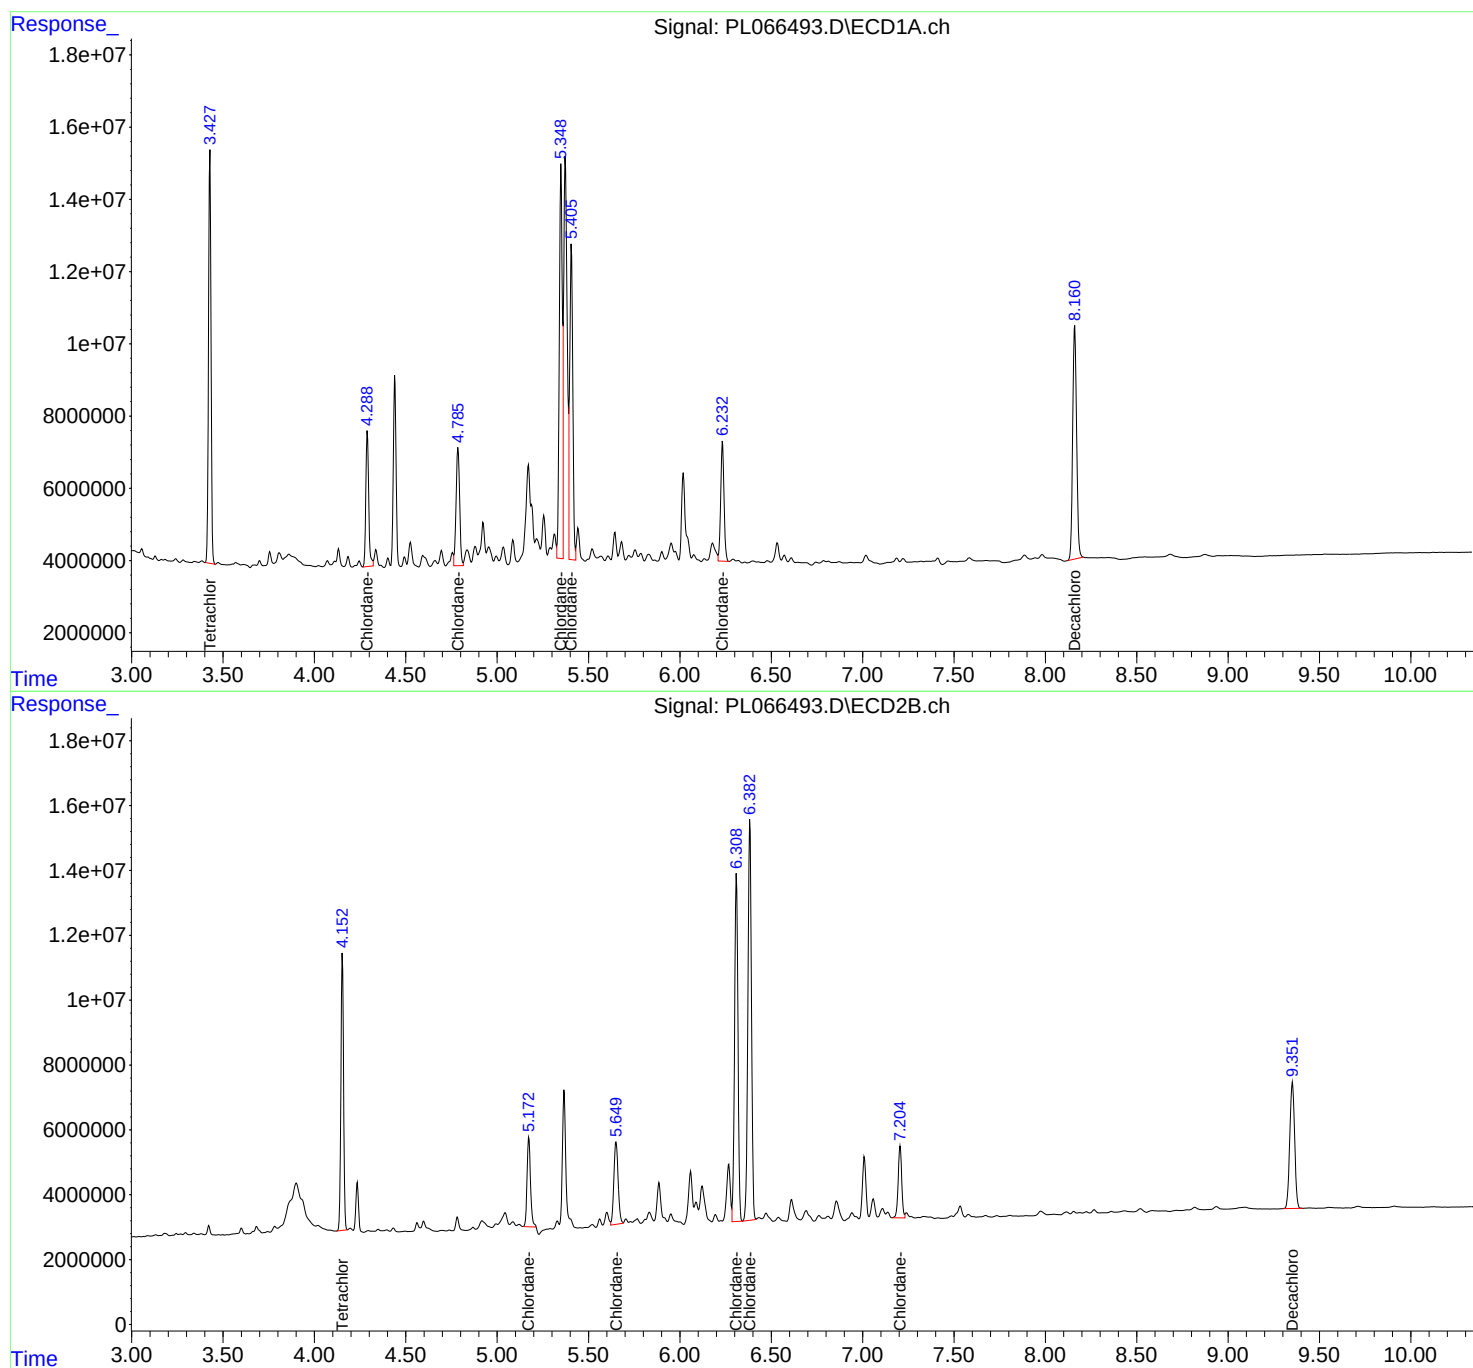


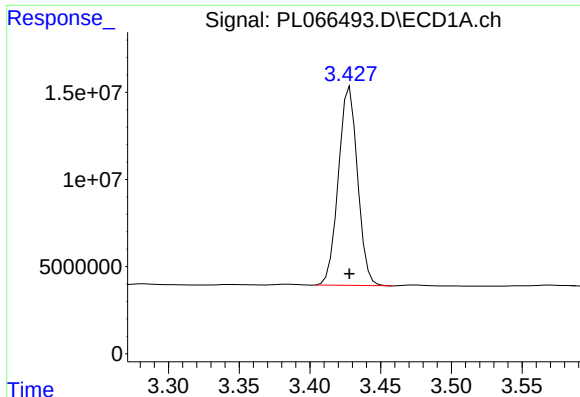

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 107501569
Conc: 24.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

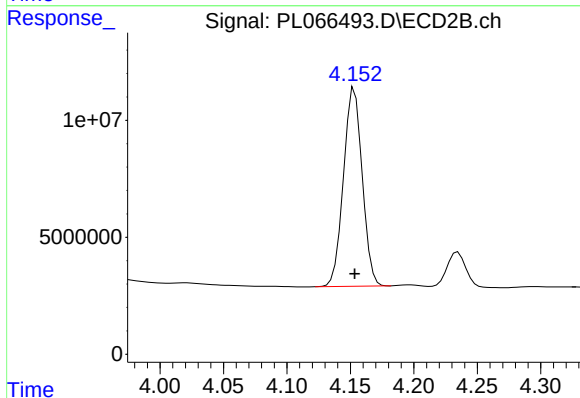


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 87152798
Conc: 25.48 ng/ml

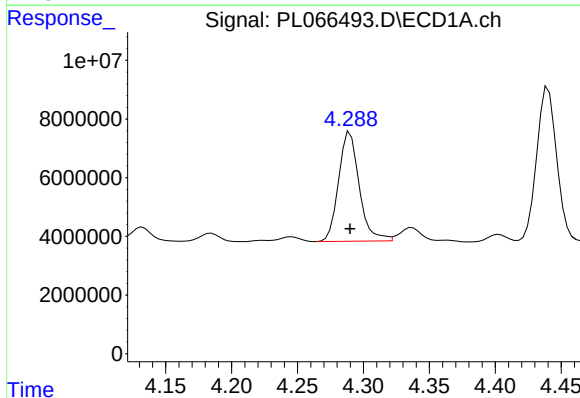


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 40533010
Conc: 258.81 ng/ml

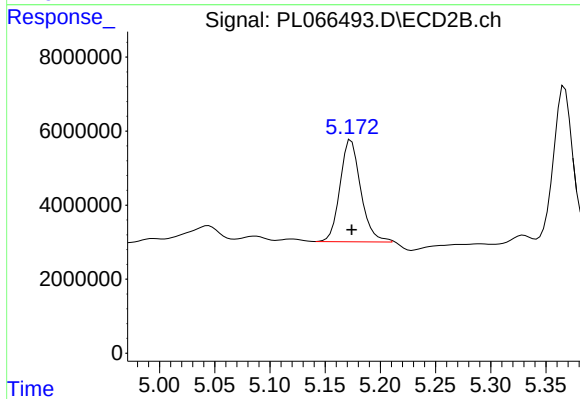

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 35913641
Conc: 255.20 ng/ml

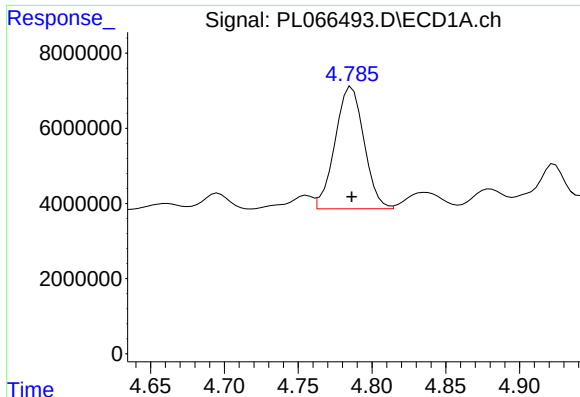

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 44354320
Conc: 256.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

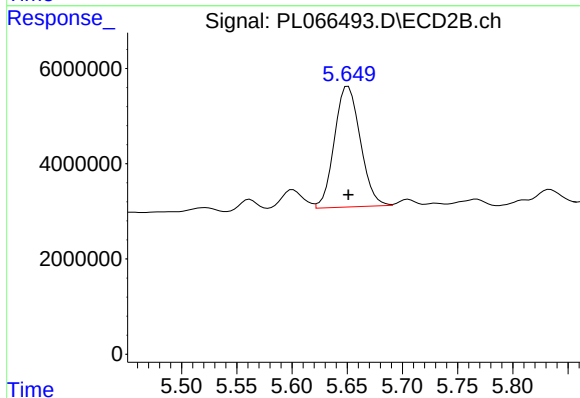


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 41423221
Conc: 268.22 ng/ml

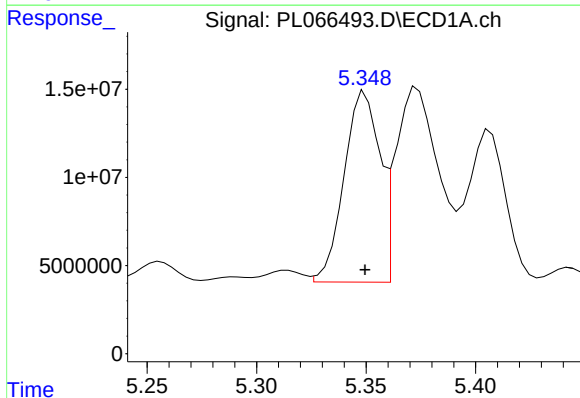


#25 Chlordane-3

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 121994230
Conc: 239.15 ng/ml

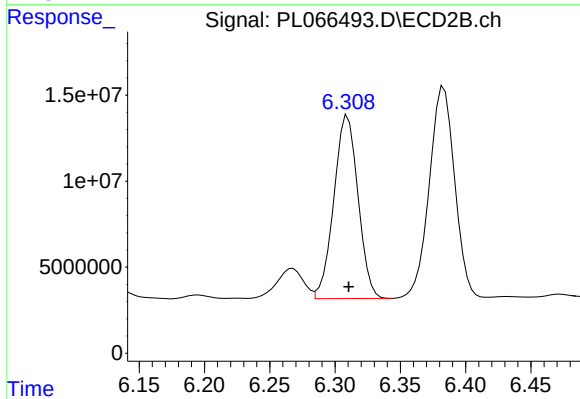

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 137384374
Conc: 242.77 ng/ml

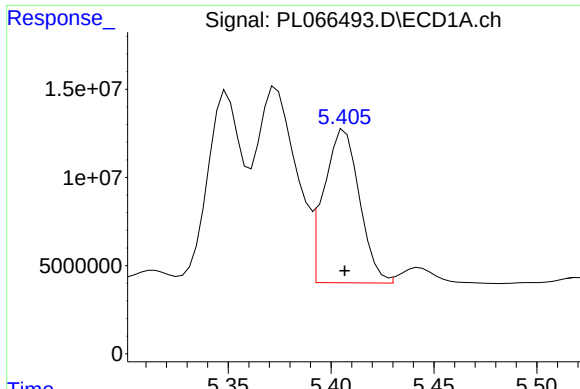

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 104413409
Conc: 243.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

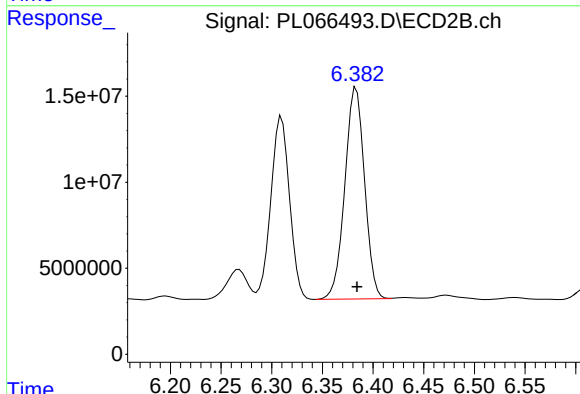


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 166266461
Conc: 247.34 ng/ml

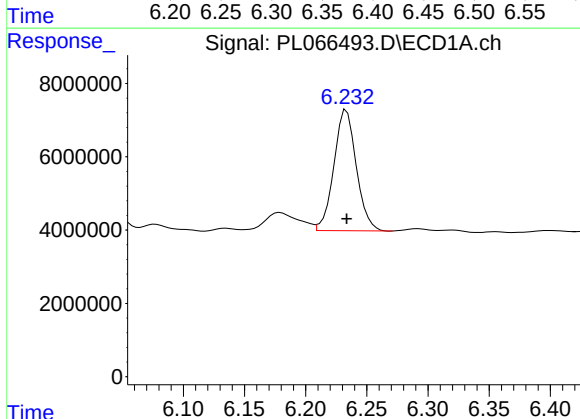


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 41985542
Conc: 244.96 ng/ml

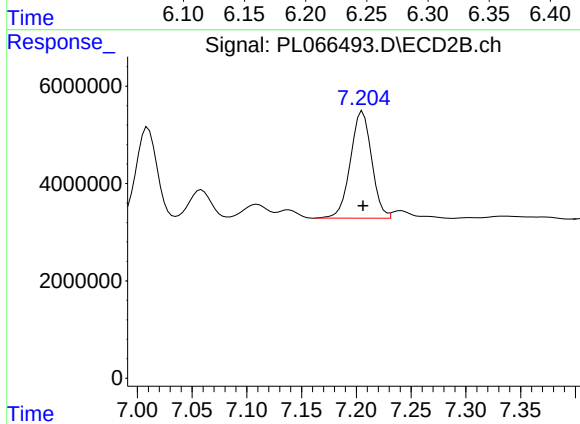

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 29651525
Conc: 242.48 ng/ml

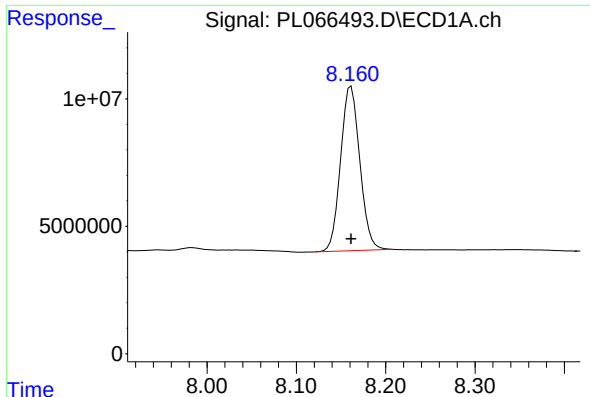

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 96385799
Conc: 25.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

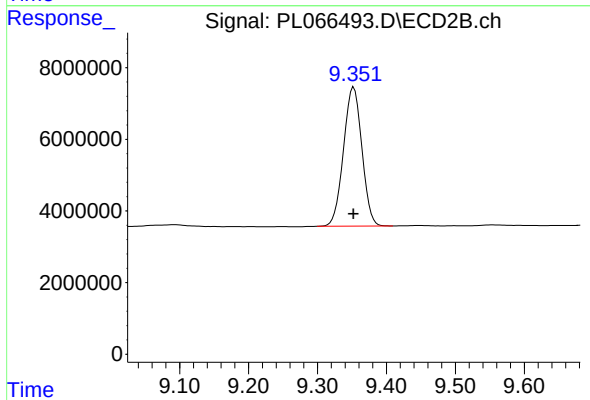

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 72013045
Conc: 25.59 ng/ml