

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
 Data File : PL066495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 11:00
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL042721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 08:48:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	217.3E6	168.3E6	50.058	49.370
28)	SA Decachlor...	8.161	9.351	189.5E6	138.9E6	50.497	49.168
Target Compounds							
23)	Chlordane-1	4.290	5.174	77252422	68736030	457.023	491.249
24)	Chlordane-2	4.786	5.651	86931629	75726376	506.007	466.263
25)	Chlordane-3	5.349	6.310	253.5E6	276.8E6	509.301	493.813
26)	Chlordane-4	5.406	6.383	213.9E6	328.5E6	506.824	489.361
27)	Chlordane-5	6.233	7.206	85939468	59235164	510.338	504.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
Data File : PL066495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 11:00
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL042721

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 08:48:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

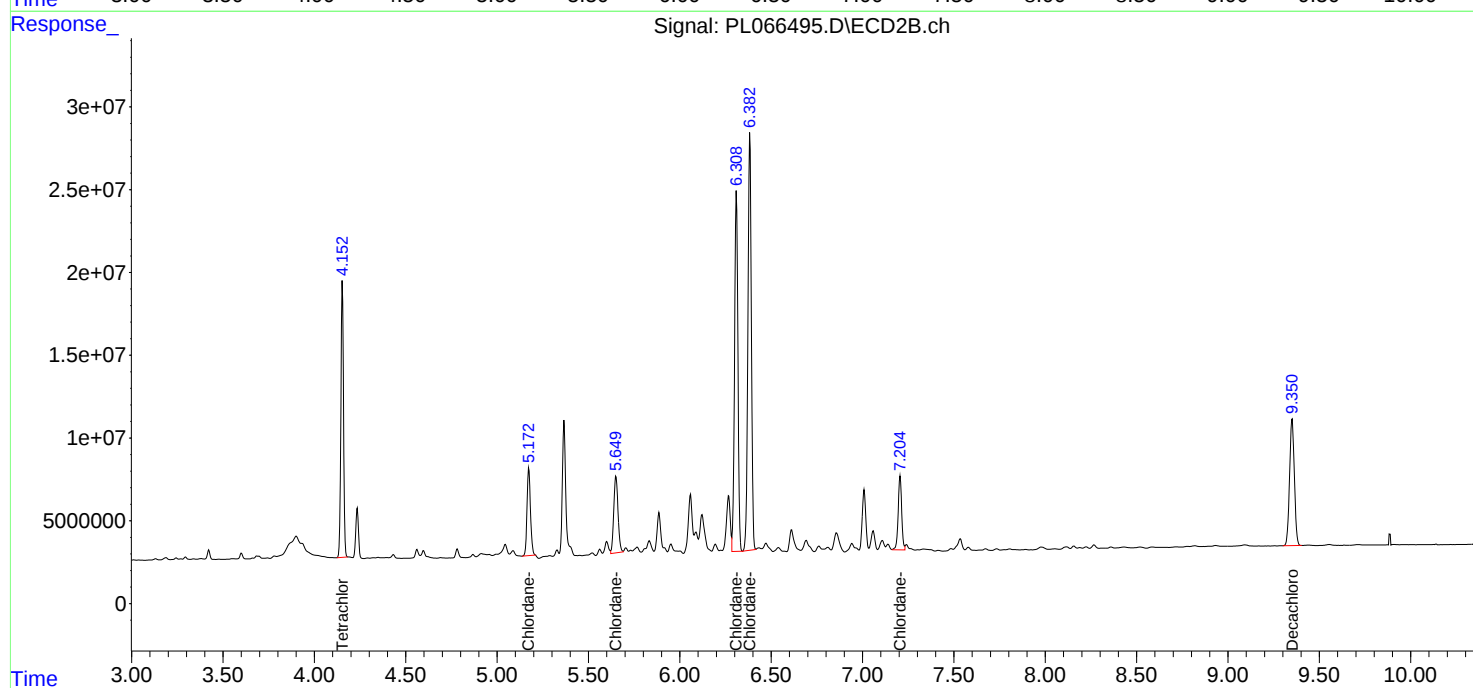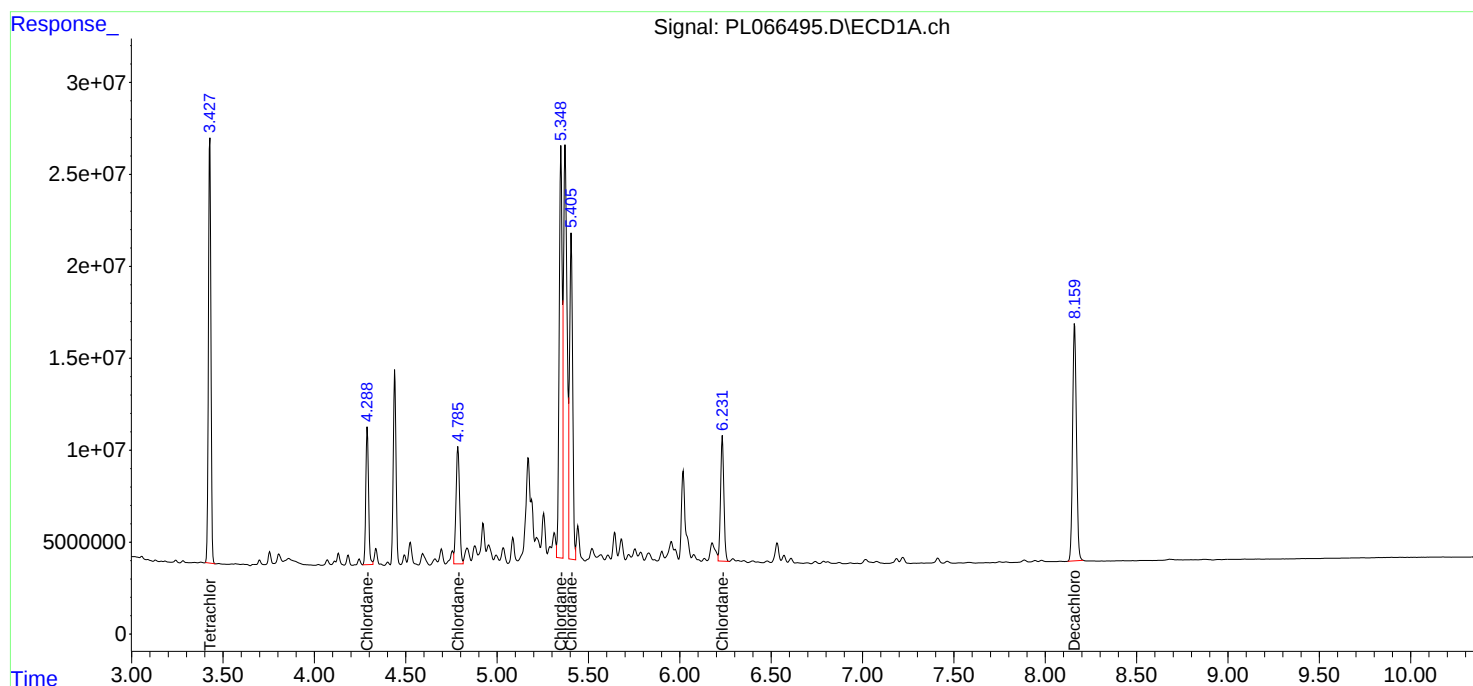


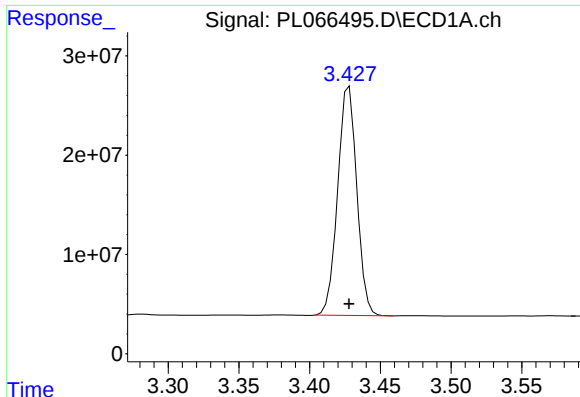

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 217259785
Conc: 50.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042721

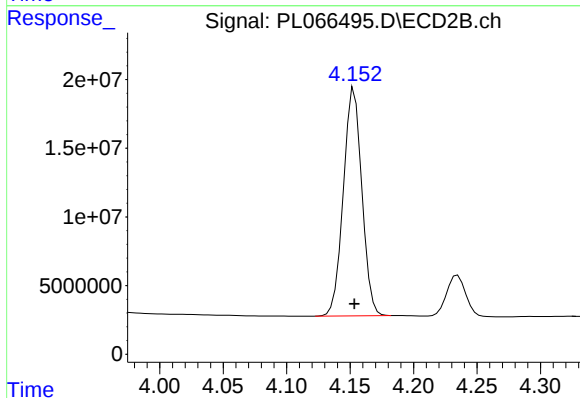


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 168311481
Conc: 49.37 ng/ml

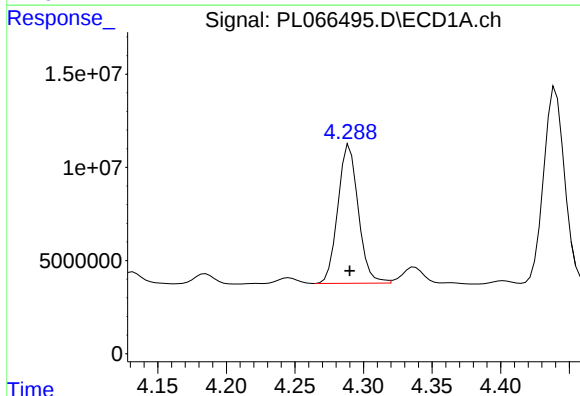


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 77252422
Conc: 457.02 ng/ml

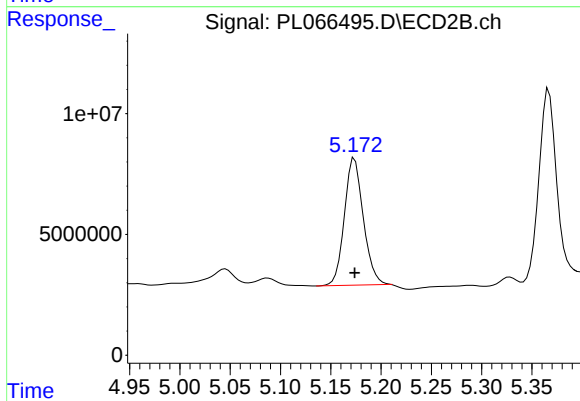

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 68736030
Conc: 491.25 ng/ml

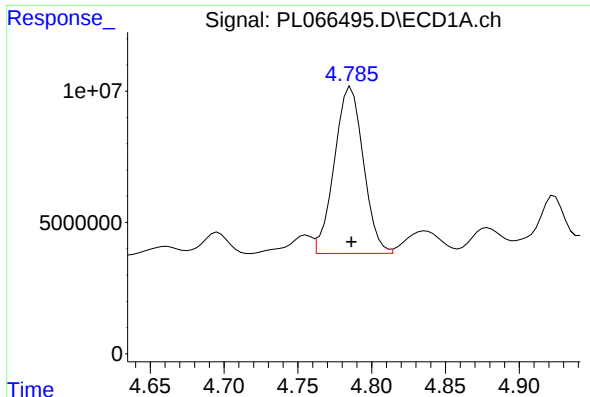

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 86931629
Conc: 506.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042721

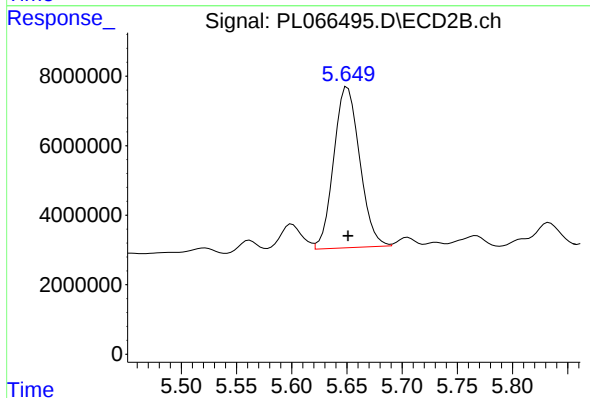


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 75726376
Conc: 466.26 ng/ml

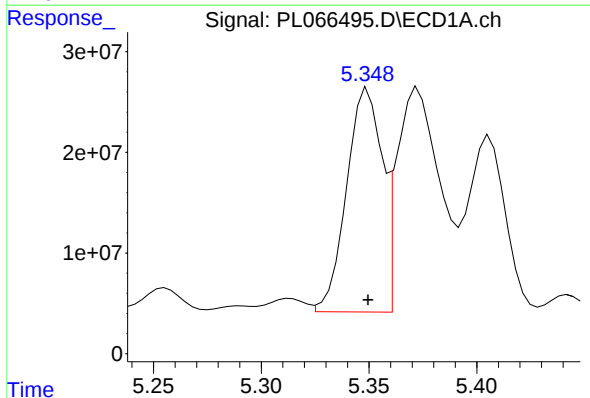


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 253452465
Conc: 509.30 ng/ml

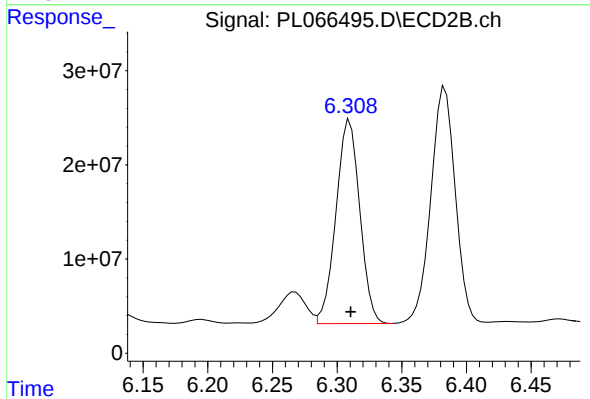

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 276791307
Conc: 493.81 ng/ml

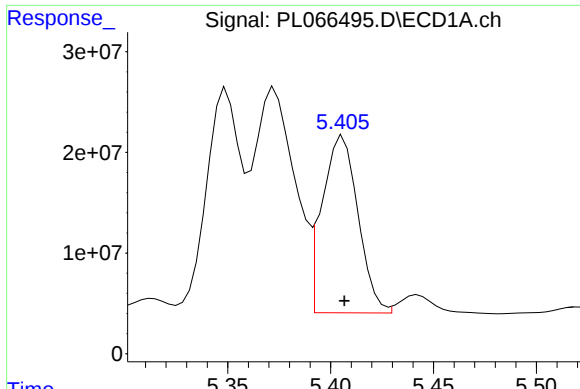

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 213883257
Conc: 506.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042721

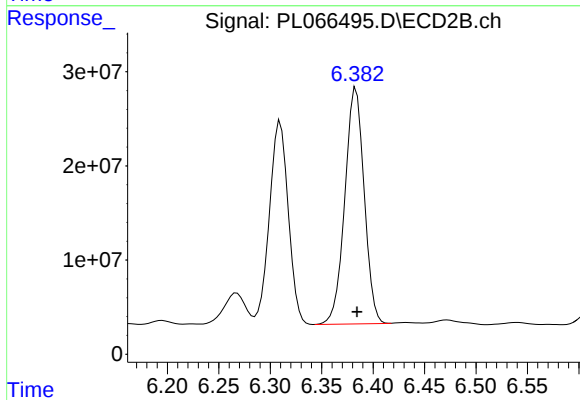


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 328547702
Conc: 489.36 ng/ml

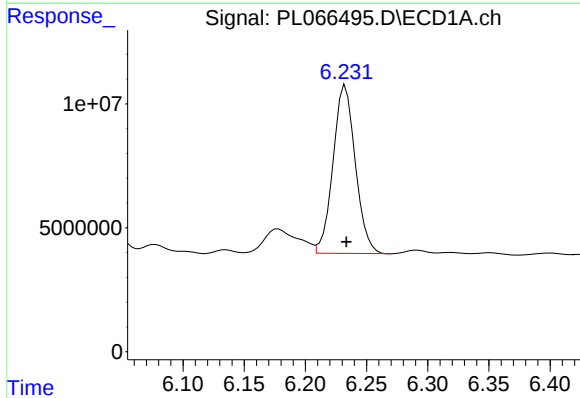


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 85939468
Conc: 510.34 ng/ml

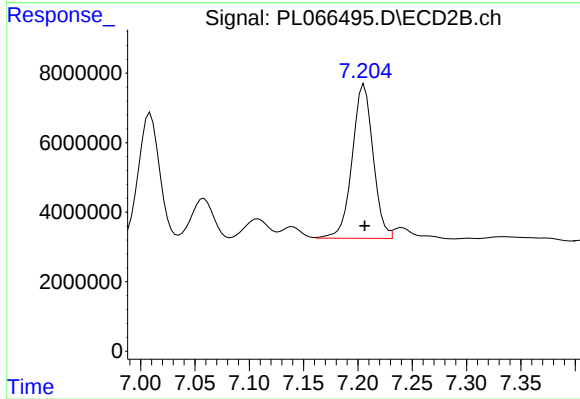

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 59235164
Conc: 504.43 ng/ml

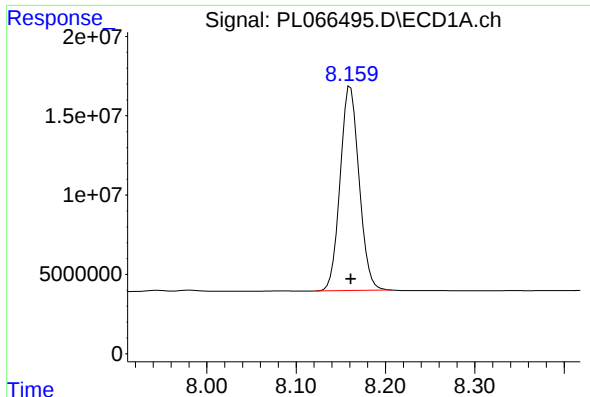

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 189516130
Conc: 50.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042721

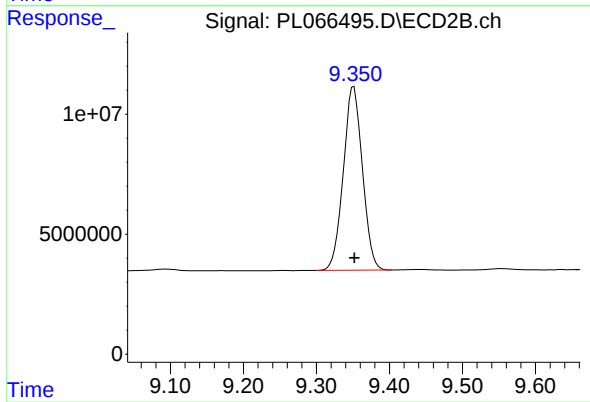

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 138921726
Conc: 49.17 ng/ml