

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
 Data File : PL066505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 15:02
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 08:52:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	4.153	210.1E6	169.2E6	55.753	48.188
28)	SA Decachlor...	8.165	9.353	187.4E6	126.2E6	48.874	40.786
Target Compounds							
23)	Chlordane-1	4.292	5.174	74668309	67902613	441.735	485.292
24)	Chlordane-2	4.788	5.651	84888286	73475794	494.113	452.406
25)	Chlordane-3	5.352	6.311	245.5E6	267.8E6	493.371	477.768
26)	Chlordane-4	5.409	6.385	208.6E6	317.9E6	494.304	473.538
27)	Chlordane-5	6.236	7.207	83917287	56152550	498.330	478.180



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042721\
Data File : PL066505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 15:02
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 08:52:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

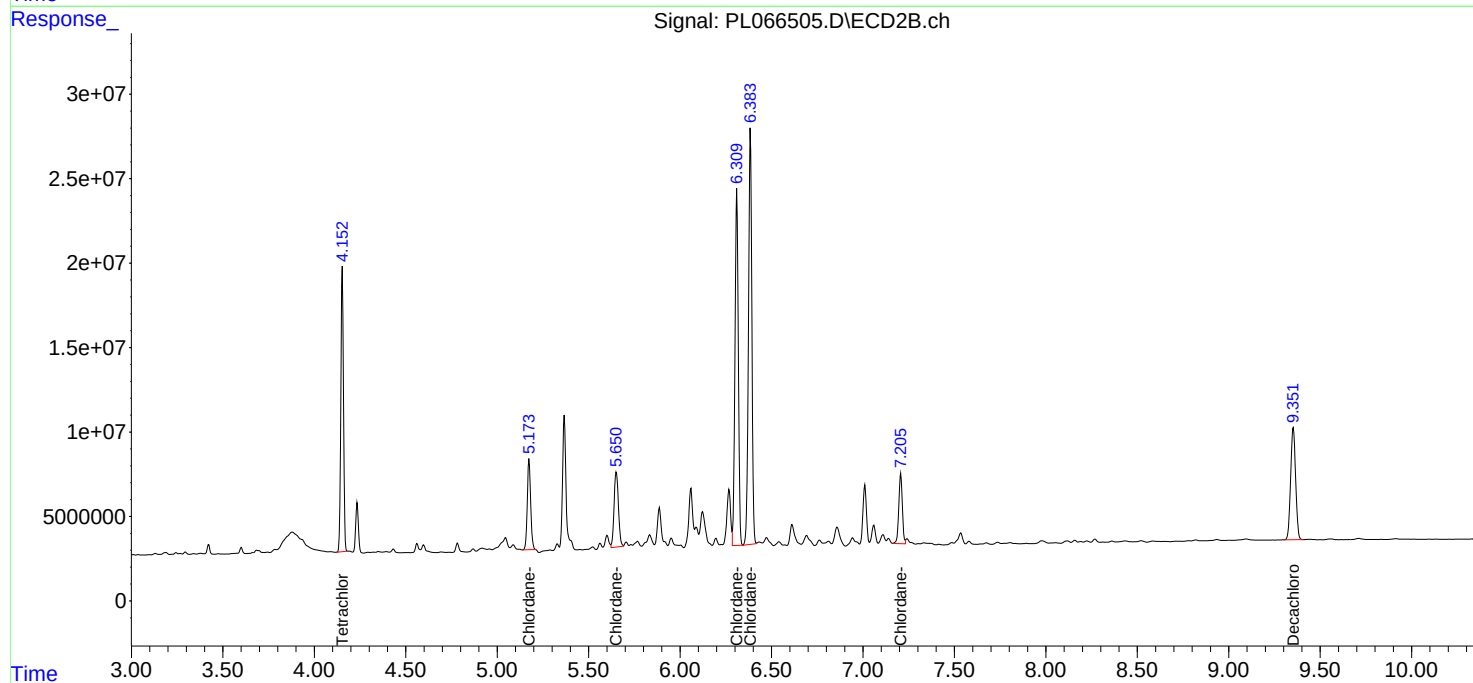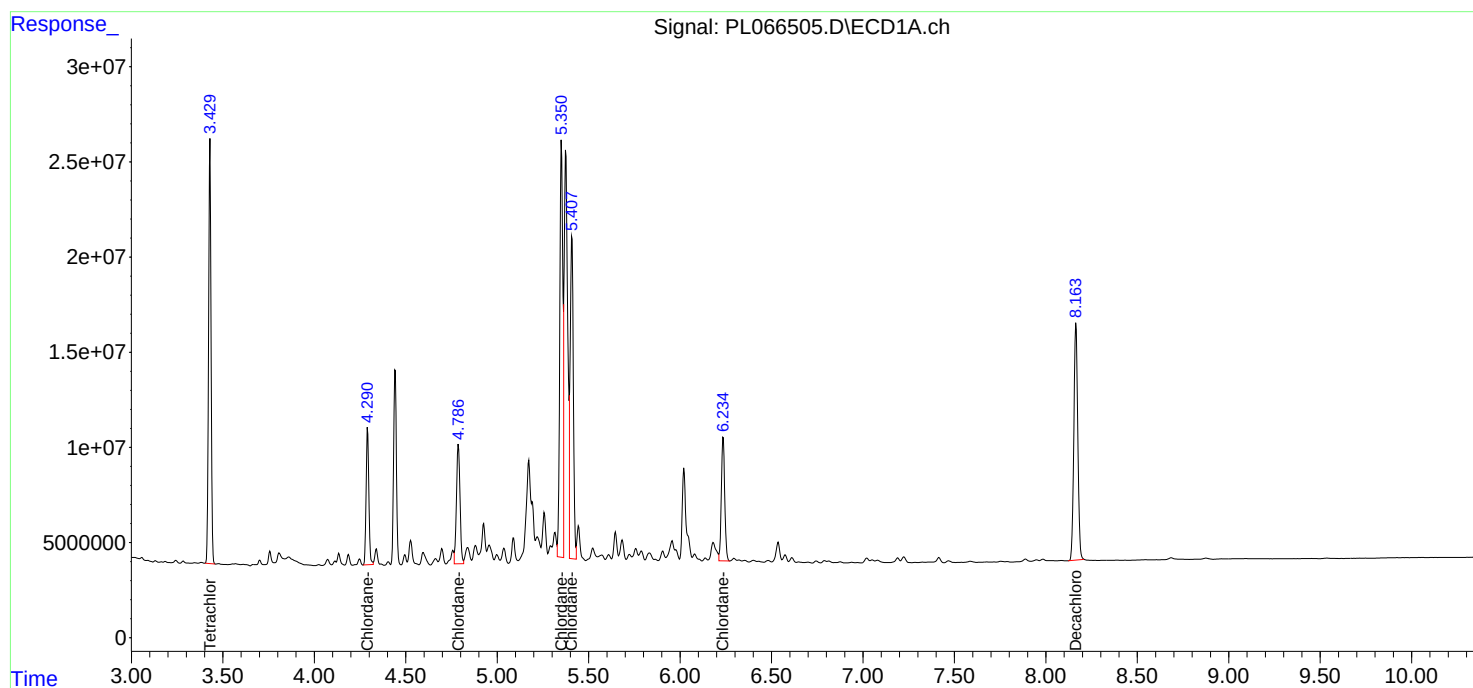


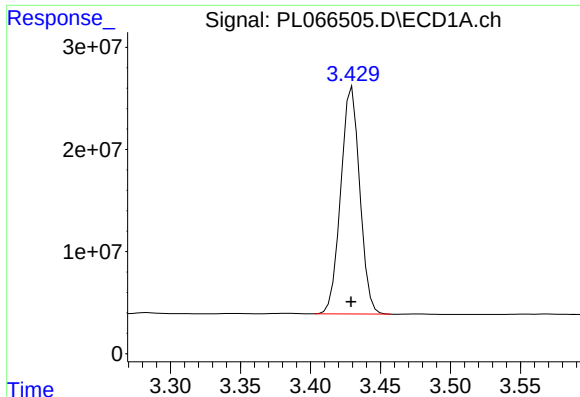

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 210080525
Conc: 55.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

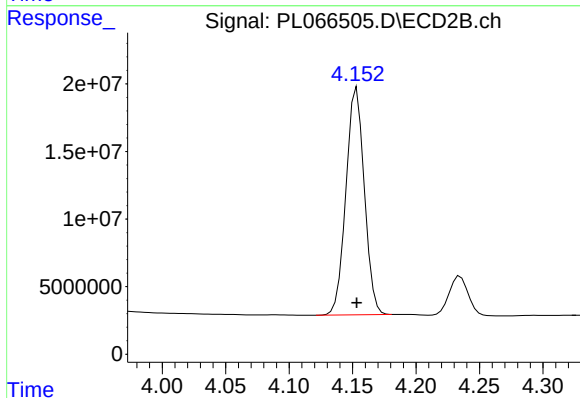


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 169238636
Conc: 48.19 ng/ml

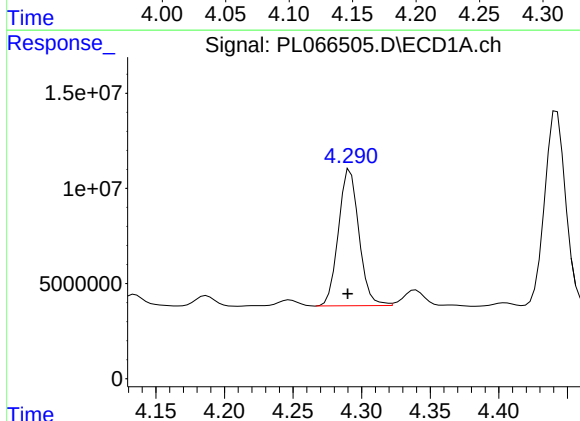


#23 Chlordane-1

R.T.: 4.292 min
Delta R.T.: 0.002 min
Response: 74668309
Conc: 441.73 ng/ml

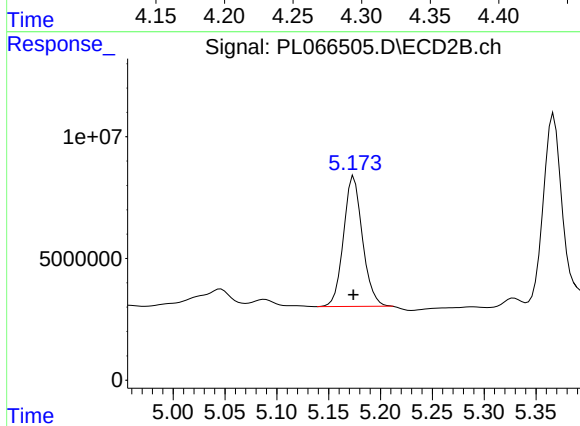

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 67902613
Conc: 485.29 ng/ml

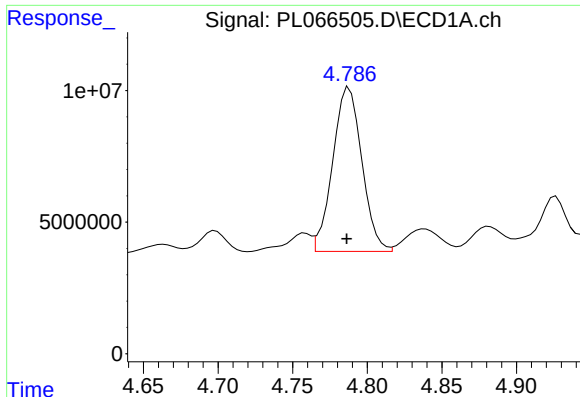

#24 Chlordane-2


R.T.: 4.788 min
Delta R.T.: 0.002 min
Response: 84888286
Conc: 494.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

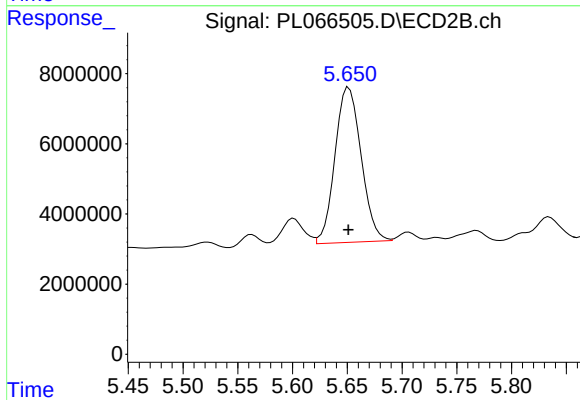


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 73475794
Conc: 452.41 ng/ml

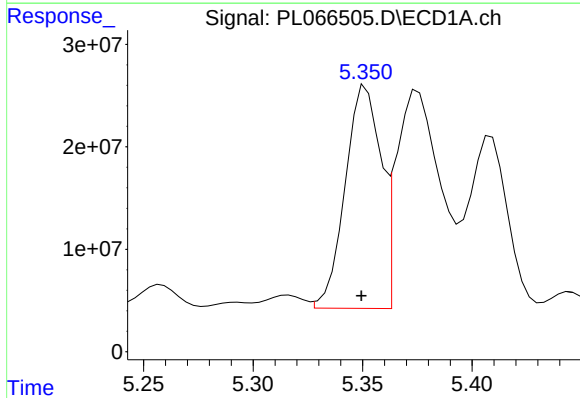


#25 Chlordane-3

R.T.: 5.352 min
Delta R.T.: 0.002 min
Response: 245525044
Conc: 493.37 ng/ml

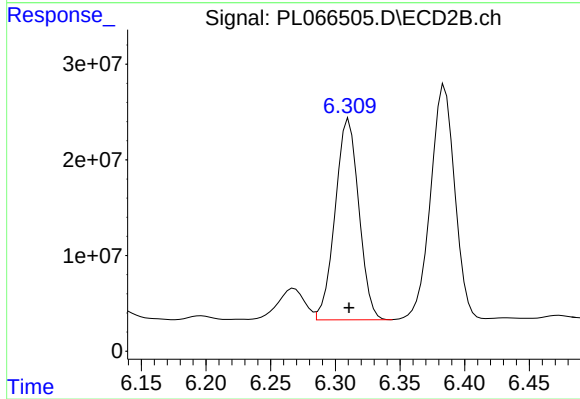

#25 Chlordane-3


R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 267797813
Conc: 477.77 ng/ml

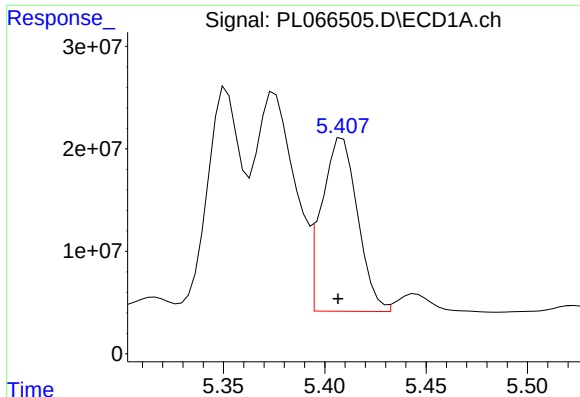

#26 Chlordane-4


R.T.: 5.409 min
Delta R.T.: 0.002 min
Response: 208600066
Conc: 494.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

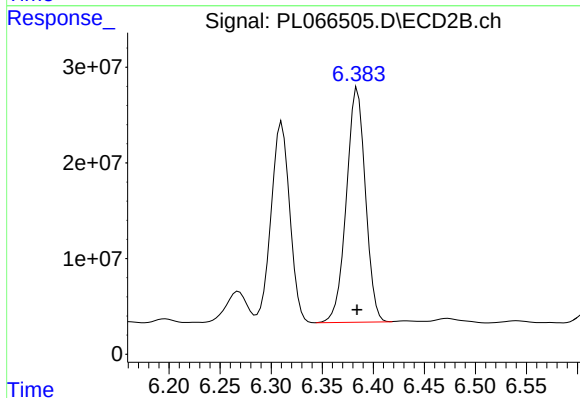


#26 Chlordane-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 317924050
Conc: 473.54 ng/ml

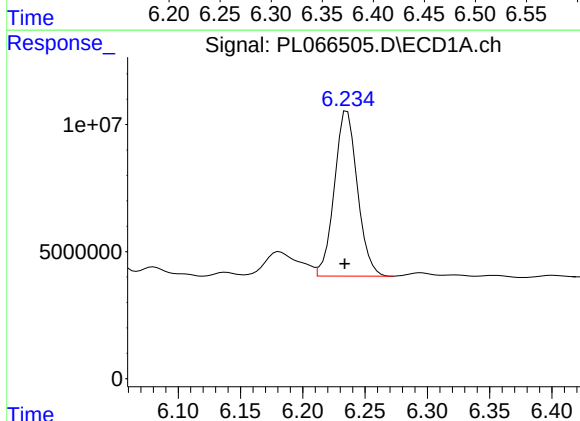


#27 Chlordane-5

R.T.: 6.236 min
Delta R.T.: 0.002 min
Response: 83917287
Conc: 498.33 ng/ml

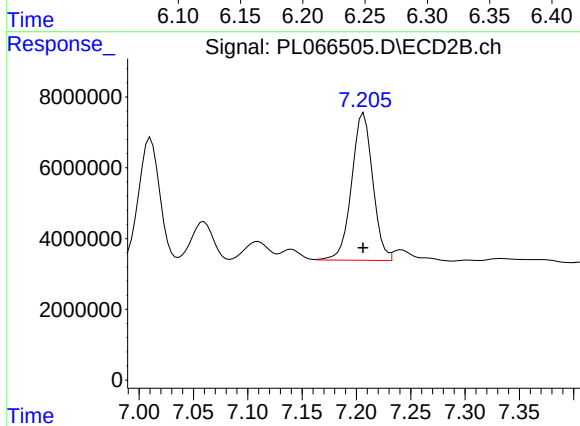

#27 Chlordane-5

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 56152550
Conc: 478.18 ng/ml

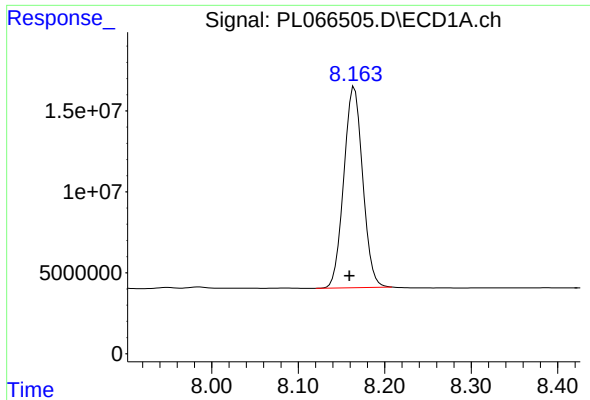

#28 Decachlorobiphenyl


R.T.: 8.165 min

Delta R.T.: 0.006 min

Response: 187393185

Conc: 48.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

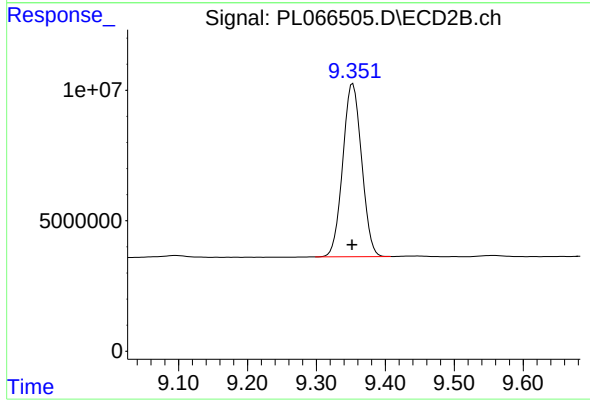

#28 Decachlorobiphenyl

R.T.: 9.353 min

Delta R.T.: 0.001 min

Response: 126176377

Conc: 40.79 ng/ml