

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl042722\
 Data File : PL074408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 17:53
 Operator : AR\AJ
 Sample : PB144407BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB144407BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/28/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 23:27:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.634	5.490	6293166	32884277	19.477	18.444
28) SA Decachlor...	10.404	11.333	10897171	37198320	20.955m	21.060

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\pl042722\
Data File : PL074408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 17:53
Operator : AR\AJ
Sample : PB144407BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB144407BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/28/2022
Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 23:27:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

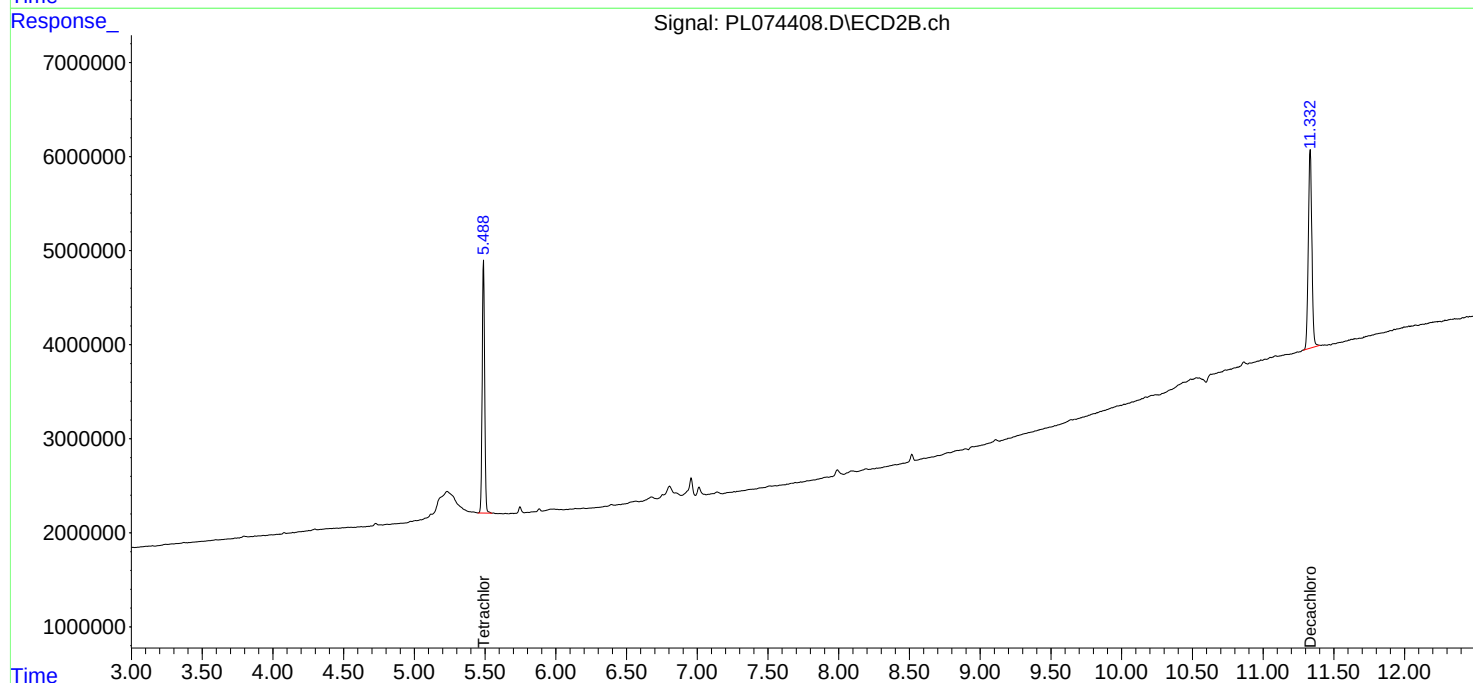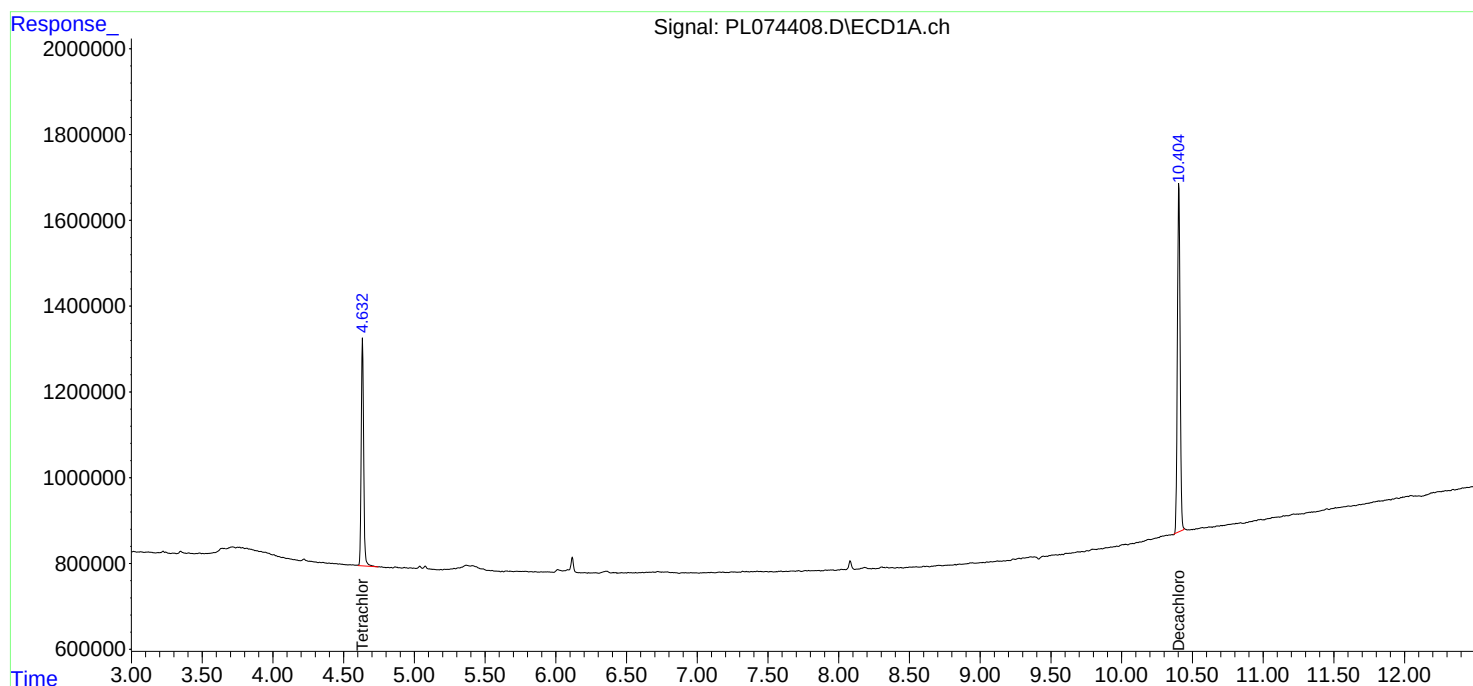

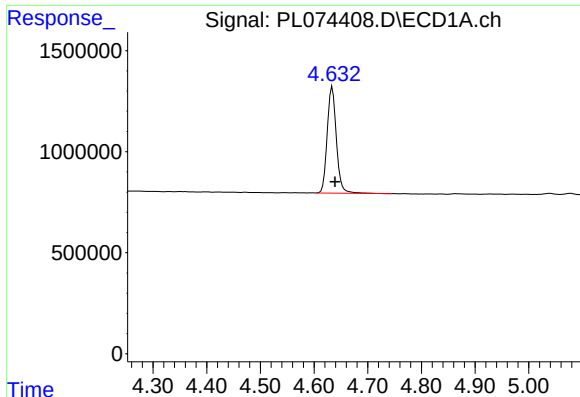


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: -0.005 min
Response: 6293166
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB144407BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/28/2022
Supervised By :mohammad ahmed 04/28/2022

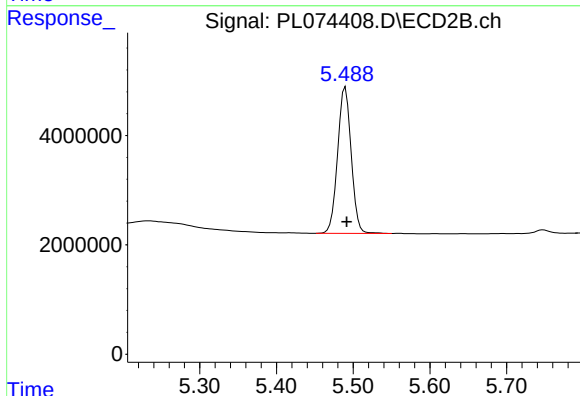


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.002 min
Response: 32884277
Conc: 18.44 ng/ml

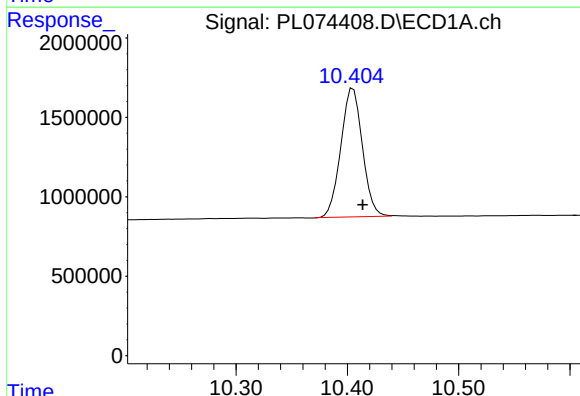

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 10897171
Conc: 20.95 ng/ml m

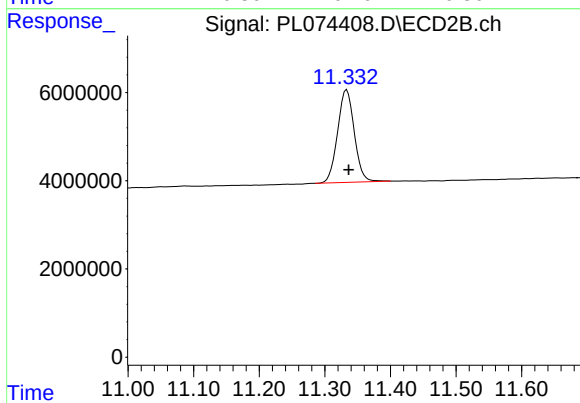

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 37198320
Conc: 21.06 ng/ml