

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042723\
 Data File : PL082358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2023 16:16
 Operator : AR\AJ
 Sample : 02503-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-305A-COMP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 21:18:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.646	53316828	44596264	19.960	19.250
28) SA Decachlor...	8.740	7.757	38737052	44918863	20.291	19.680

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042723\
Data File : PL082358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2023 16:16
Operator : AR\AJ
Sample : 02503-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-305A-COMP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 21:18:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

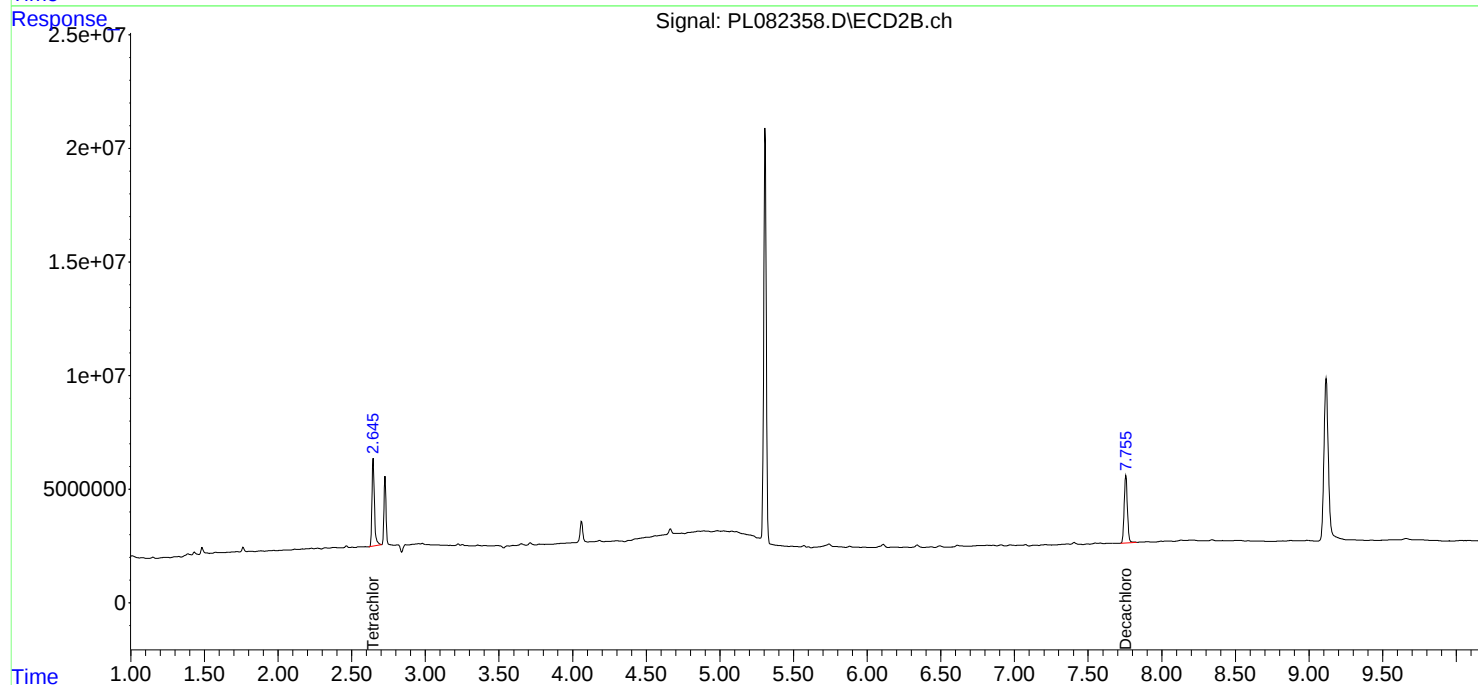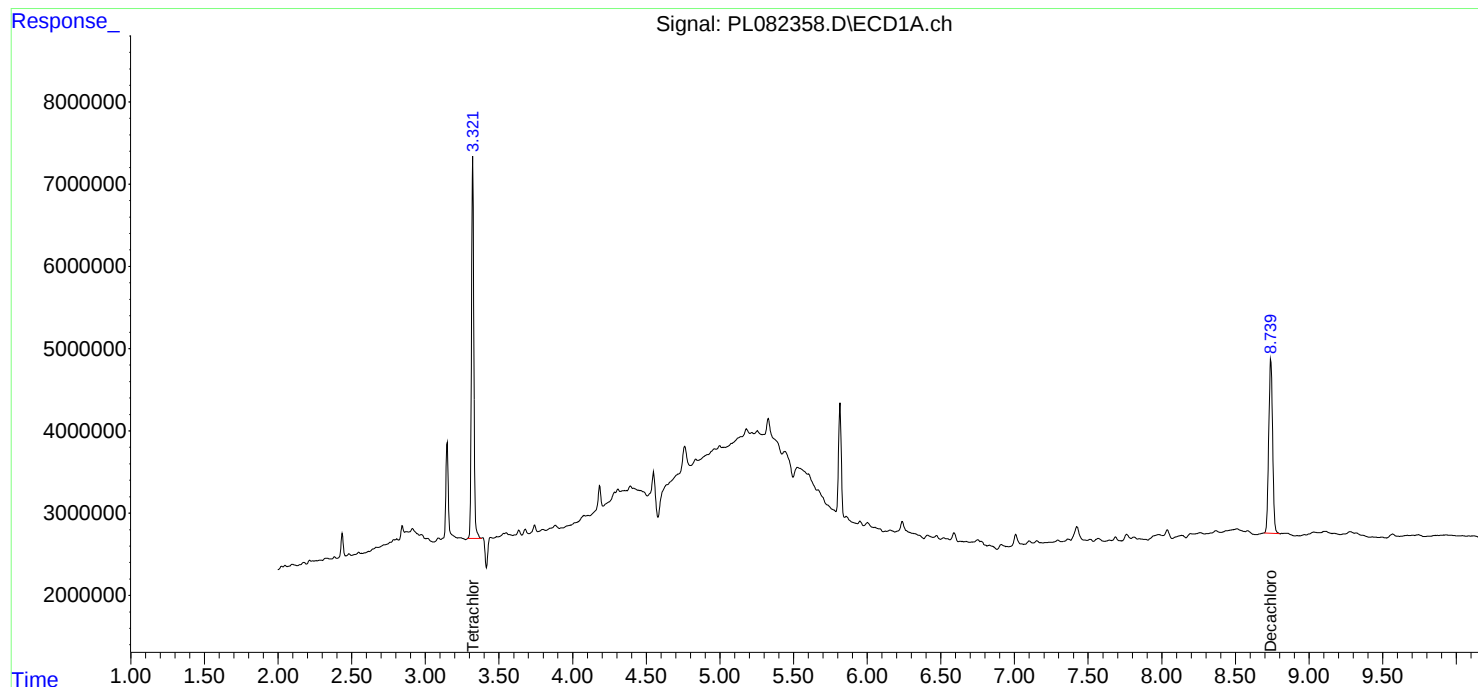


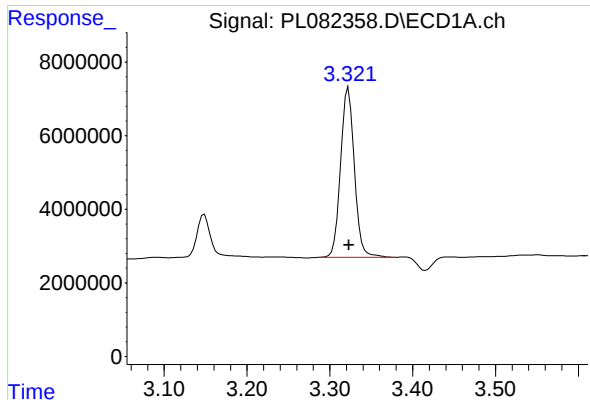

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 53316828
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-305A-COMP-01

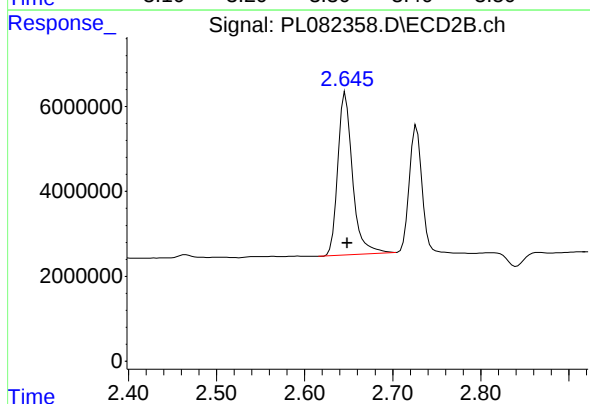


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.002 min
Response: 44596264
Conc: 19.25 ng/ml

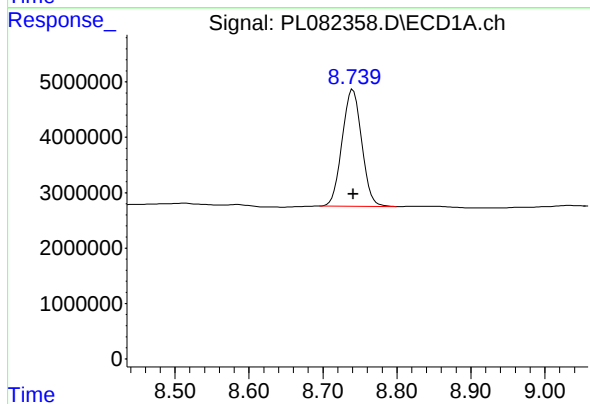

#28 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: 0.000 min
Response: 38737052
Conc: 20.29 ng/ml

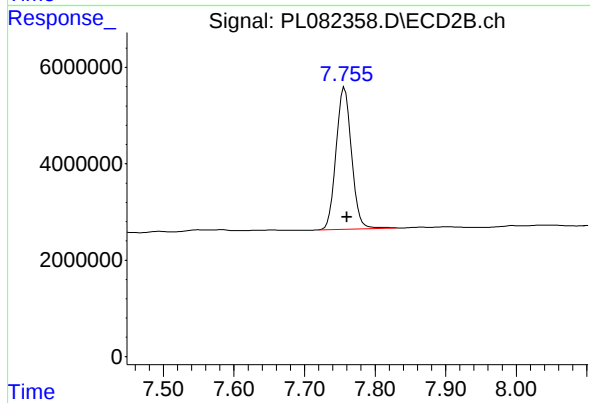

#28 Decachlorobiphenyl

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 44918863
Conc: 19.68 ng/ml