

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042820\
 Data File : PL058413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2020 12:21
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 12:41:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 28 12:41:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.953	592.9E6	99642253	50.000	50.000
28)	SA Decachlor...	8.199	8.972	493.8E6	101.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.322	4.936	214.9E6	41671825	500.000	500.000
24)	Chlordane-2	4.823	5.402	207.6E6	49562558	500.000	500.000
25)	Chlordane-3	5.392	6.043	656.7E6	200.0E6	500.000	500.000
26)	Chlordane-4	5.448	6.116	548.8E6	243.0E6	500.000	500.000
27)	Chlordane-5	6.283	6.916	203.4E6	37435386	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042820\
Data File : PL058413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2020 12:21
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 12:41:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Tue Apr 28 12:41:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

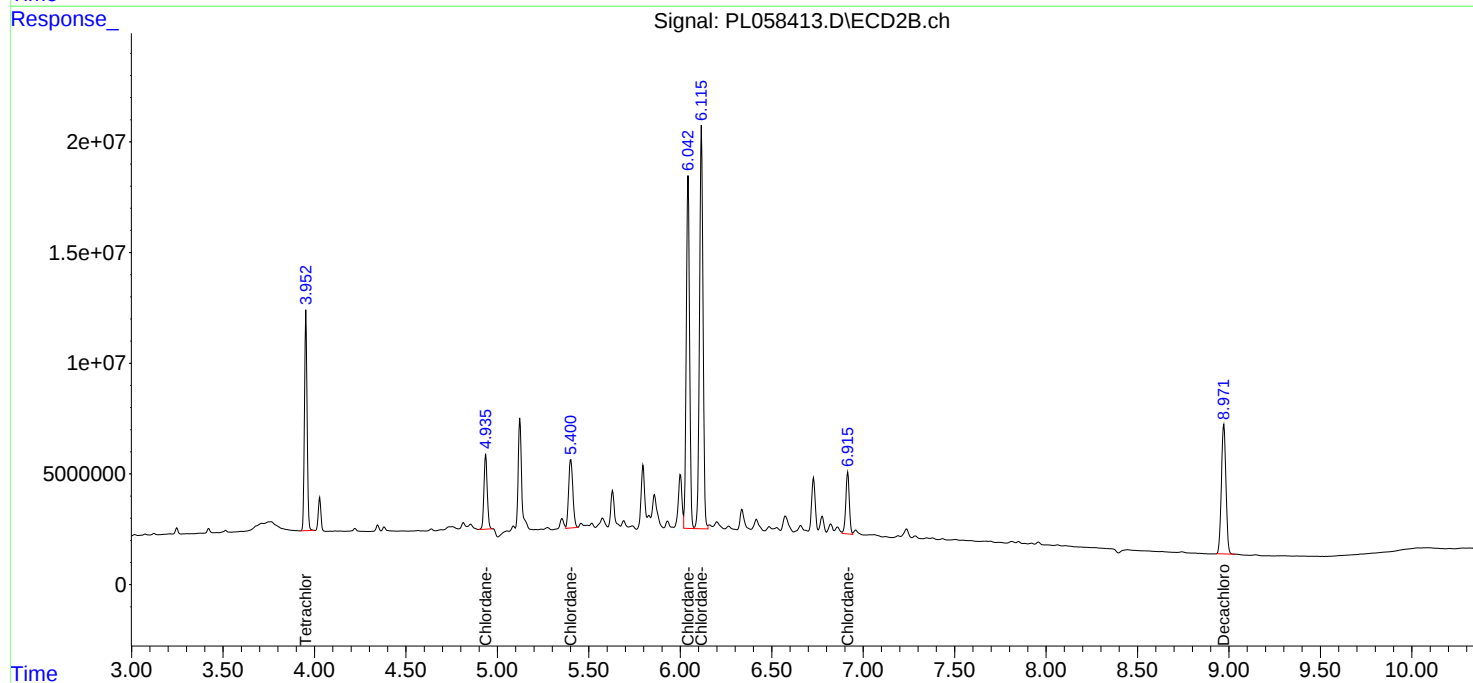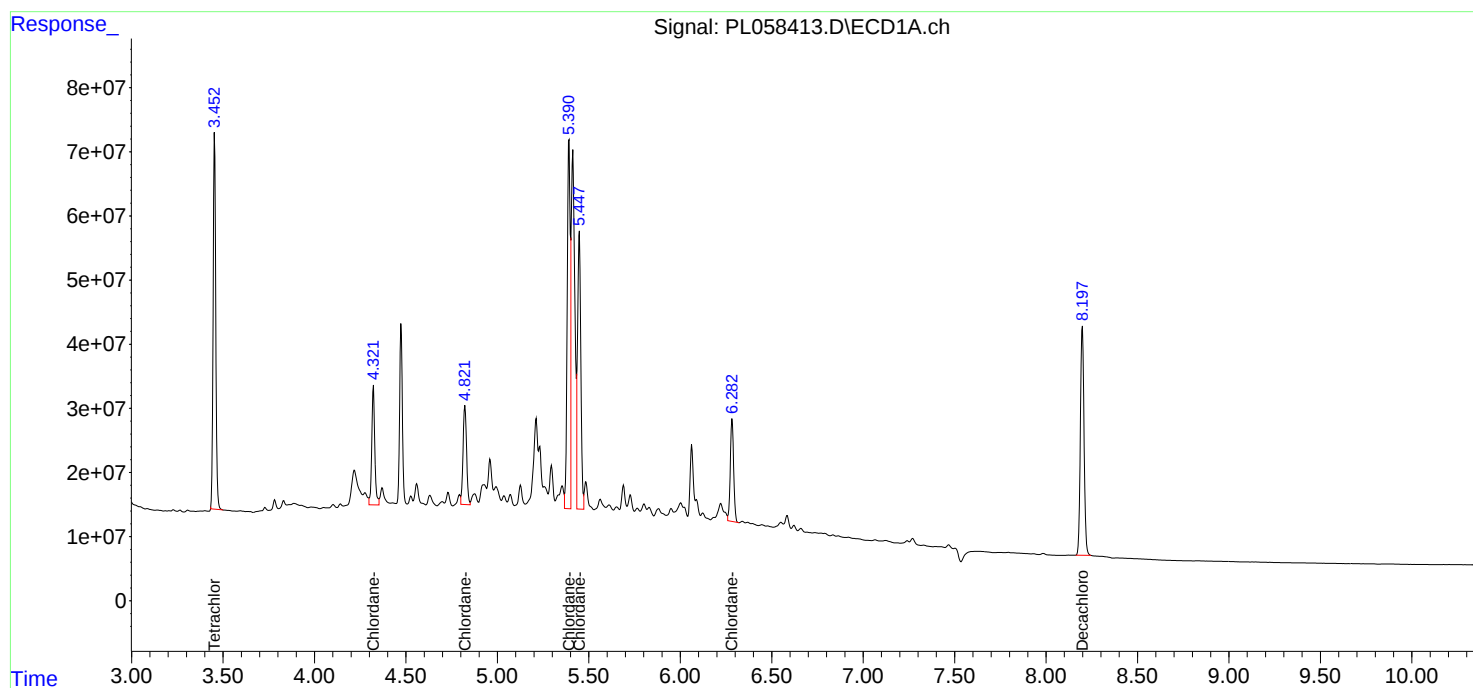


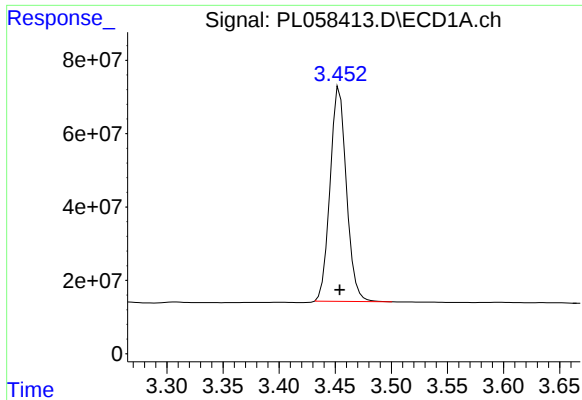

#1 Tetrachloro-m-xylene


R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 592922428
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

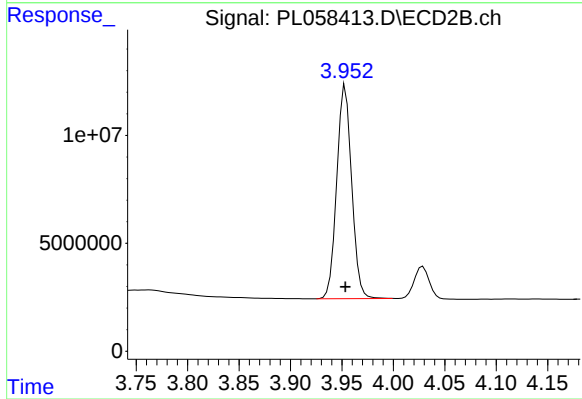


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: 0.000 min
Response: 99642253
Conc: 50.00 ng/ml

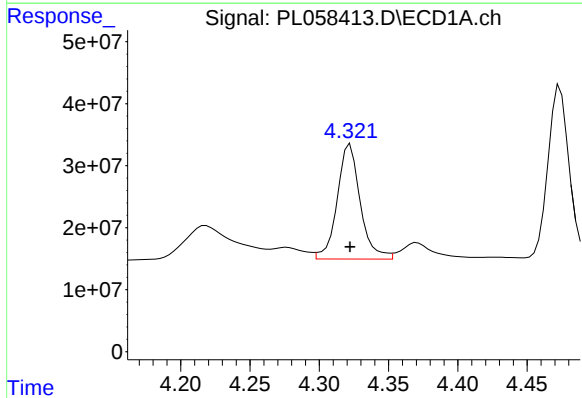


#23 Chlordane-1

R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 214918674
Conc: 500.00 ng/ml

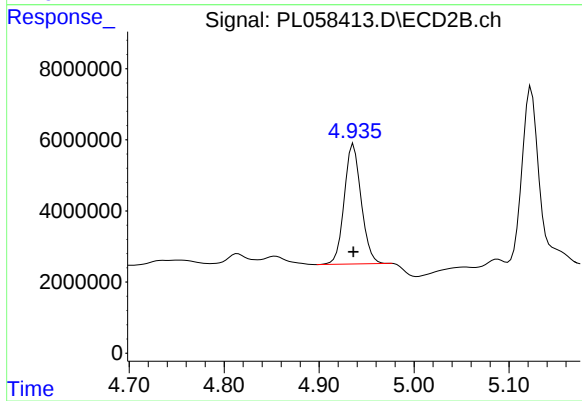

#23 Chlordane-1


R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 41671825
Conc: 500.00 ng/ml

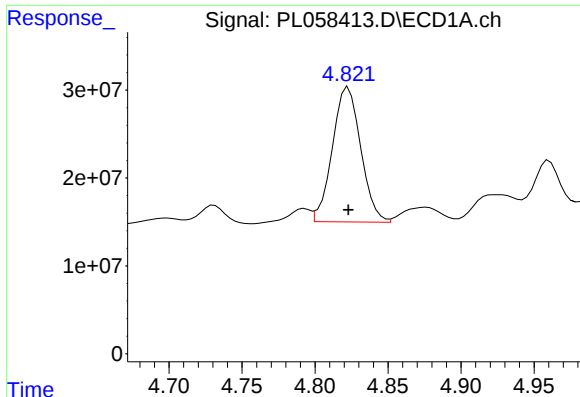

#24 Chlordane-2


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 207641650
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

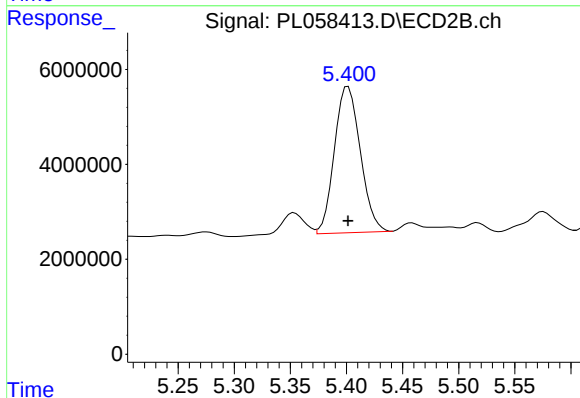


#24 Chlordane-2

R.T.: 5.402 min
Delta R.T.: 0.000 min
Response: 49562558
Conc: 500.00 ng/ml

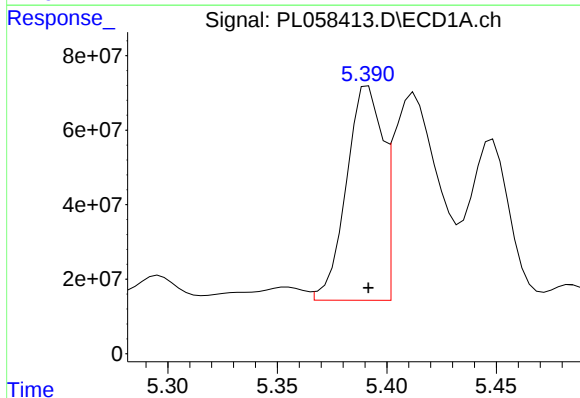


#25 Chlordane-3

R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 656729317
Conc: 500.00 ng/ml

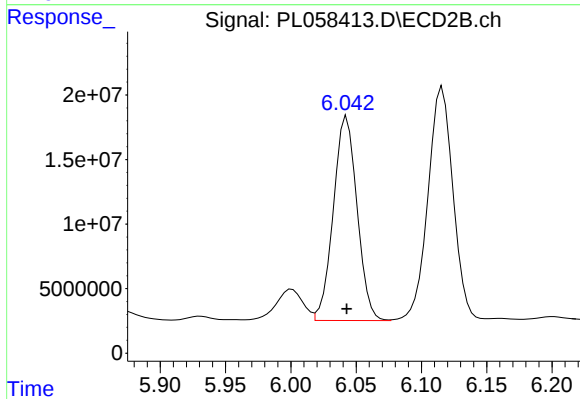

#25 Chlordane-3


R.T.: 6.043 min
Delta R.T.: 0.000 min
Response: 199980322
Conc: 500.00 ng/ml

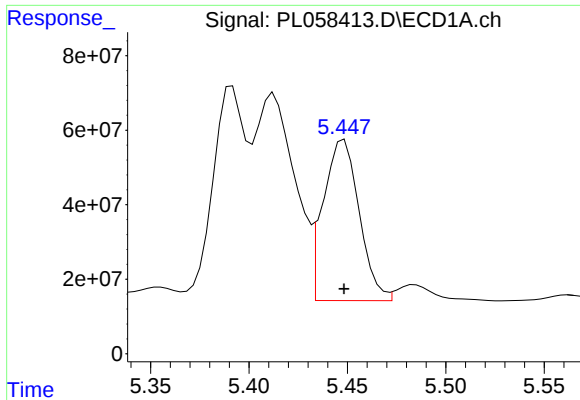

#26 Chlordane-4


R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 548810364
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

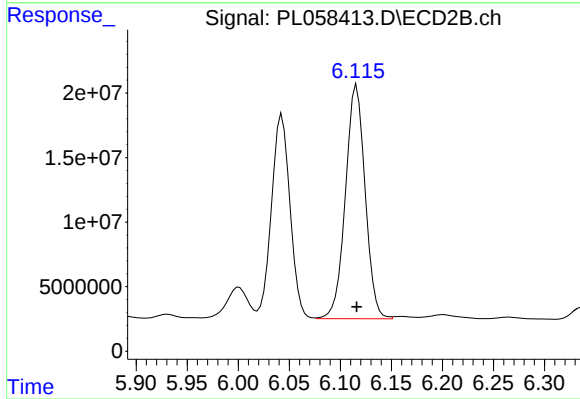


#26 Chlordane-4

R.T.: 6.116 min
Delta R.T.: 0.000 min
Response: 243023158
Conc: 500.00 ng/ml

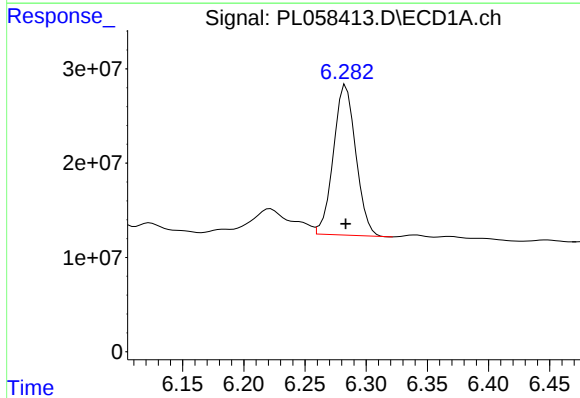


#27 Chlordane-5

R.T.: 6.283 min
Delta R.T.: 0.000 min
Response: 203376115
Conc: 500.00 ng/ml

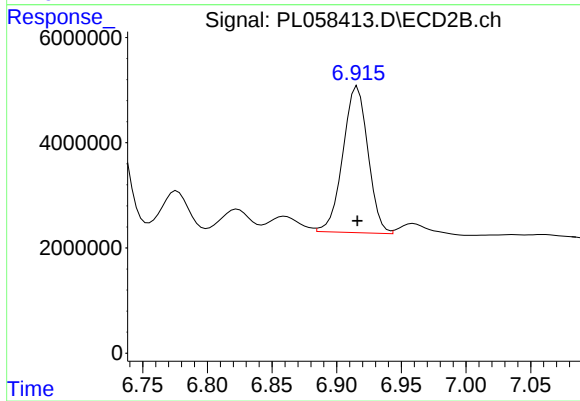

#27 Chlordane-5


R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 37435386
Conc: 500.00 ng/ml

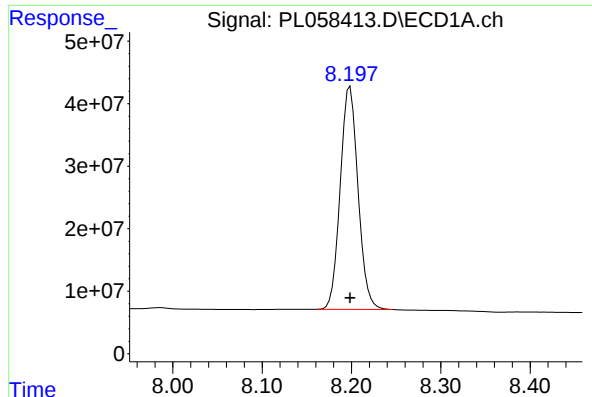

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 493829243
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

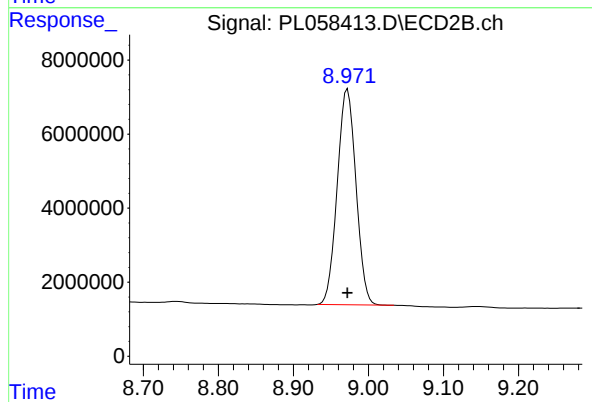

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 101218375
Conc: 50.00 ng/ml