

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042821\
 Data File : PL066518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2021 09:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 03:56:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	4.153	78103640	69052700	20.728	19.662
28)	SA Decachlor...	8.168	9.353	66188818	50930683	17.263	16.463
Target Compounds							
2)	A alpha-BHC	3.851	0.000	4759600	0	0.765	N.D. #
6)	B beta-BHC	0.000	5.032	0	9235342	N.D.	0.935 #
10)	B gamma-Chl...	0.000	6.310	0	1096419	N.D.	0.263 #
14)	MA Endrin	5.960	0.000	834551	0	0.192	N.D. #
15)	B Endosulfa...	6.224	0.000	5235667	0	1.269	N.D. #
17)	MA 4,4'-DDT	0.000	7.338	0	8767273	N.D.	2.709 #
21)	B Endrin ke...	0.000	7.969	0	5596119	N.D.	1.577 #
23)	Chlordane-1	4.314f	0.000	3548587	0	20.993	N.D. #
25)	Chlordane-3	0.000	6.310	0	1096419	N.D.	1.956 #
27)	Chlordane-5	6.224	0.000	5235667	0	31.091	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042821\
Data File : PL066518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2021 09:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 03:56:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

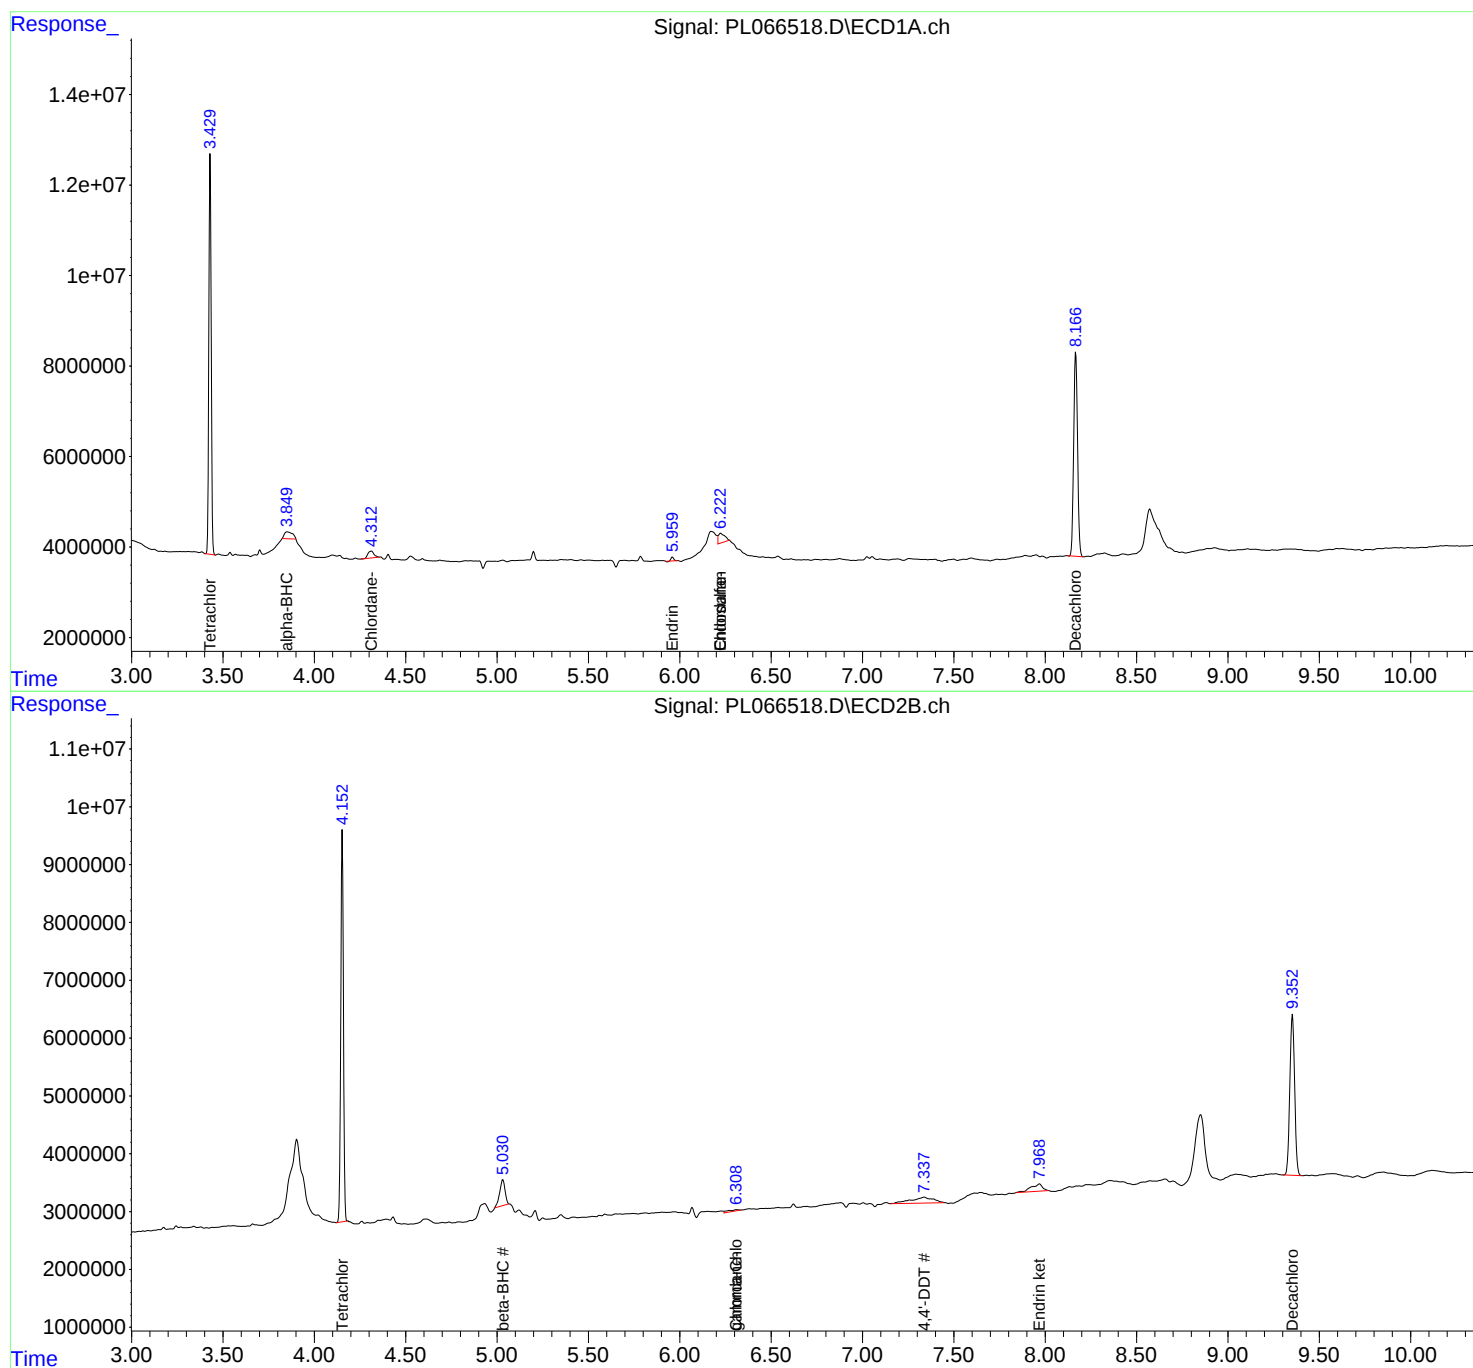


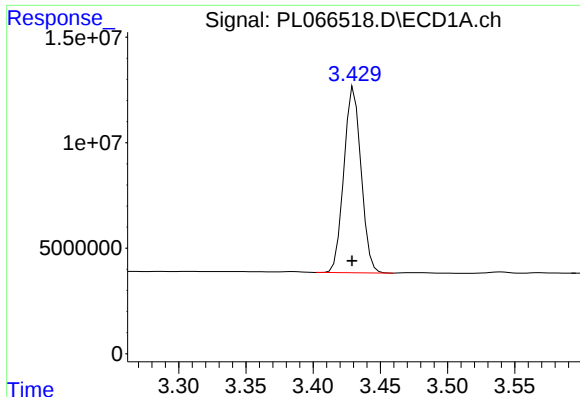

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.001 min
Response: 78103640
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

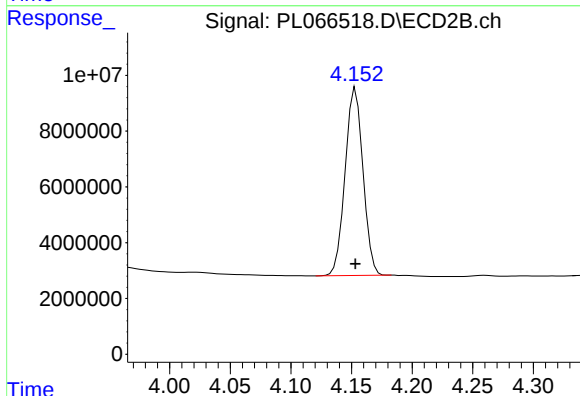


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 69052700
Conc: 19.66 ng/ml

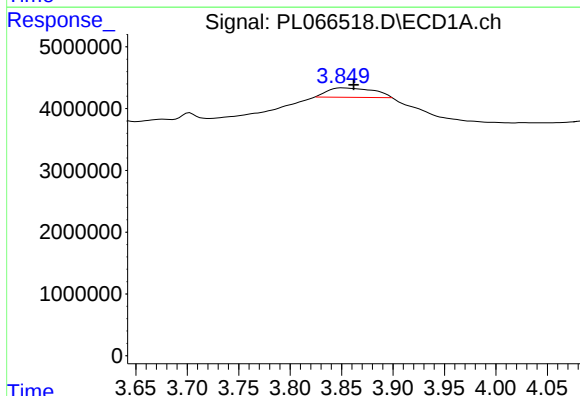


#2 alpha-BHC

R.T.: 3.851 min
Delta R.T.: -0.011 min
Response: 4759600
Conc: 0.76 ng/ml

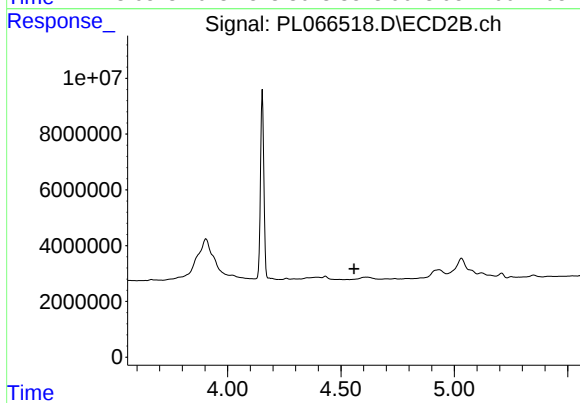

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

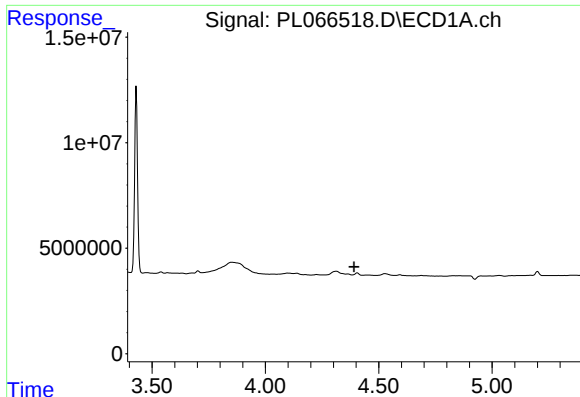

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

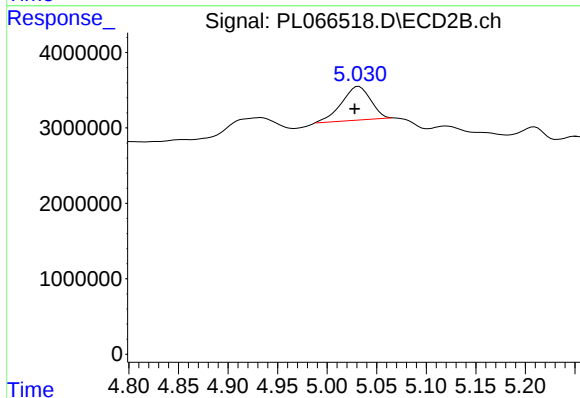


#6 beta-BHC

R.T.: 5.032 min
Delta R.T.: 0.004 min
Response: 9235342
Conc: 0.94 ng/ml

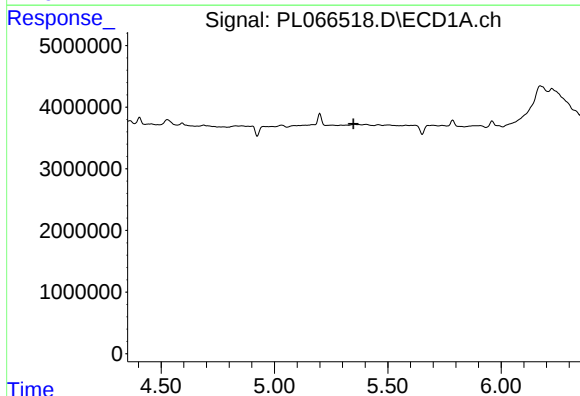


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

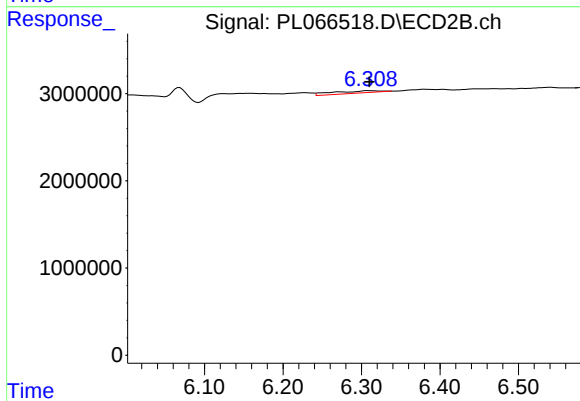

#10 gamma-Chlordane


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 1096419
Conc: 0.26 ng/ml

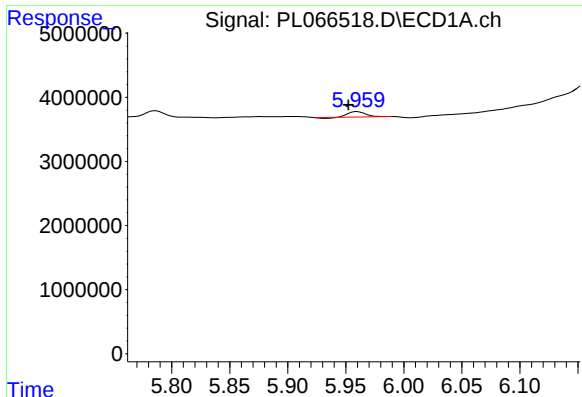

#14 Endrin


R.T.: 5.960 min
Delta R.T.: 0.008 min
Response: 834551
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

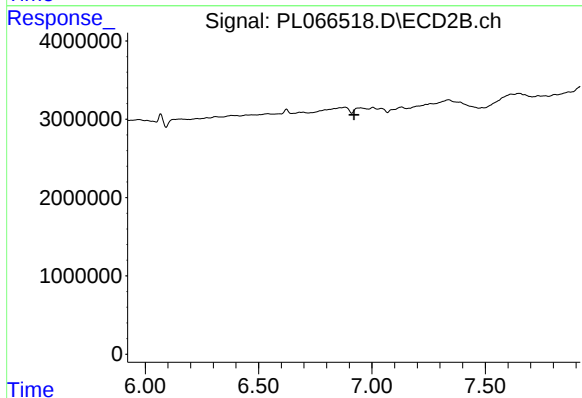


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

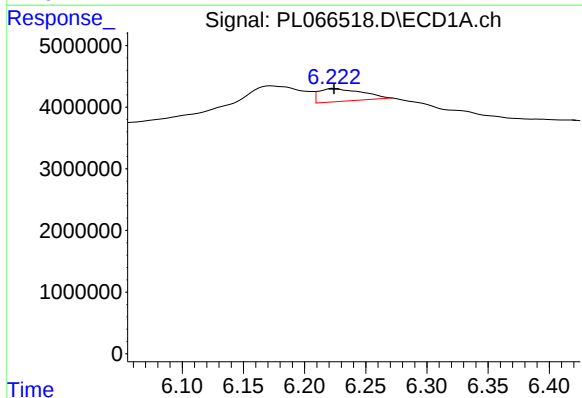


#15 Endosulfan II

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 5235667
Conc: 1.27 ng/ml

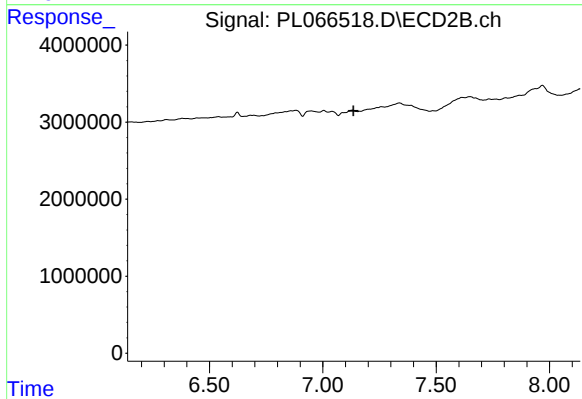

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

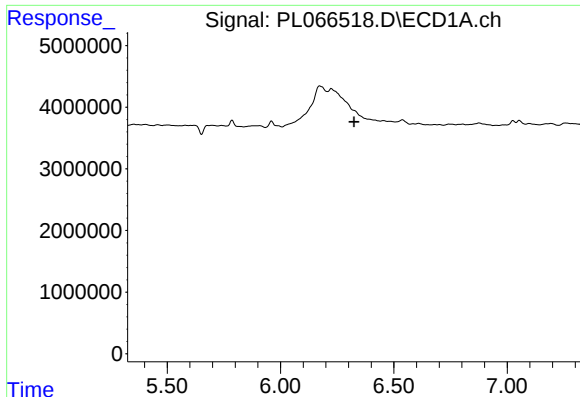

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.325 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

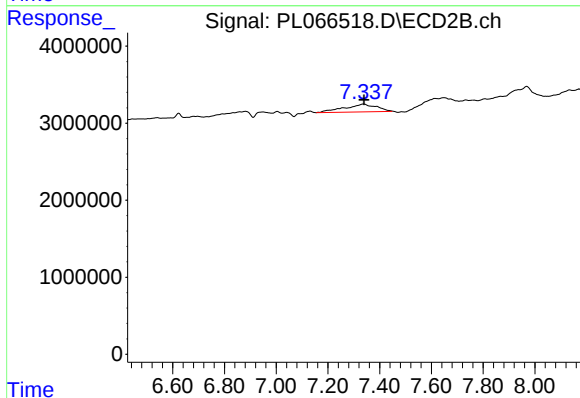


#17 4,4'-DDT

R.T.: 7.338 min
Delta R.T.: -0.001 min
Response: 8767273
Conc: 2.71 ng/ml

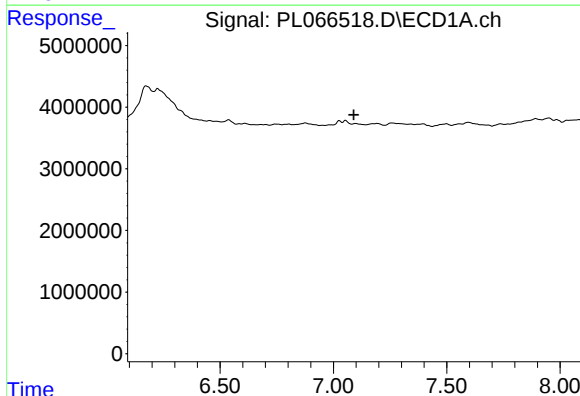


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

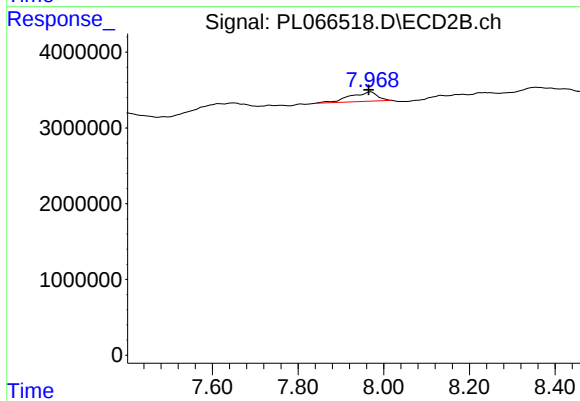

#21 Endrin ketone


R.T.: 7.969 min
Delta R.T.: 0.004 min
Response: 5596119
Conc: 1.58 ng/ml

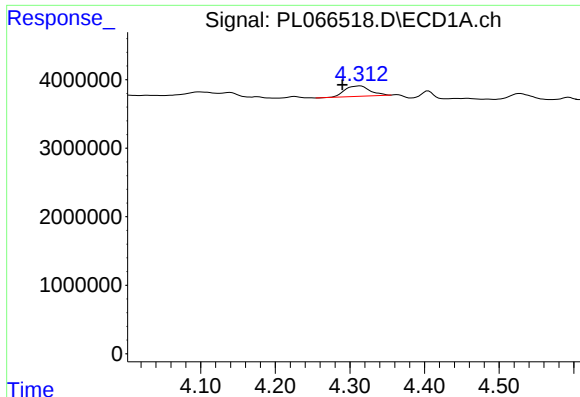

#23 Chlordane-1


R.T.: 4.314 min
Delta R.T.: 0.024 min
Response: 3548587
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

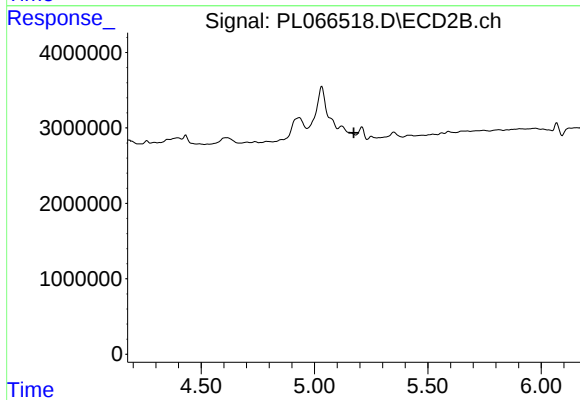


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

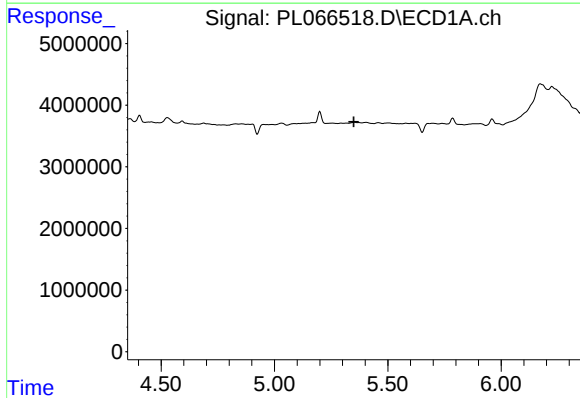


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

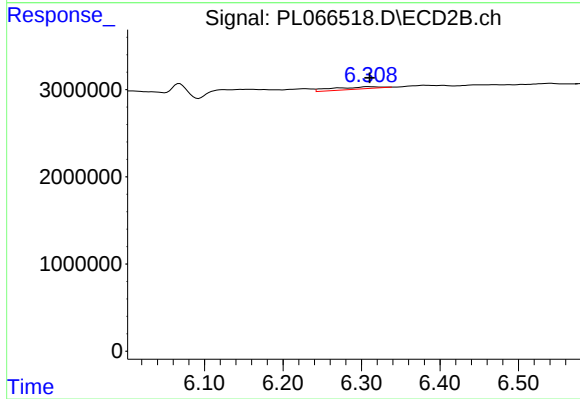

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 1096419
Conc: 1.96 ng/ml

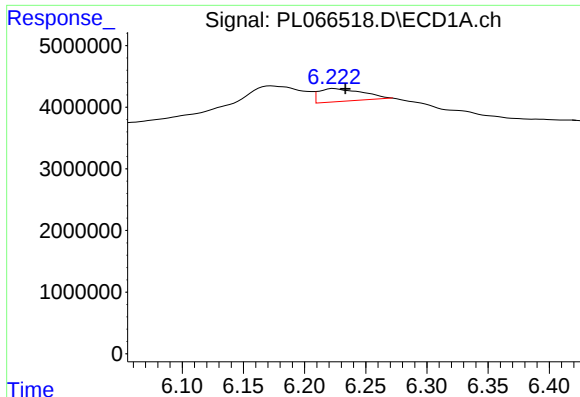

#27 Chlordane-5


R.T.: 6.224 min
Delta R.T.: -0.009 min
Response: 5235667
Conc: 31.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

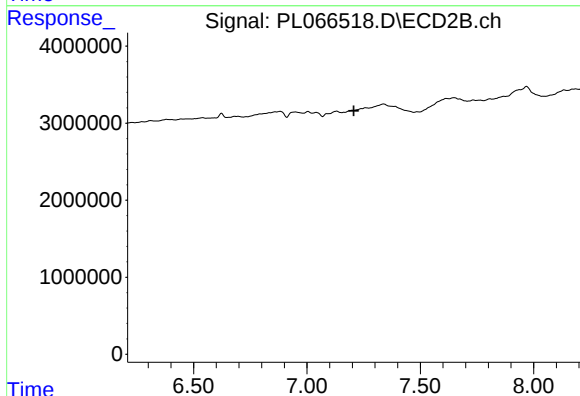


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

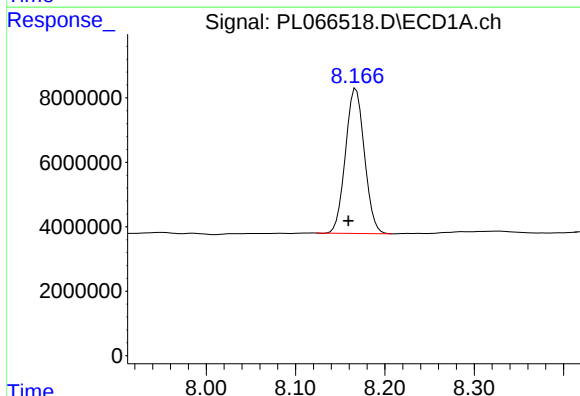

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.009 min
Response: 66188818
Conc: 17.26 ng/ml

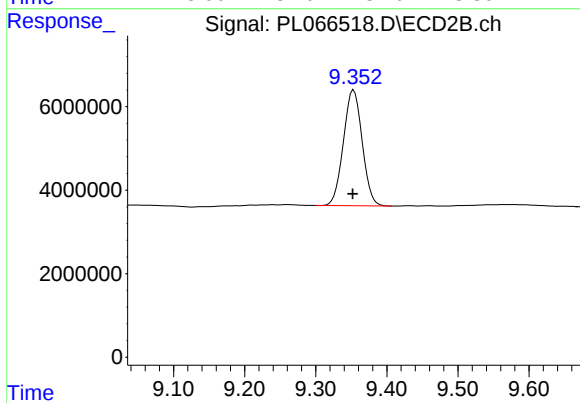

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.002 min
Response: 50930683
Conc: 16.46 ng/ml