

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042821\
 Data File : PL066544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2021 17:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 04:05:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	77036652	72397048	20.445	20.614
28)	SA Decachlor...	8.166	9.354	64408185	54900186	16.798	17.746
Target Compounds							
2)	A alpha-BHC	3.854	0.000	3941106	0	0.633	N.D. #
6)	B beta-BHC	4.404	5.033	1015001	6510569	0.384	N.D. #
8)	B Heptachlo...	0.000	6.068	0	5228163	N.D.	1.413 #
10)	B gamma-Chl...	0.000	6.310	0	782850	N.D.	0.188 #
13)	MA Dieldrin	5.678f	0.000	3005416	0	0.619	N.D. #
14)	MA Endrin	5.958	0.000	1261260	0	0.290	N.D. #
21)	B Endrin ke...	0.000	7.973	0	1698155	N.D.	0.478 #
25)	Chlordane-3	0.000	6.310	0	782850	N.D.	1.397 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042821\
Data File : PL066544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2021 17:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 04:05:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

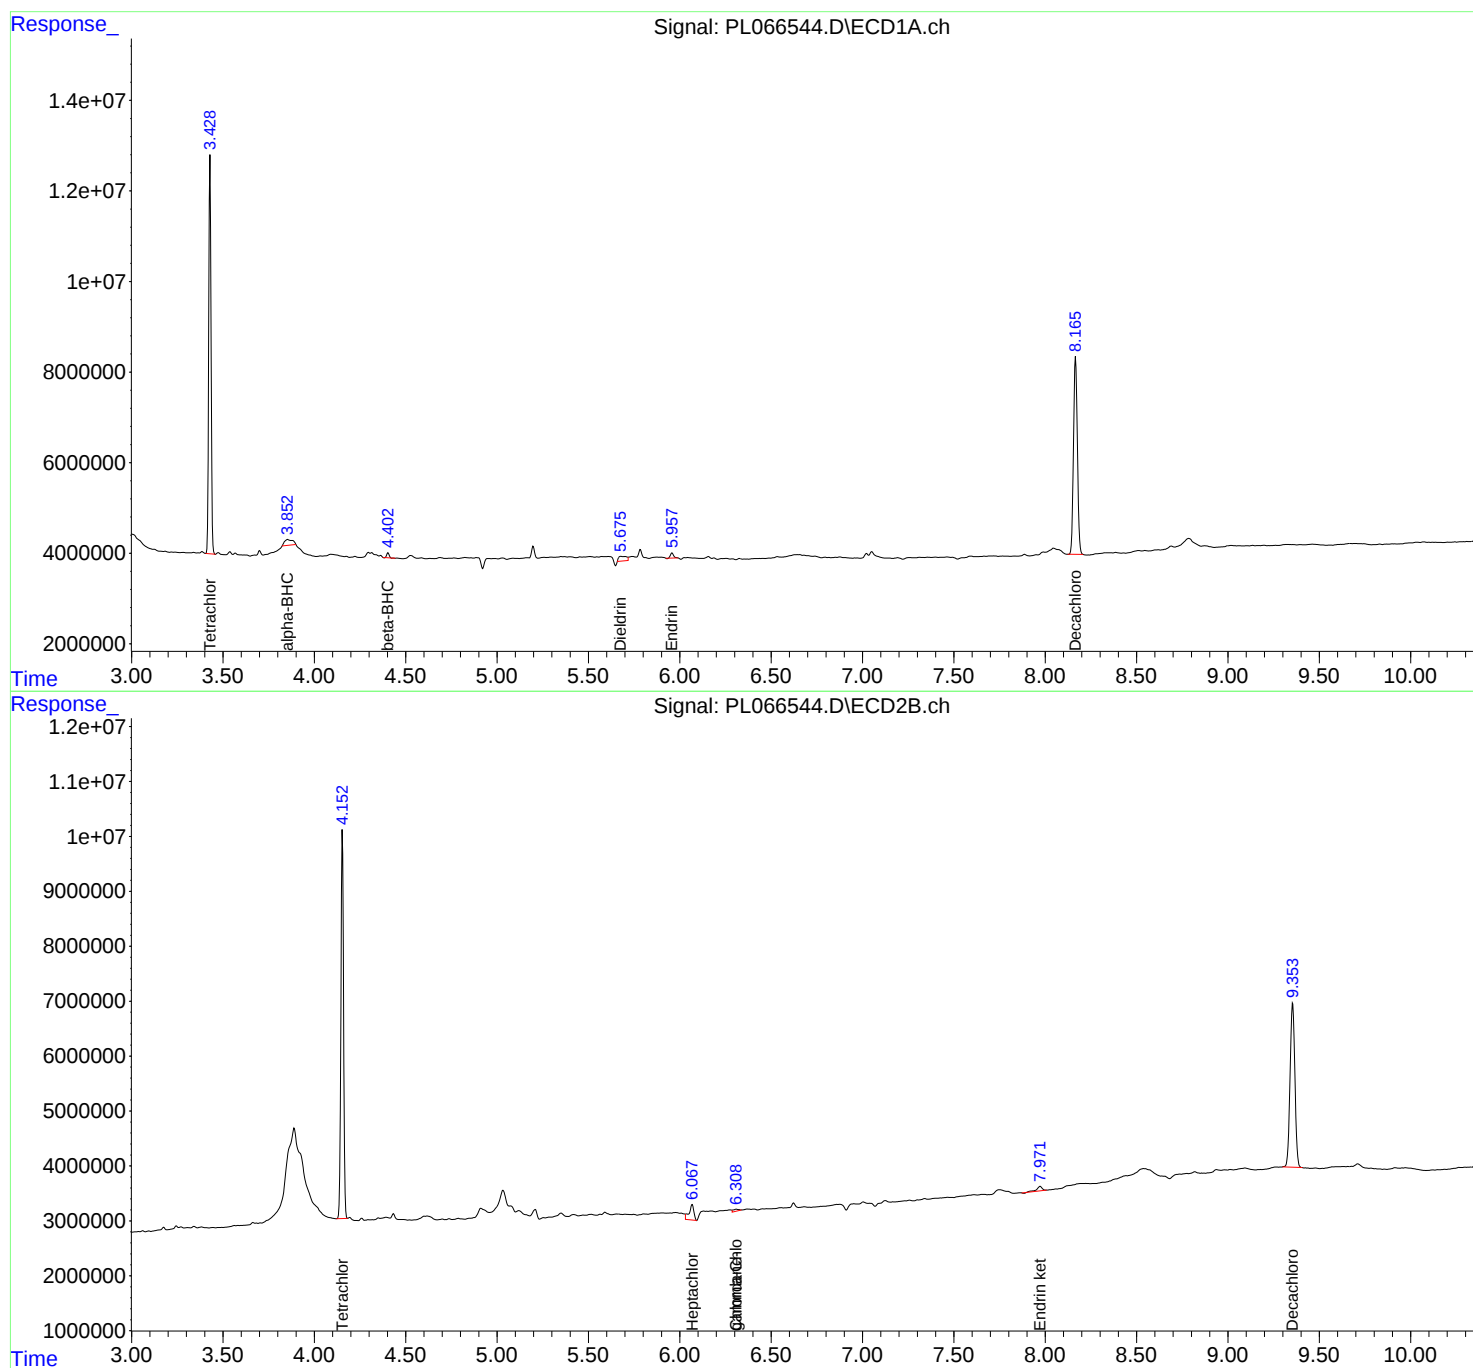


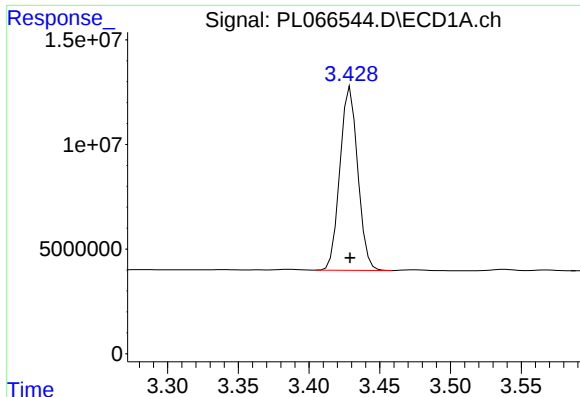

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 77036652
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

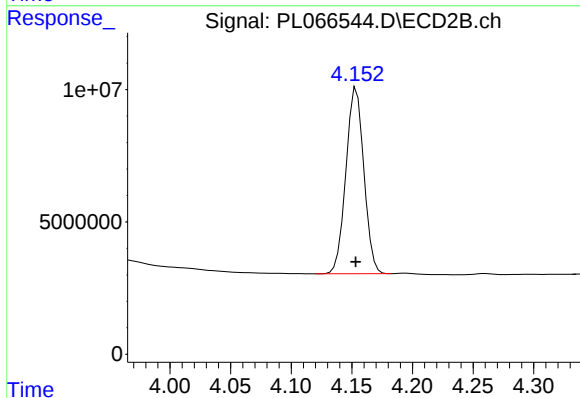


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 72397048
Conc: 20.61 ng/ml

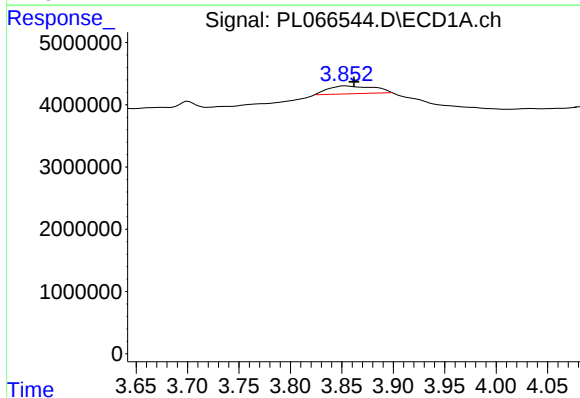


#2 alpha-BHC

R.T.: 3.854 min
Delta R.T.: -0.008 min
Response: 3941106
Conc: 0.63 ng/ml

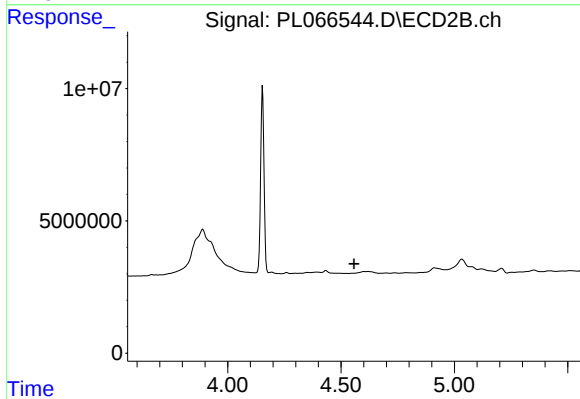

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

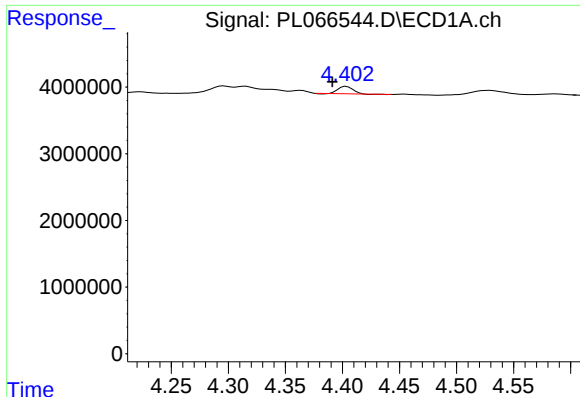

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: 0.012 min
Response: 1015001
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

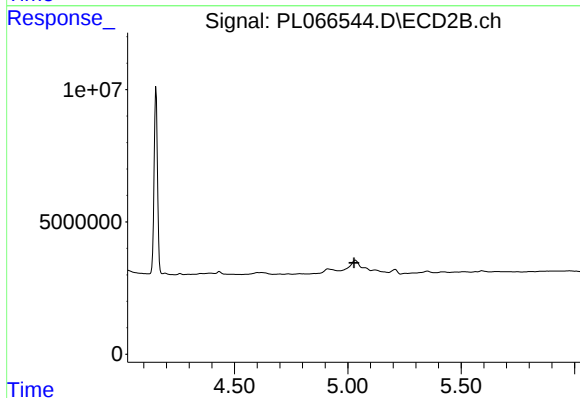


#6 beta-BHC

R.T.: 5.033 min
Delta R.T.: 0.005 min
Response: 6510569
Conc: N.D.

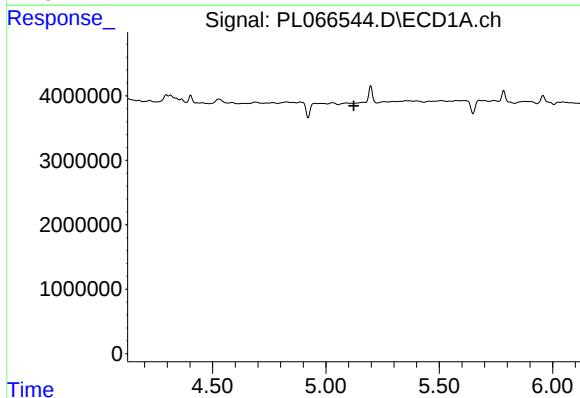


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

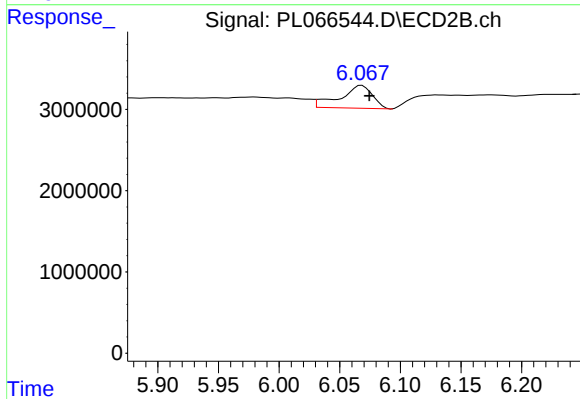

#8 Heptachlor epoxide


R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 5228163
Conc: 1.41 ng/ml

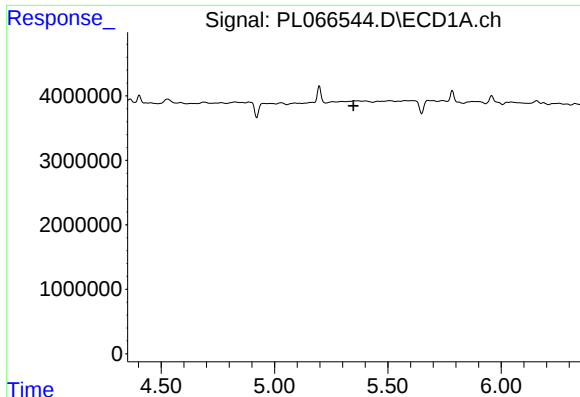

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

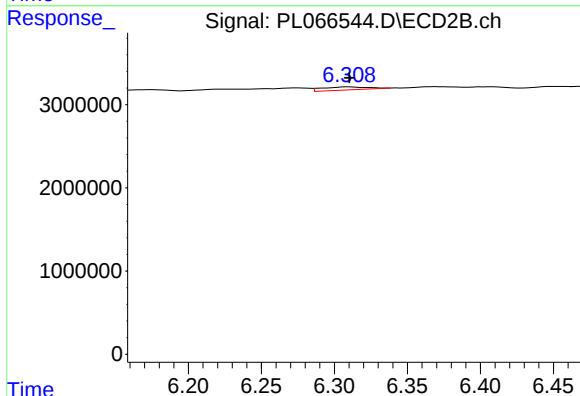


#10 gamma-Chlordane

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 782850
Conc: 0.19 ng/ml

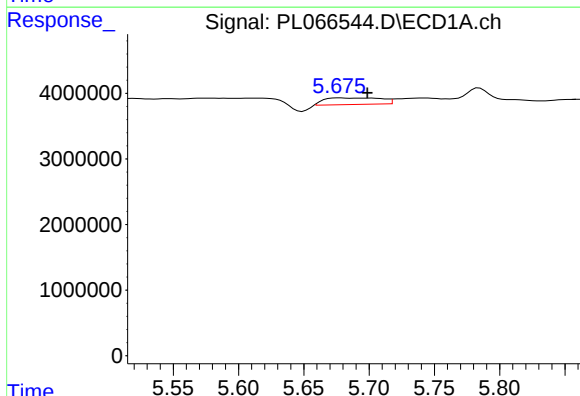


#13 Dieldrin

R.T.: 5.678 min
Delta R.T.: -0.021 min
Response: 3005416
Conc: 0.62 ng/ml

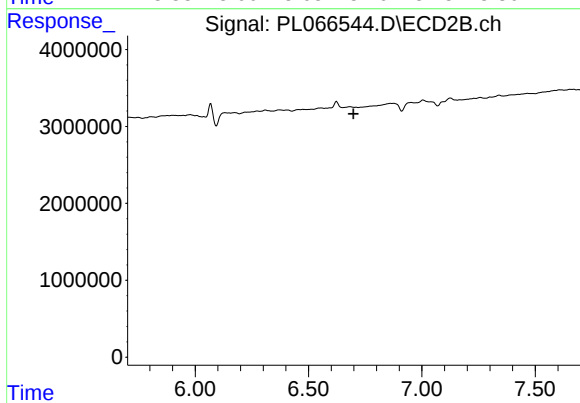

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

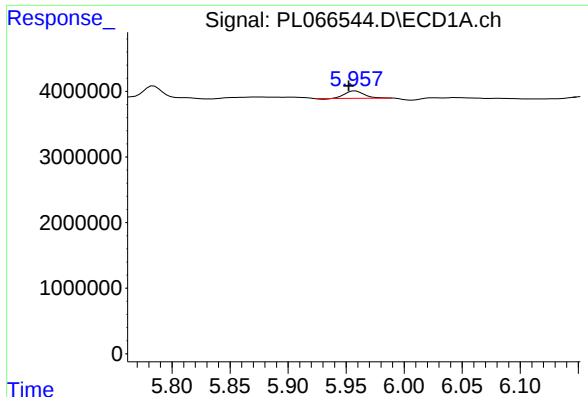

#14 Endrin


R.T.: 5.958 min
Delta R.T.: 0.006 min
Response: 1261260
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

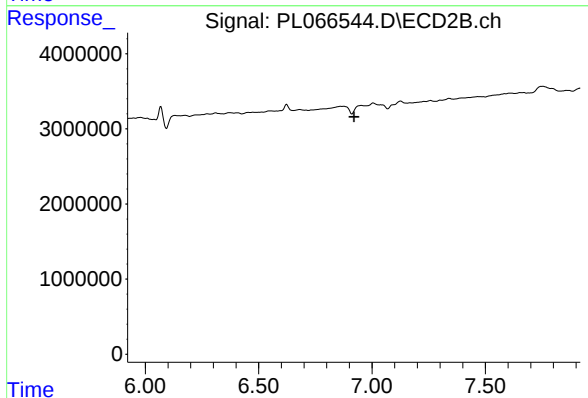


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

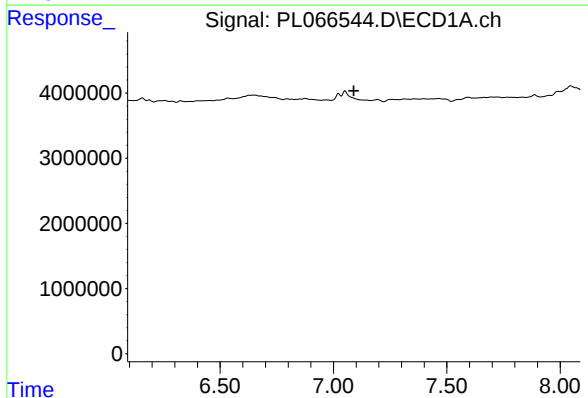


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

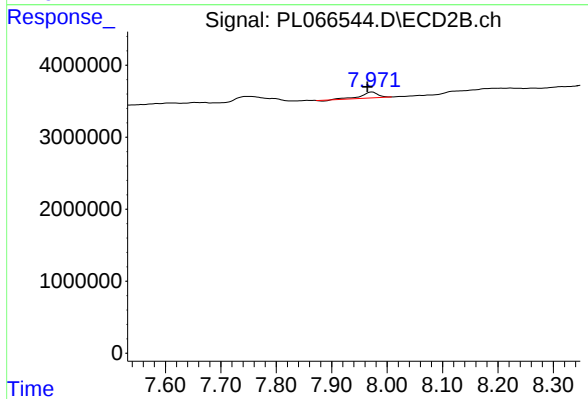

#21 Endrin ketone


R.T.: 7.973 min
Delta R.T.: 0.008 min
Response: 1698155
Conc: 0.48 ng/ml

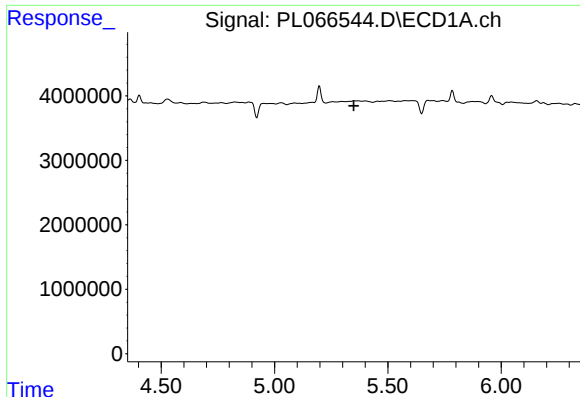

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

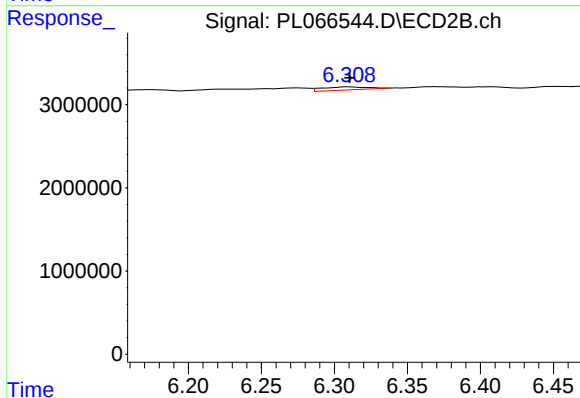


#25 Chlordane-3

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 782850
Conc: 1.40 ng/ml

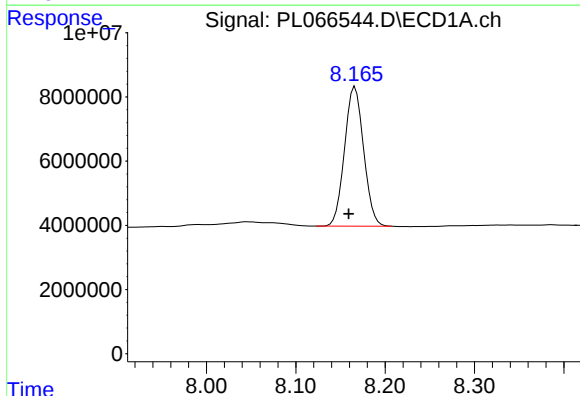

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.007 min
Response: 64408185
Conc: 16.80 ng/ml

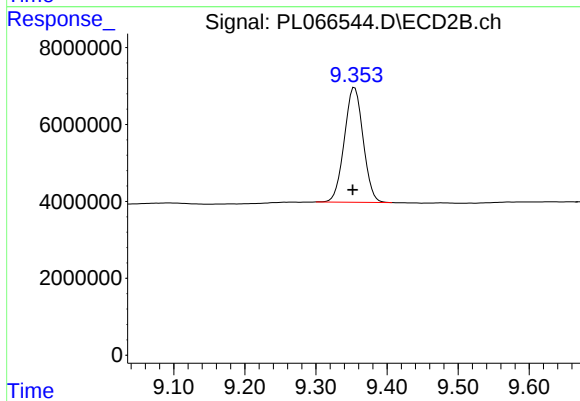

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.003 min
Response: 54900186
Conc: 17.75 ng/ml