

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042822\
 Data File : PL074427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2022 15:13
 Operator : AR\AJ
 Sample : N2588-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 05:54:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.485	3668447	17796971	11.354	9.982
28)	SA Decachlor...	10.413	11.336	7154222	23839709	13.757	13.497
Target Compounds							
7)	B delta-BHC	0.000	6.955	0	594612	N.D.	0.243 #
11)	B alpha-Chl...	0.000	8.252f	0	34260	N.D.	0.016 #
12)	B 4,4'-DDE	0.000	8.473	0	71058	N.D.	0.036 #
14)	MA Endrin	8.091f	0.000	71098	0	0.175	N.D. #
16)	A 4,4'-DDD	0.000	9.004	0	31025	N.D.	0.020 #
17)	MA 4,4'-DDT	0.000	9.291f	0	106542	N.D.	0.060 #
20)	A Methoxychlor	0.000	9.777	0	228765	N.D.	0.238 #
21)	B Endrin ke...	0.000	9.923	0	169760	N.D.	0.098 #
27)	Chlordane-5	0.000	9.174f	0	22865	N.D.	0.380 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042822\
Data File : PL074427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2022 15:13
Operator : AR\AJ
Sample : N2588-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 05:54:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

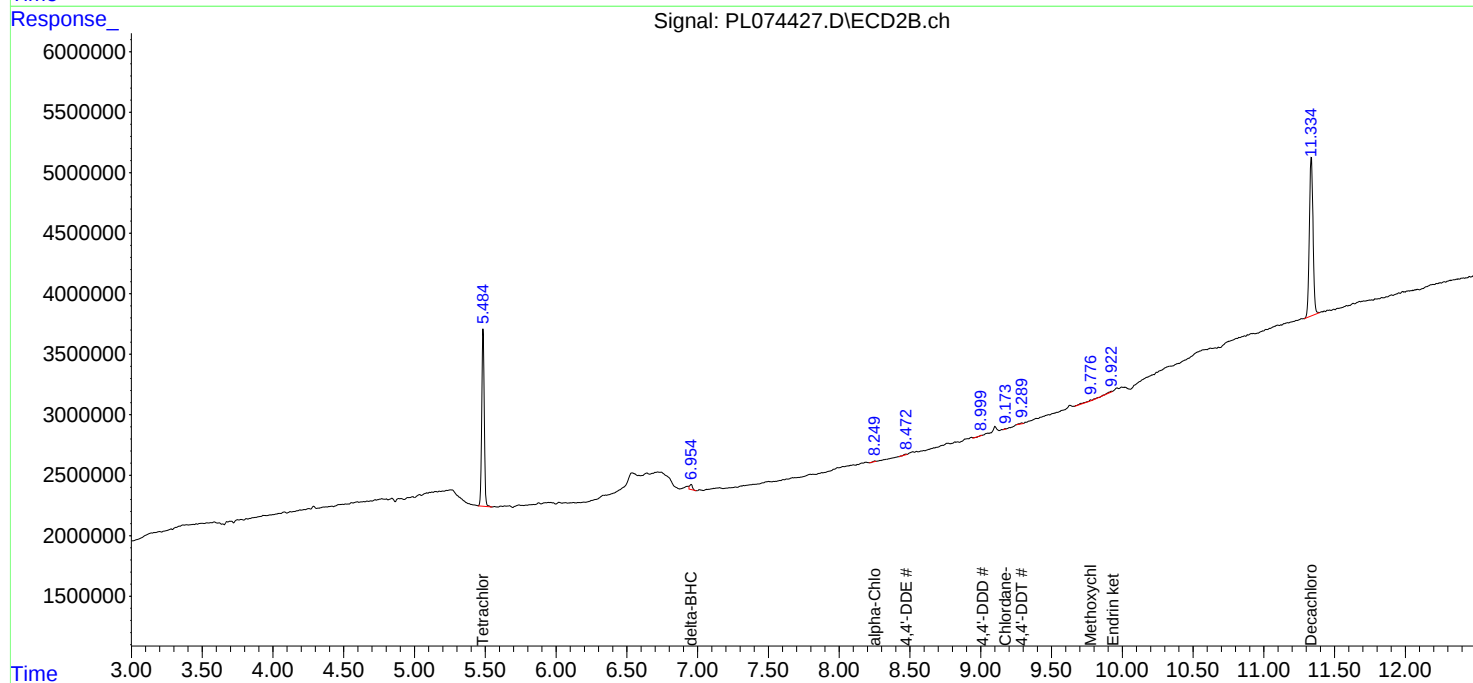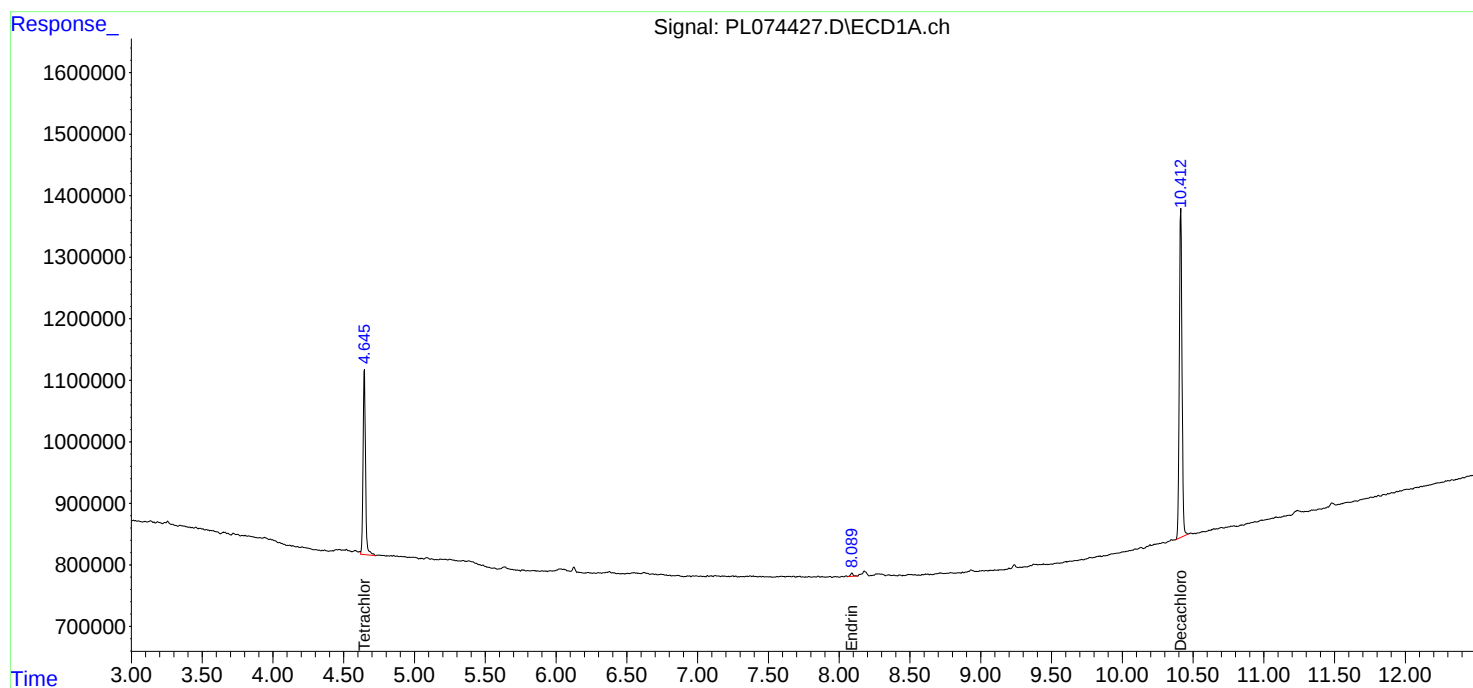


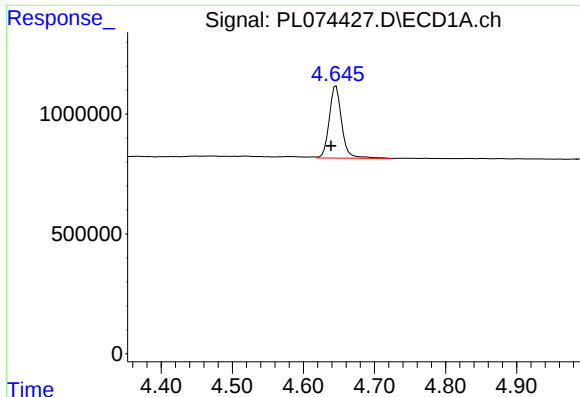

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.007 min
Response: 3668447
Conc: 11.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

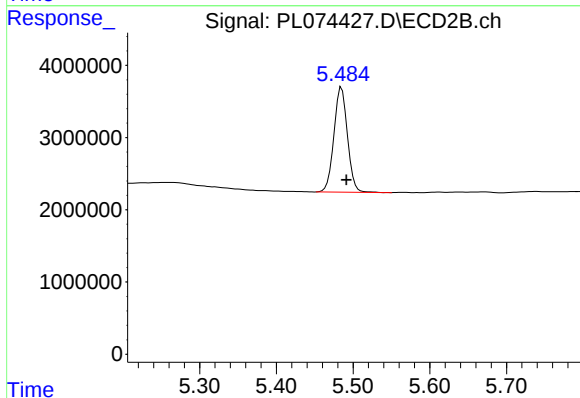


#1 Tetrachloro-m-xylene

R.T.: 5.485 min
Delta R.T.: -0.006 min
Response: 17796971
Conc: 9.98 ng/ml

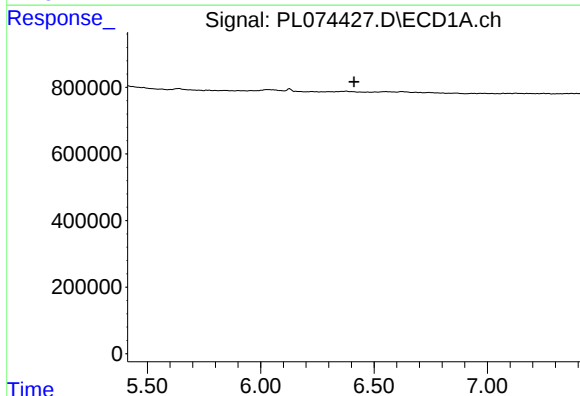


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

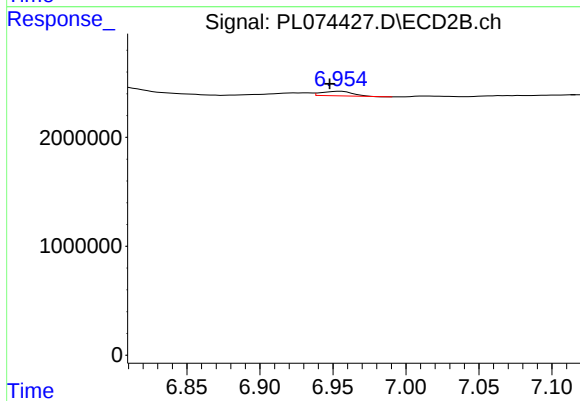

#7 delta-BHC


R.T.: 6.955 min
Delta R.T.: 0.007 min
Response: 594612
Conc: 0.24 ng/ml

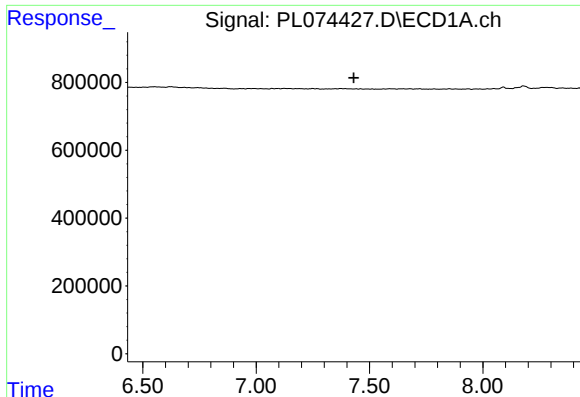

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

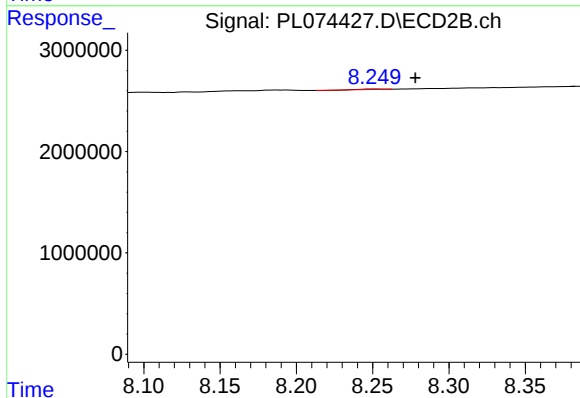


#11 alpha-Chlordane

R.T.: 8.252 min
Delta R.T.: -0.026 min
Response: 34260
Conc: 0.02 ng/ml

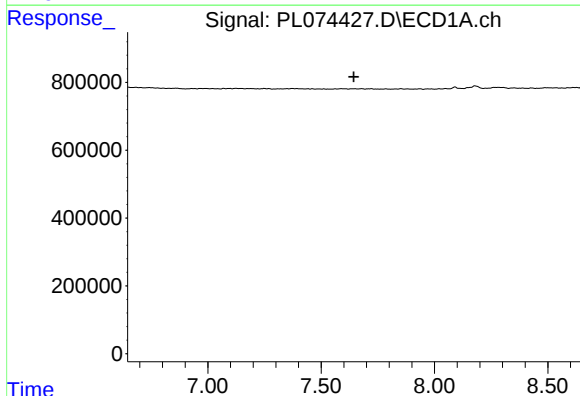


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

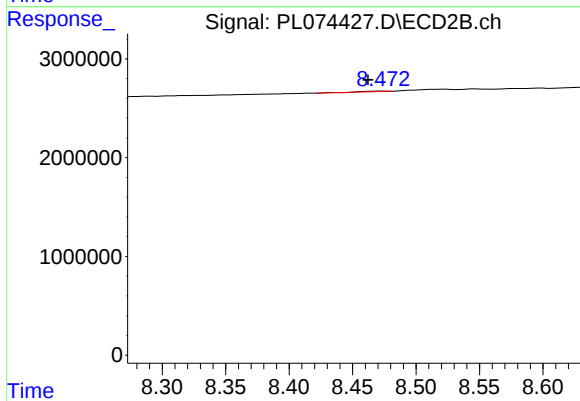

#12 4,4'-DDE


R.T.: 8.473 min
Delta R.T.: 0.011 min
Response: 71058
Conc: 0.04 ng/ml

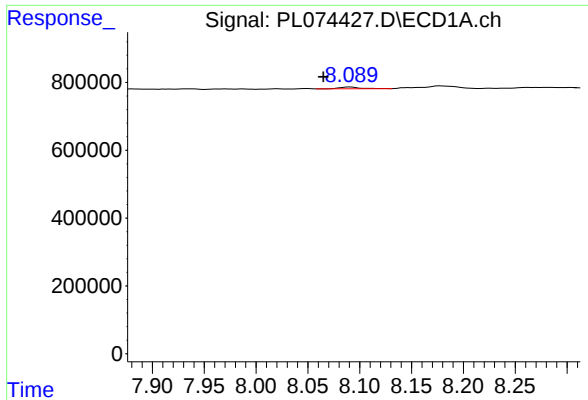

#14 Endrin


R.T.: 8.091 min
Delta R.T.: 0.026 min
Response: 71098
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

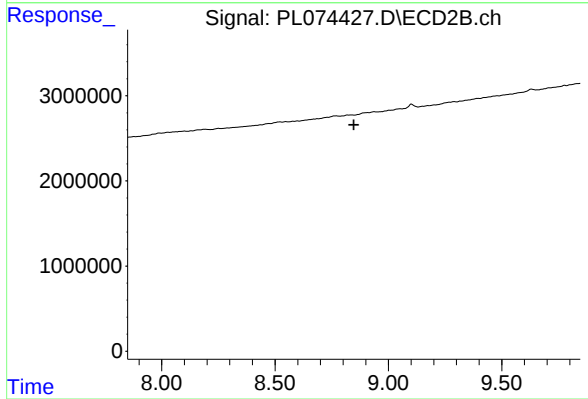


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.847 min
Response: 0
Conc: N.D.

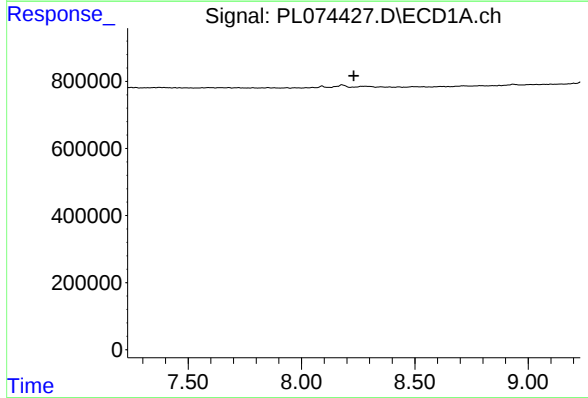




#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 8.231 min
Response: 0
Conc: N.D.

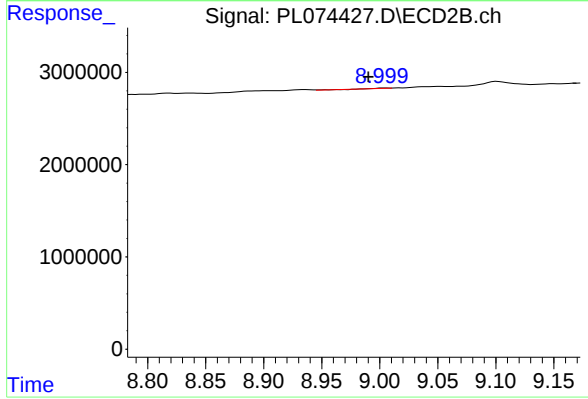

#16 4,4'-DDD

R.T.: 9.004 min
Delta R.T.: 0.014 min
Response: 31025
Conc: 0.02 ng/ml




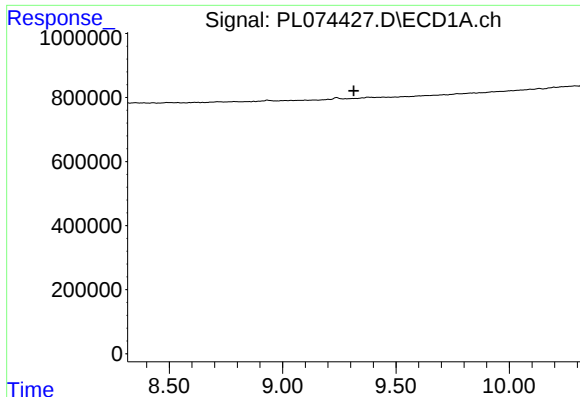

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

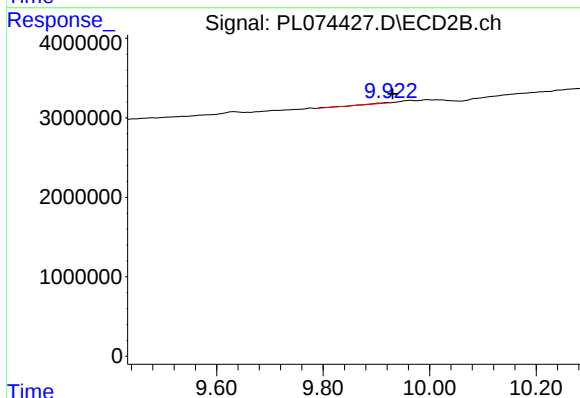


#21 Endrin ketone

R.T.: 9.923 min
Delta R.T.: -0.008 min
Response: 169760
Conc: 0.10 ng/ml

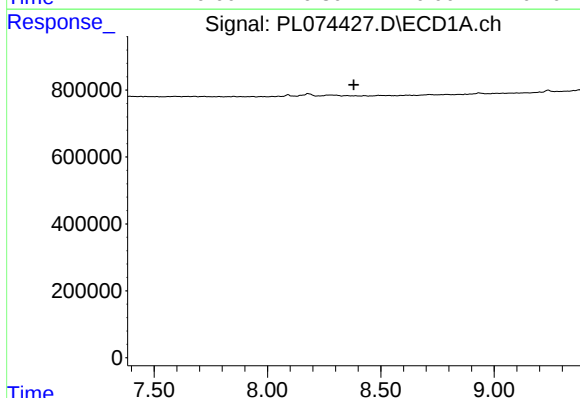


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.381 min
Response: 0
Conc: N.D.

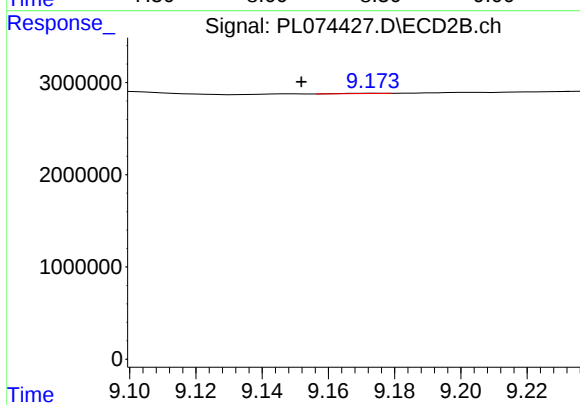

#27 Chlordane-5


R.T.: 9.174 min
Delta R.T.: 0.022 min
Response: 22865
Conc: 0.38 ng/ml

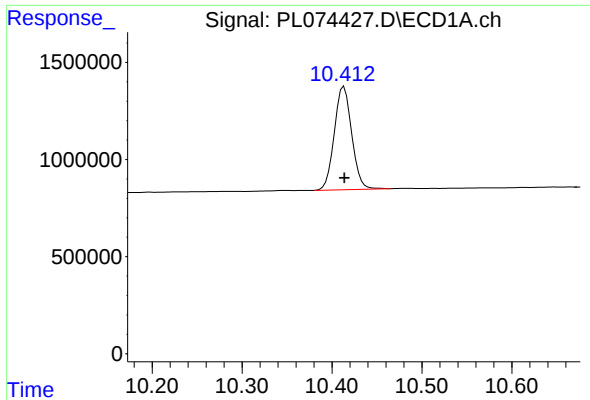

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: 0.000 min
Response: 7154222
Conc: 13.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

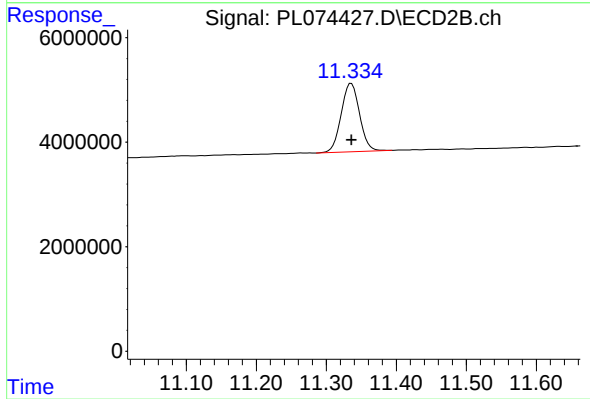

#28 Decachlorobiphenyl

R.T.: 11.336 min
Delta R.T.: 0.000 min
Response: 23839709
Conc: 13.50 ng/ml