

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042822\
 Data File : PL074436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2022 04:37
 Operator : AR\AJ
 Sample : N2600-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 05:57:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.486	8022886	41249044	24.830	23.135
28)	SA Decachlor...	10.412	11.334	13048265	42913410	25.091	24.296
Target Compounds							
5)	MB Aldrin	0.000	7.486	0	326150	N.D.	0.139 #
7)	B delta-BHC	0.000	6.956	0	289481	N.D.	0.119 #
9)	A Endosulfan I	0.000	8.354f	0	76949	N.D.	0.039 #
10)	B gamma-Chl...	0.000	8.190	0	142842	N.D.	0.064 #
11)	B alpha-Chl...	0.000	8.289	0	24244	N.D.	0.011 #
12)	B 4,4'-DDE	0.000	8.447f	0	27048	N.D.	0.014 #
15)	B Endosulfa...	0.000	9.051f	0	290486	N.D.	0.167 #
17)	MA 4,4'-DDT	8.509f	0.000	102213	0	0.277	N.D. #
25)	Chlordane-3	0.000	8.190	0	142842	N.D.	0.422 #
26)	Chlordane-4	0.000	8.289	0	24244	N.D.	0.061 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042822\
Data File : PL074436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2022 04:37
Operator : AR\AJ
Sample : N2600-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 05:57:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

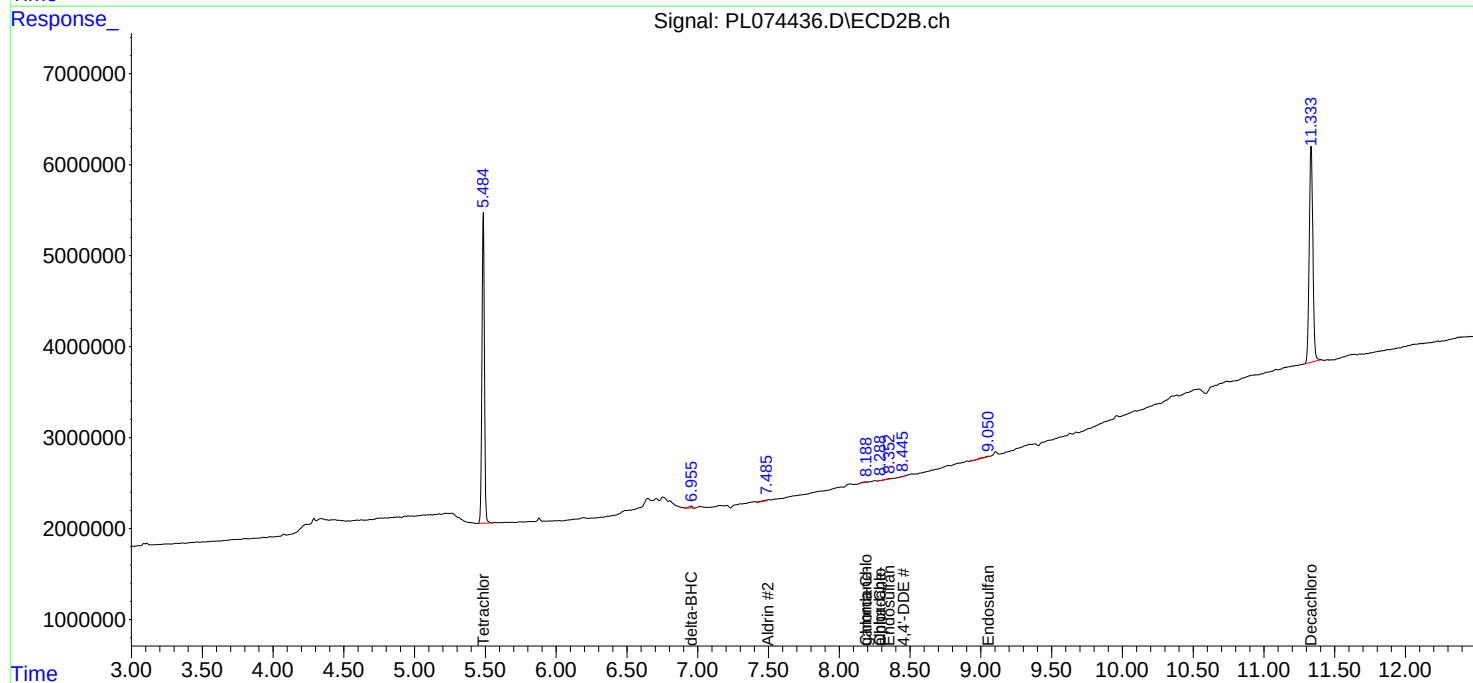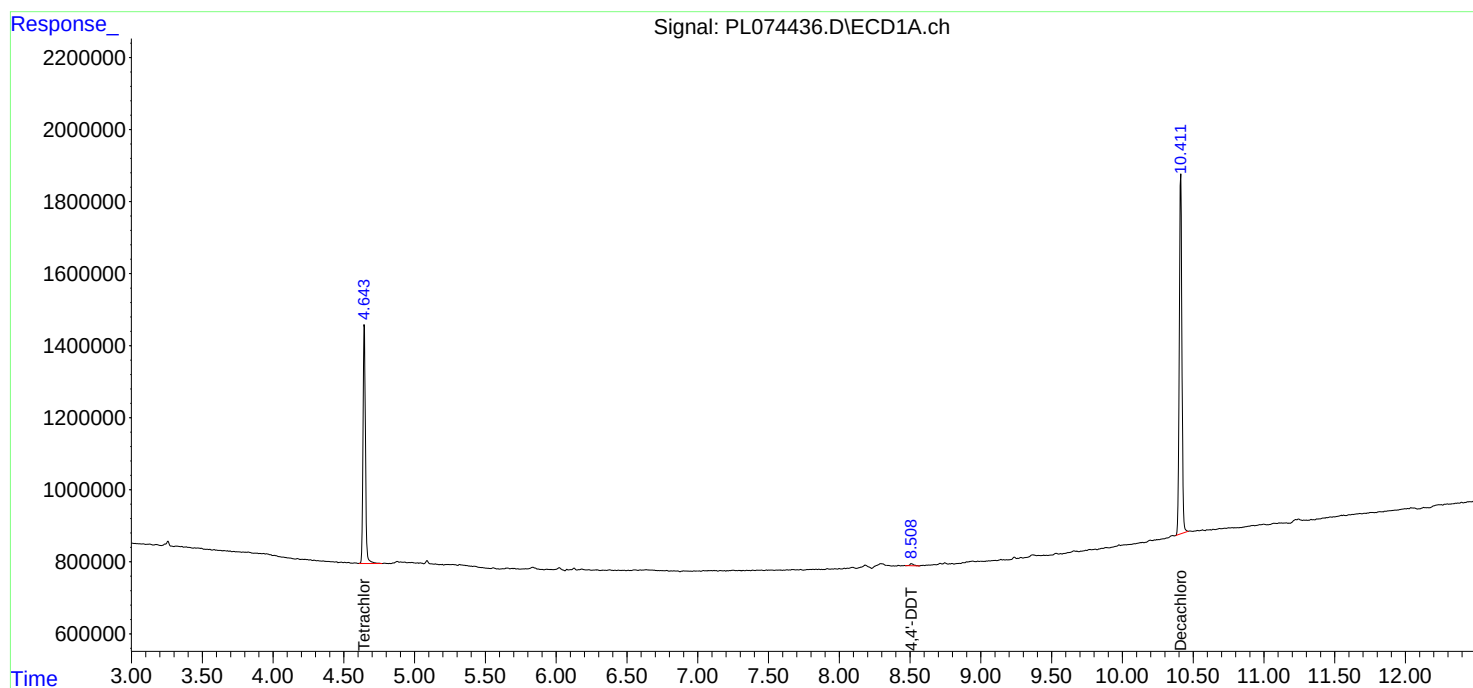


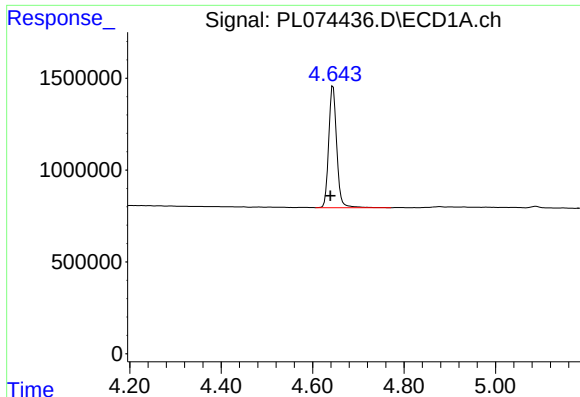

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.006 min
Response: 8022886
Conc: 24.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

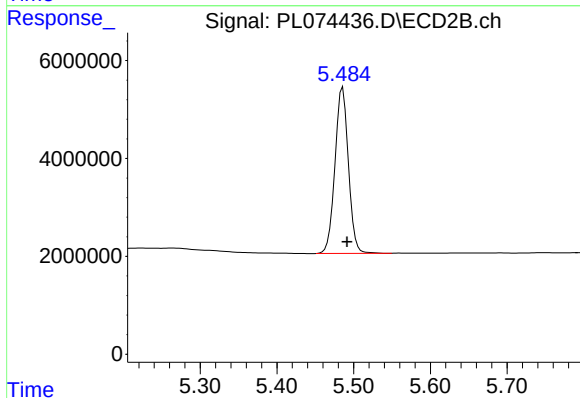


#1 Tetrachloro-m-xylene

R.T.: 5.486 min
Delta R.T.: -0.006 min
Response: 41249044
Conc: 23.14 ng/ml

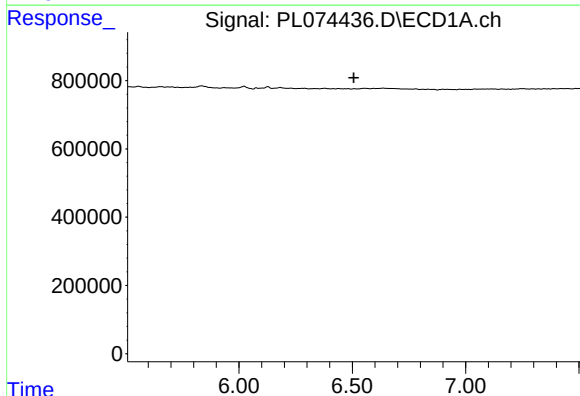


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

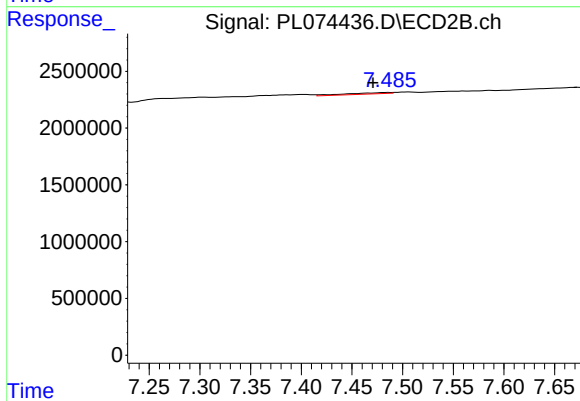

#5 Aldrin


R.T.: 7.486 min
Delta R.T.: 0.015 min
Response: 326150
Conc: 0.14 ng/ml

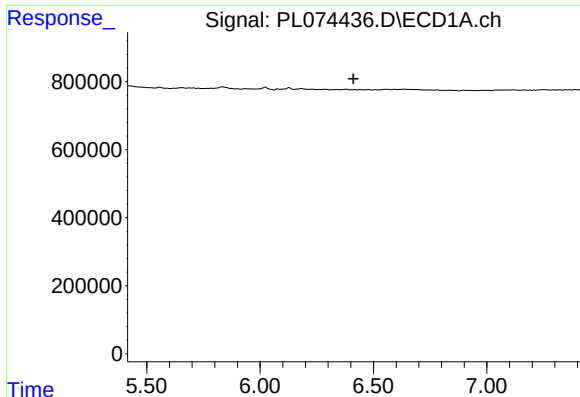

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

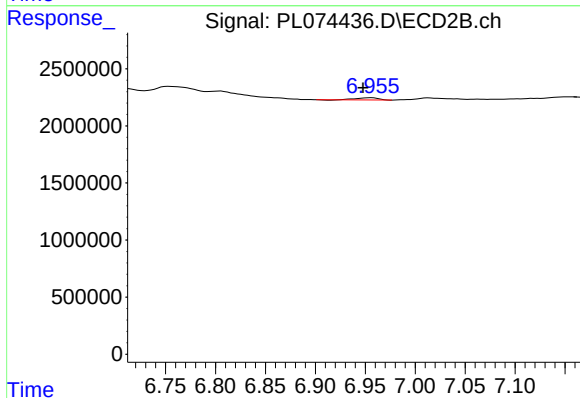


#7 delta-BHC

R.T.: 6.956 min
Delta R.T.: 0.008 min
Response: 289481
Conc: 0.12 ng/ml

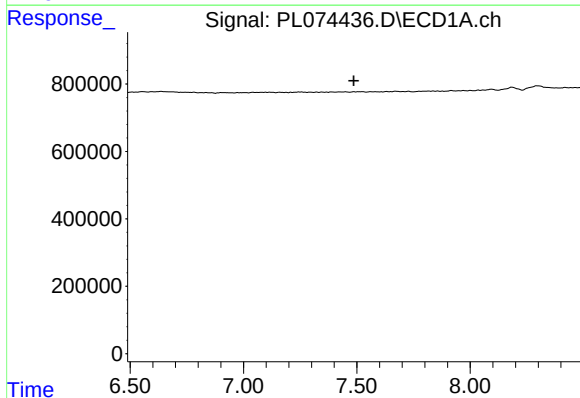


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

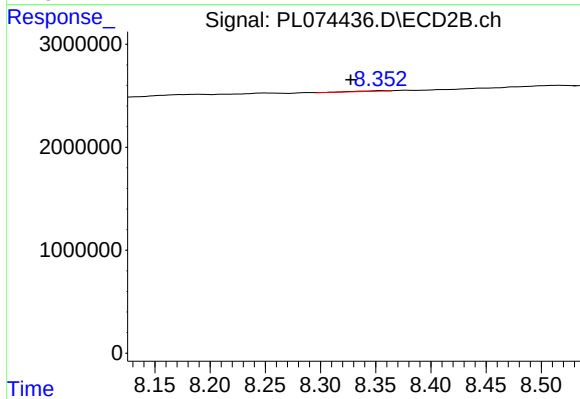

#9 Endosulfan I


R.T.: 8.354 min
Delta R.T.: 0.027 min
Response: 76949
Conc: 0.04 ng/ml

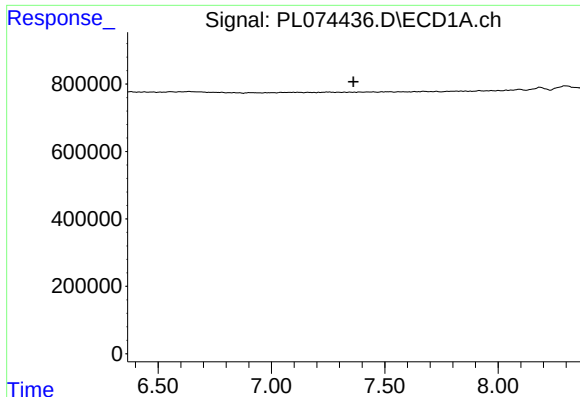

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

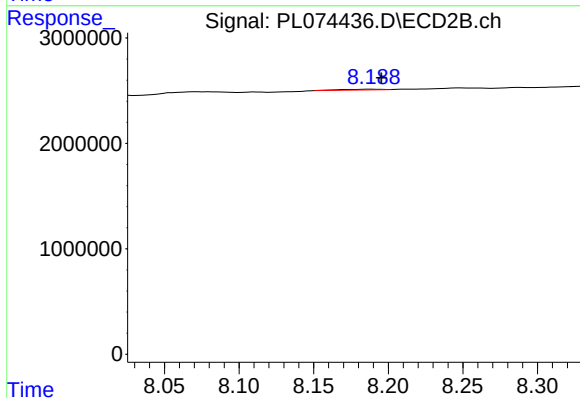


#10 gamma-Chlordane

R.T.: 8.190 min
Delta R.T.: -0.006 min
Response: 142842
Conc: 0.06 ng/ml

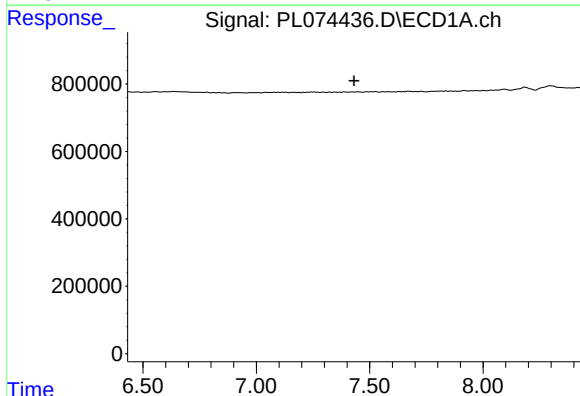


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

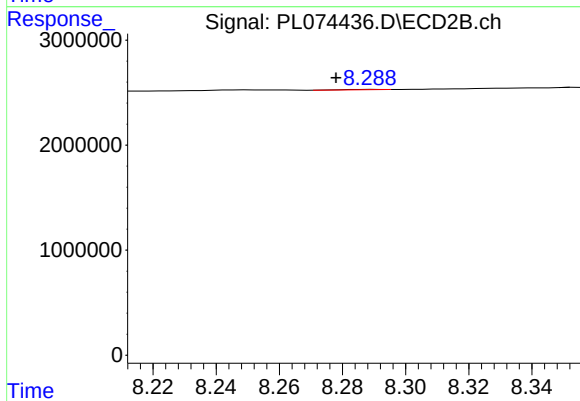

#11 alpha-Chlordane


R.T.: 8.289 min
Delta R.T.: 0.011 min
Response: 24244
Conc: 0.01 ng/ml

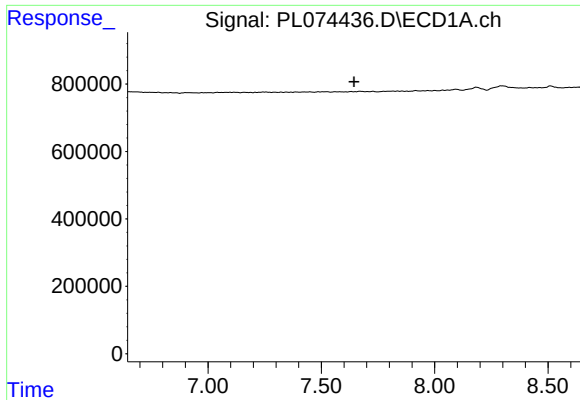

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

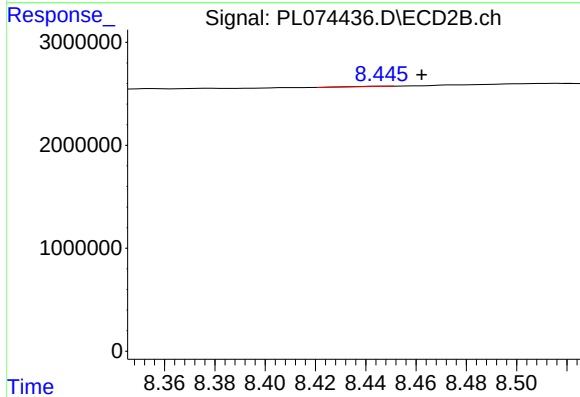


#12 4,4'-DDE

R.T.: 8.447 min
Delta R.T.: -0.016 min
Response: 27048
Conc: 0.01 ng/ml

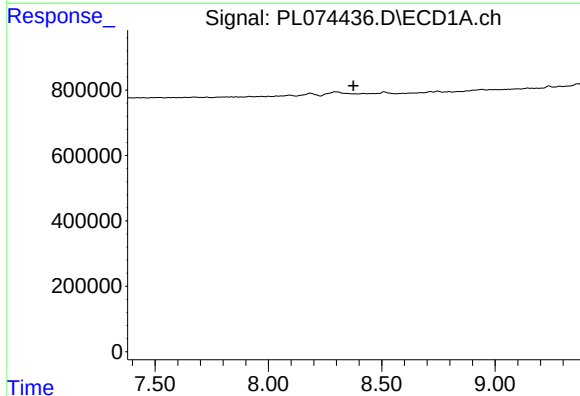


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

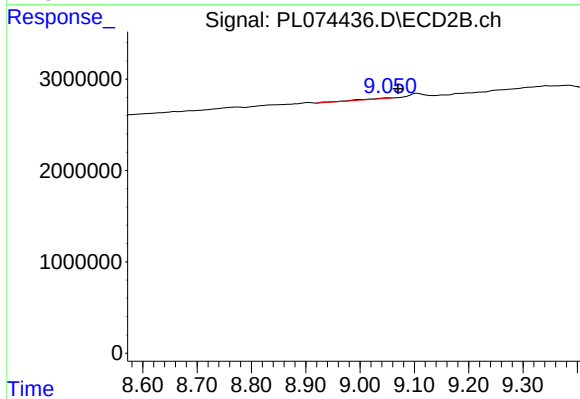

#15 Endosulfan II


R.T.: 9.051 min
Delta R.T.: -0.019 min
Response: 290486
Conc: 0.17 ng/ml

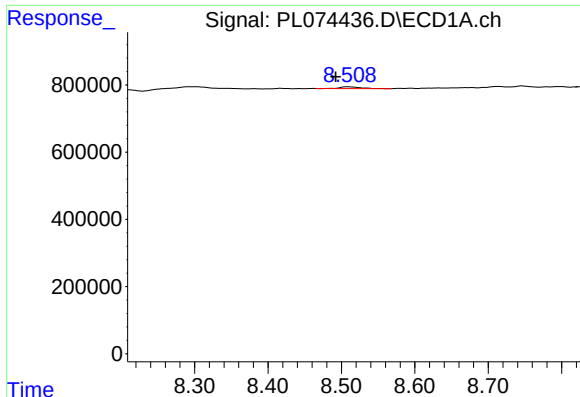

#17 4,4'-DDT


R.T.: 8.509 min
Delta R.T.: 0.017 min
Response: 102213
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

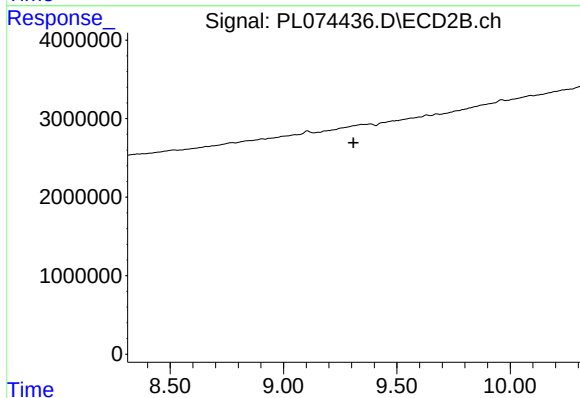


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.309 min
Response: 0
Conc: N.D.

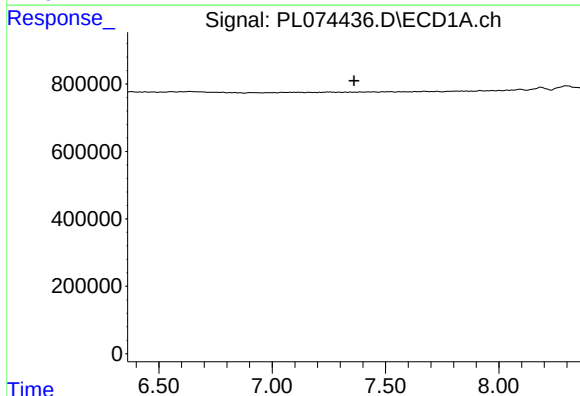


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

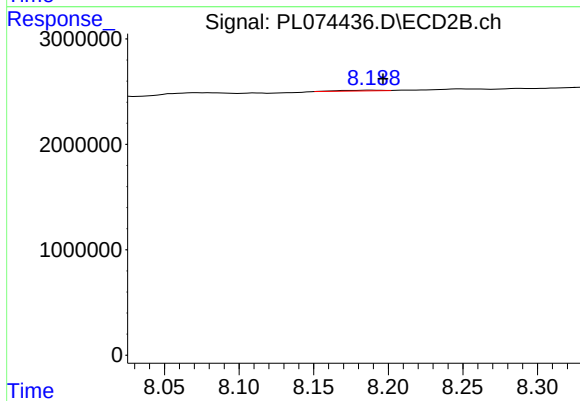

#25 Chlordane-3


R.T.: 8.190 min
Delta R.T.: -0.007 min
Response: 142842
Conc: 0.42 ng/ml

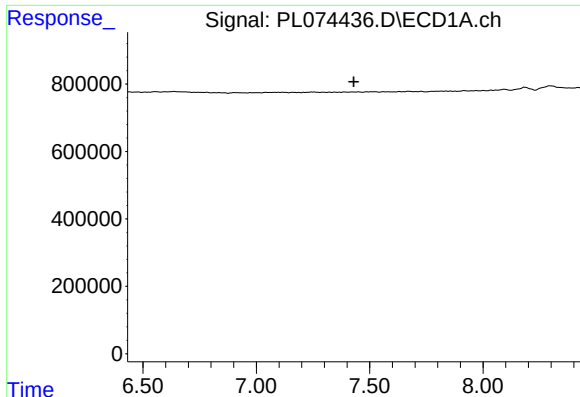

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

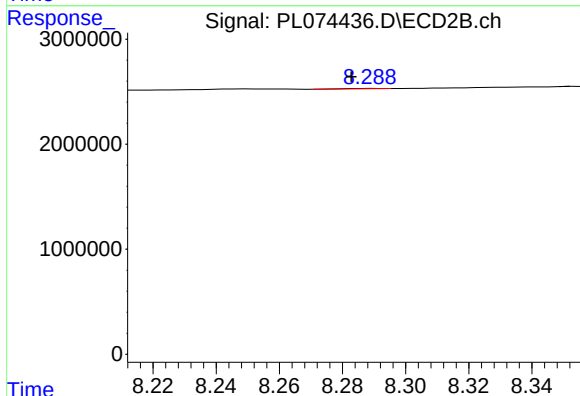


#26 Chlordane-4

R.T.: 8.289 min
Delta R.T.: 0.006 min
Response: 24244
Conc: 0.06 ng/ml

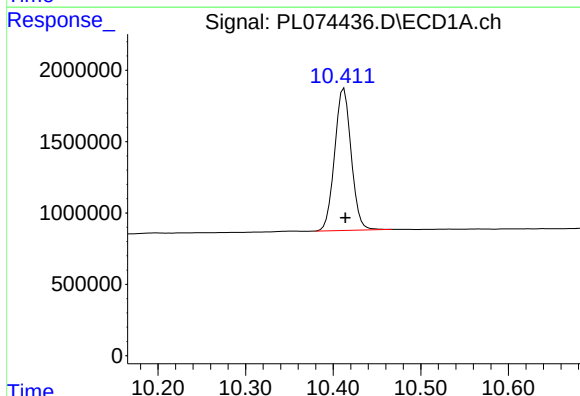

#28 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.001 min
Response: 13048265
Conc: 25.09 ng/ml

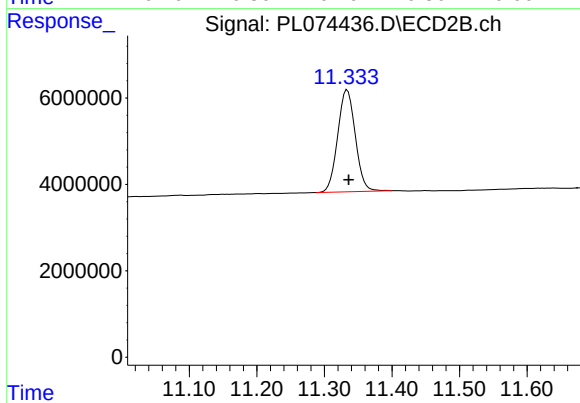

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: -0.002 min
Response: 42913410
Conc: 24.30 ng/ml