

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042823\
 Data File : PL082375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Apr 2023 10:28
 Operator : AR\AJ
 Sample : 02513-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 28 22:05:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	2.646	41564433	29058885	15.560	12.543
28) SA Decachlor...	8.746	7.754	108.8E6	36641226	56.997	16.053 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042823\
Data File : PL082375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Apr 2023 10:28
Operator : AR\AJ
Sample : 02513-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 28 22:05:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

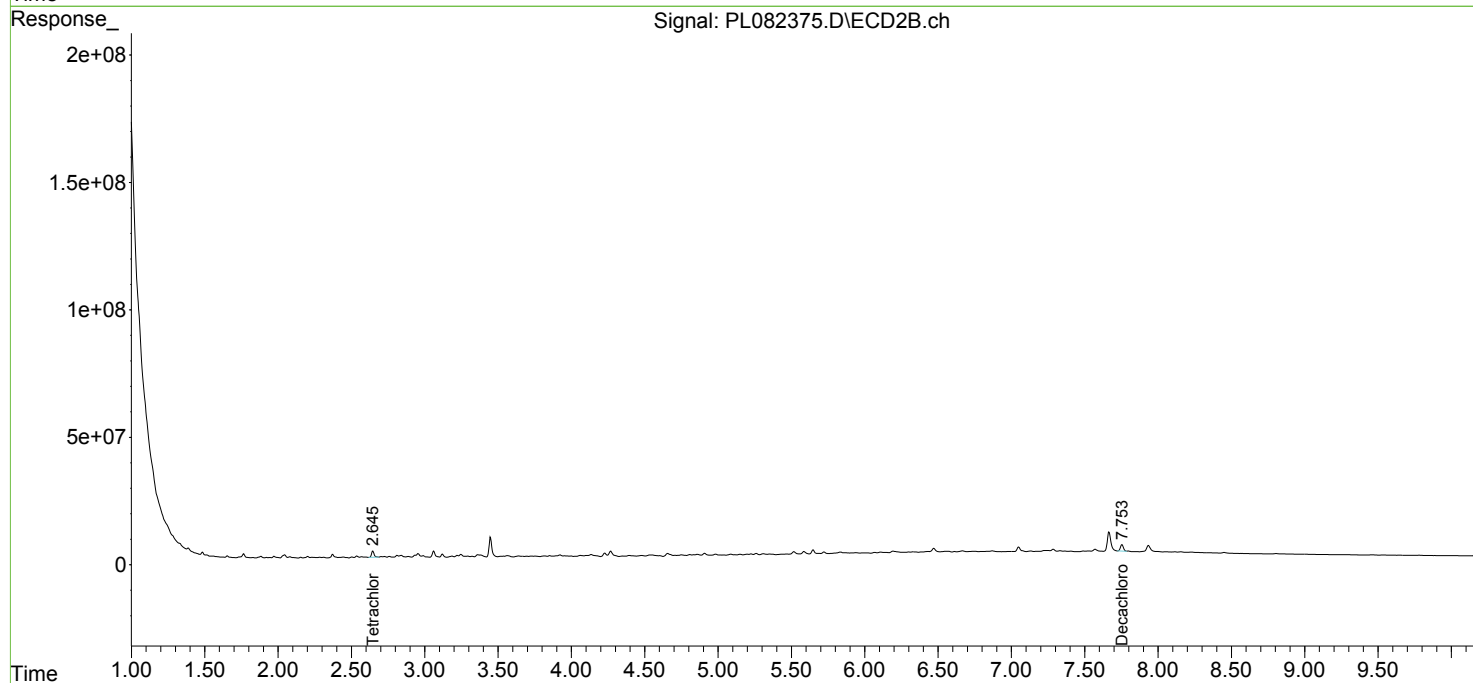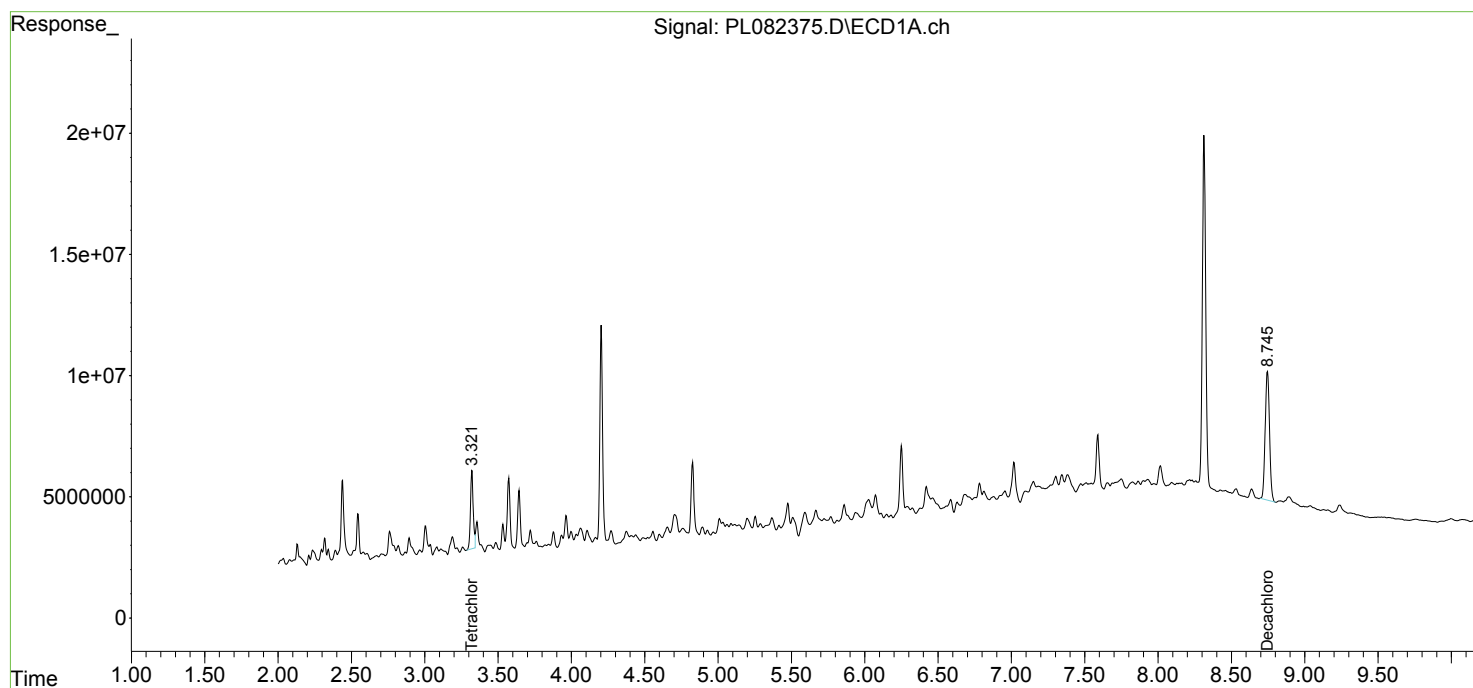


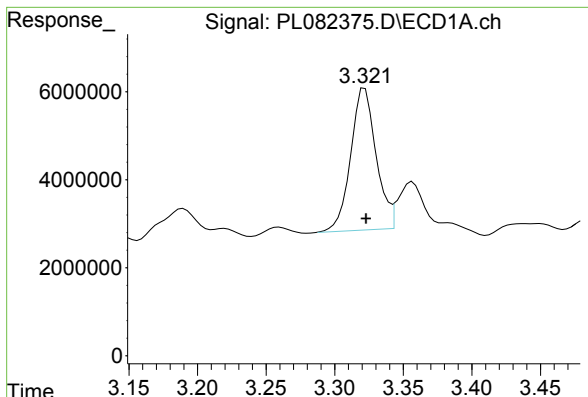

#1 Tetrachloro-m-xylene


R.T.: 3.322 min
Delta R.T.: -0.001 min
Response: 41564433
Conc: 15.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT

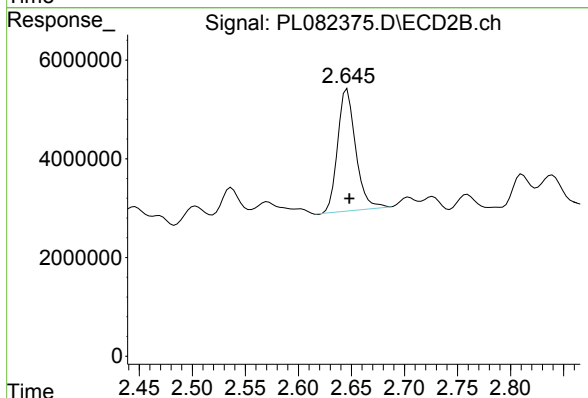


#1 Tetrachloro-m-xylene

R.T.: 2.646 min
Delta R.T.: -0.002 min
Response: 29058885
Conc: 12.54 ng/ml

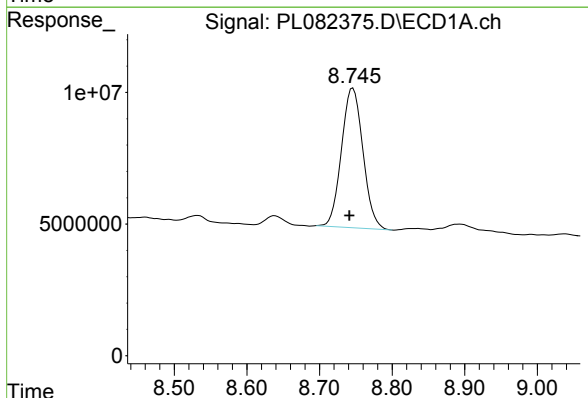

#28 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: 0.005 min
Response: 108812424
Conc: 57.00 ng/ml

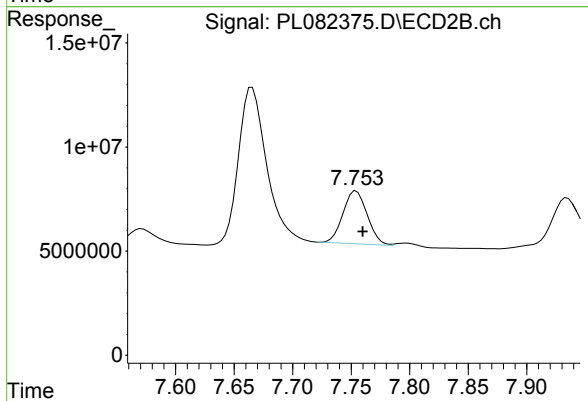

#28 Decachlorobiphenyl

R.T.: 7.754 min
Delta R.T.: -0.006 min
Response: 36641226
Conc: 16.05 ng/ml