

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
 Data File : PL047957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2019 11:30
 Operator : AJ\SJ
 Sample : K2582-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0419-S-DH-6-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 11:48:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	112.7E6	30519069	12.182	12.784
28)	SA Decachlor...	7.997	8.975	147.1E6	40036717	13.143	14.025
Target Compounds							
8)	B Heptachlo...	0.000	5.835f	0	47267756	N.D.	16.913 #
12)	B 4,4'-DDE	5.439	6.269	14307400	5375010	1.150	1.947 #
13)	MA Dieldrin	5.561	0.000	11803975	0	0.909	N.D. #
14)	MA Endrin	0.000	6.628	0	2099040	N.D.	0.822 #
16)	A 4,4'-DDD	0.000	6.763	0	5433644	N.D.	2.420 #
17)	MA 4,4'-DDT	6.180	7.056	26265109	2092268	2.634	0.878 #
19)	B Endosulfa...	6.461	0.000	3856641	0	0.346	N.D. #
20)	A Methoxychlor	6.708f	0.000	18102601	0	3.404	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
Data File : PL047957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2019 11:30
Operator : AJ\SJ
Sample : K2582-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 11:48:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

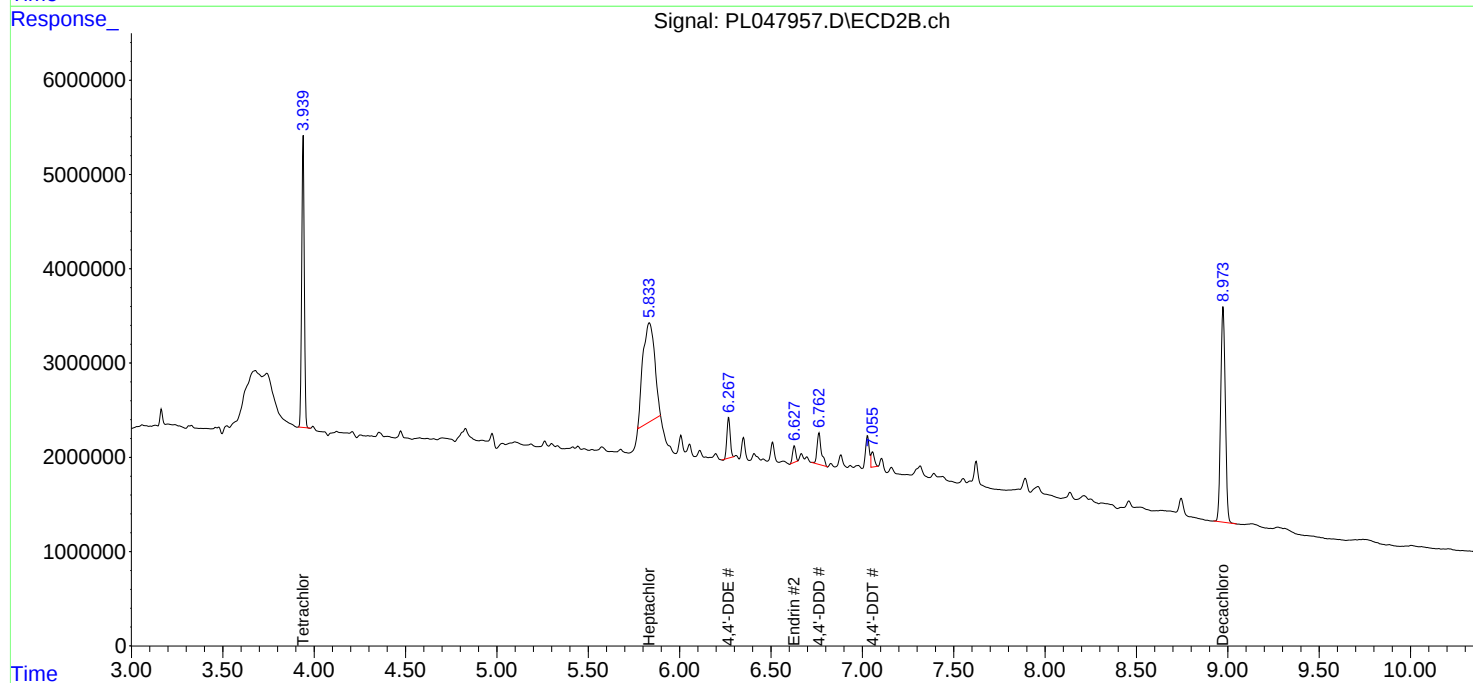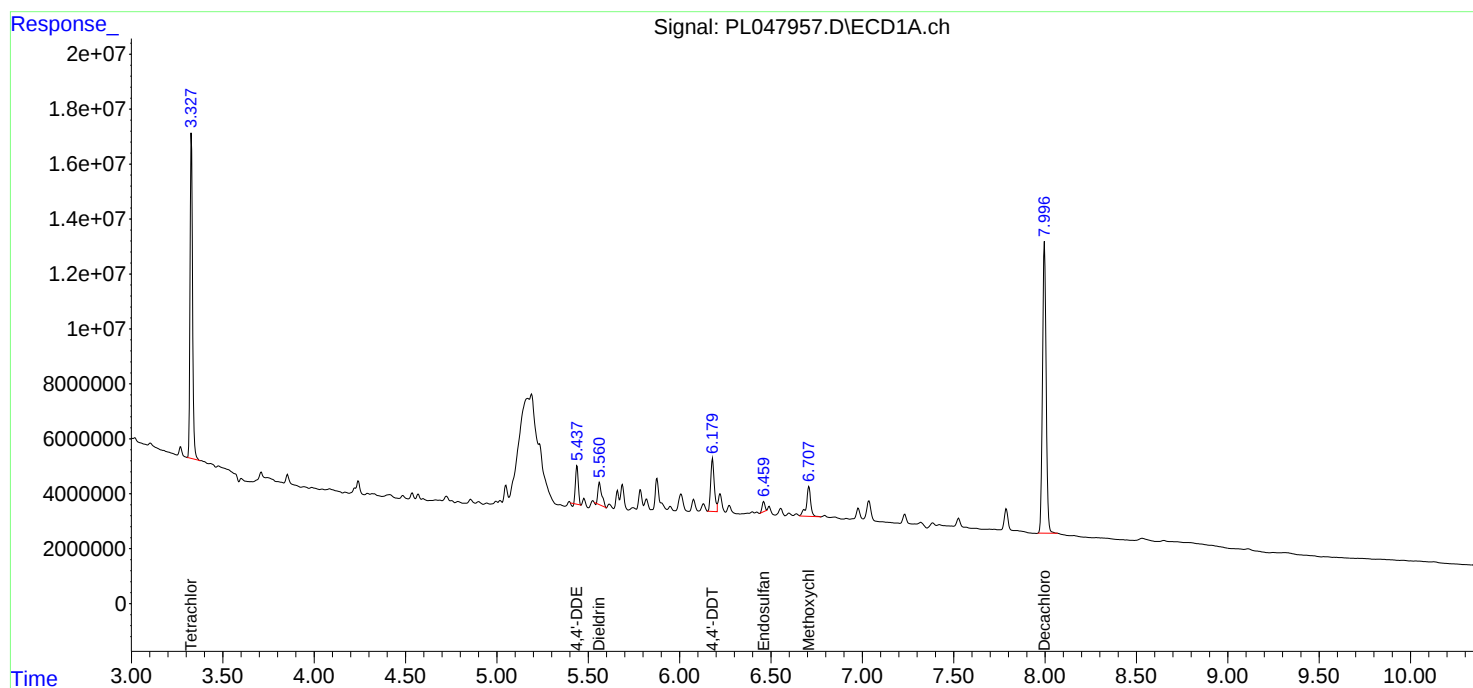


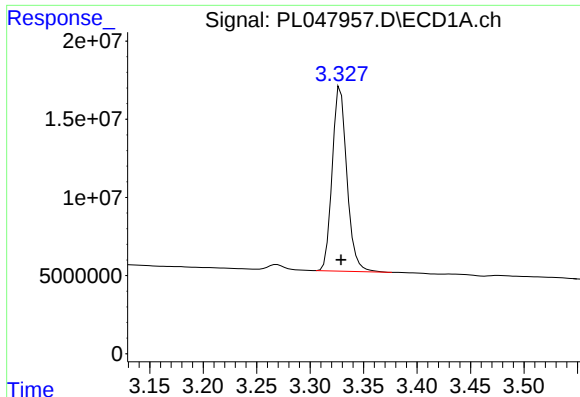

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 112664952
Conc: 12.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

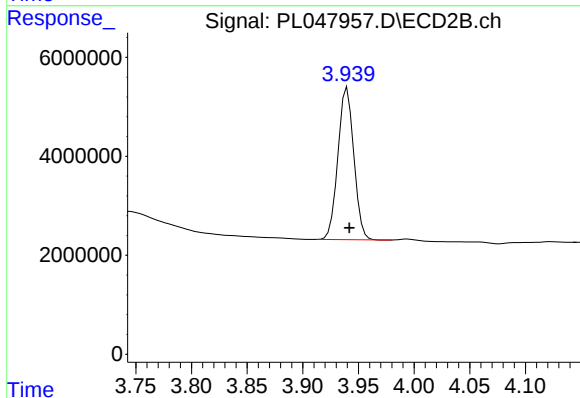


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.002 min
Response: 30519069
Conc: 12.78 ng/ml

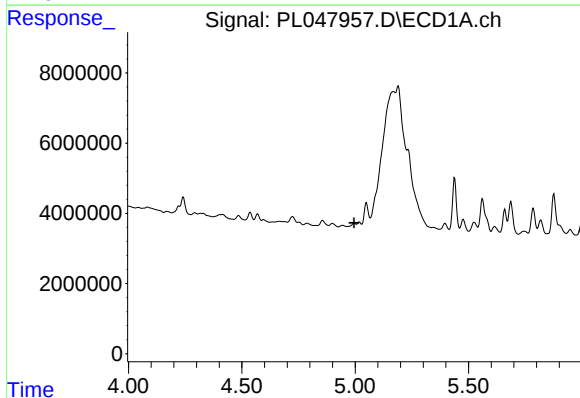


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.995 min
Response: 0
Conc: N.D.

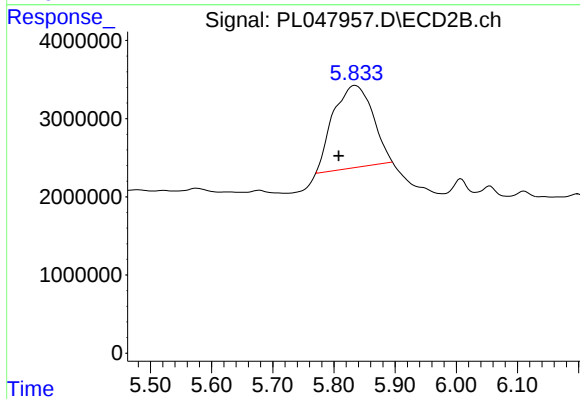

#8 Heptachlor epoxide


R.T.: 5.835 min
Delta R.T.: 0.027 min
Response: 47267756
Conc: 16.91 ng/ml

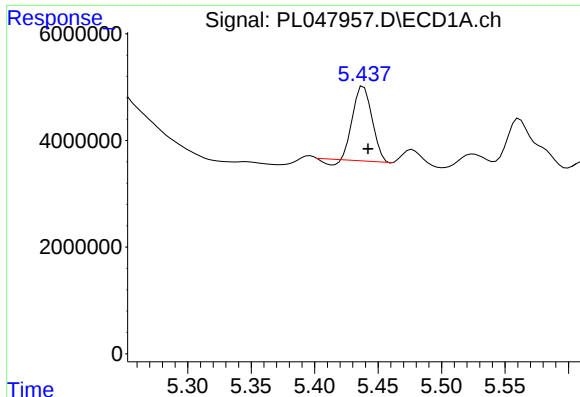

#12 4,4'-DDE


R.T.: 5.439 min
Delta R.T.: -0.004 min
Response: 14307400
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

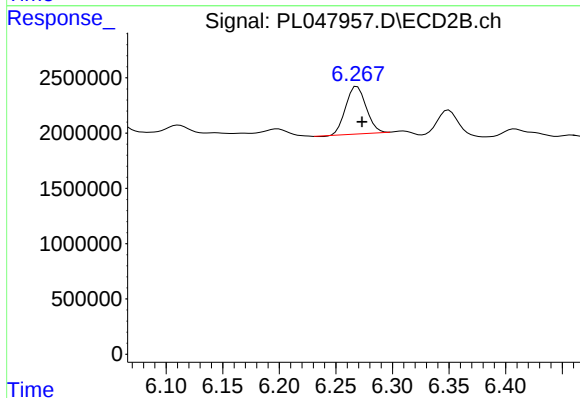


#12 4,4'-DDE

R.T.: 6.269 min
Delta R.T.: -0.004 min
Response: 5375010
Conc: 1.95 ng/ml

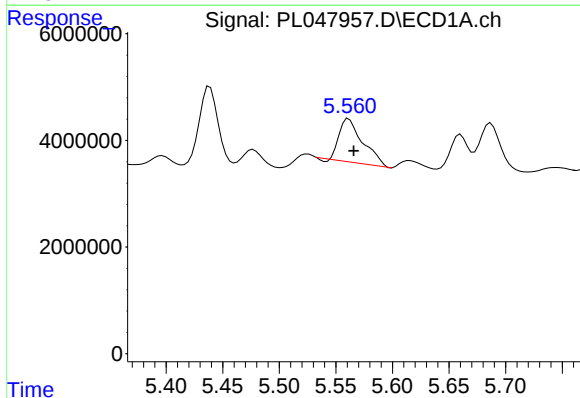


#13 Dieldrin

R.T.: 5.561 min
Delta R.T.: -0.005 min
Response: 11803975
Conc: 0.91 ng/ml

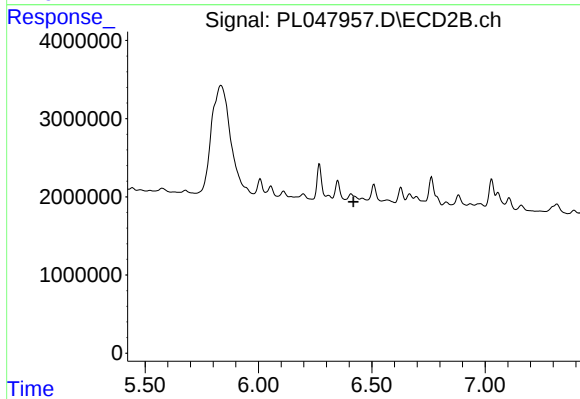

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

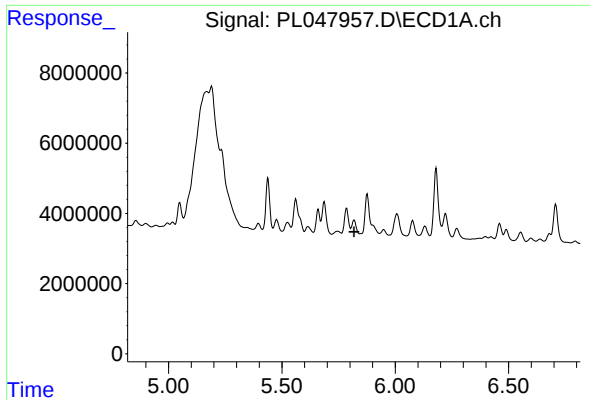

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

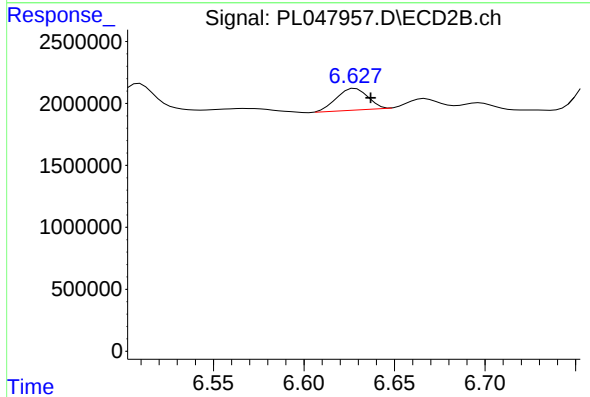


#14 Endrin

R.T.: 6.628 min
Delta R.T.: -0.008 min
Response: 2099040
Conc: 0.82 ng/ml

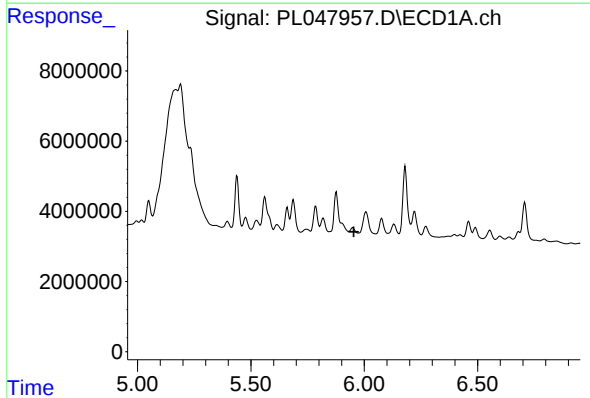


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

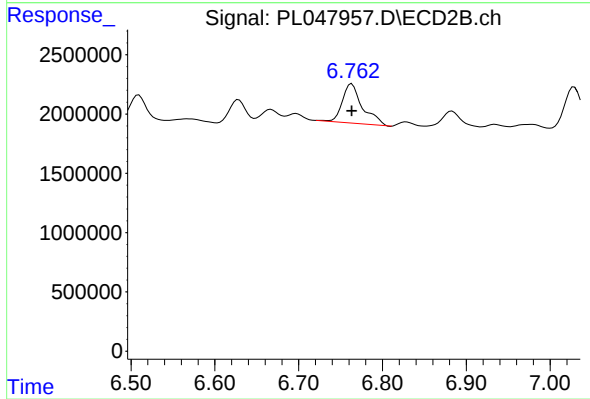

#16 4,4'-DDD


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 5433644
Conc: 2.42 ng/ml

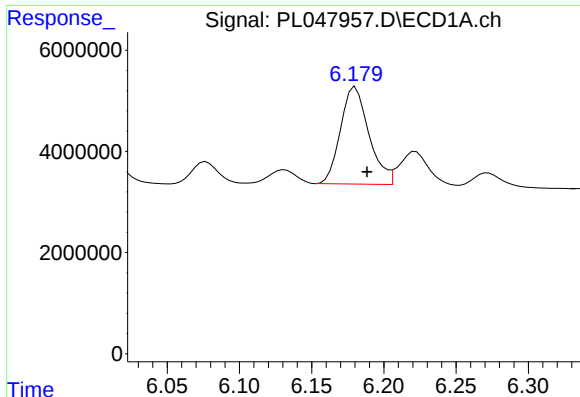

#17 4,4'-DDT


R.T.: 6.180 min
Delta R.T.: -0.008 min
Response: 26265109
Conc: 2.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

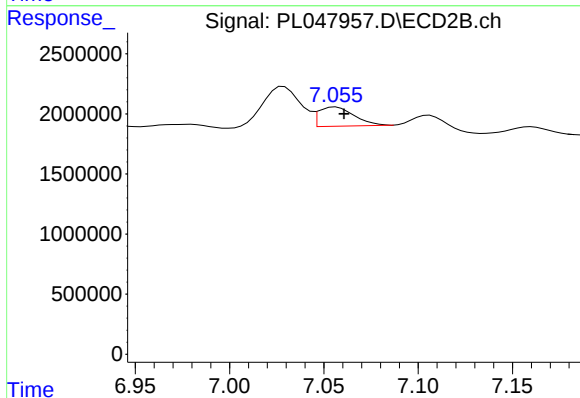


#17 4,4'-DDT

R.T.: 7.056 min
Delta R.T.: -0.004 min
Response: 2092268
Conc: 0.88 ng/ml

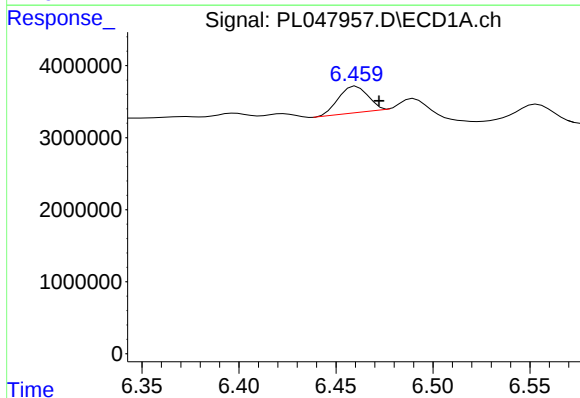


#19 Endosulfan Sulfate

R.T.: 6.461 min
Delta R.T.: -0.012 min
Response: 3856641
Conc: 0.35 ng/ml

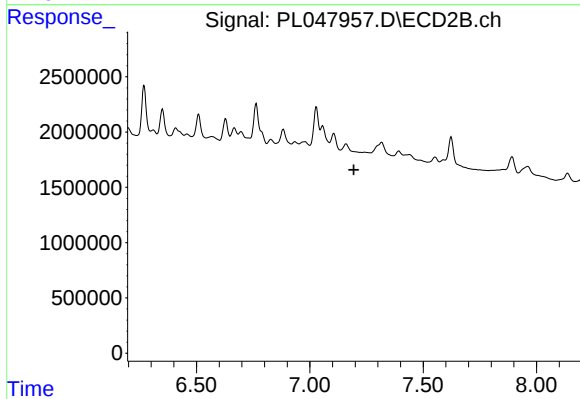

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

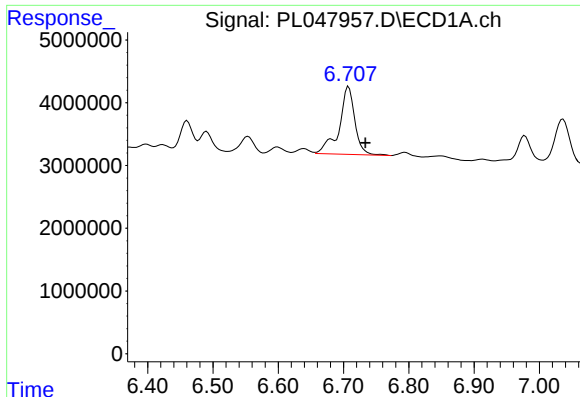

#20 Methoxychlor


R.T.: 6.708 min
Delta R.T.: -0.026 min
Response: 18102601
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

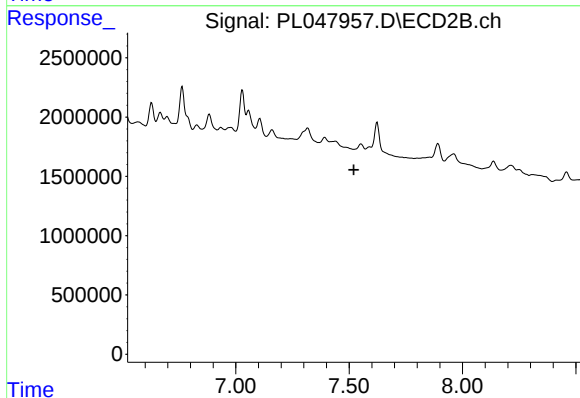


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

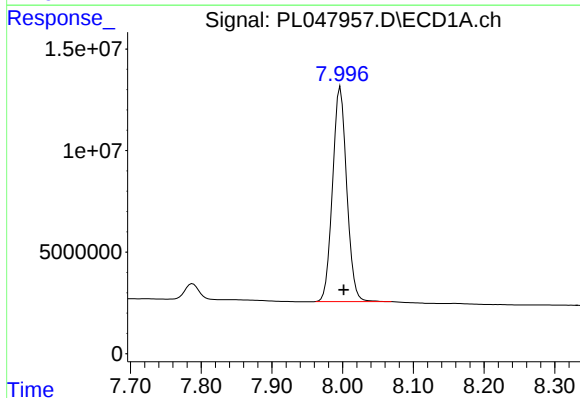

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: -0.005 min
Response: 147128942
Conc: 13.14 ng/ml

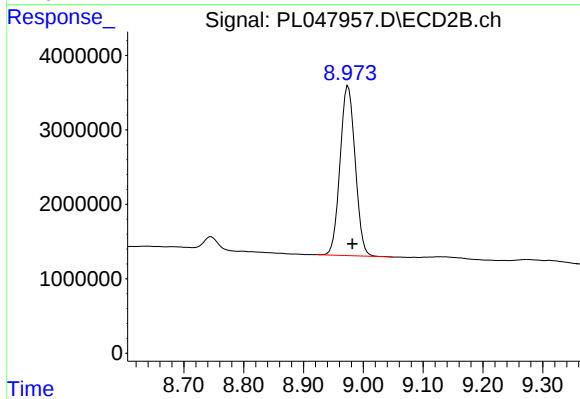

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: -0.007 min
Response: 40036717
Conc: 14.03 ng/ml