

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
 Data File : PL047960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2019 12:15
 Operator : AJ\SJ
 Sample : K2582-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0419-S-DH-6-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 13:03:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	111.5E6	30291980	12.061	12.689
28)	SA Decachlor...	7.996	8.976	146.7E6	40376602	13.101	14.144
Target Compounds							
8)	B Heptachlo...	0.000	5.835f	0	48107570	N.D.	17.214 #
12)	B 4,4'-DDE	5.439	6.269	6463425	5371479	0.520	1.945 #
13)	MA Dieldrin	5.562	0.000	11428396	0	0.880	N.D. #
14)	MA Endrin	5.826	6.630	4039627	4137051	0.340	1.620 #
16)	A 4,4'-DDD	0.000	6.764	0	5798765	N.D.	2.583 #
17)	MA 4,4'-DDT	6.181	7.057	25977794	2236678	2.606	0.939 #
19)	B Endosulfa...	6.462	0.000	3830884	0	0.344	N.D. #
20)	A Methoxychlor	6.708f	0.000	15748326	0	2.961	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
Data File : PL047960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2019 12:15
Operator : AJ\SJ
Sample : K2582-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 13:03:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

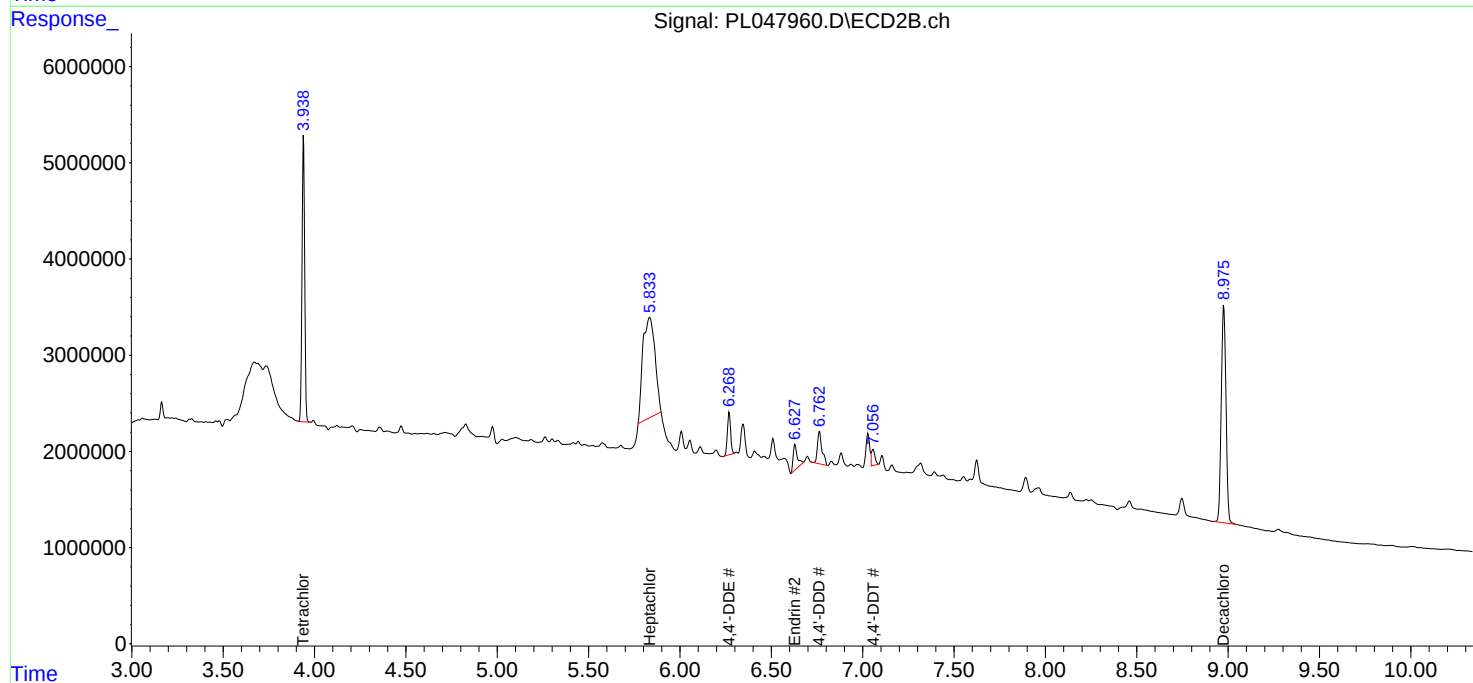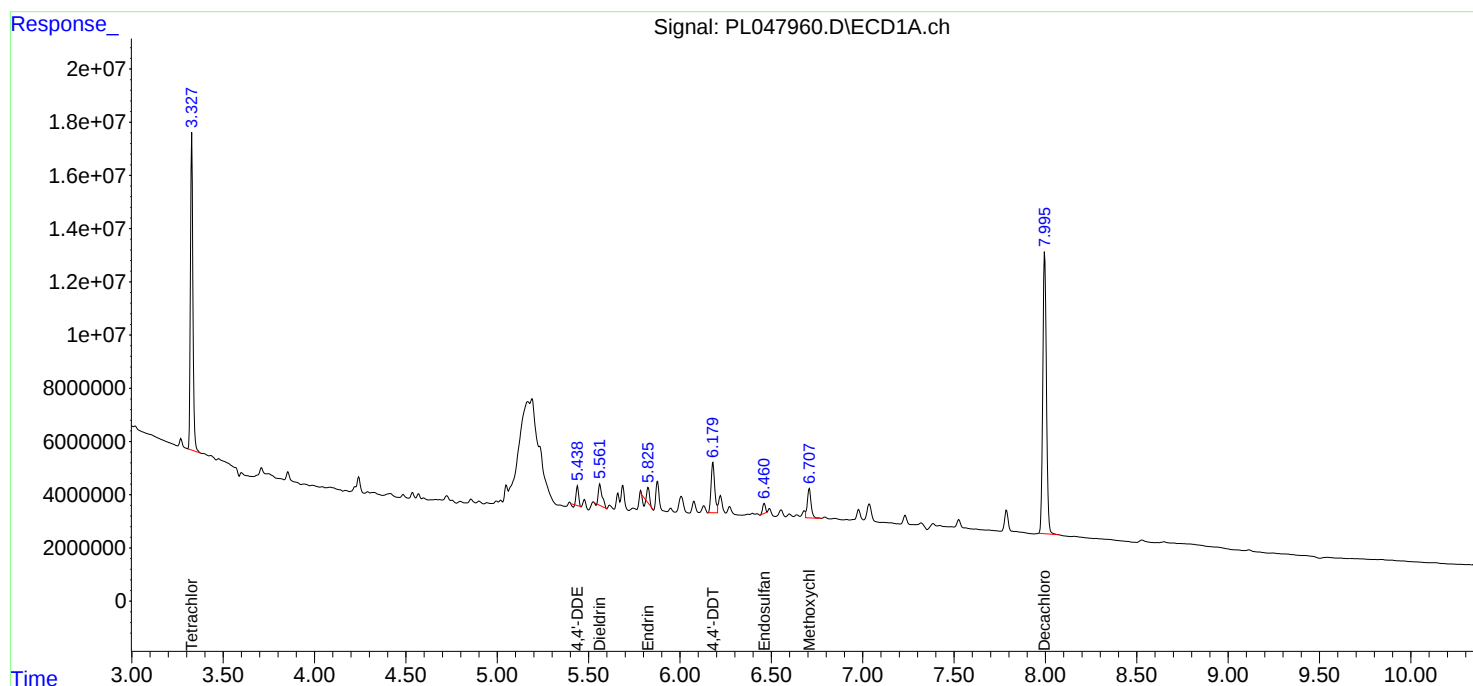


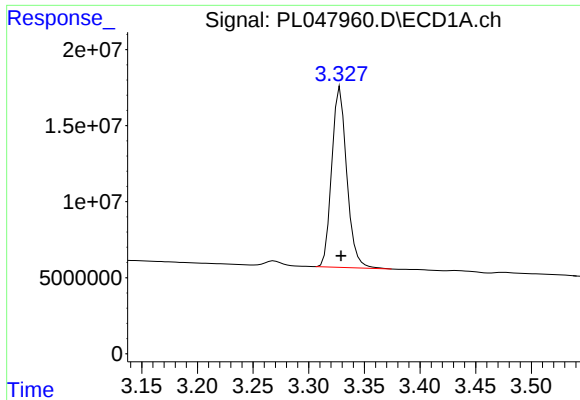

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 111547392
Conc: 12.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

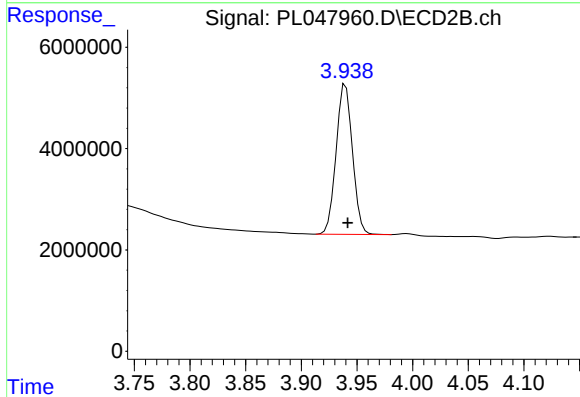


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.002 min
Response: 30291980
Conc: 12.69 ng/ml

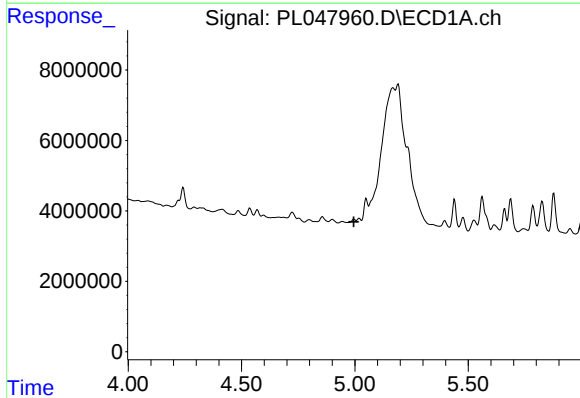


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.995 min
Response: 0
Conc: N.D.

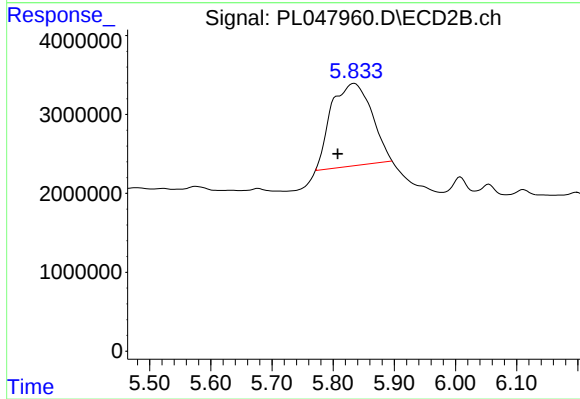

#8 Heptachlor epoxide


R.T.: 5.835 min
Delta R.T.: 0.027 min
Response: 48107570
Conc: 17.21 ng/ml

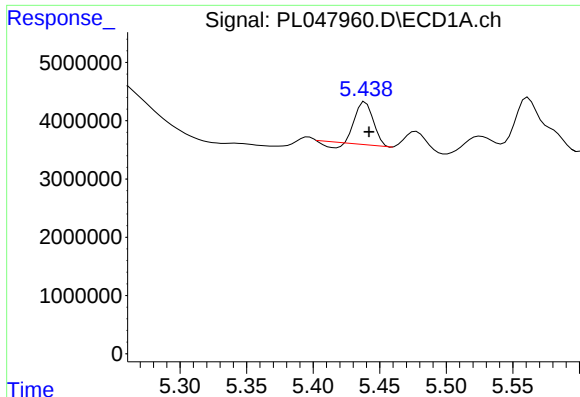

#12 4,4'-DDE


R.T.: 5.439 min
Delta R.T.: -0.003 min
Response: 6463425
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

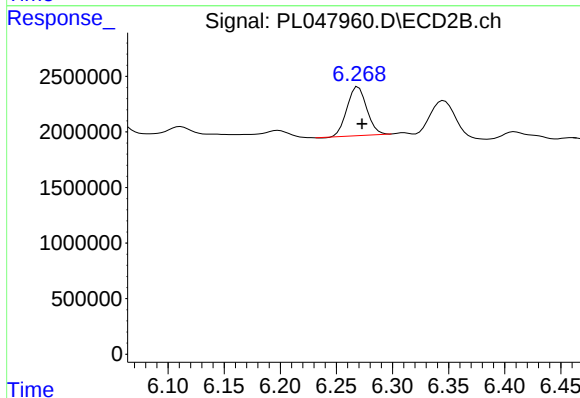


#12 4,4'-DDE

R.T.: 6.269 min
Delta R.T.: -0.004 min
Response: 5371479
Conc: 1.95 ng/ml

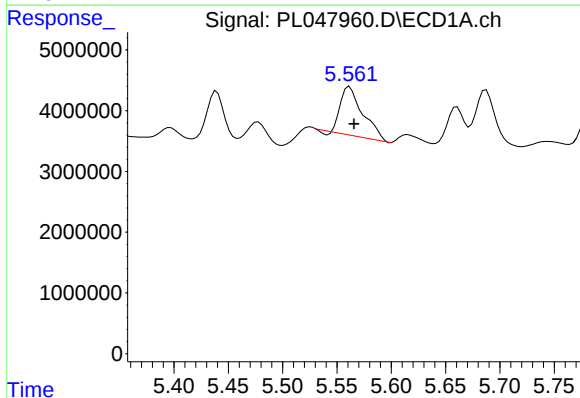


#13 Dieldrin

R.T.: 5.562 min
Delta R.T.: -0.004 min
Response: 11428396
Conc: 0.88 ng/ml

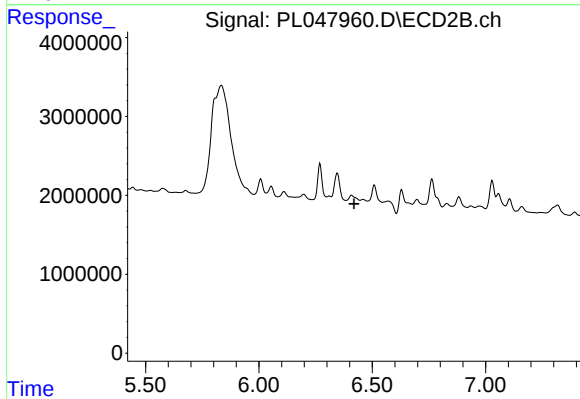

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

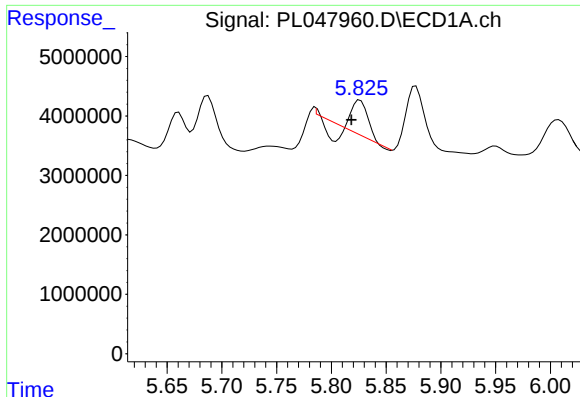

#14 Endrin


R.T.: 5.826 min
Delta R.T.: 0.008 min
Response: 4039627
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

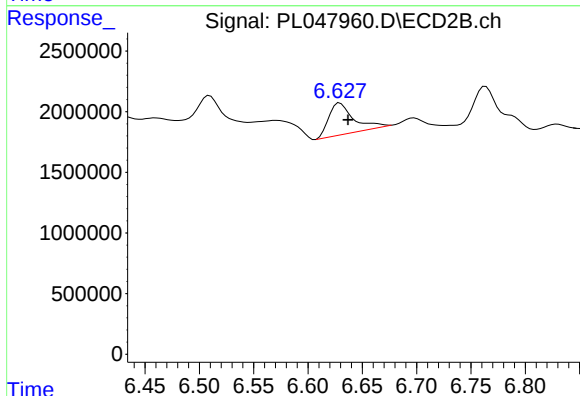


#14 Endrin

R.T.: 6.630 min
Delta R.T.: -0.007 min
Response: 4137051
Conc: 1.62 ng/ml

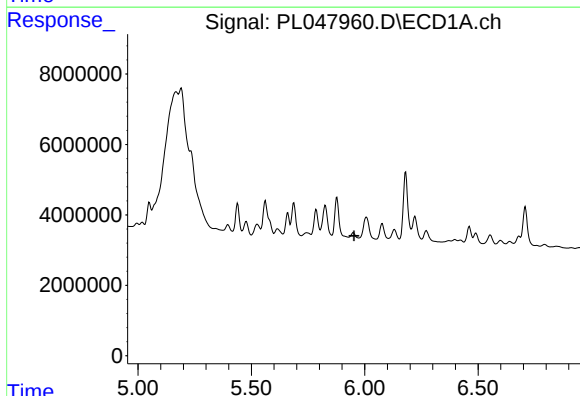


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

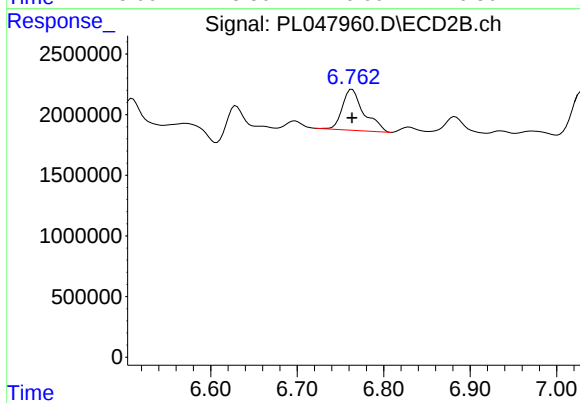

#16 4,4'-DDD


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 5798765
Conc: 2.58 ng/ml

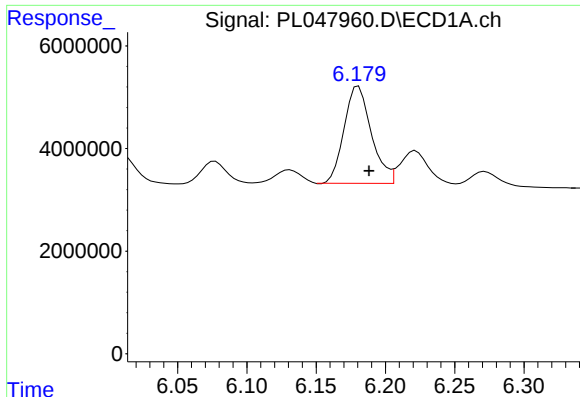

#17 4,4'-DDT


R.T.: 6.181 min
Delta R.T.: -0.008 min
Response: 25977794
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

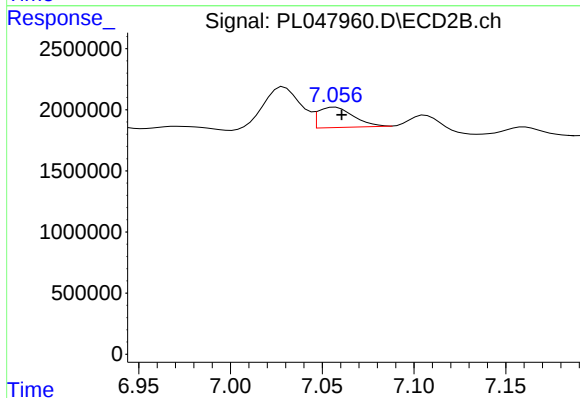


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: -0.004 min
Response: 2236678
Conc: 0.94 ng/ml

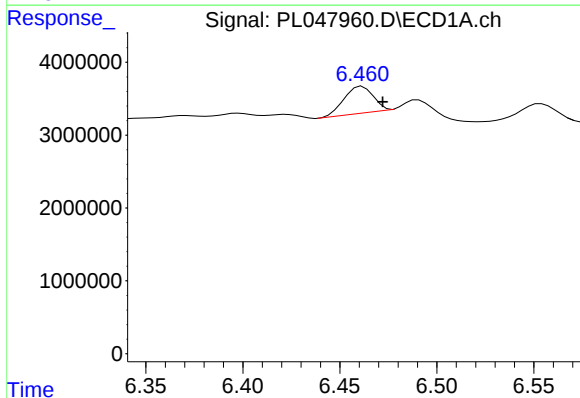


#19 Endosulfan Sulfate

R.T.: 6.462 min
Delta R.T.: -0.011 min
Response: 3830884
Conc: 0.34 ng/ml

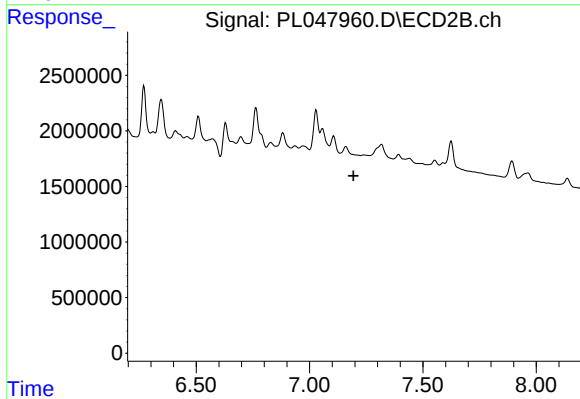

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

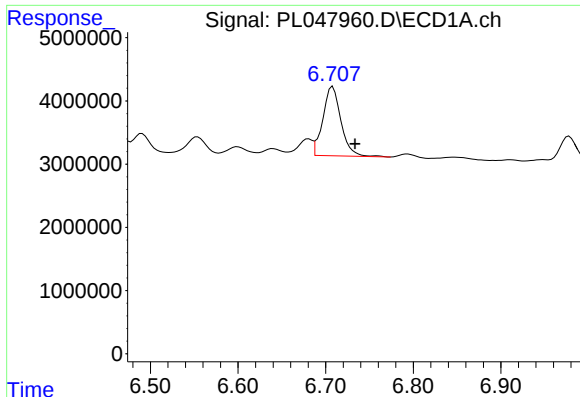

#20 Methoxychlor


R.T.: 6.708 min
Delta R.T.: -0.026 min
Response: 15748326
Conc: 2.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

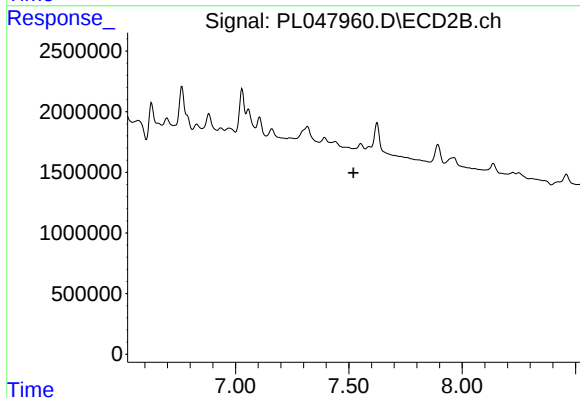


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

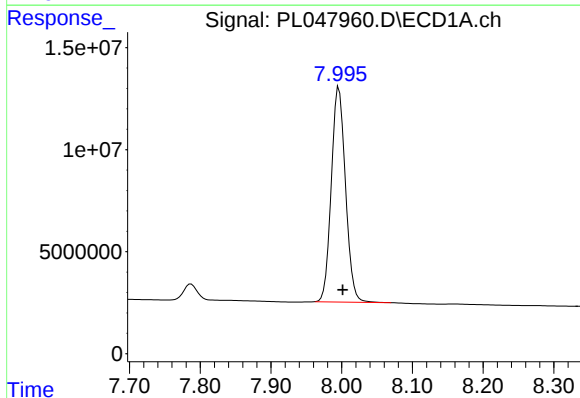

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: -0.006 min
Response: 146660014
Conc: 13.10 ng/ml

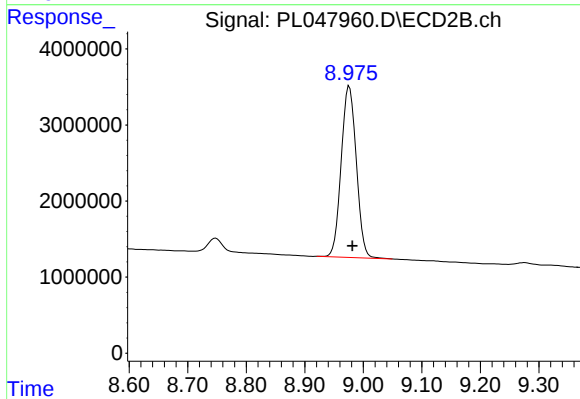

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 40376602
Conc: 14.14 ng/ml