

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
 Data File : PL047960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2019 12:15
 Operator : AJ\SJ
 Sample : K2582-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SSSI-0419-S-DH-6-B

Manual Integrations
 APPROVED

mohammad
 4/30/2019 3:22:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 29 13:03:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	3.940	111.5E6	30291980	12.061	12.689
28) SA Decachlor...	7.996	8.976	146.7E6	40376602	13.101	14.144
Target Compounds						
12) B 4,4'-DDE	5.438	6.269	8056196	5371479	0.648m	1.945 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042919\
Data File : PL047960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2019 12:15
Operator : AJ\SJ
Sample : K2582-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B


Manual Integrations
APPROVED

mohammad
4/30/2019 3:22:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 29 13:03:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

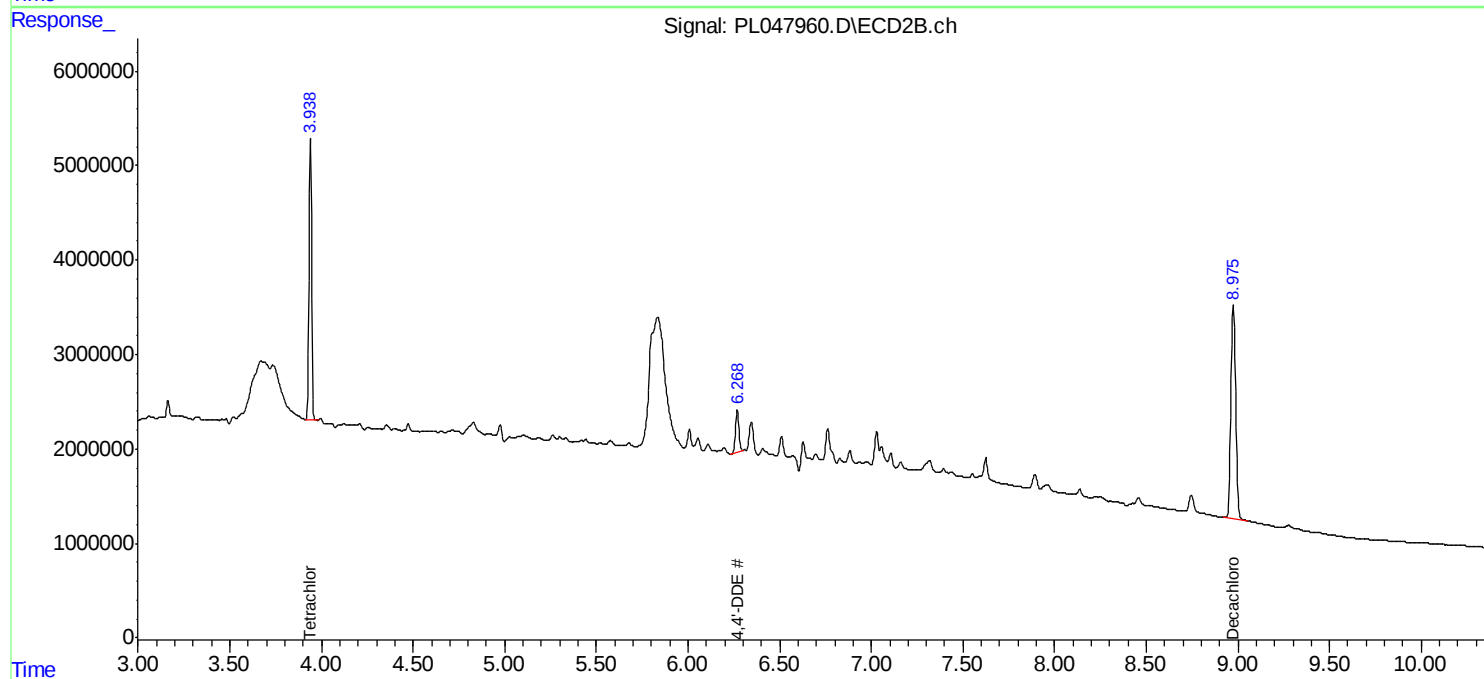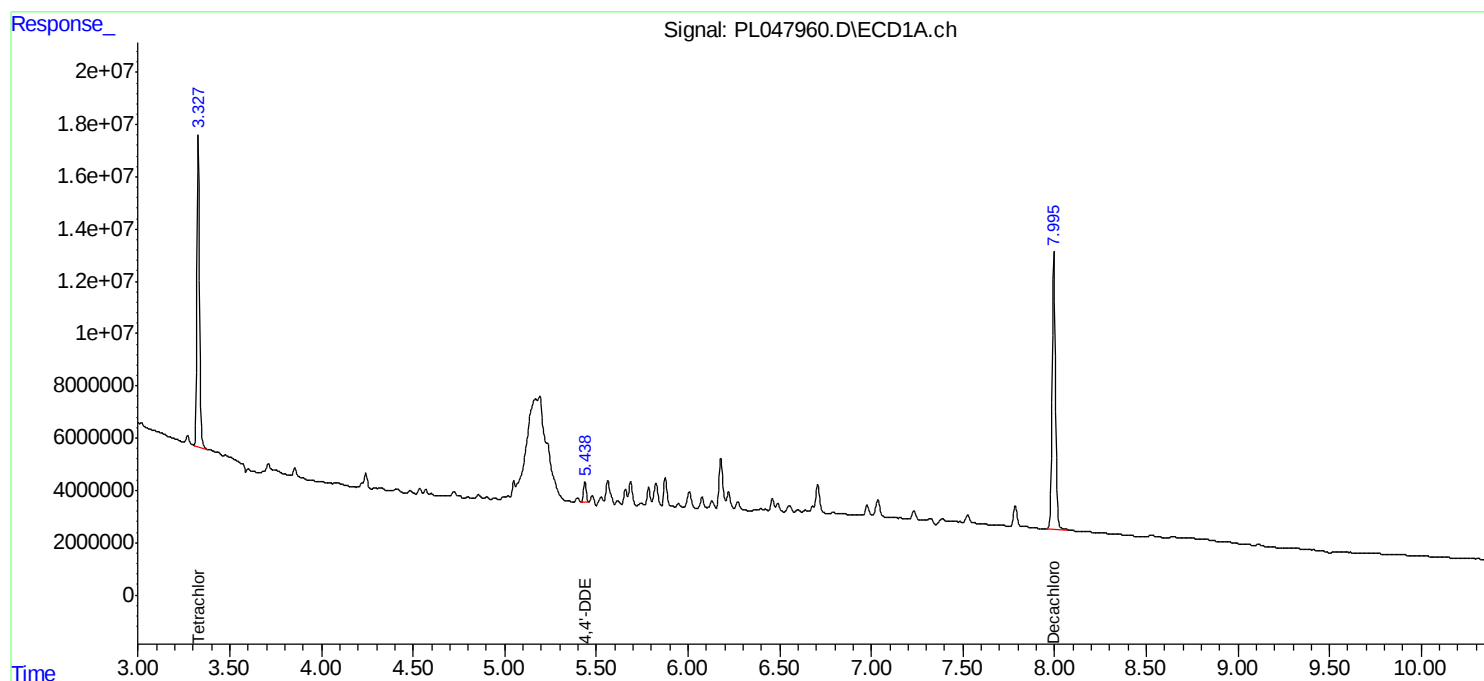

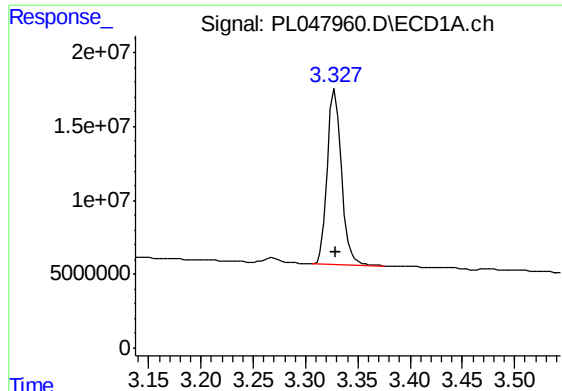


#1 Tetrachloro-m-xylene

R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 111547392
Conc: 12.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B


Manual Integrations
APPROVED

mohammad
4/30/2019 3:22:57 PM

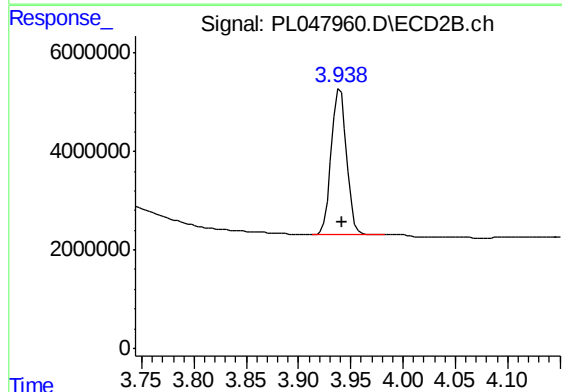


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.002 min
Response: 30291980
Conc: 12.69 ng/ml

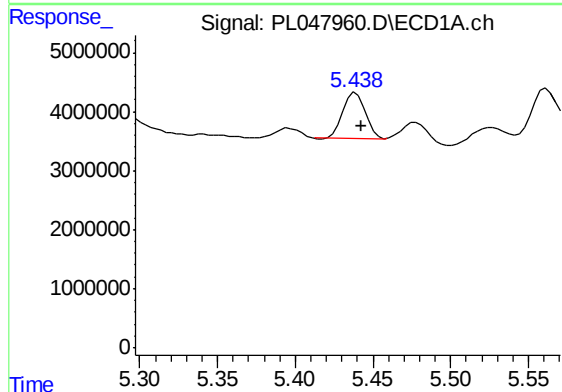


#12 4,4'-DDE

R.T.: 5.438 min
Delta R.T.: -0.004 min
Response: 8056196
Conc: 0.65 ng/ml m

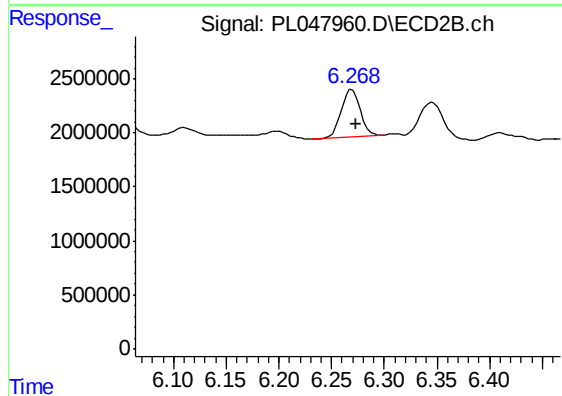

#12 4,4'-DDE

R.T.: 6.269 min
Delta R.T.: -0.004 min
Response: 5371479
Conc: 1.95 ng/ml

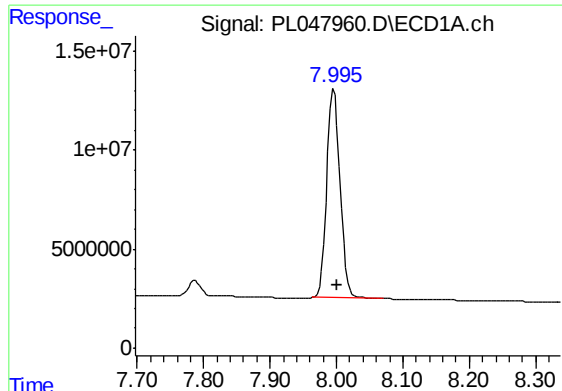


#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: -0.006 min
Response: 146660014
Conc: 13.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
SSSI-0419-S-DH-6-B

Manual Integrations
APPROVED

mohammad
4/30/2019 3:22:57 PM

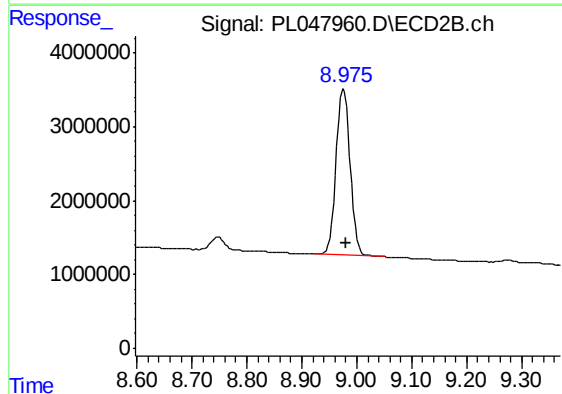

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 40376602
Conc: 14.14 ng/ml