

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 21:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:55:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.155	82977177	81784196	22.021	23.287
28)	SA Decachlor...	8.168	9.357	77180206	66099978	20.129	21.367
Target Compounds							
2)	A alpha-BHC	3.850	0.000	2452734	0	0.394	N.D. #
6)	B beta-BHC	4.404	5.034	916586	8762804	0.346	0.717 #
8)	B Heptachlo...	0.000	6.072	0	2426637	N.D.	0.656 #
9)	A Endosulfan I	0.000	6.408f	0	5367825	N.D.	1.410 #
11)	B alpha-Chl...	0.000	6.408f	0	5367825	N.D.	1.294 #
14)	MA Endrin	5.958	0.000	1602374	0	0.368	N.D. #
21)	B Endrin ke...	0.000	7.974	0	2476947	N.D.	0.698 #
23)	Chlordane-1	4.315f	0.000	4148337	0	24.541	N.D. #
26)	Chlordane-4	0.000	6.408f	0	5367825	N.D.	7.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 21:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:55:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

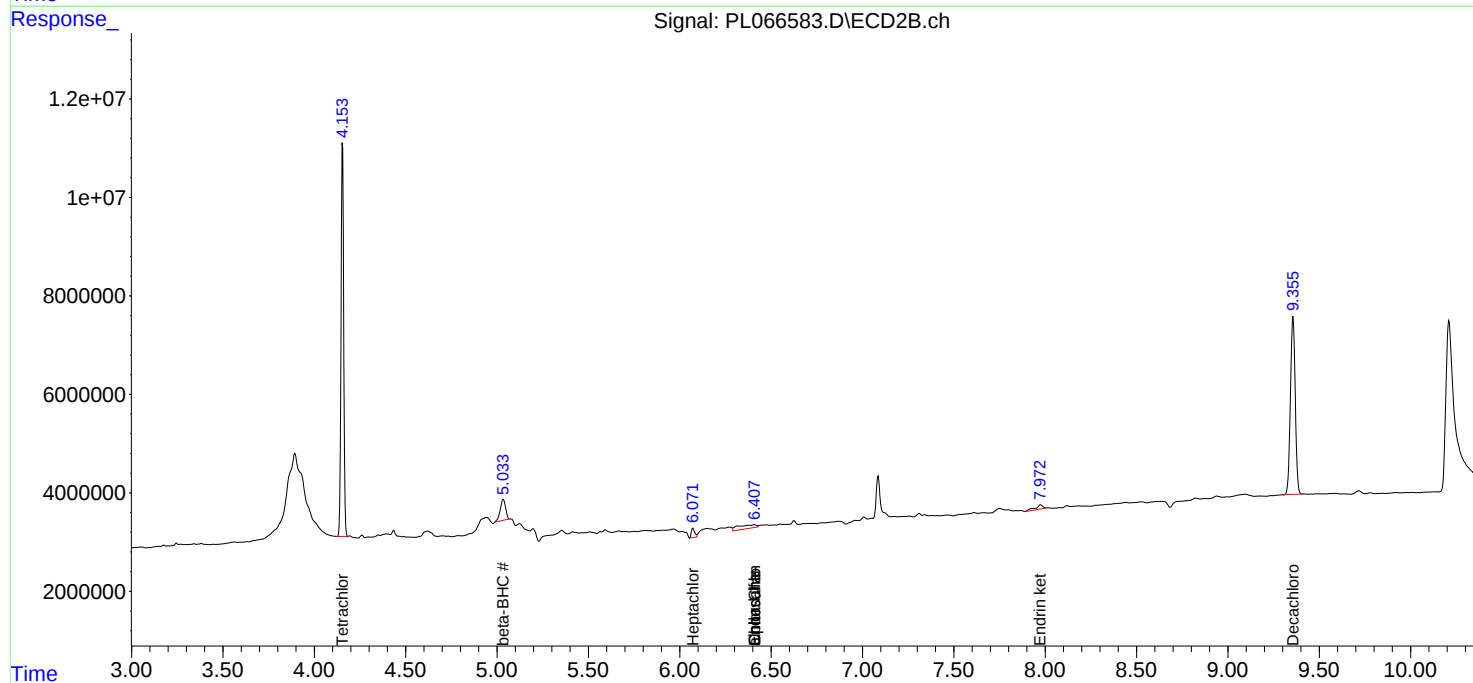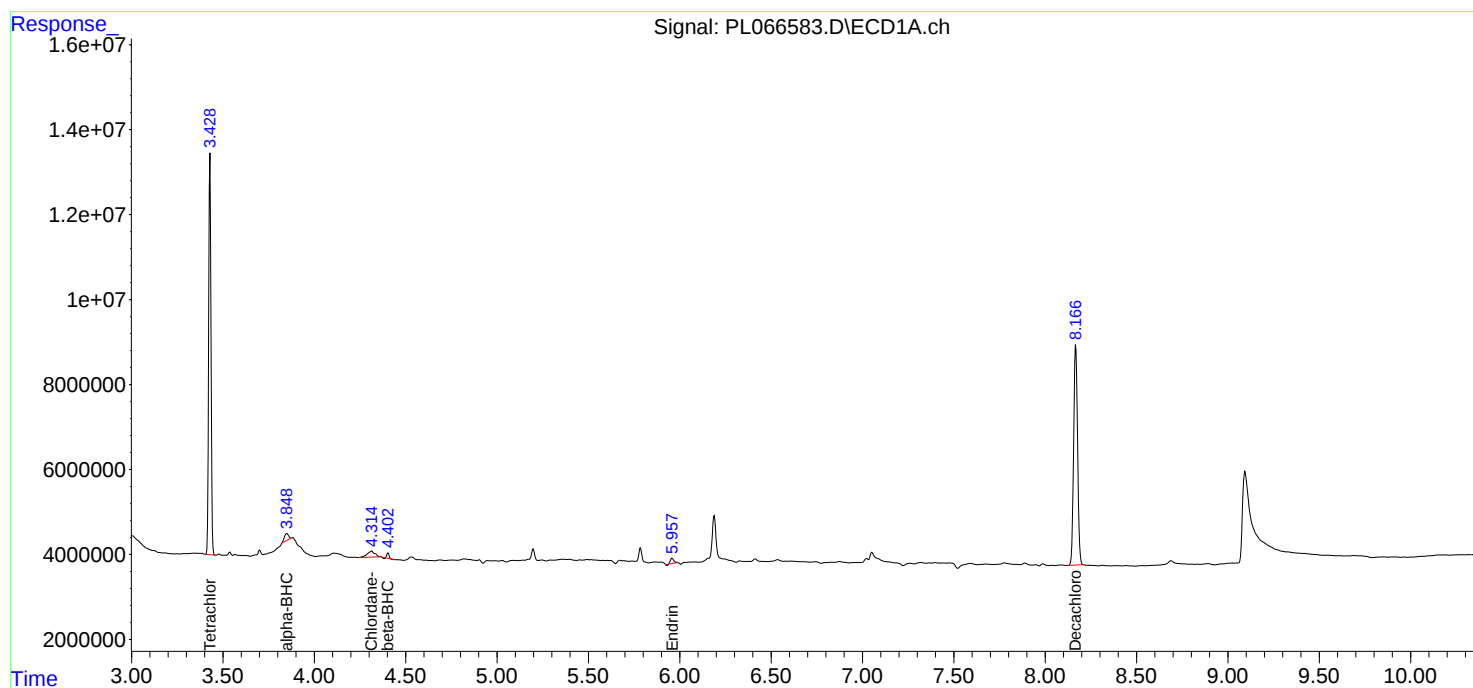


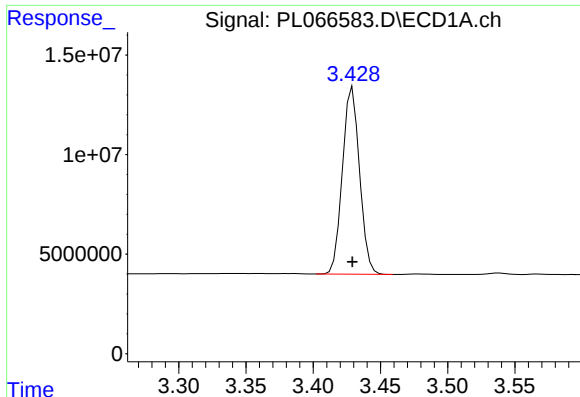

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 82977177
Conc: 22.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

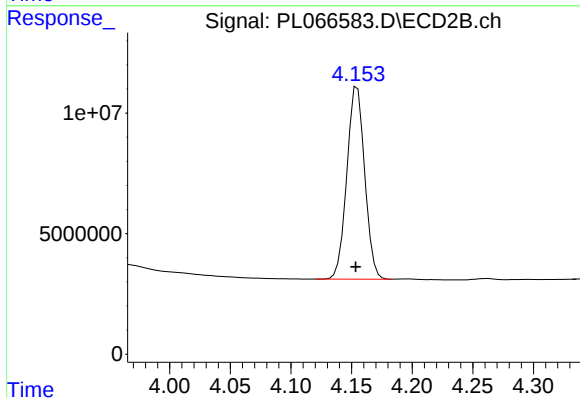


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 81784196
Conc: 23.29 ng/ml

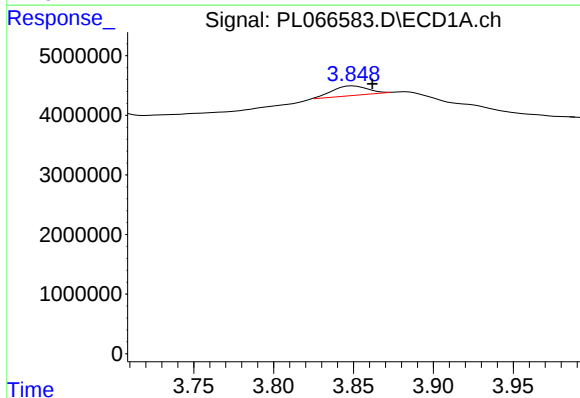


#2 alpha-BHC

R.T.: 3.850 min
Delta R.T.: -0.012 min
Response: 2452734
Conc: 0.39 ng/ml

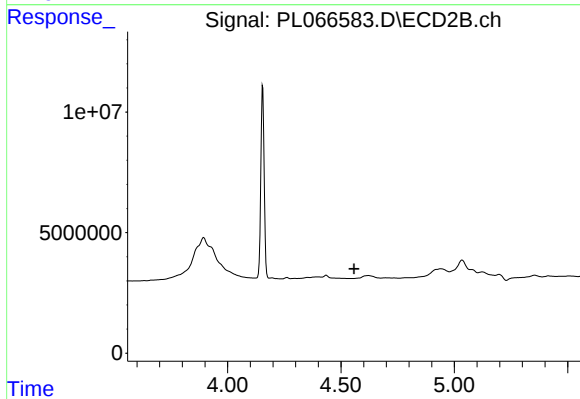

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.557 min
Response: 0
Conc: N.D.

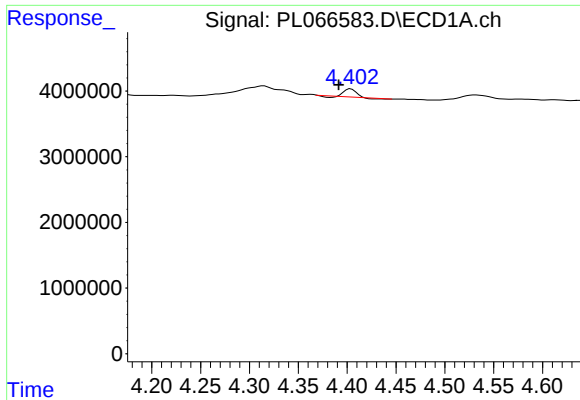

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: 0.013 min
Response: 916586
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

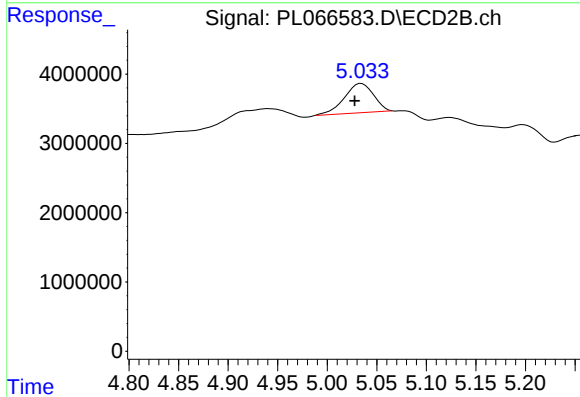


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 8762804
Conc: 0.72 ng/ml

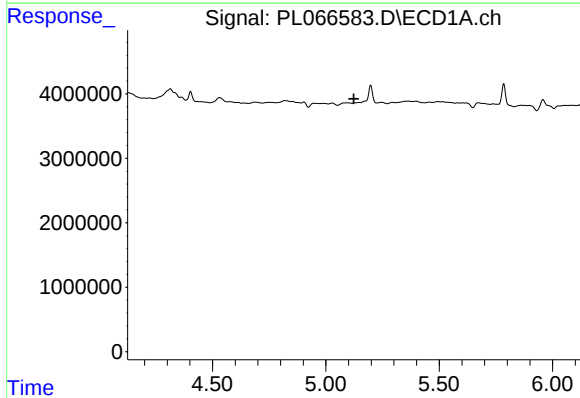


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

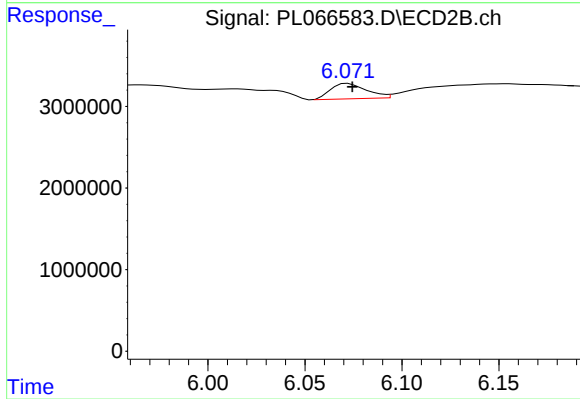

#8 Heptachlor epoxide


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 2426637
Conc: 0.66 ng/ml

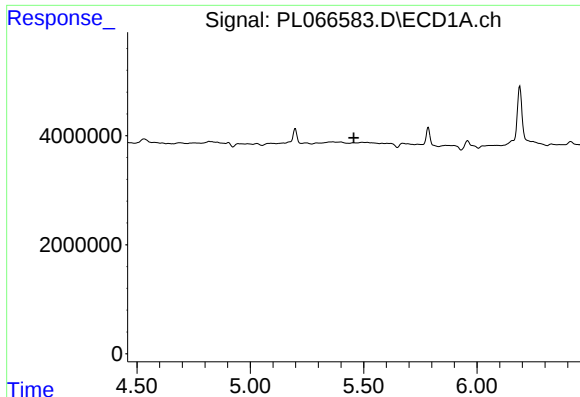

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

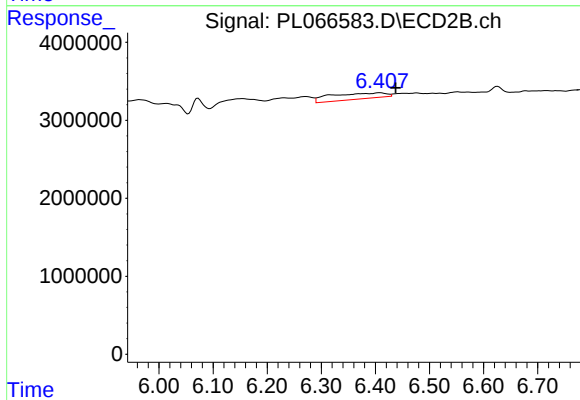


#9 Endosulfan I

R.T.: 6.408 min
Delta R.T.: -0.029 min
Response: 5367825
Conc: 1.41 ng/ml

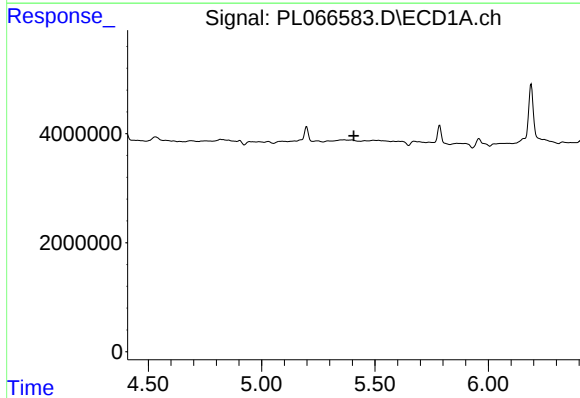


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

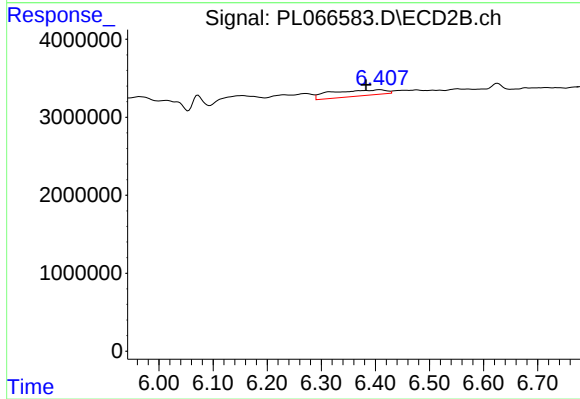

#11 alpha-Chlordane


R.T.: 6.408 min
Delta R.T.: 0.025 min
Response: 5367825
Conc: 1.29 ng/ml

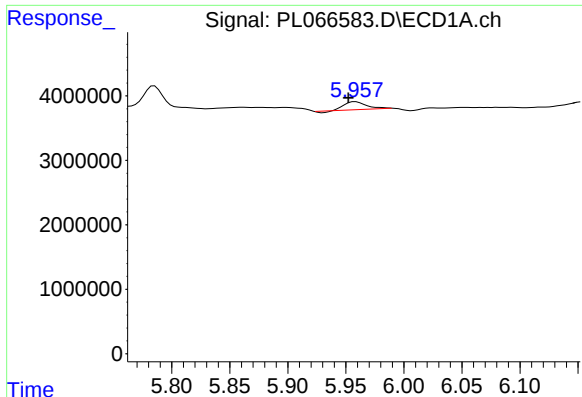

#14 Endrin


R.T.: 5.958 min
Delta R.T.: 0.006 min
Response: 1602374
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

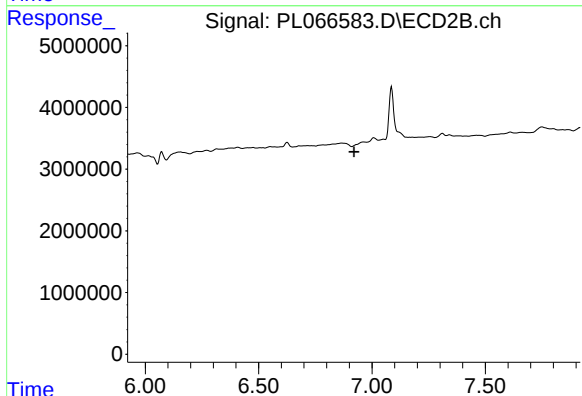


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

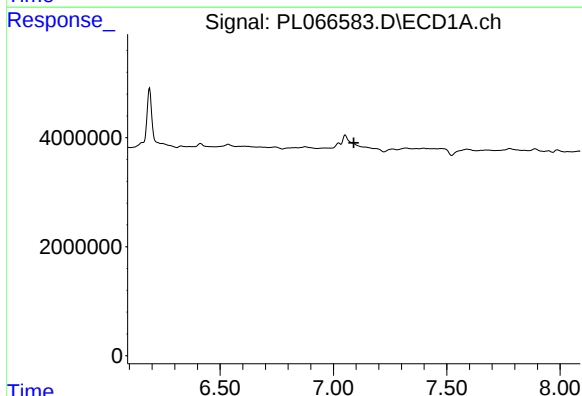


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

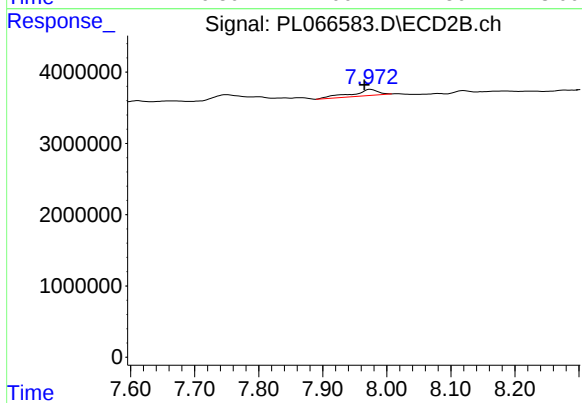

#21 Endrin ketone


R.T.: 7.974 min
Delta R.T.: 0.010 min
Response: 2476947
Conc: 0.70 ng/ml

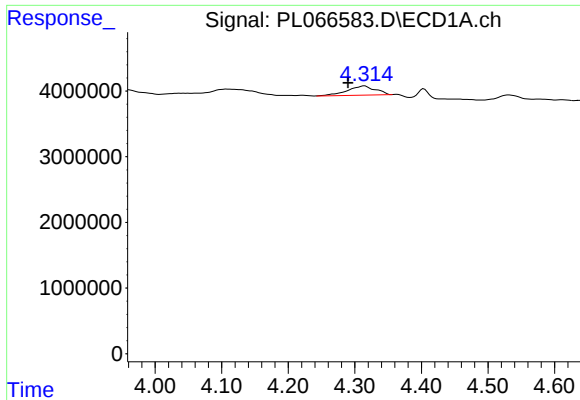

#23 Chlordane-1


R.T.: 4.315 min
Delta R.T.: 0.025 min
Response: 4148337
Conc: 24.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

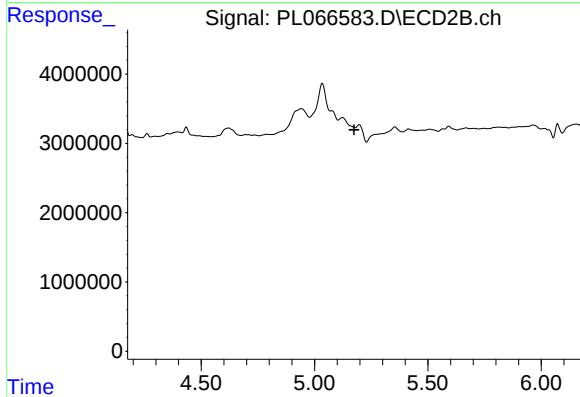


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

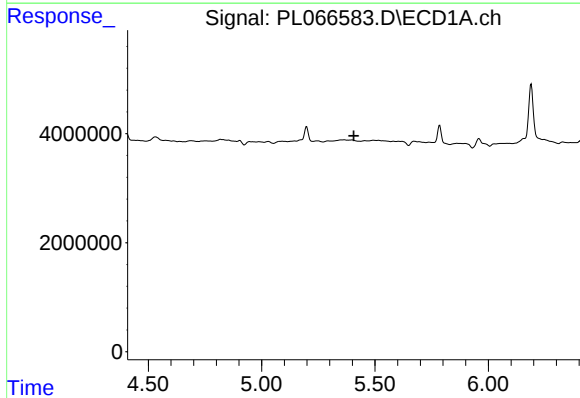


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

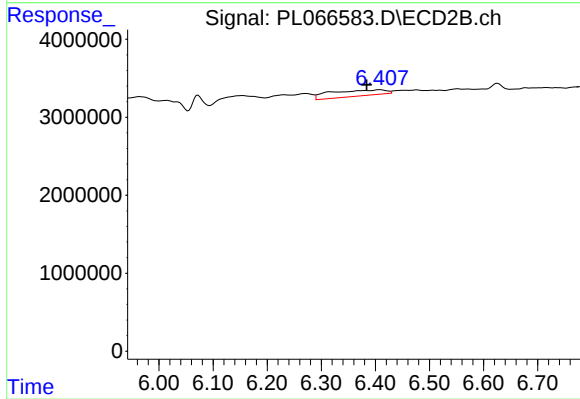

#26 Chlordane-4


R.T.: 6.408 min
Delta R.T.: 0.024 min
Response: 5367825
Conc: 8.00 ng/ml

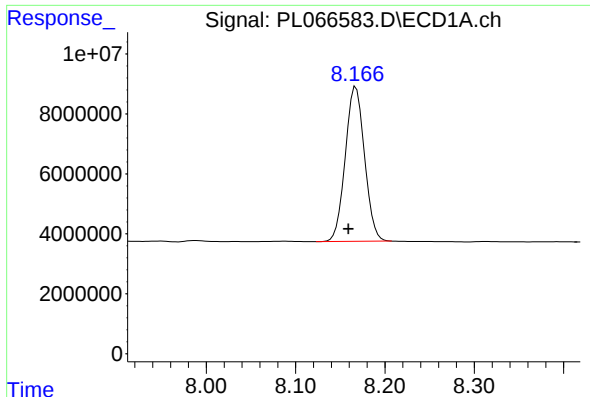

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.008 min
Response: 77180206
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

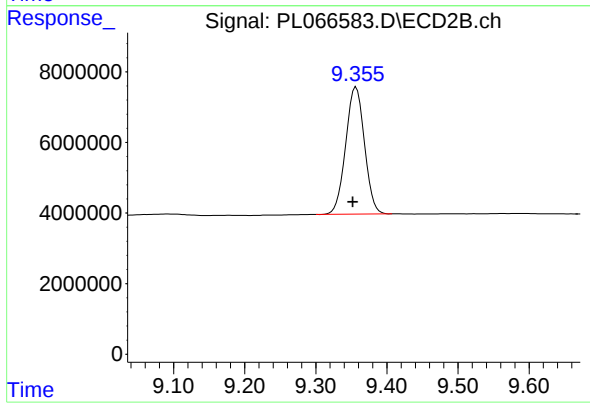

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 66099978
Conc: 21.37 ng/ml