

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 22:53
 Operator : AR\AJ
 Sample : M2196-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:56:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	4.155	79567974	78615438	21.116	22.384
28)	SA Decachlor...	8.168	9.357	60122370	52488088	15.680	16.967
Target Compounds							
2)	A alpha-BHC	3.853	0.000	3510304	0	0.564	N.D. #
6)	B beta-BHC	0.000	5.035	0	7993853	N.D.	0.362 #
9)	A Endosulfan I	0.000	6.452	0	714267	N.D.	0.188 #
10)	B gamma-Chl...	5.375f	6.313	3690220	7310672	0.724	1.756 #
11)	B alpha-Chl...	0.000	6.407f	0	3565082	N.D.	0.859 #
14)	MA Endrin	5.961	0.000	1370753	0	0.315	N.D. #
23)	Chlordane-1	4.298	0.000	819308	0	4.847	N.D. #
25)	Chlordane-3	5.375f	6.313	3690220	7310672	7.415	13.043 #
26)	Chlordane-4	0.000	6.407f	0	3565082	N.D.	5.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 22:53
Operator : AR\AJ
Sample : M2196-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:56:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

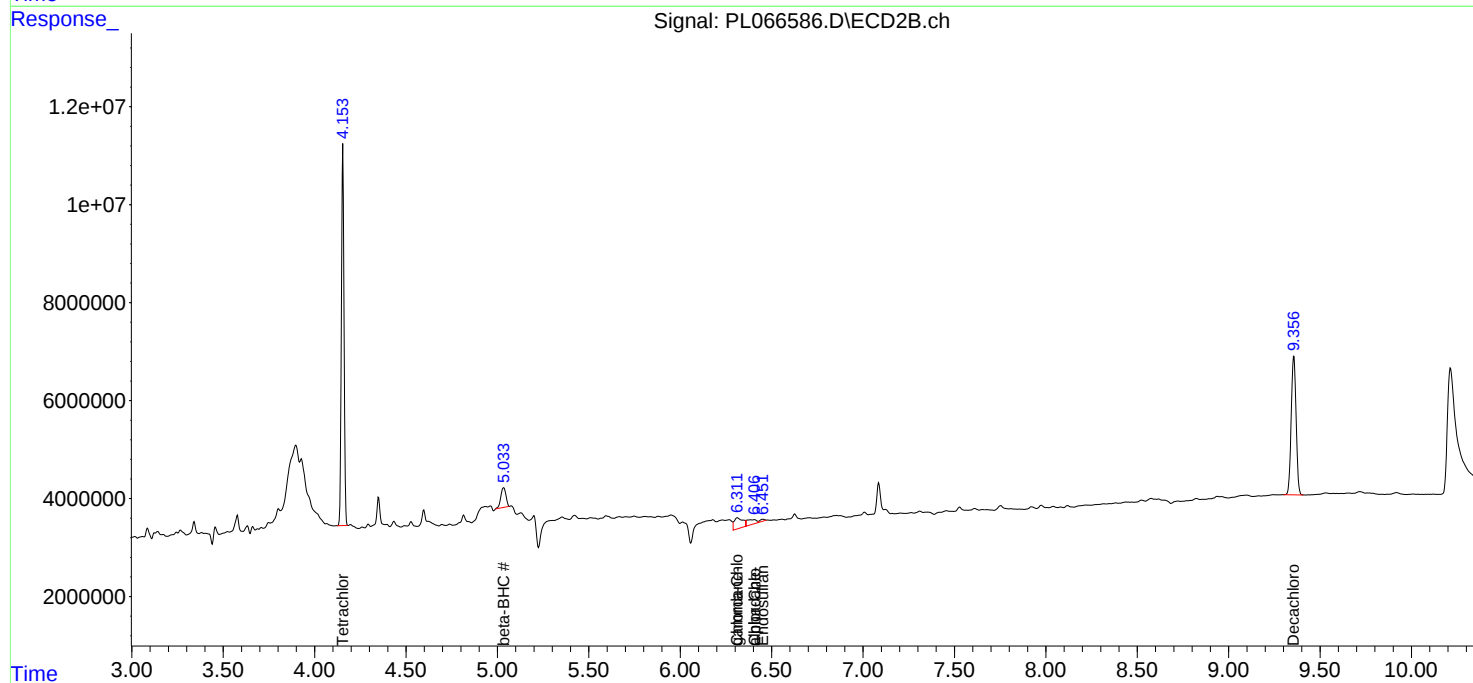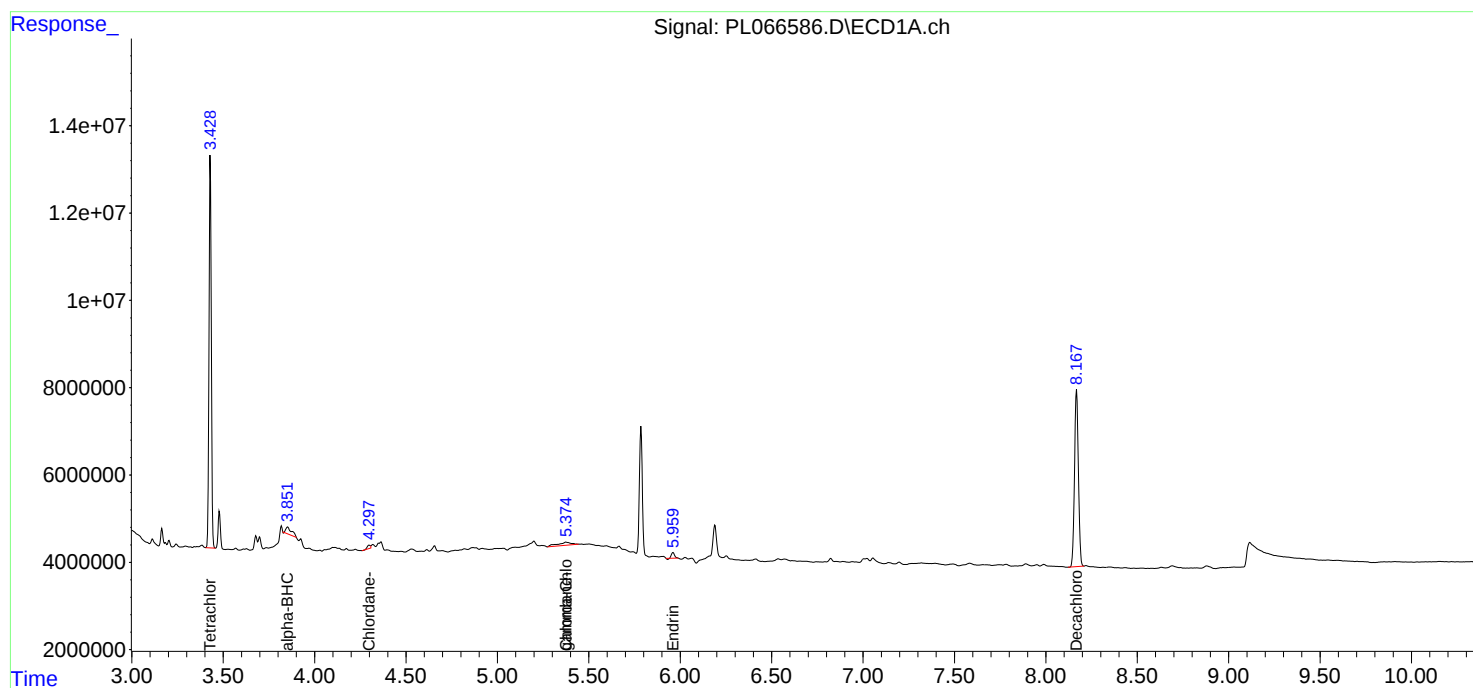


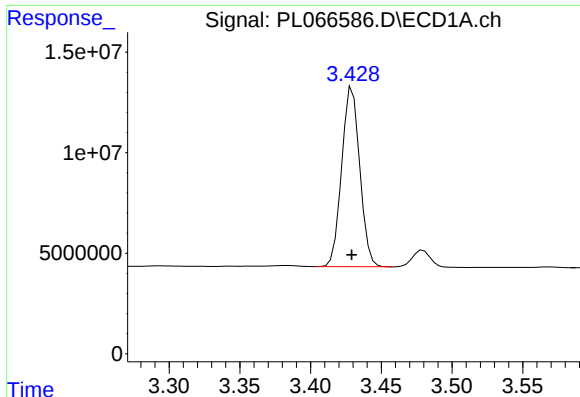

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 79567974
Conc: 21.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

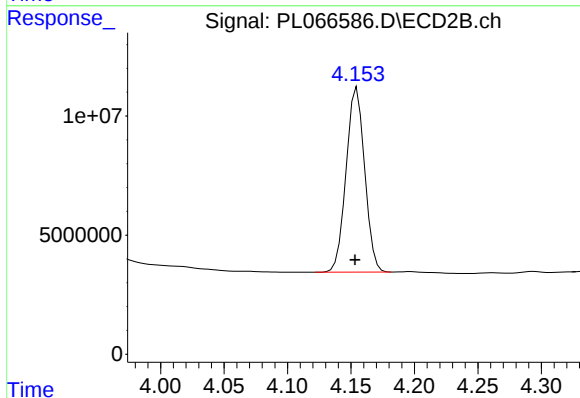


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 78615438
Conc: 22.38 ng/ml

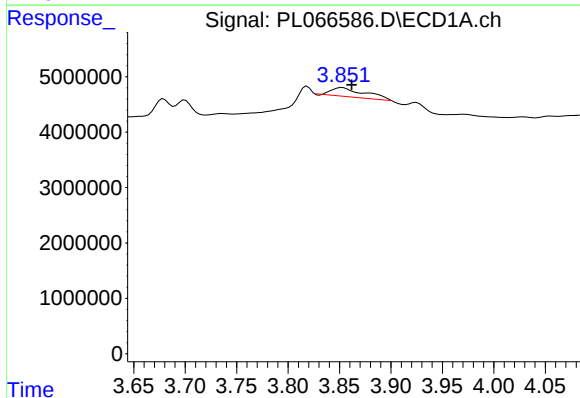


#2 alpha-BHC

R.T.: 3.853 min
Delta R.T.: -0.009 min
Response: 3510304
Conc: 0.56 ng/ml

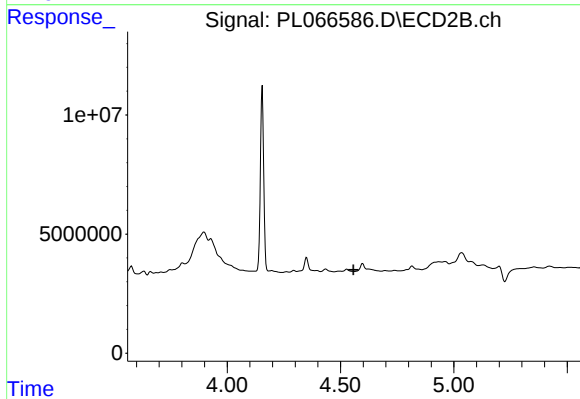

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.557 min
Response: 0
Conc: N.D.

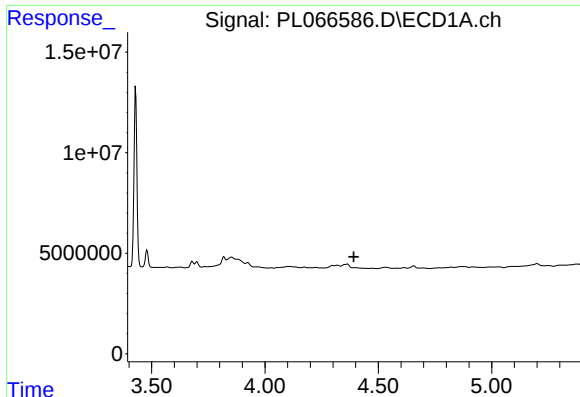

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

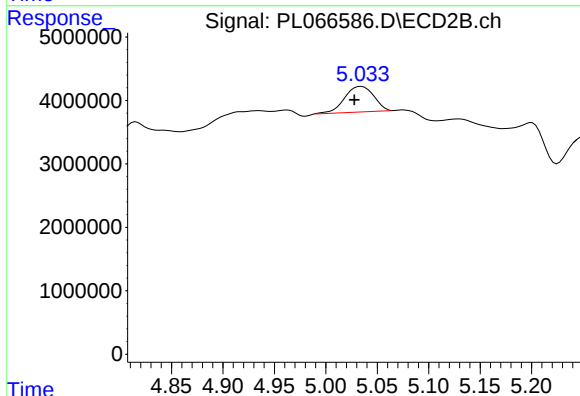


#6 beta-BHC

R.T.: 5.035 min
Delta R.T.: 0.007 min
Response: 7993853
Conc: 0.36 ng/ml

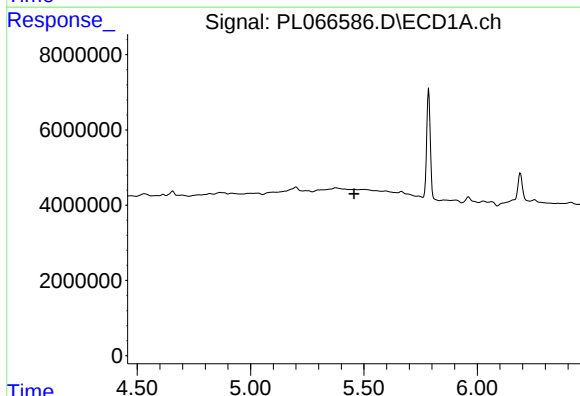


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.457 min
Response: 0
Conc: N.D.

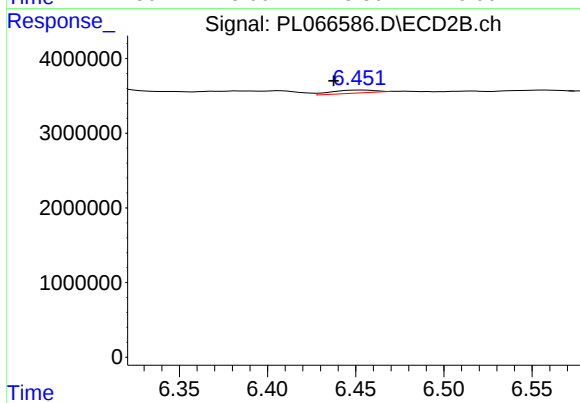

#9 Endosulfan I


R.T.: 6.452 min
Delta R.T.: 0.015 min
Response: 714267
Conc: 0.19 ng/ml

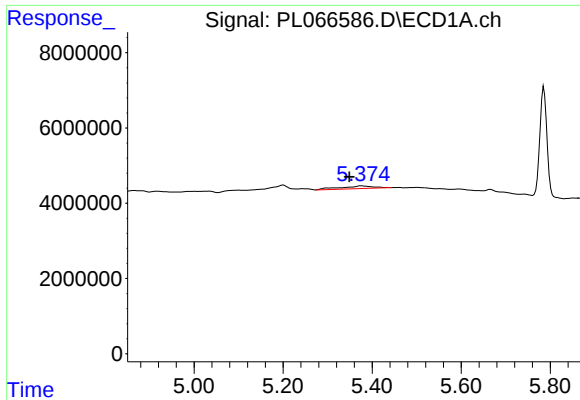

#10 gamma-Chlordane


R.T.: 5.375 min
Delta R.T.: 0.026 min
Response: 3690220
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

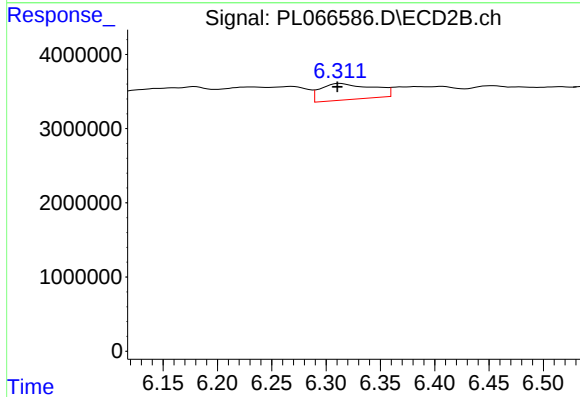


#10 gamma-Chlordane

R.T.: 6.313 min
Delta R.T.: 0.003 min
Response: 7310672
Conc: 1.76 ng/ml

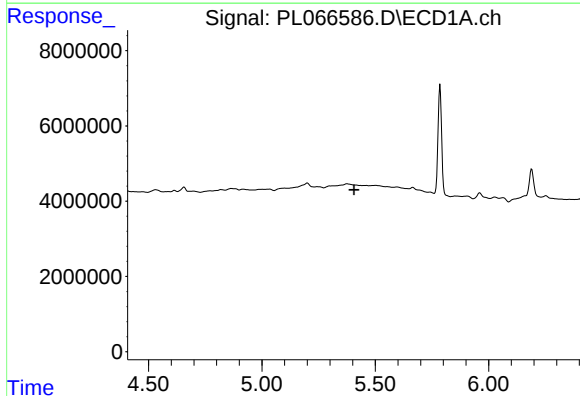


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

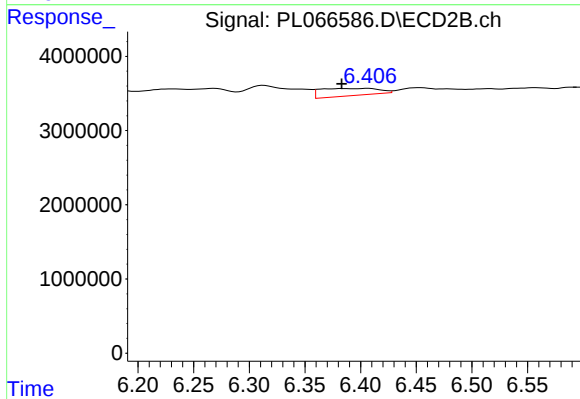

#11 alpha-Chlordane


R.T.: 6.407 min
Delta R.T.: 0.024 min
Response: 3565082
Conc: 0.86 ng/ml

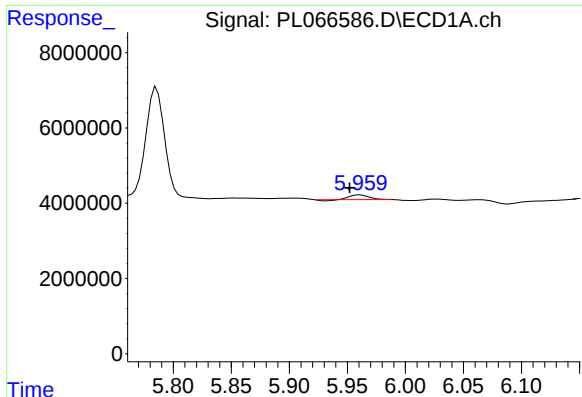

#14 Endrin


R.T.: 5.961 min
Delta R.T.: 0.008 min
Response: 1370753
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

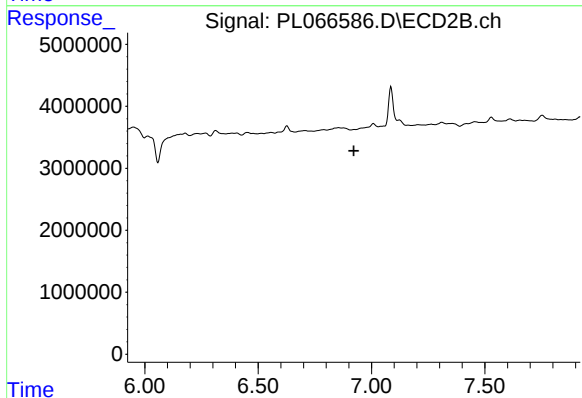


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

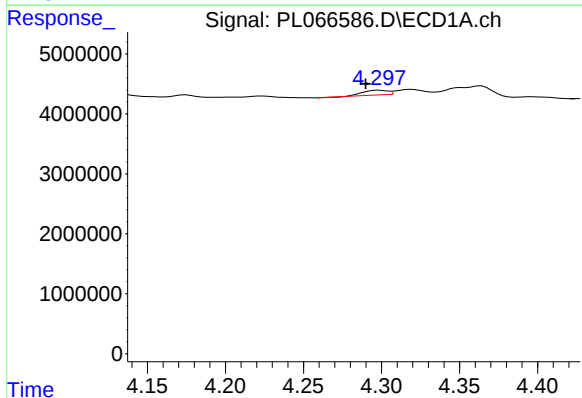


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.008 min
Response: 819308
Conc: 4.85 ng/ml

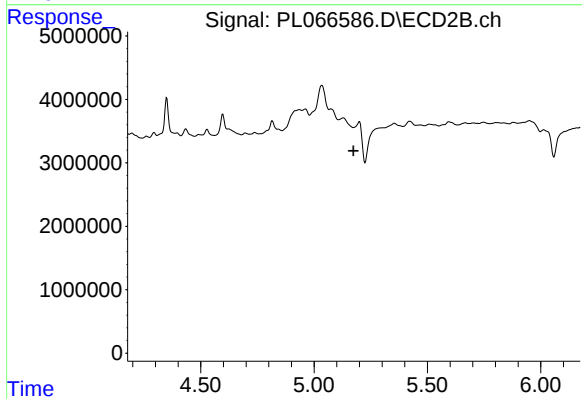

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

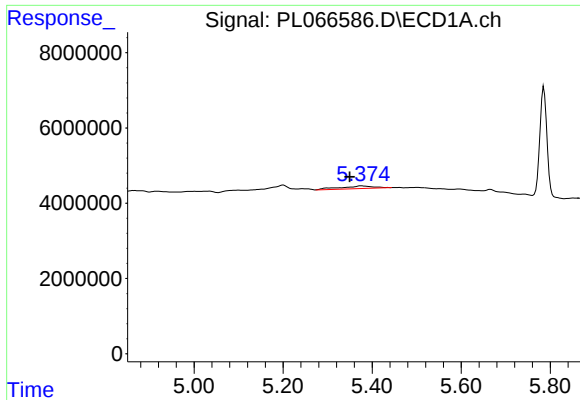

#25 Chlordane-3


R.T.: 5.375 min
Delta R.T.: 0.026 min
Response: 3690220
Conc: 7.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

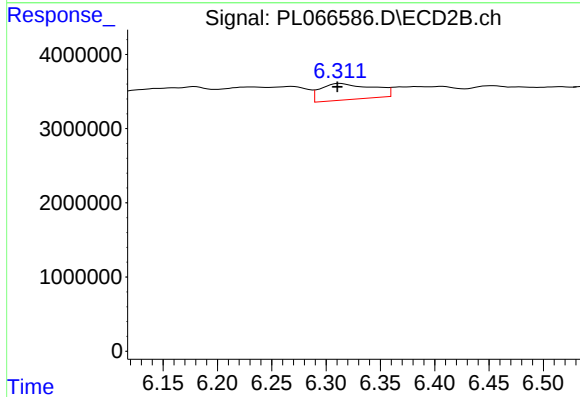


#25 Chlordane-3

R.T.: 6.313 min
Delta R.T.: 0.002 min
Response: 7310672
Conc: 13.04 ng/ml

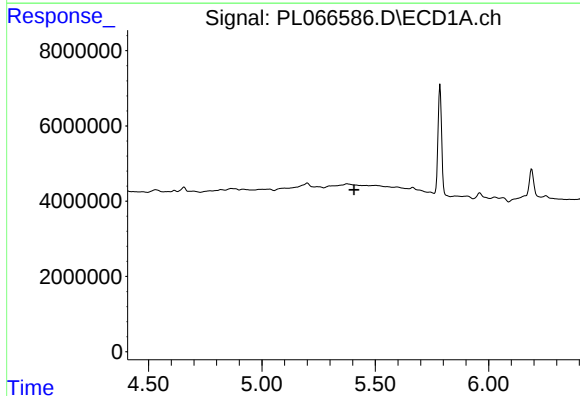


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

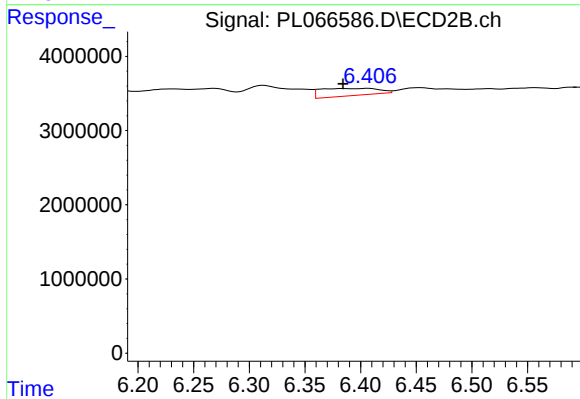

#26 Chlordane-4


R.T.: 6.407 min
Delta R.T.: 0.023 min
Response: 3565082
Conc: 5.31 ng/ml

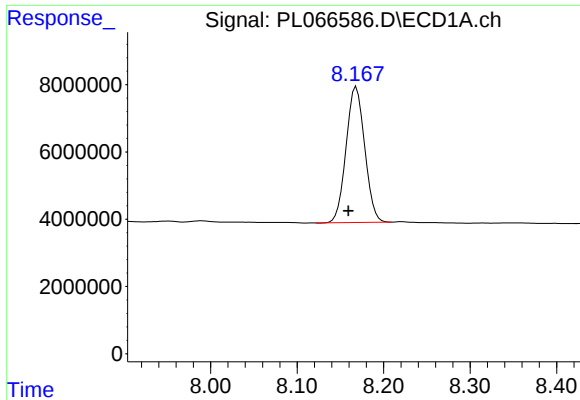

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.009 min
Response: 60122370
Conc: 15.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

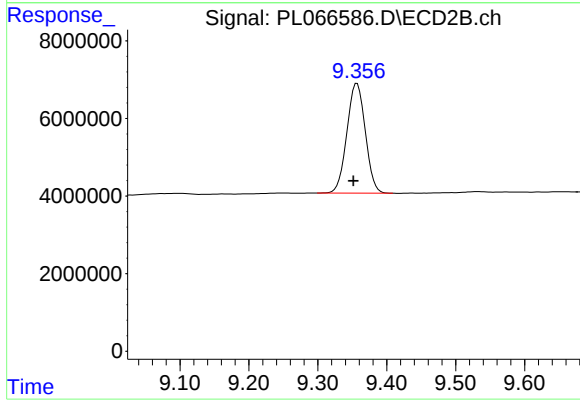

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 52488088
Conc: 16.97 ng/ml