

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 23:36
 Operator : AR\AJ
 Sample : M2196-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:56:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	82295584	84310395	21.840	24.006
28)	SA Decachlor...	8.166	9.357	67693398	60309677	17.655	19.495
Target Compounds							
2)	A alpha-BHC	3.855	0.000	4611641	0	0.741	N.D. #
6)	B beta-BHC	0.000	5.034	0	8206199	N.D.	0.460 #
9)	A Endosulfan I	0.000	6.453f	0	1018989	N.D.	0.268 #
10)	B gamma-Chl...	0.000	6.313	0	7635929	N.D.	1.834 #
11)	B alpha-Chl...	0.000	6.407f	0	5960197	N.D.	1.437 #
23)	Chlordane-1	4.296	0.000	1101303	0	6.515	N.D. #
25)	Chlordane-3	0.000	6.313	0	7635929	N.D.	13.623 #
26)	Chlordane-4	0.000	6.407f	0	5960197	N.D.	8.878 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 23:36
Operator : AR\AJ
Sample : M2196-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:56:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

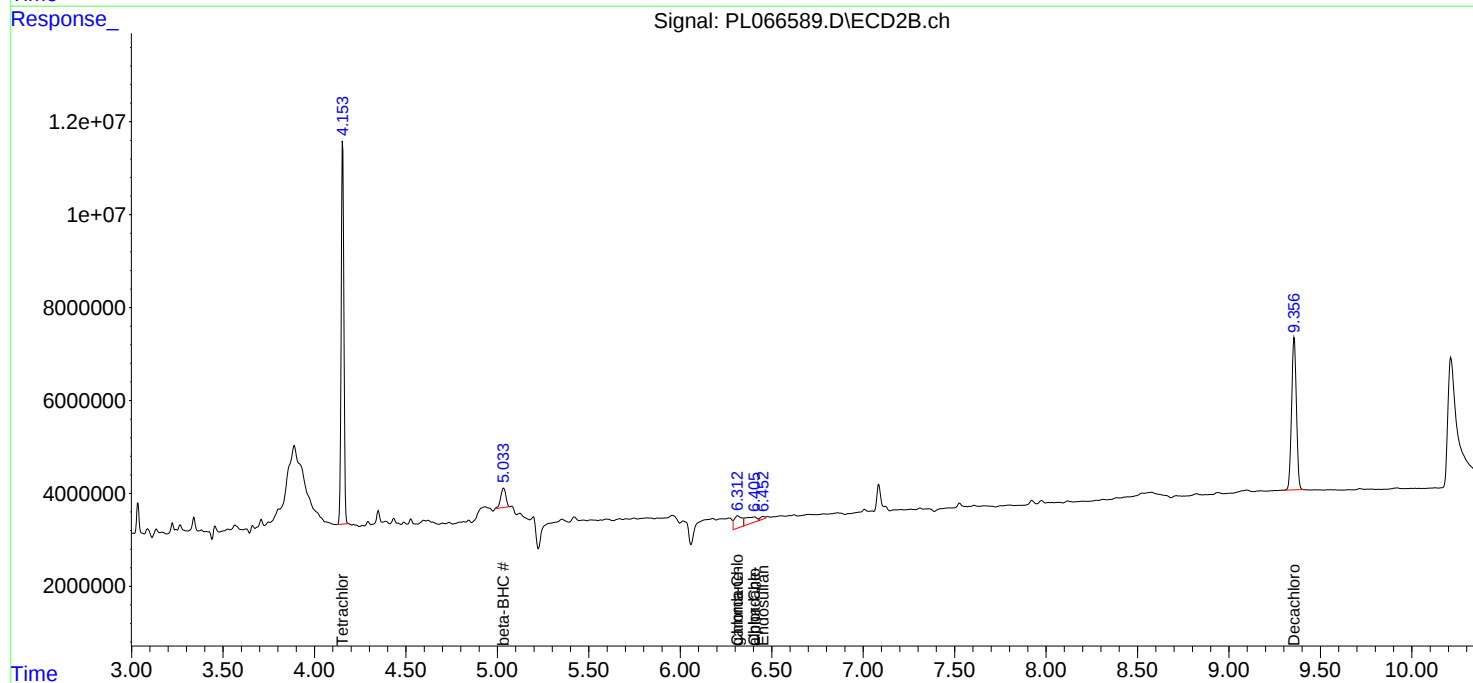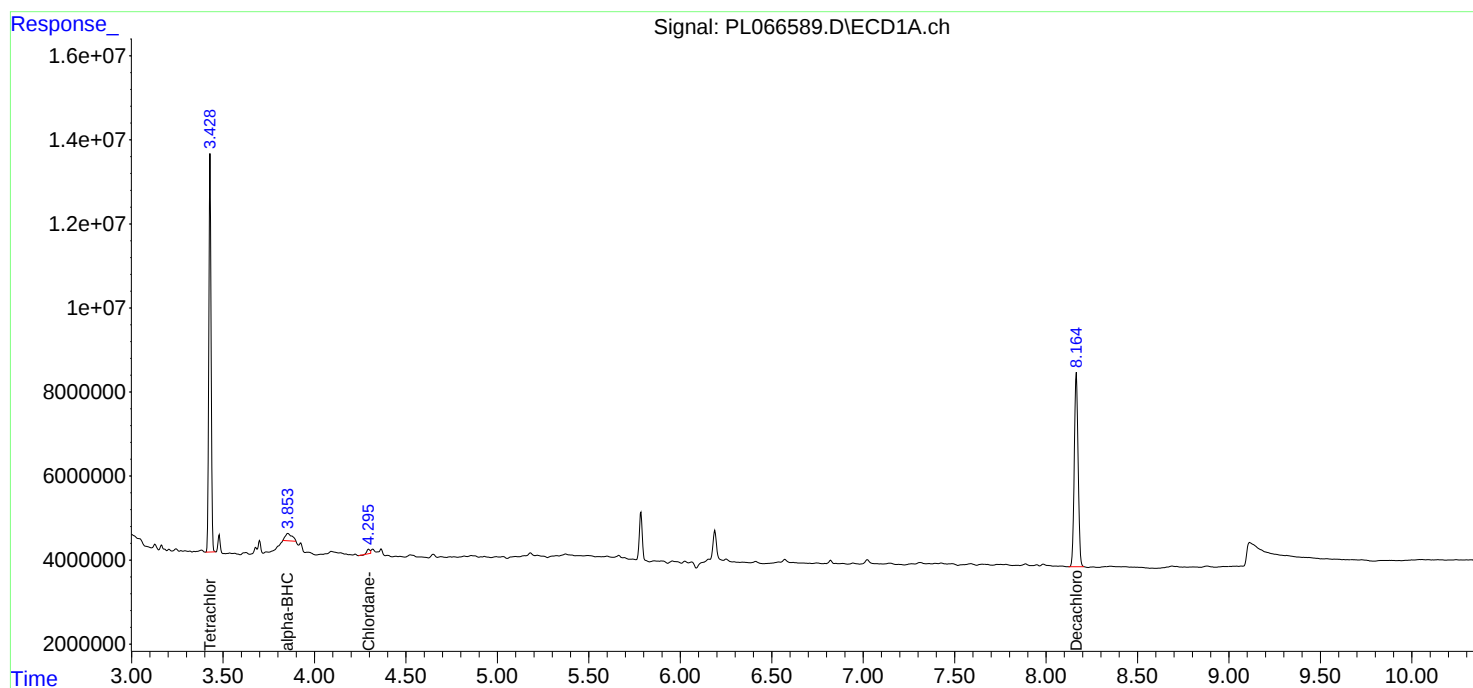


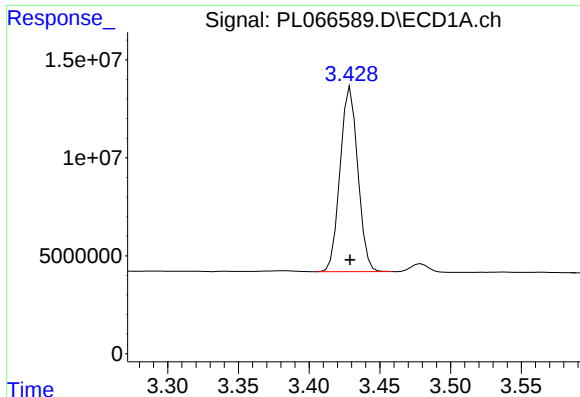

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 82295584
Conc: 21.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

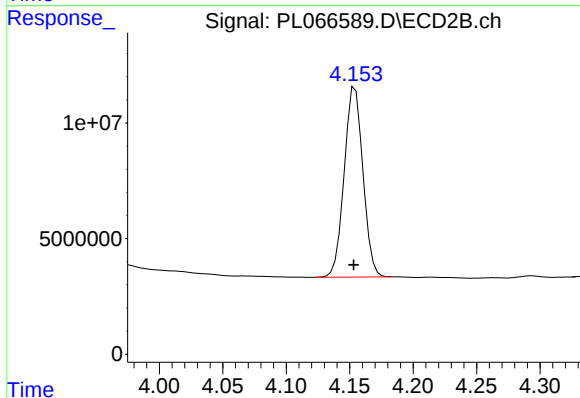


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 84310395
Conc: 24.01 ng/ml

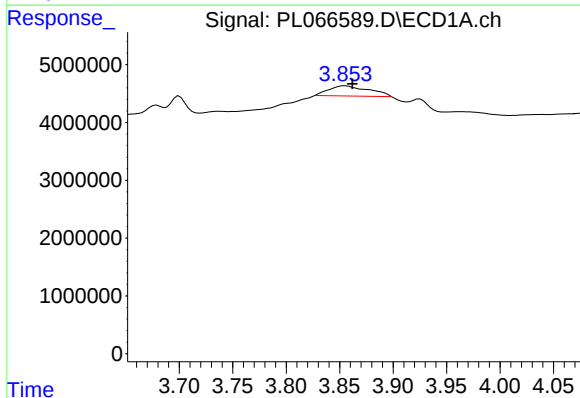


#2 alpha-BHC

R.T.: 3.855 min
Delta R.T.: -0.007 min
Response: 4611641
Conc: 0.74 ng/ml

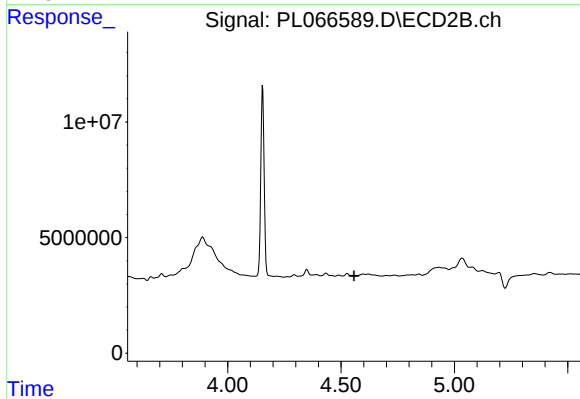

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.557 min
Response: 0
Conc: N.D.

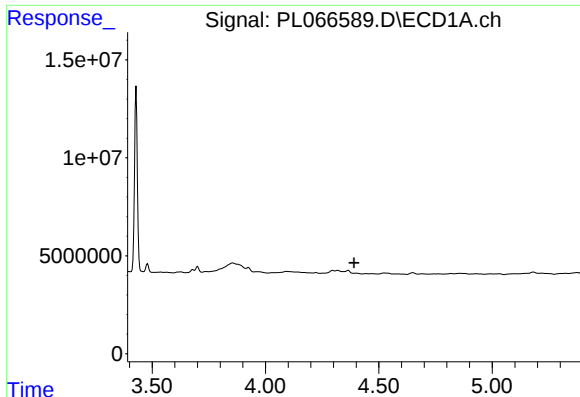

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

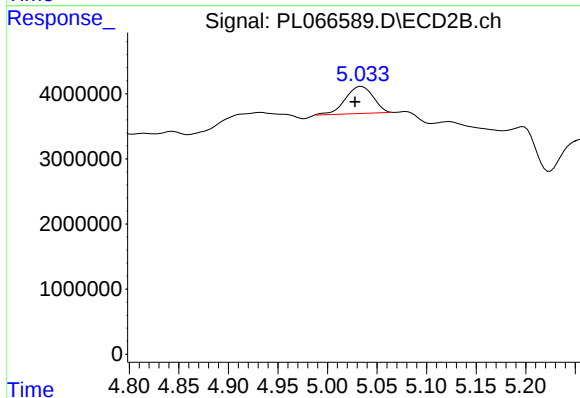


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 8206199
Conc: 0.46 ng/ml

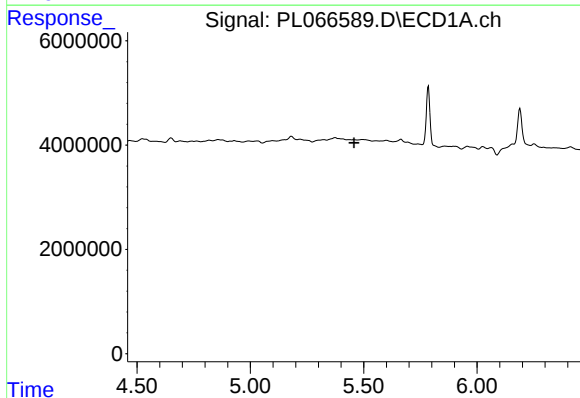


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.457 min
Response: 0
Conc: N.D.

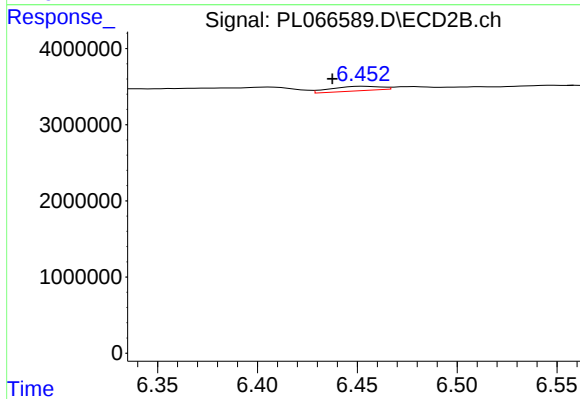

#9 Endosulfan I


R.T.: 6.453 min
Delta R.T.: 0.015 min
Response: 1018989
Conc: 0.27 ng/ml

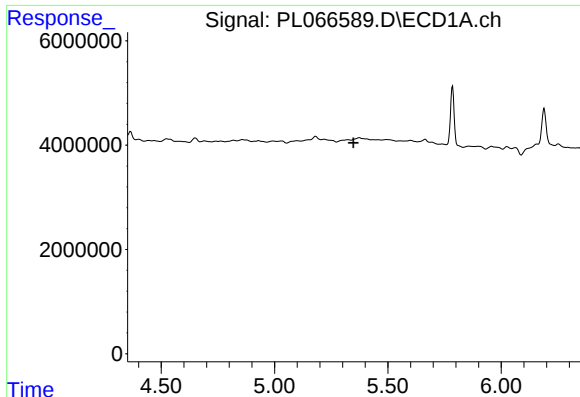

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

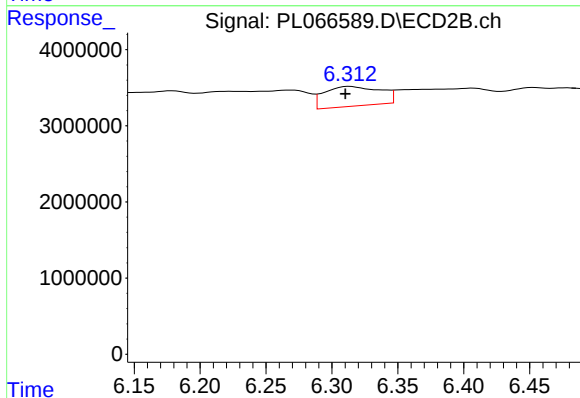


#10 gamma-Chlordane

R.T.: 6.313 min
Delta R.T.: 0.003 min
Response: 7635929
Conc: 1.83 ng/ml

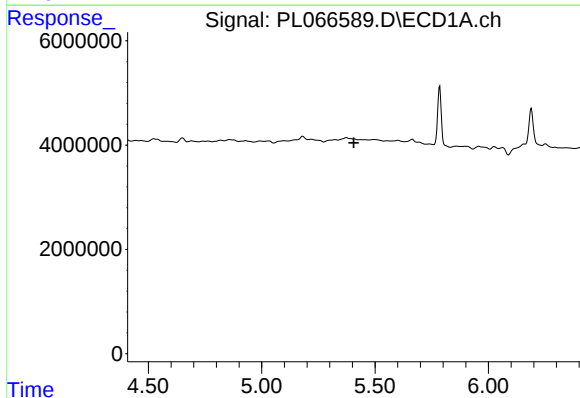


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

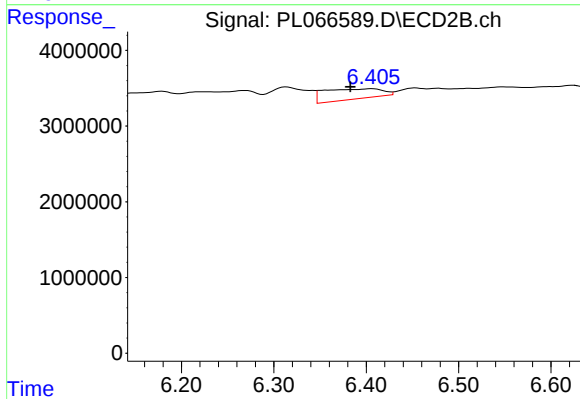

#11 alpha-Chlordane


R.T.: 6.407 min
Delta R.T.: 0.024 min
Response: 5960197
Conc: 1.44 ng/ml

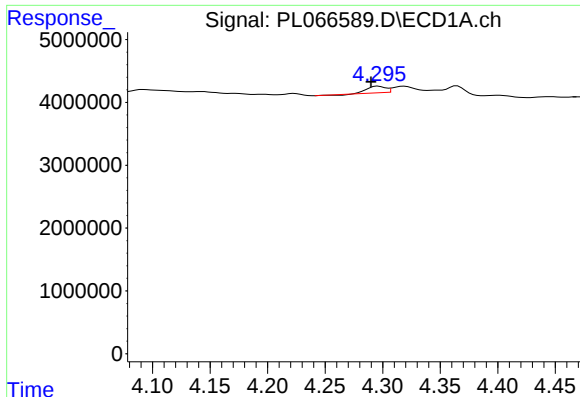

#23 Chlordane-1


R.T.: 4.296 min
Delta R.T.: 0.006 min
Response: 1101303
Conc: 6.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

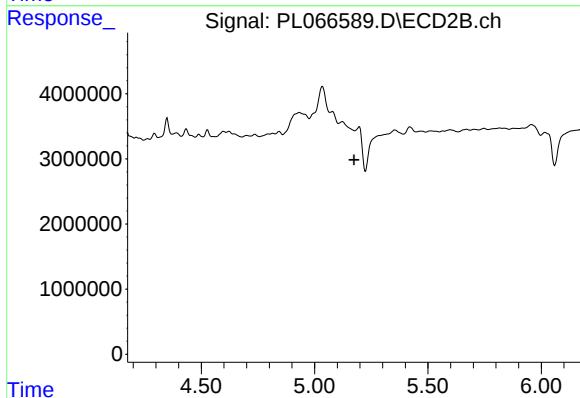


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

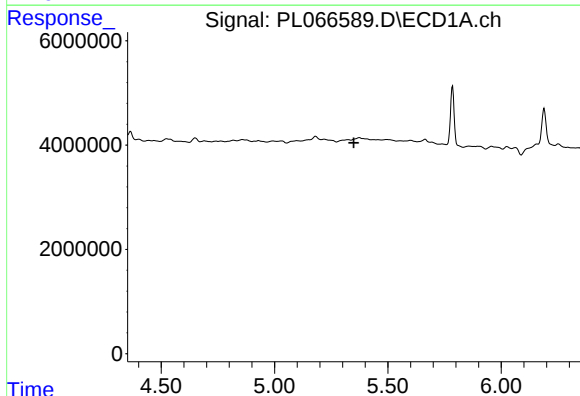


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

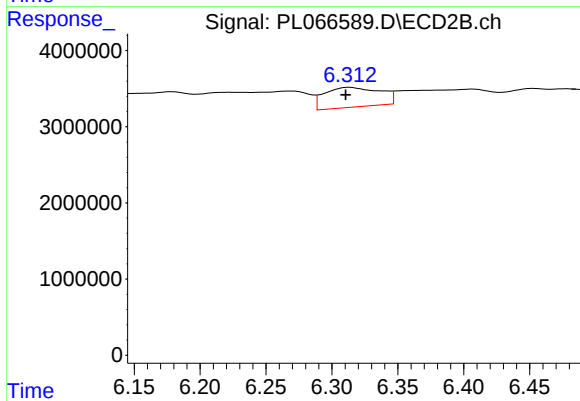

#25 Chlordane-3


R.T.: 6.313 min
Delta R.T.: 0.003 min
Response: 7635929
Conc: 13.62 ng/ml

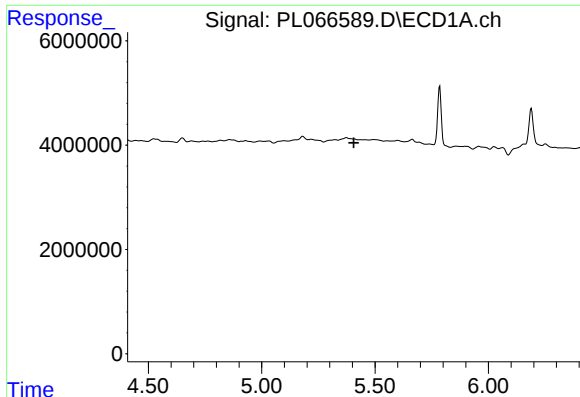

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

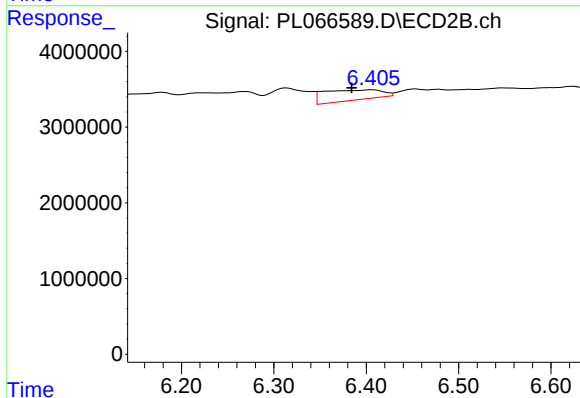


#26 Chlordane-4

R.T.: 6.407 min
Delta R.T.: 0.022 min
Response: 5960197
Conc: 8.88 ng/ml

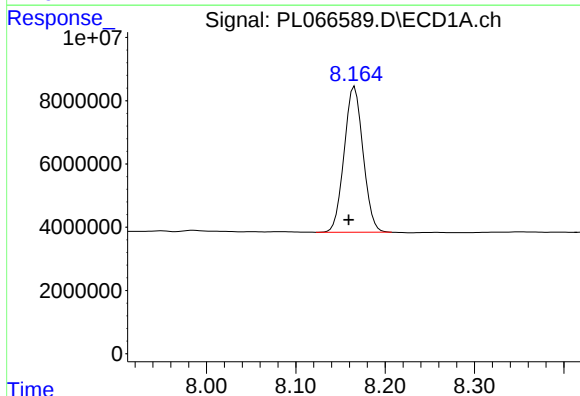

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.007 min
Response: 67693398
Conc: 17.66 ng/ml

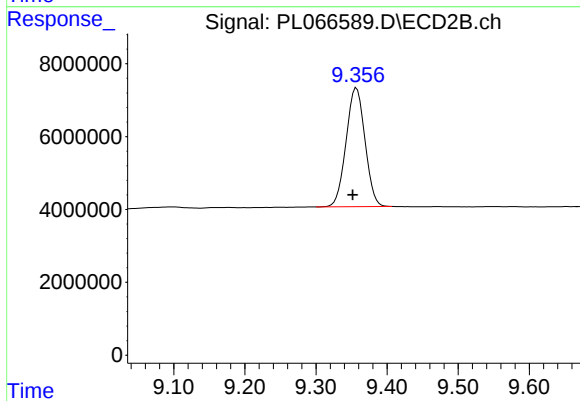

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 60309677
Conc: 19.50 ng/ml