

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 00:05
 Operator : AR\AJ
 Sample : M2202-02
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:56:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	79763749	79608523	21.168	22.667
28)	SA Decachlor...	8.166	9.358	66919943	59851114	17.453	19.347
Target Compounds							
2)	A alpha-BHC	3.855	0.000	5912469	0	0.950	N.D. #
6)	B beta-BHC	0.000	5.035	0	8430260	N.D.	0.563 #
9)	A Endosulfan I	0.000	6.453f	0	264031	N.D.	0.069 #
10)	B gamma-Chl...	0.000	6.315	0	4300675	N.D.	1.033 #
11)	B alpha-Chl...	0.000	6.408f	0	3630265	N.D.	0.875 #
15)	B Endosulfa...	0.000	7.122	0	1351274	N.D.	0.409 #
23)	Chlordane-1	4.297	0.000	1658253	0	9.810	N.D. #
25)	Chlordane-3	0.000	6.315	0	4300675	N.D.	7.673 #
26)	Chlordane-4	0.000	6.408f	0	3630265	N.D.	5.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 00:05
Operator : AR\AJ
Sample : M2202-02
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:56:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

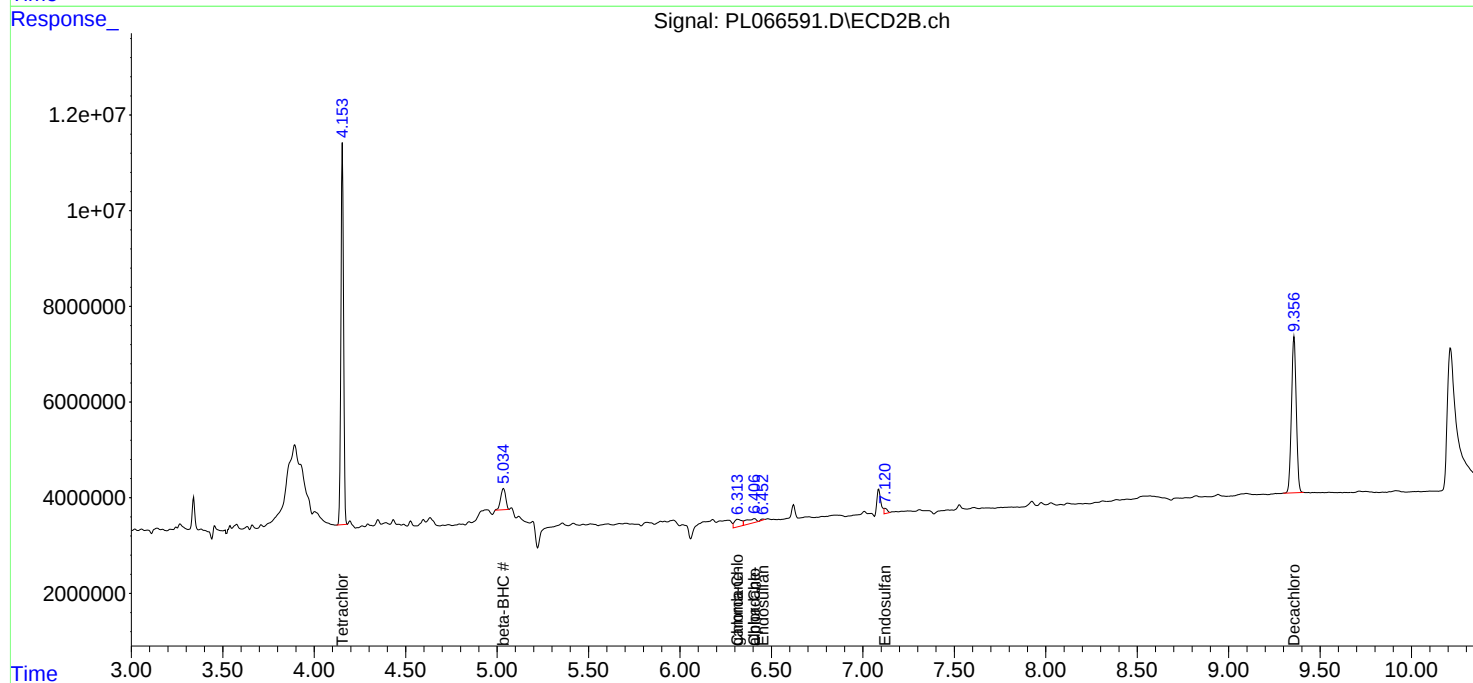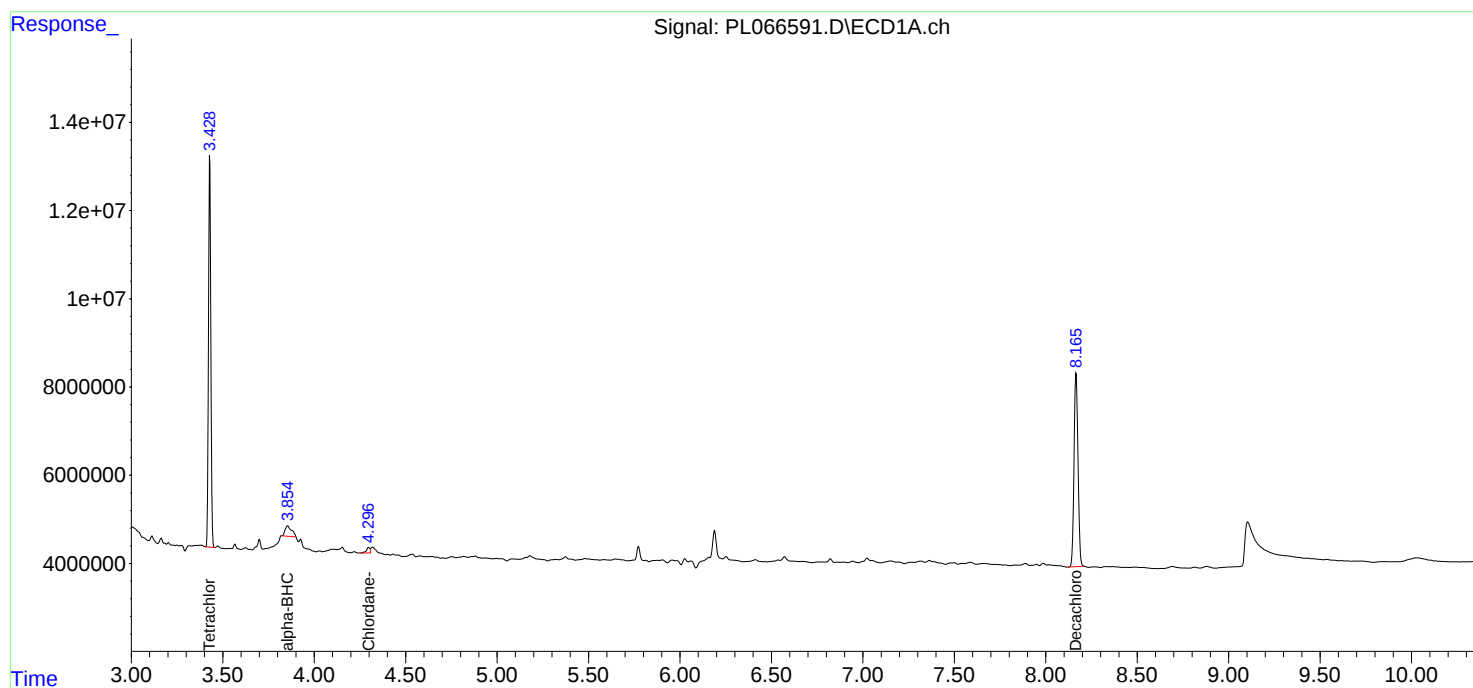


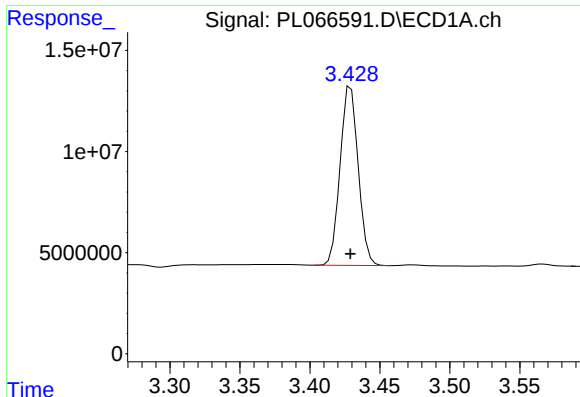

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 79763749
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

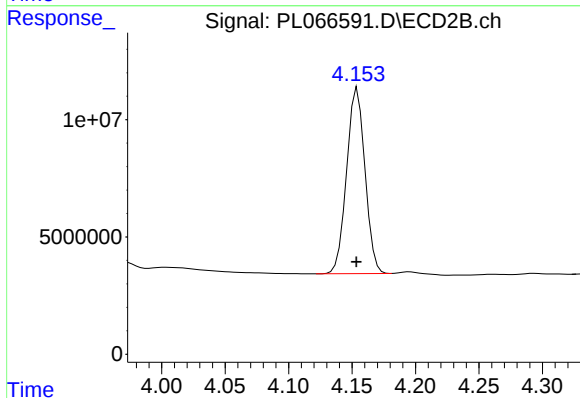


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 79608523
Conc: 22.67 ng/ml

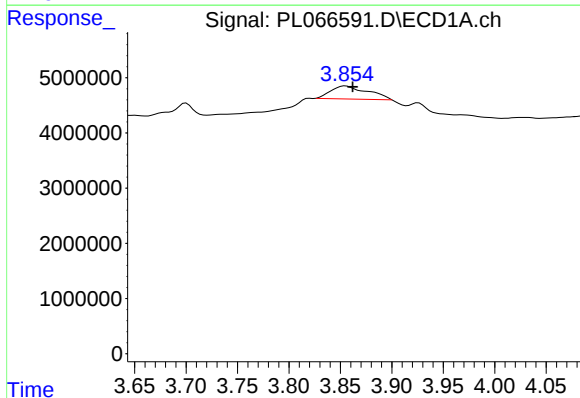


#2 alpha-BHC

R.T.: 3.855 min
Delta R.T.: -0.007 min
Response: 5912469
Conc: 0.95 ng/ml

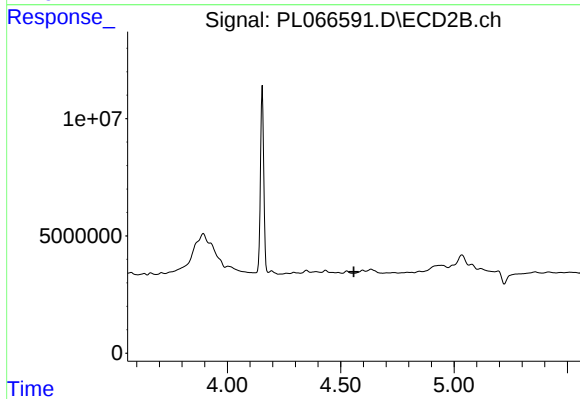

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

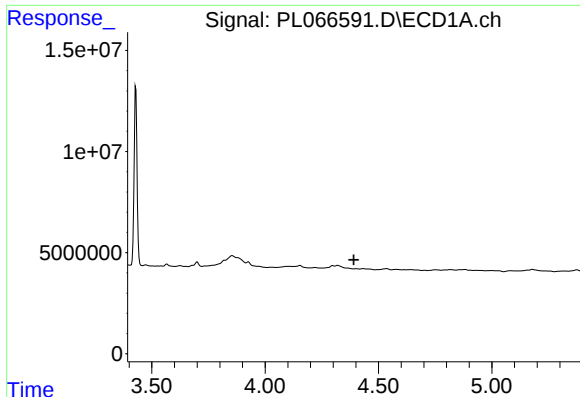

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

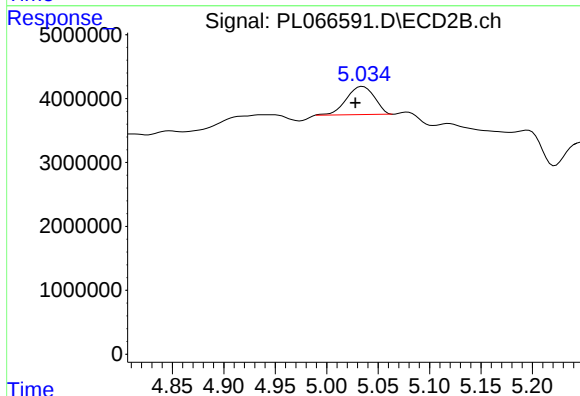


#6 beta-BHC

R.T.: 5.035 min
Delta R.T.: 0.007 min
Response: 8430260
Conc: 0.56 ng/ml

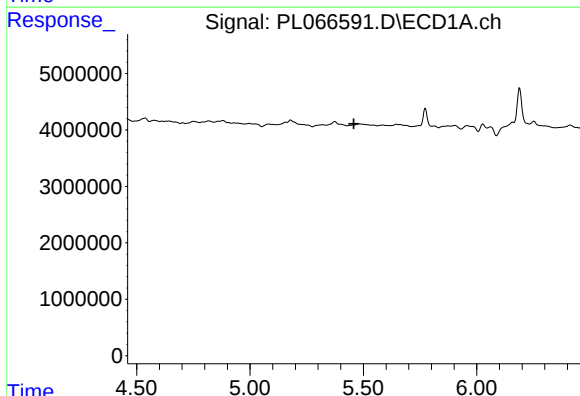


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.457 min
Response: 0
Conc: N.D.

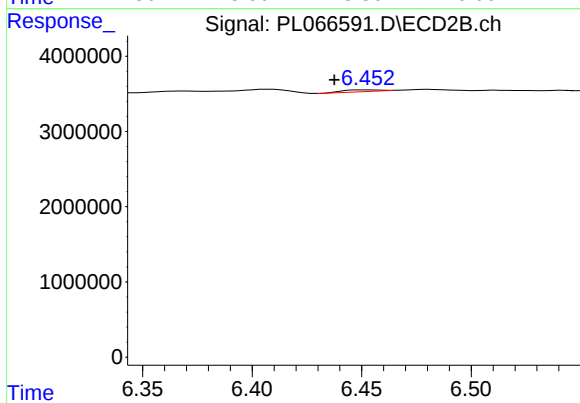

#9 Endosulfan I


R.T.: 6.453 min
Delta R.T.: 0.015 min
Response: 264031
Conc: 0.07 ng/ml

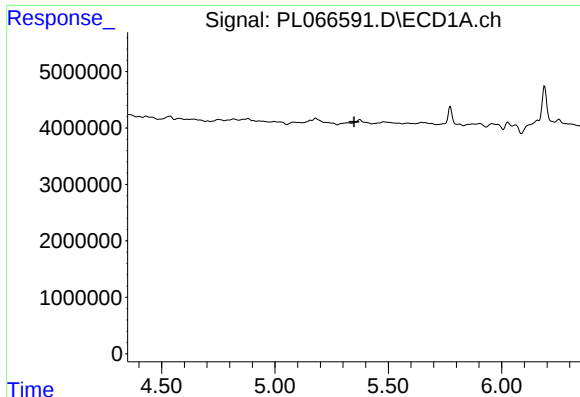

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

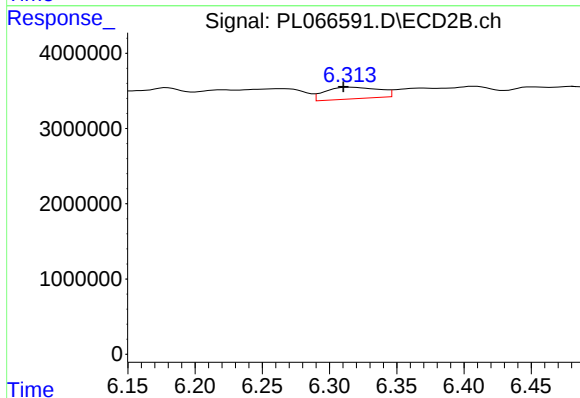


#10 gamma-Chlordane

R.T.: 6.315 min
Delta R.T.: 0.004 min
Response: 4300675
Conc: 1.03 ng/ml

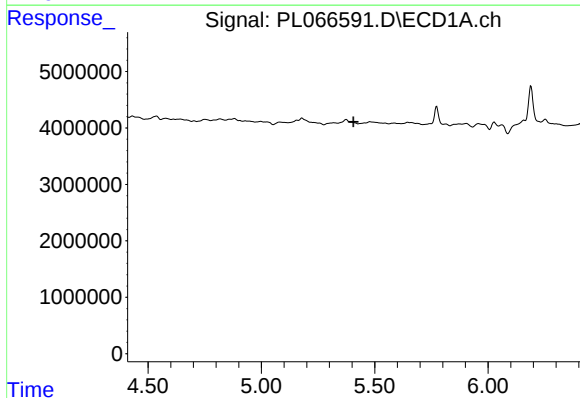


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

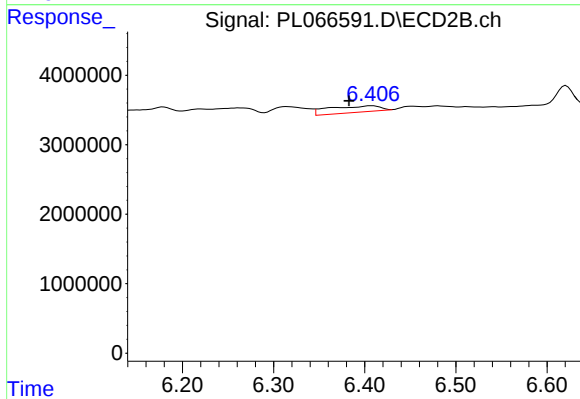

#11 alpha-Chlordane


R.T.: 6.408 min
Delta R.T.: 0.025 min
Response: 3630265
Conc: 0.88 ng/ml

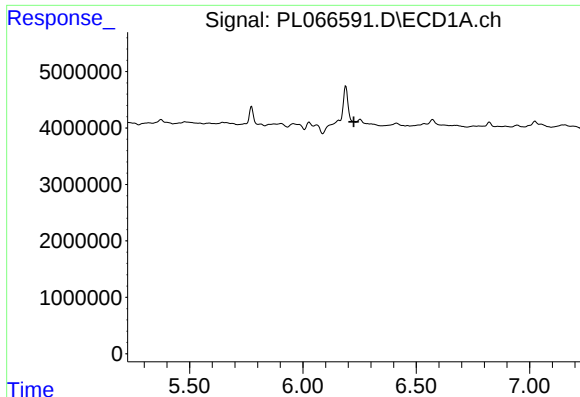

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.224 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

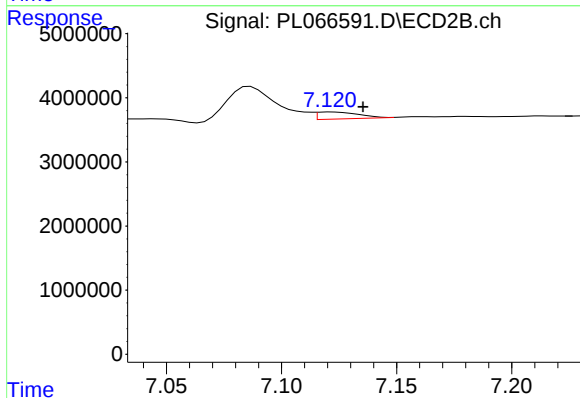


#15 Endosulfan II

R.T.: 7.122 min
Delta R.T.: -0.014 min
Response: 1351274
Conc: 0.41 ng/ml

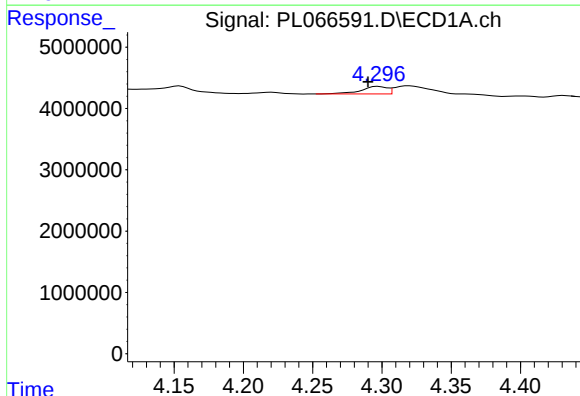


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.007 min
Response: 1658253
Conc: 9.81 ng/ml

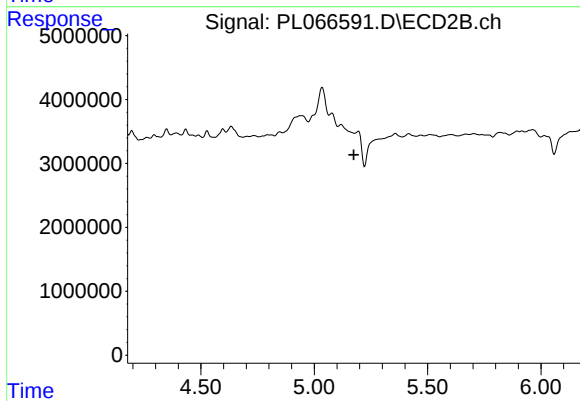

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

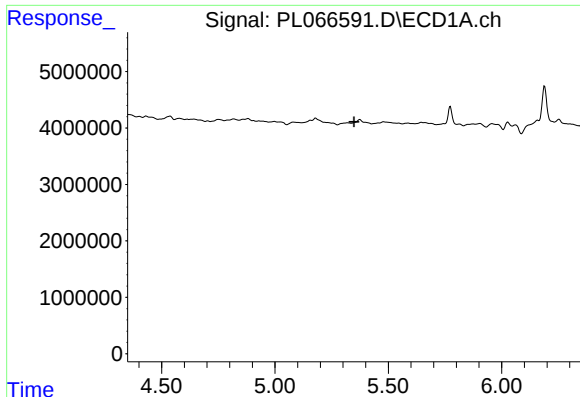

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

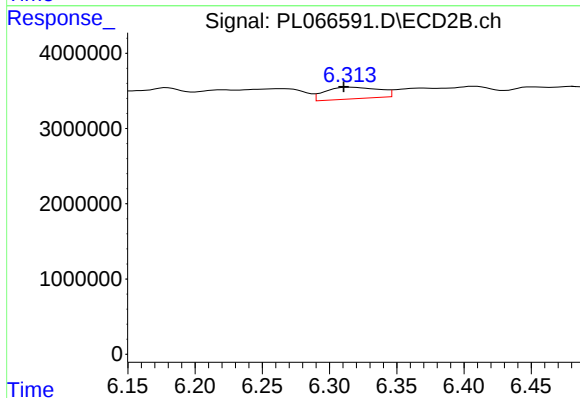


#25 Chlordane-3

R.T.: 6.315 min
Delta R.T.: 0.004 min
Response: 4300675
Conc: 7.67 ng/ml

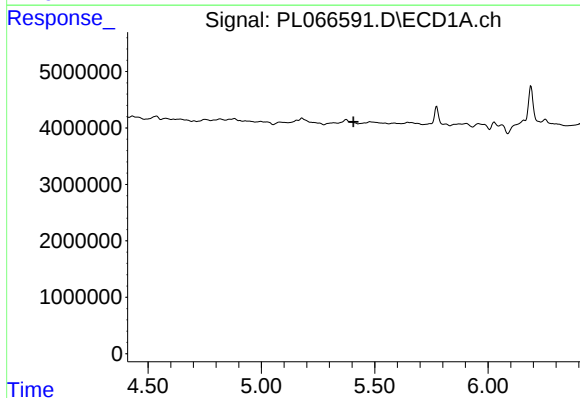


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

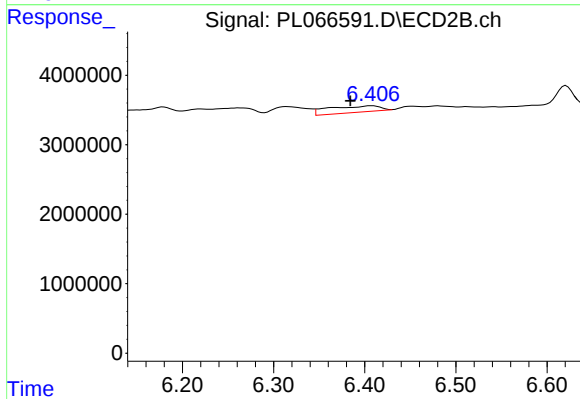

#26 Chlordane-4


R.T.: 6.408 min
Delta R.T.: 0.024 min
Response: 3630265
Conc: 5.41 ng/ml

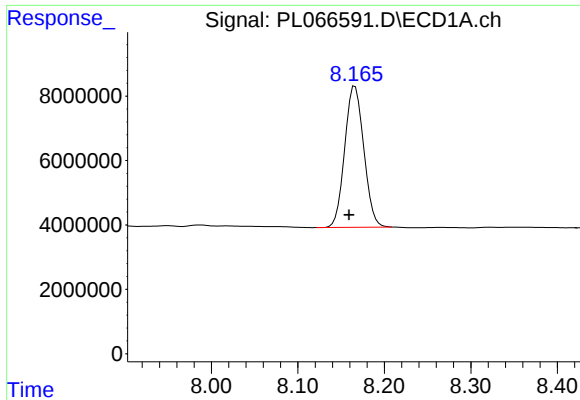

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.007 min
Response: 66919943
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

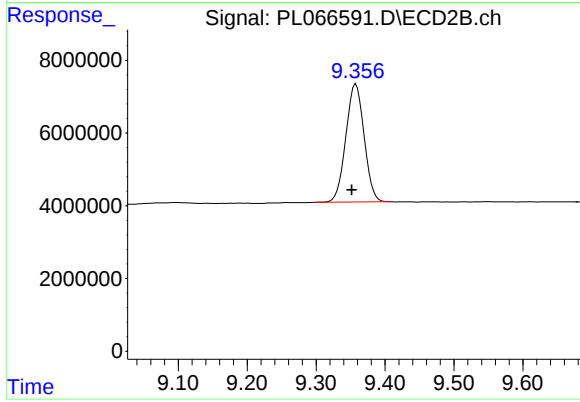

#28 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: 0.006 min
Response: 59851114
Conc: 19.35 ng/ml