

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 00:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:57:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	88398245	87929965	23.460	25.037
28)	SA Decachlor...	8.167	9.357	76166863	67791549	19.865	21.914
Target Compounds							
2)	A alpha-BHC	3.850	0.000	5652672	0	0.908	N.D. #
6)	B beta-BHC	4.404	5.034	1260345	8686388	0.476	0.682 #
8)	B Heptachlo...	0.000	6.072	0	2610440	N.D.	0.706 #
10)	B gamma-Chl...	0.000	6.316	0	818046	N.D.	0.197 #
14)	MA Endrin	5.959	0.000	1599493	0	0.367	N.D. #
21)	B Endrin ke...	0.000	7.975	0	871299	N.D.	0.245 #
23)	Chlordane-1	4.316f	0.000	4085101	0	24.167	N.D. #
25)	Chlordane-3	0.000	6.316	0	818046	N.D.	1.459 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 00:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:57:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

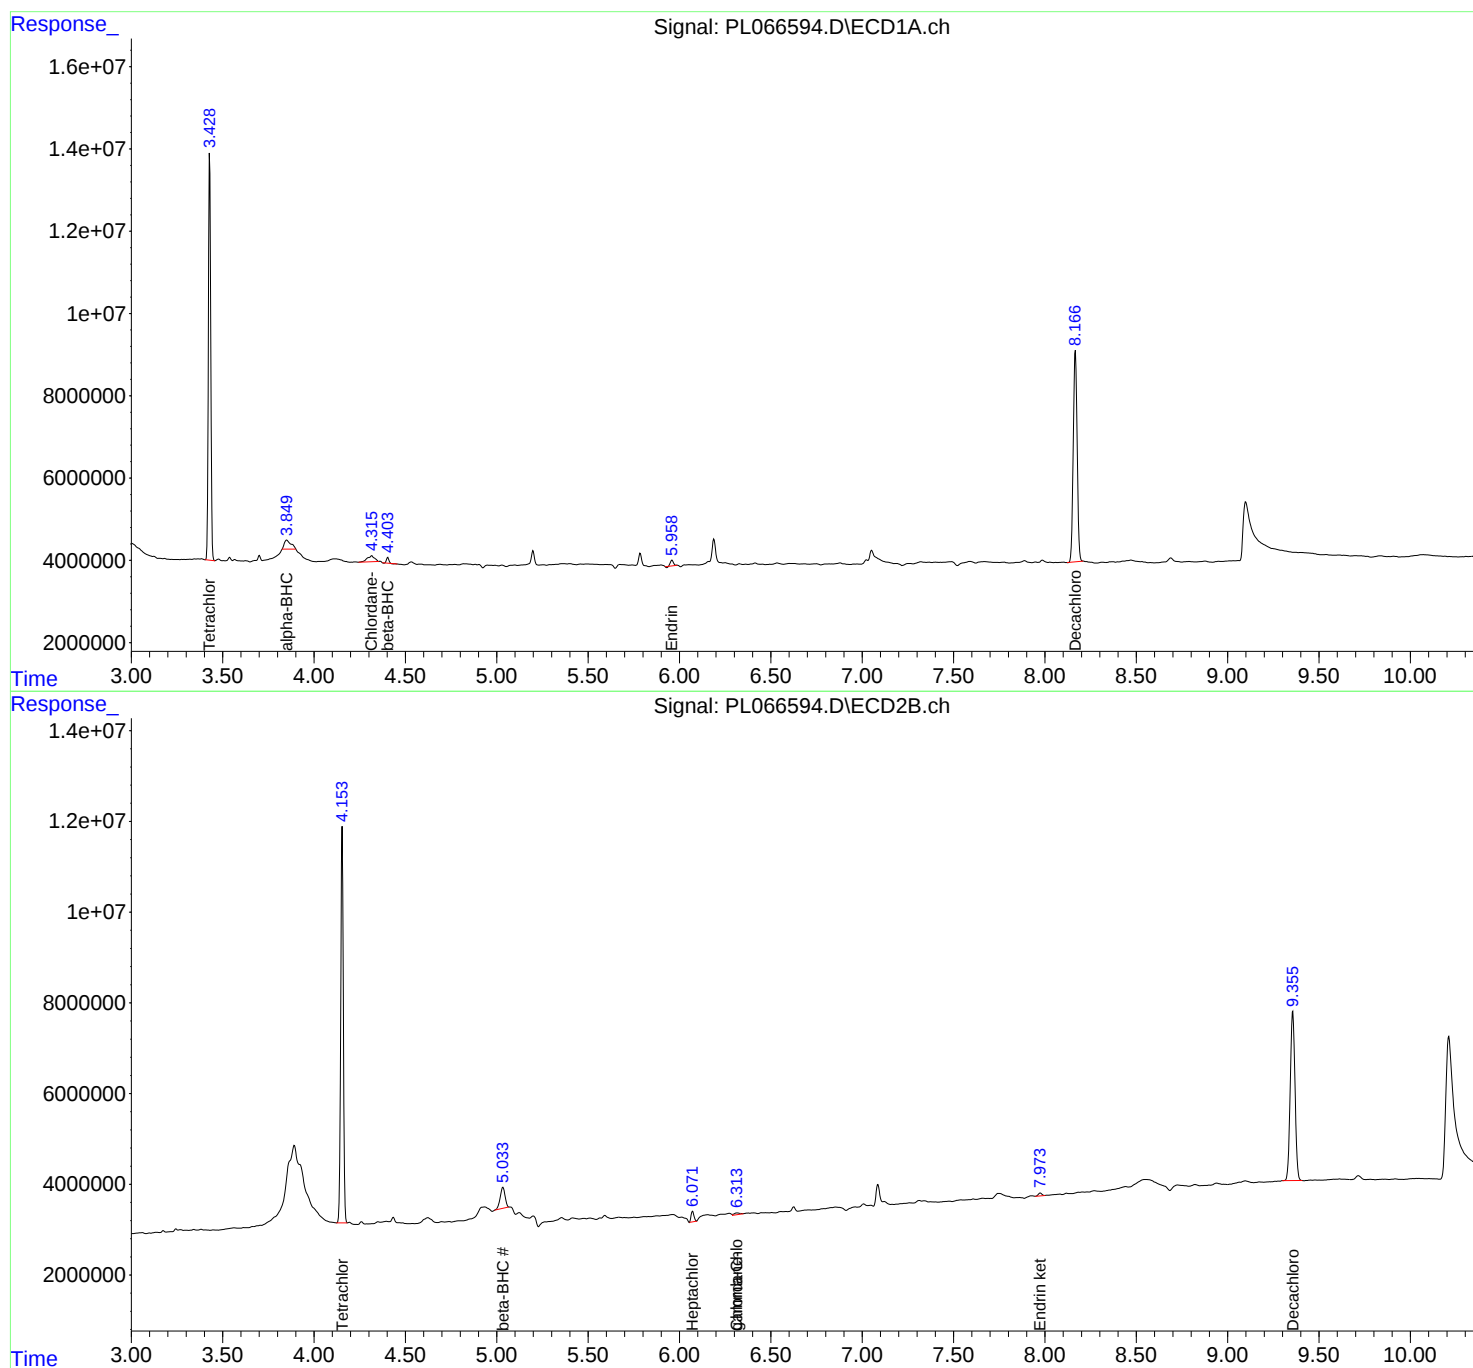


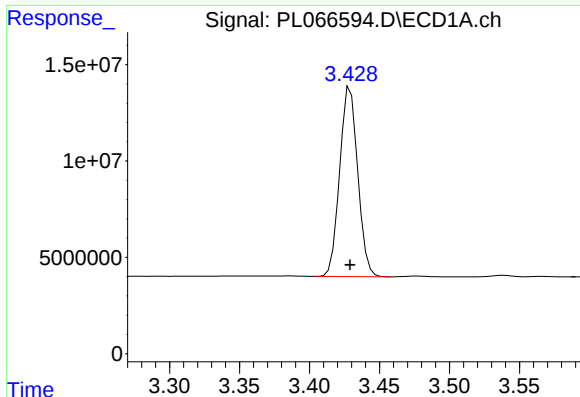

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 88398245
Conc: 23.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

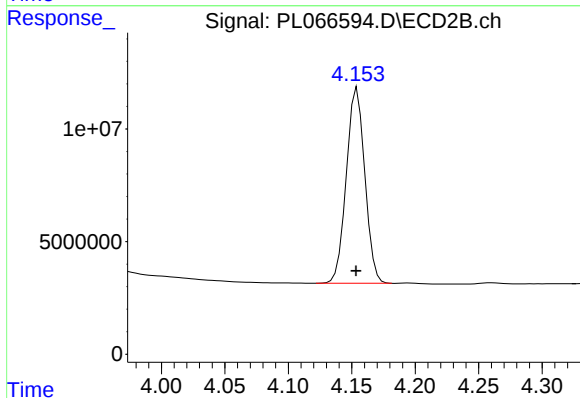


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 87929965
Conc: 25.04 ng/ml

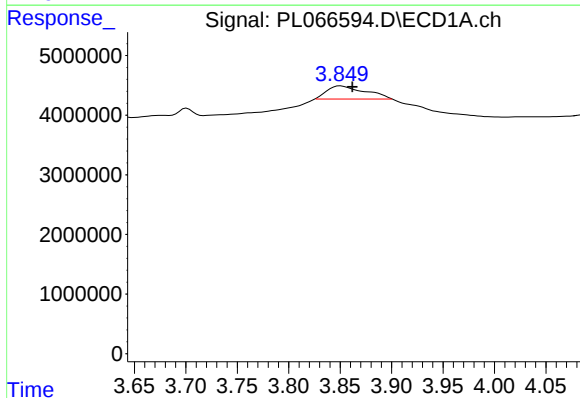


#2 alpha-BHC

R.T.: 3.850 min
Delta R.T.: -0.011 min
Response: 5652672
Conc: 0.91 ng/ml

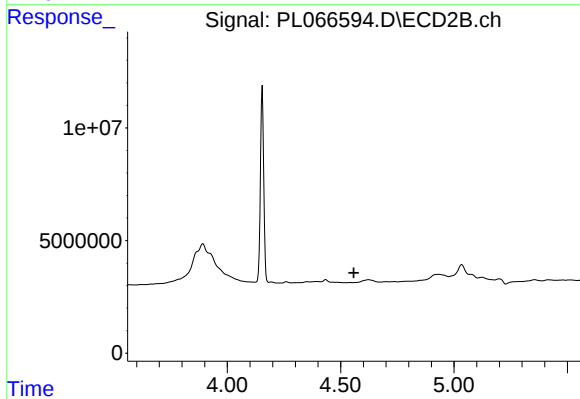

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.557 min
Response: 0
Conc: N.D.

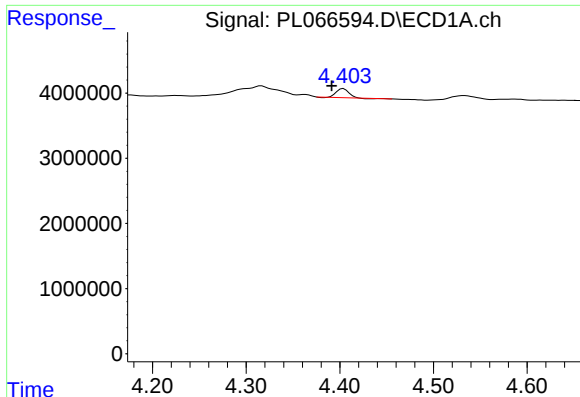

#6 beta-BHC


R.T.: 4.404 min
Delta R.T.: 0.013 min
Response: 1260345
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

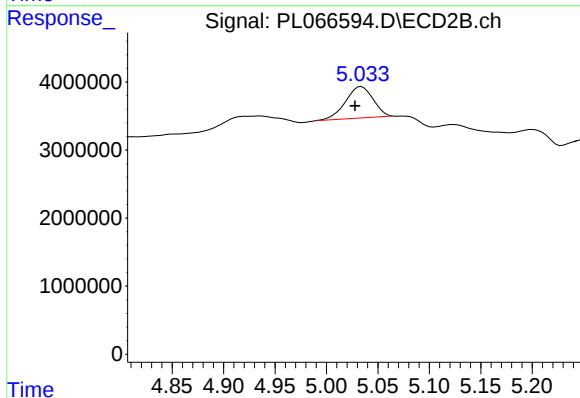


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 8686388
Conc: 0.68 ng/ml

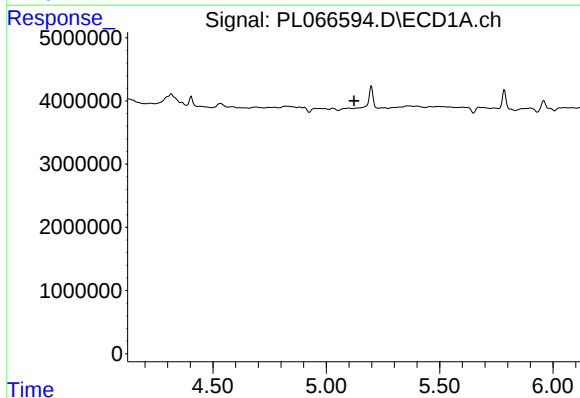


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

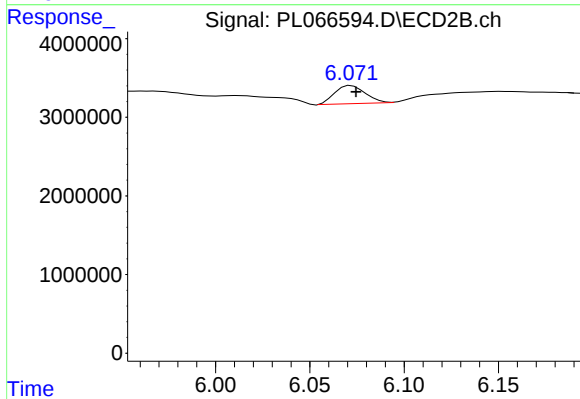

#8 Heptachlor epoxide


R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 2610440
Conc: 0.71 ng/ml

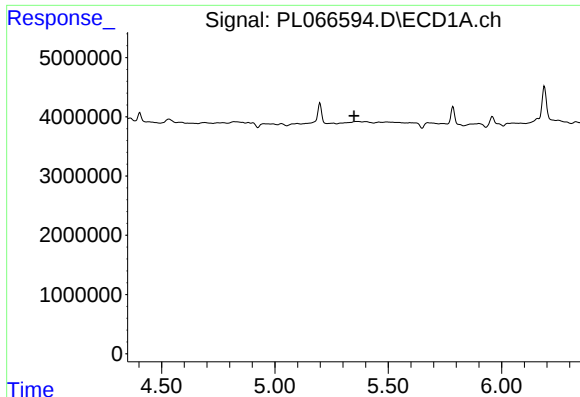

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

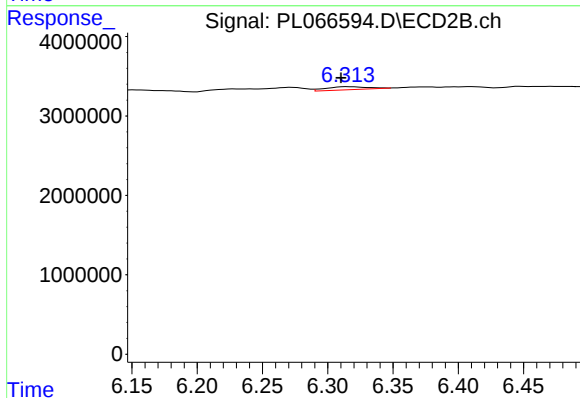


#10 gamma-Chlordane

R.T.: 6.316 min
Delta R.T.: 0.006 min
Response: 818046
Conc: 0.20 ng/ml

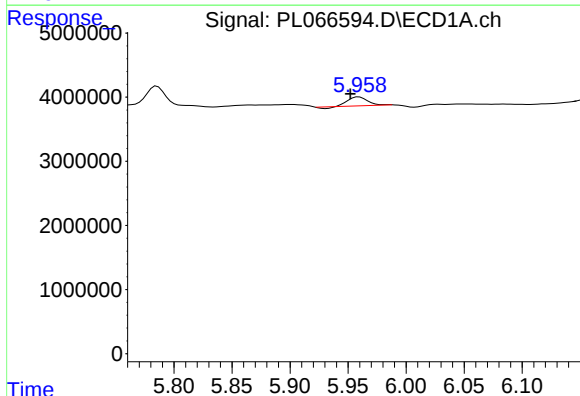


#14 Endrin

R.T.: 5.959 min
Delta R.T.: 0.007 min
Response: 1599493
Conc: 0.37 ng/ml

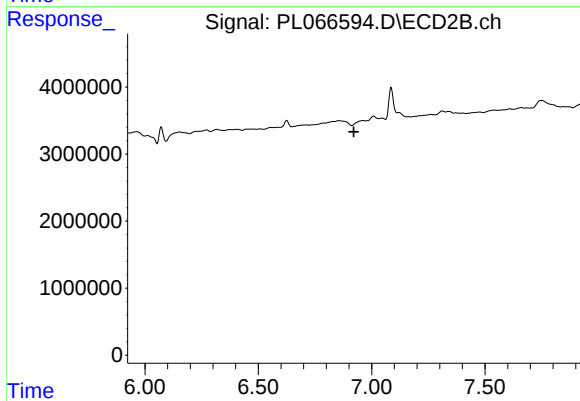

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.921 min
Response: 0
Conc: N.D.

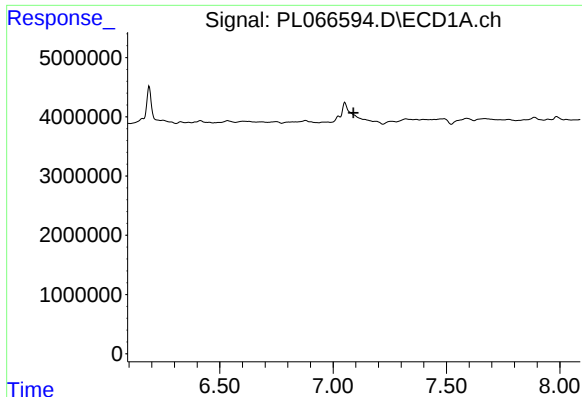

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

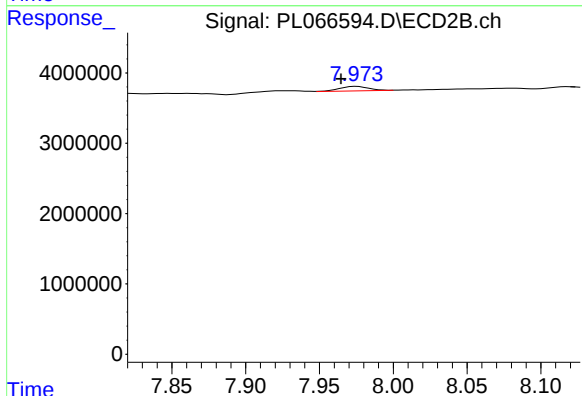


#21 Endrin ketone

R.T.: 7.975 min
Delta R.T.: 0.010 min
Response: 871299
Conc: 0.25 ng/ml

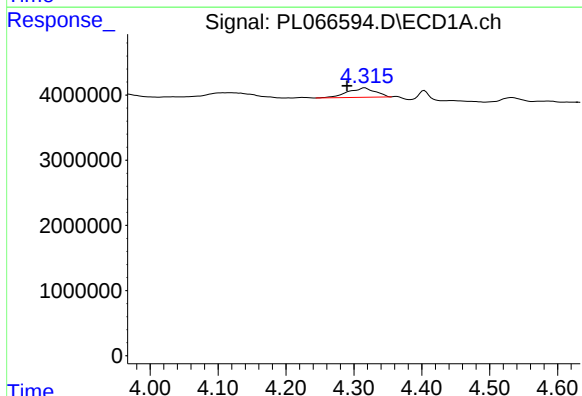


#23 Chlordane-1

R.T.: 4.316 min
Delta R.T.: 0.026 min
Response: 4085101
Conc: 24.17 ng/ml

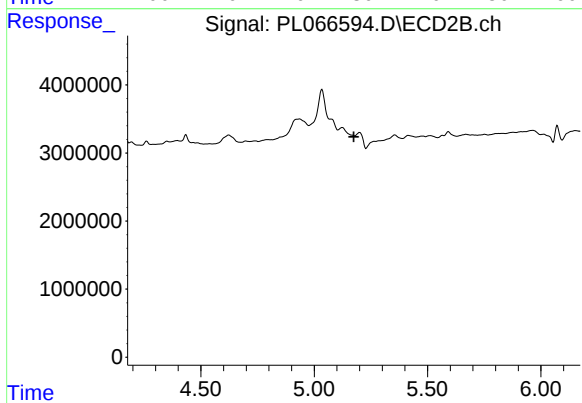

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

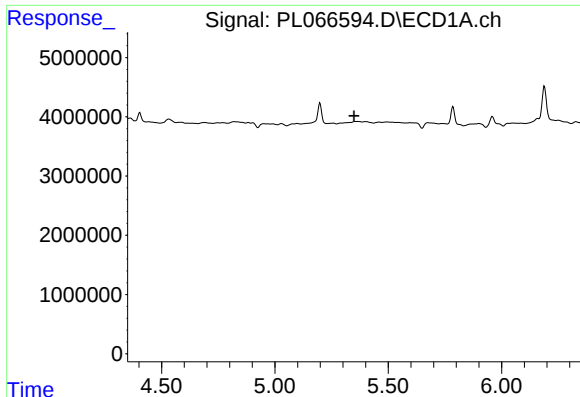

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

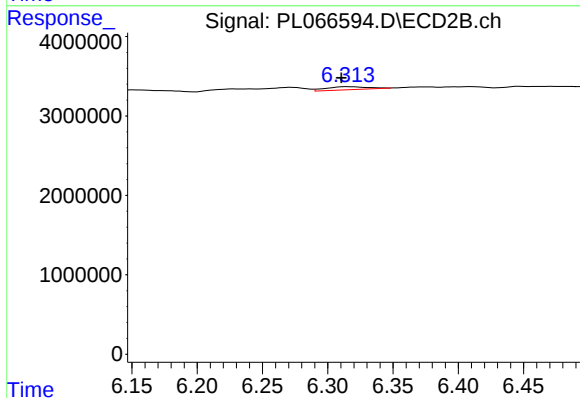


#25 Chlordane-3

R.T.: 6.316 min
Delta R.T.: 0.005 min
Response: 818046
Conc: 1.46 ng/ml

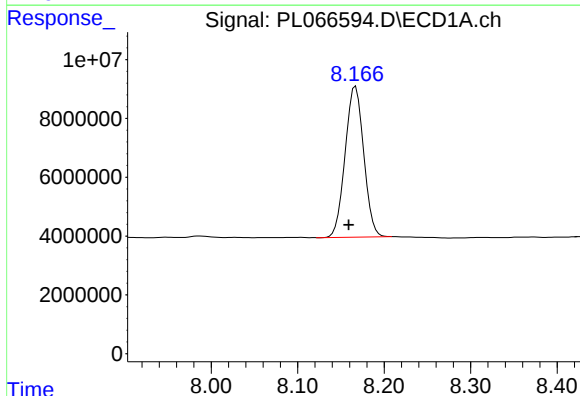

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.008 min
Response: 76166863
Conc: 19.87 ng/ml

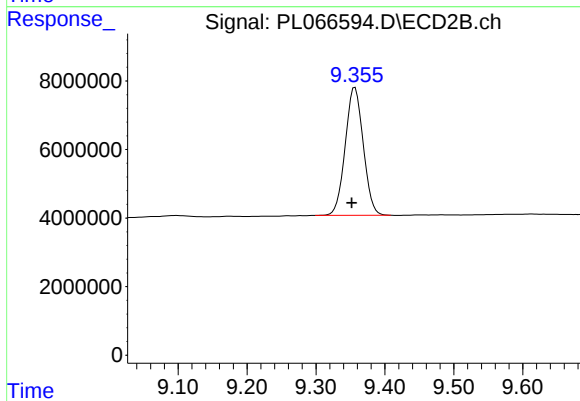

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 67791549
Conc: 21.91 ng/ml