

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 18:49
 Operator : AR\AJ
 Sample : M2217-19
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HTRCV2-GRAB-TS01-01

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:26:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:53:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	4.155	68011870	66296279	18.050	18.877
28)	SA Decachlor...	8.166	9.357	44292375	45411426	11.552	14.679 #
Target Compounds							
12)	B 4,4'-DDE	5.576	6.539	11030476	10987991	2.417	2.896m
17)	MA 4,4'-DDT	6.327	7.341	4296620	4069482	1.102	1.257m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 18:49
Operator : AR\AJ
Sample : M2217-19
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-01


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:53:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

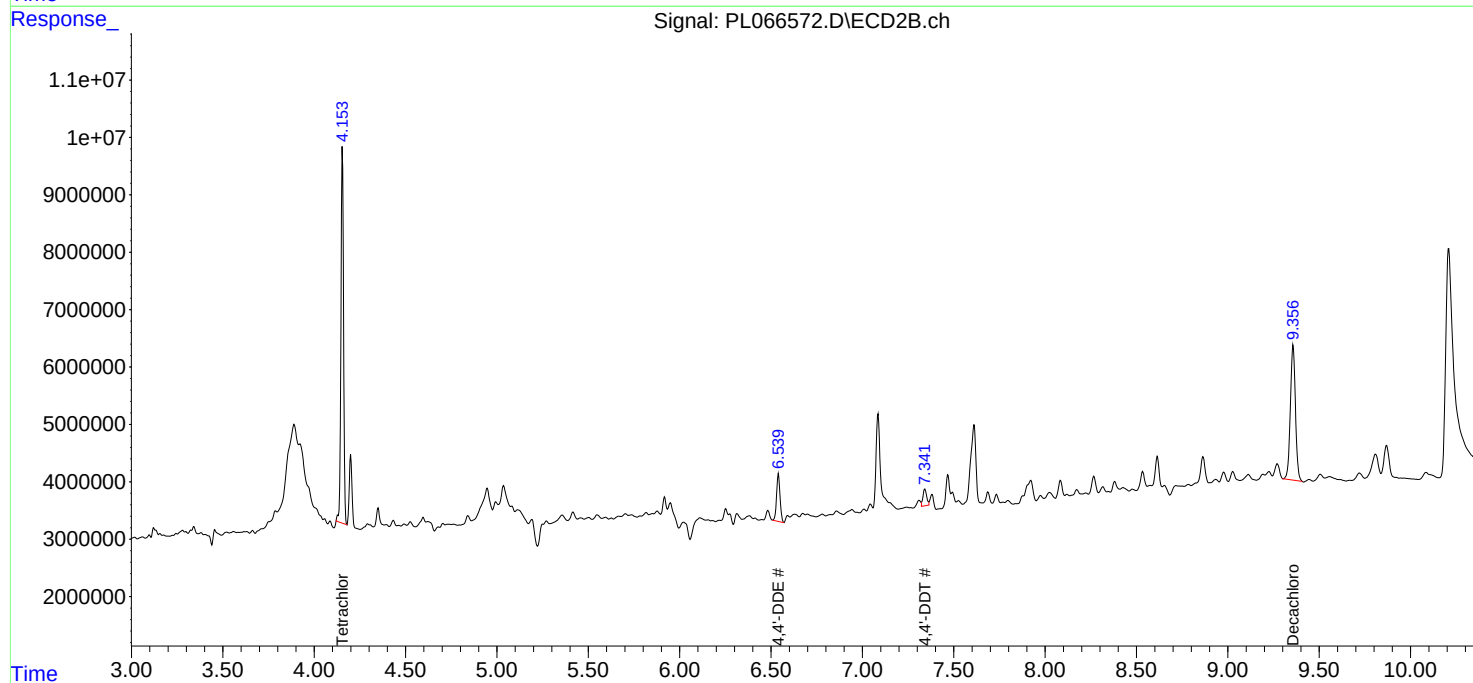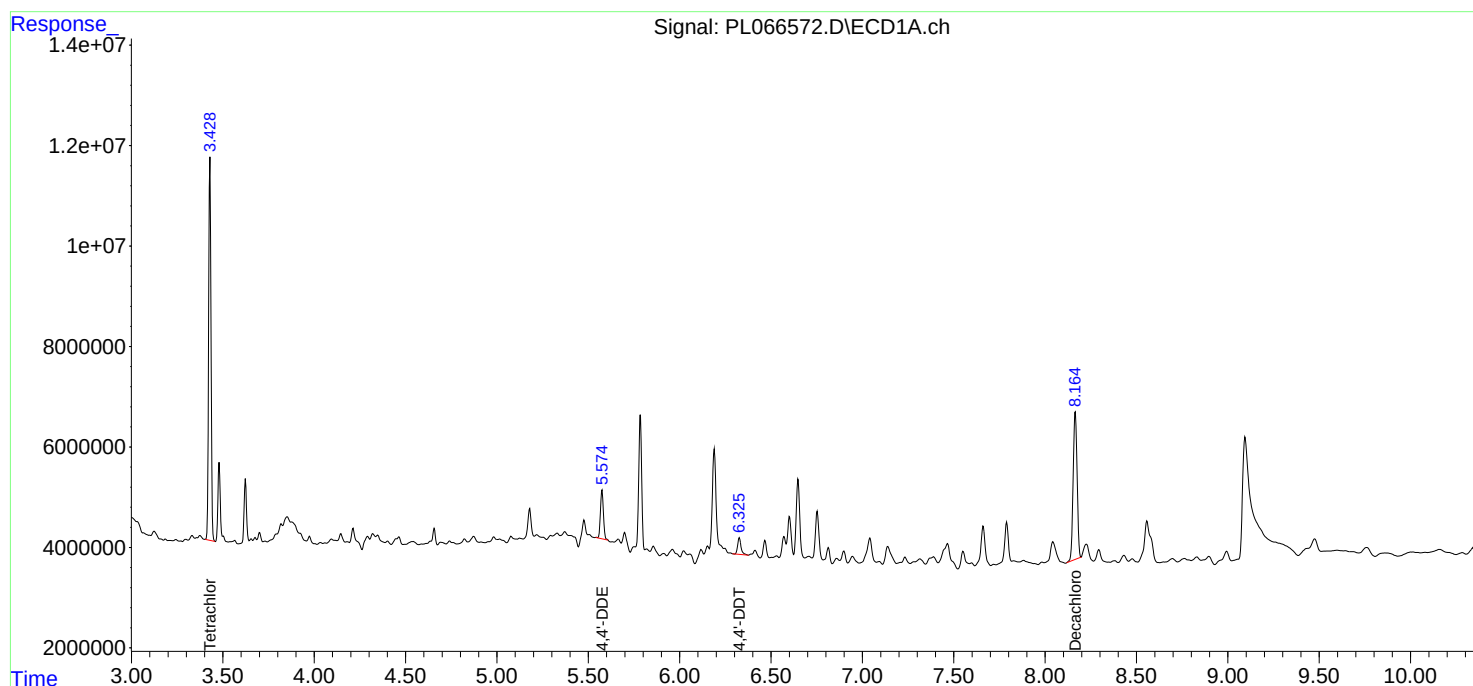

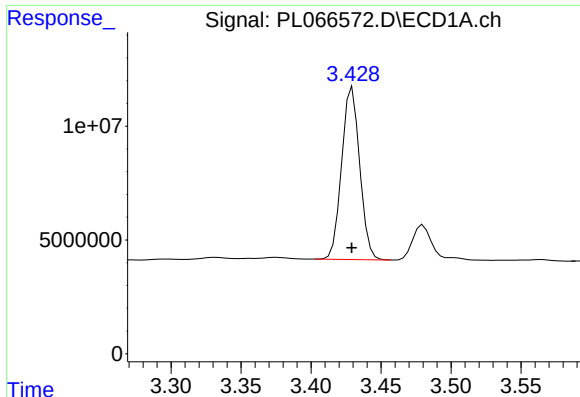


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 68011870
Conc: 18.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-01


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:32 PM

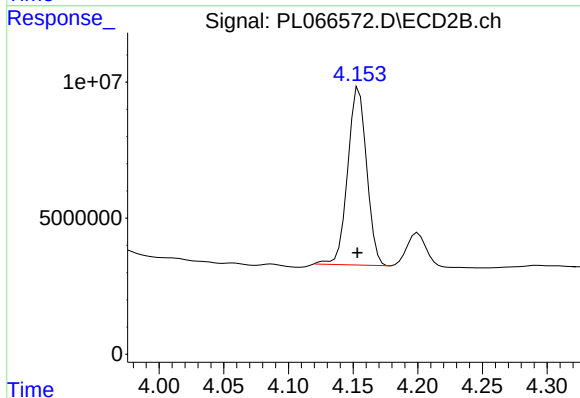


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 66296279
Conc: 18.88 ng/ml

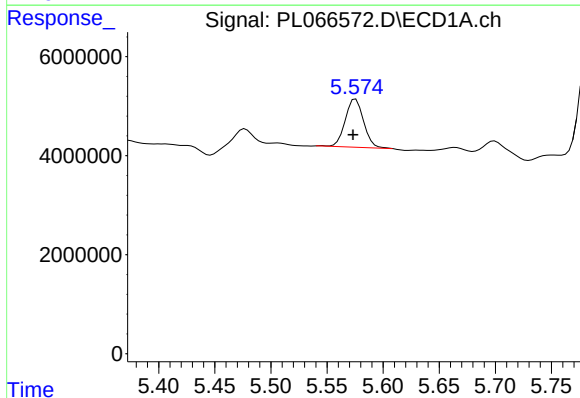


#12 4,4'-DDE

R.T.: 5.576 min
Delta R.T.: 0.002 min
Response: 11030476
Conc: 2.42 ng/ml

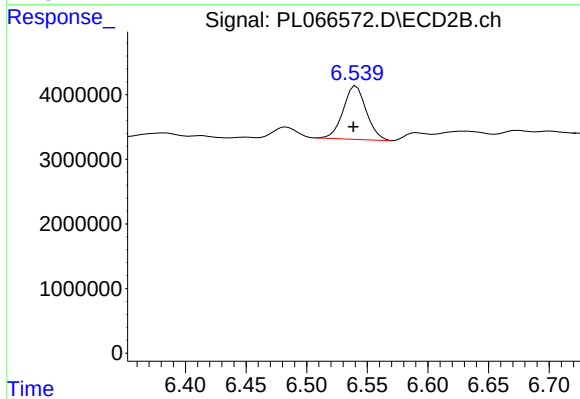

#12 4,4'-DDE

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 10987991
Conc: 2.90 ng/ml m

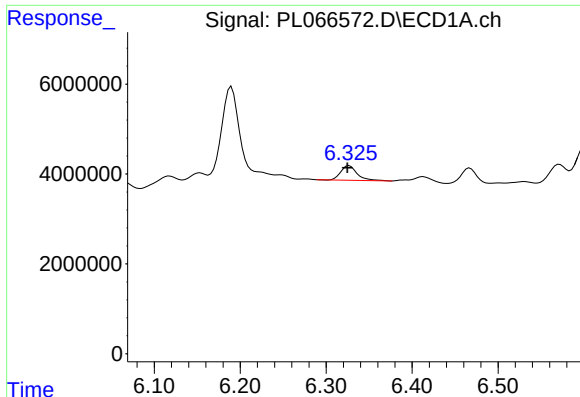


#17 4,4'-DDT

R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 4296620
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-01


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:32 PM

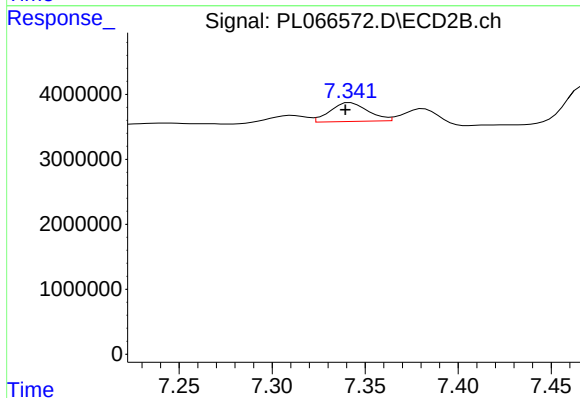


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 4069482
Conc: 1.26 ng/ml m

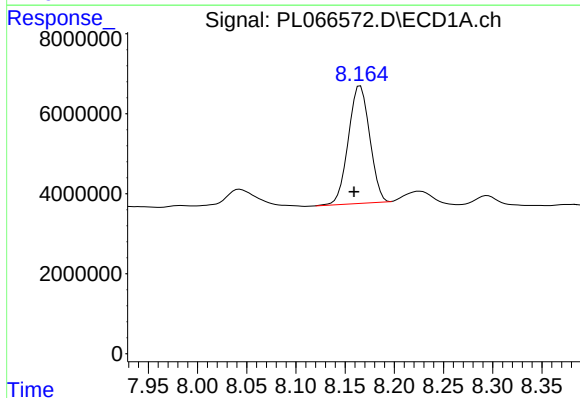

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.006 min
Response: 44292375
Conc: 11.55 ng/ml

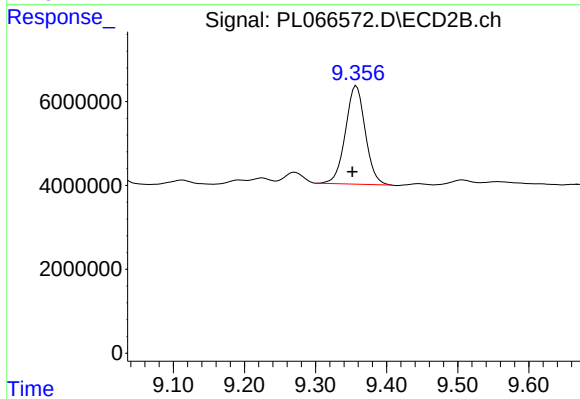

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.006 min
Response: 45411426
Conc: 14.68 ng/ml