

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 19:32
 Operator : AR\AJ
 Sample : M2217-22
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HTRCV2-GRAB-TS01-02

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:26:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 03:49:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	60722783	57803070	16.115	16.458
28)	SA Decachlor...	8.166	9.356	47748877	42162653	12.453	13.629
Target Compounds							
12)	B 4,4'-DDE	5.576	6.541	6005020	5562054	1.316	1.466
17)	MA 4,4'-DDT	6.325	7.339	1986423	2175426	0.509m	0.672m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 19:32
Operator : AR\AJ
Sample : M2217-22
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-02


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 03:49:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

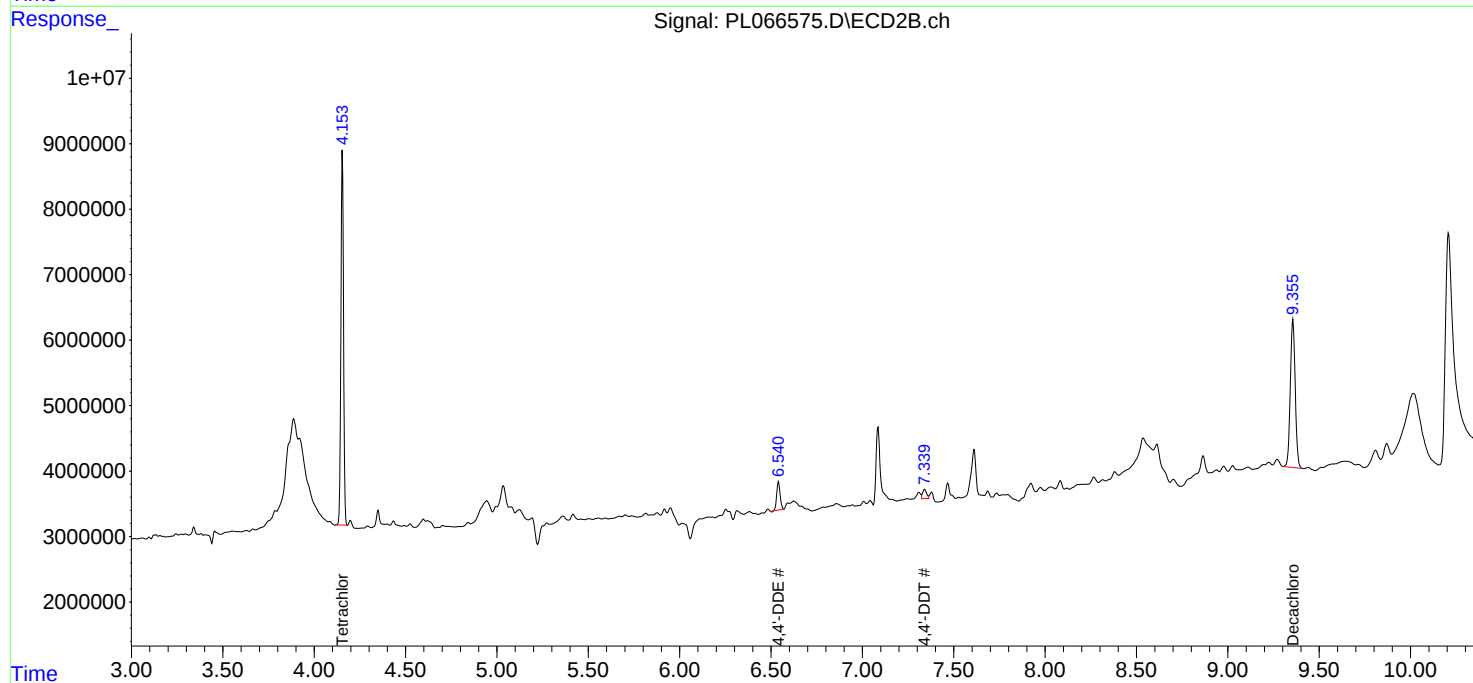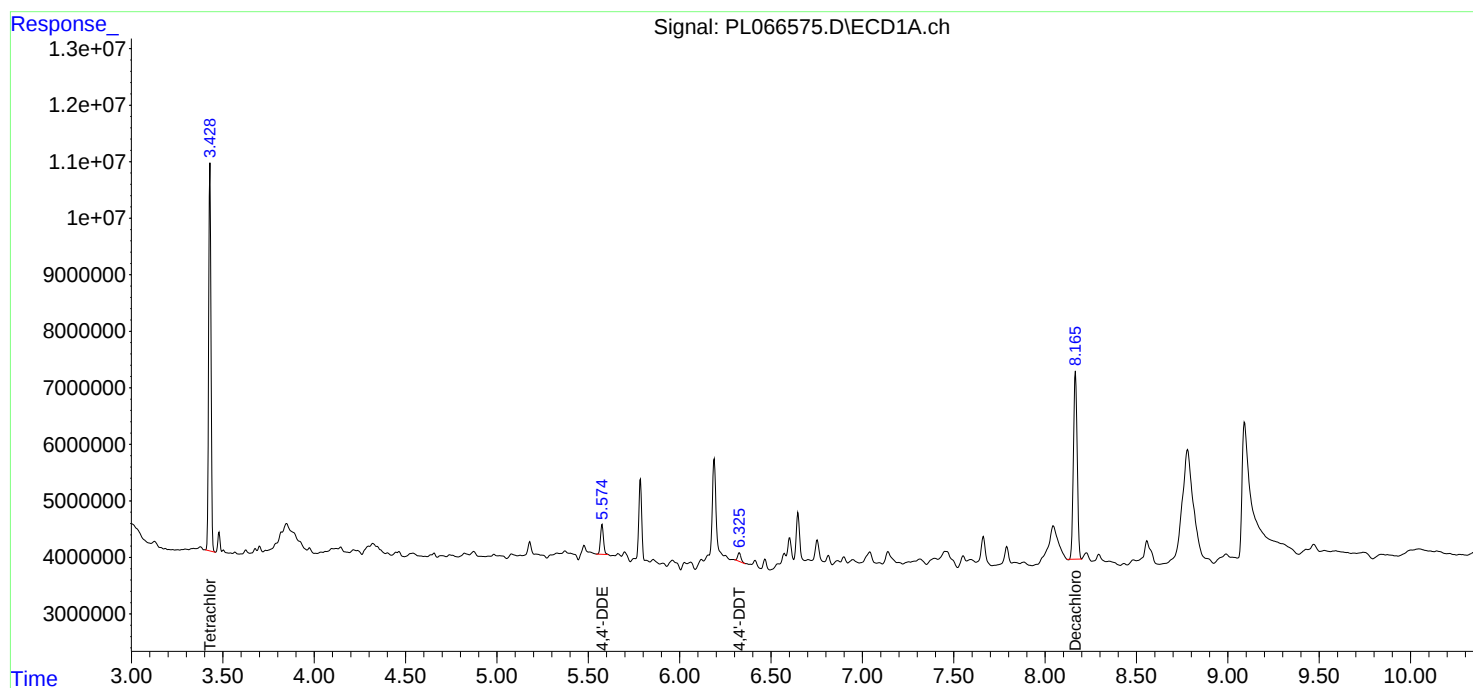

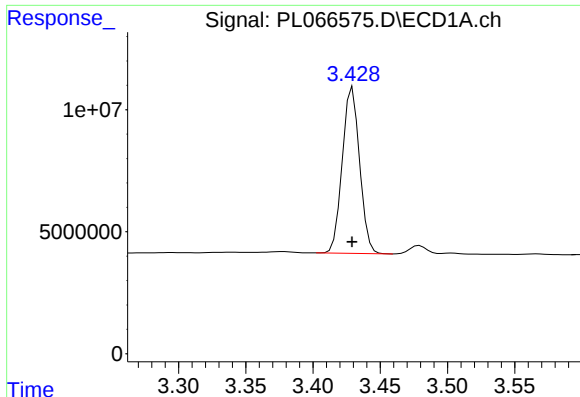


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 60722783
Conc: 16.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-02


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:33 PM

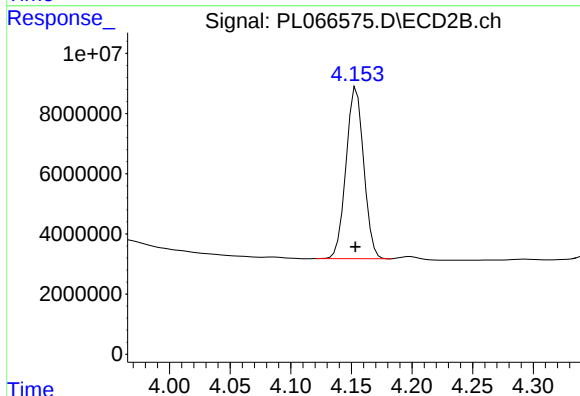


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 57803070
Conc: 16.46 ng/ml

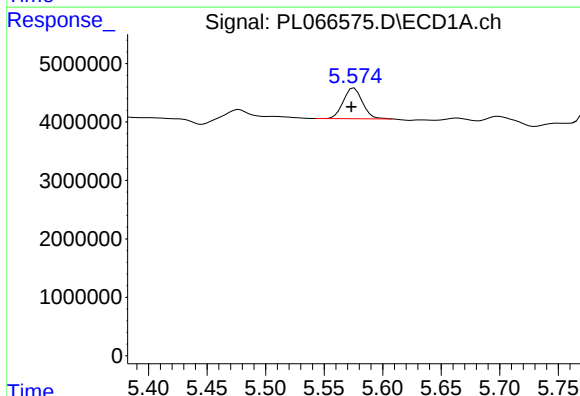


#12 4,4'-DDE

R.T.: 5.576 min
Delta R.T.: 0.002 min
Response: 6005020
Conc: 1.32 ng/ml

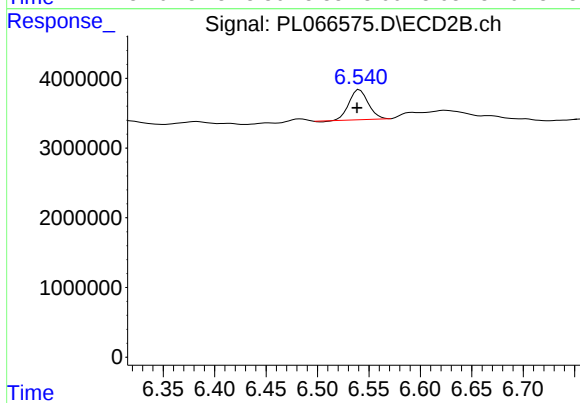

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 5562054
Conc: 1.47 ng/ml

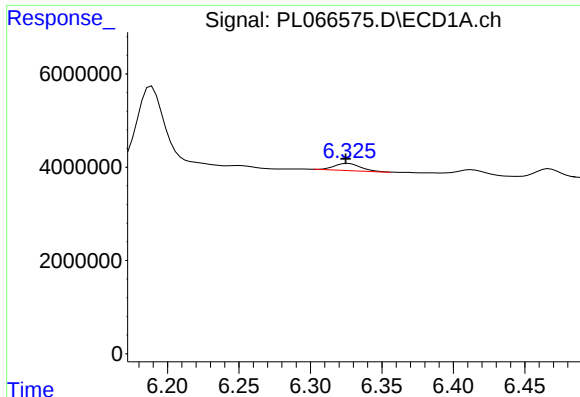


#17 4,4'-DDT

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 1986423
Conc: 0.51 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HTCRV2-GRAB-TS01-02


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:33 PM

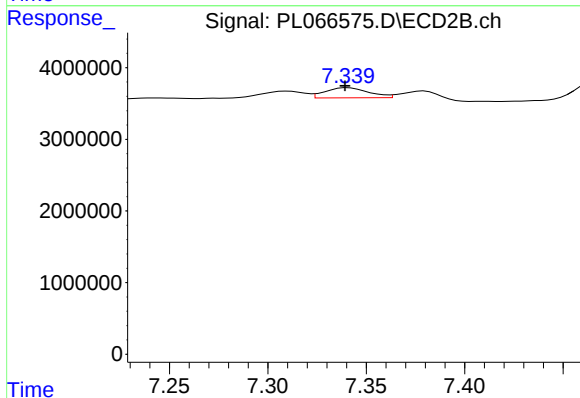


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 2175426
Conc: 0.67 ng/ml m

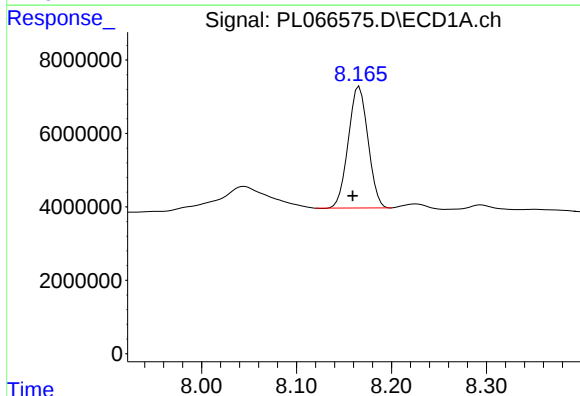

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.007 min
Response: 47748877
Conc: 12.45 ng/ml

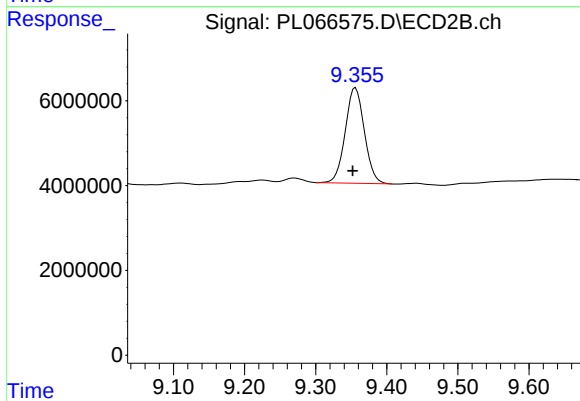

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.004 min
Response: 42162653
Conc: 13.63 ng/ml