

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
 Data File : PL066577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2021 20:01
 Operator : AR\AJ
 Sample : M2219-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-071

Manual Integrations
 APPROVED

Ankita
 4/30/2021 2:26:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 02:54:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.429	4.154	39181616	38230418	10.398	10.885
2) SA Decachlor...	8.166	9.356	24355010	19291128	6.352	6.236
Target Compounds						
11) B alpha-Chl...	5.406	6.383	1959709	3661505	0.398m	0.883m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042921\
Data File : PL066577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2021 20:01
Operator : AR\AJ
Sample : M2219-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-071


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 02:54:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

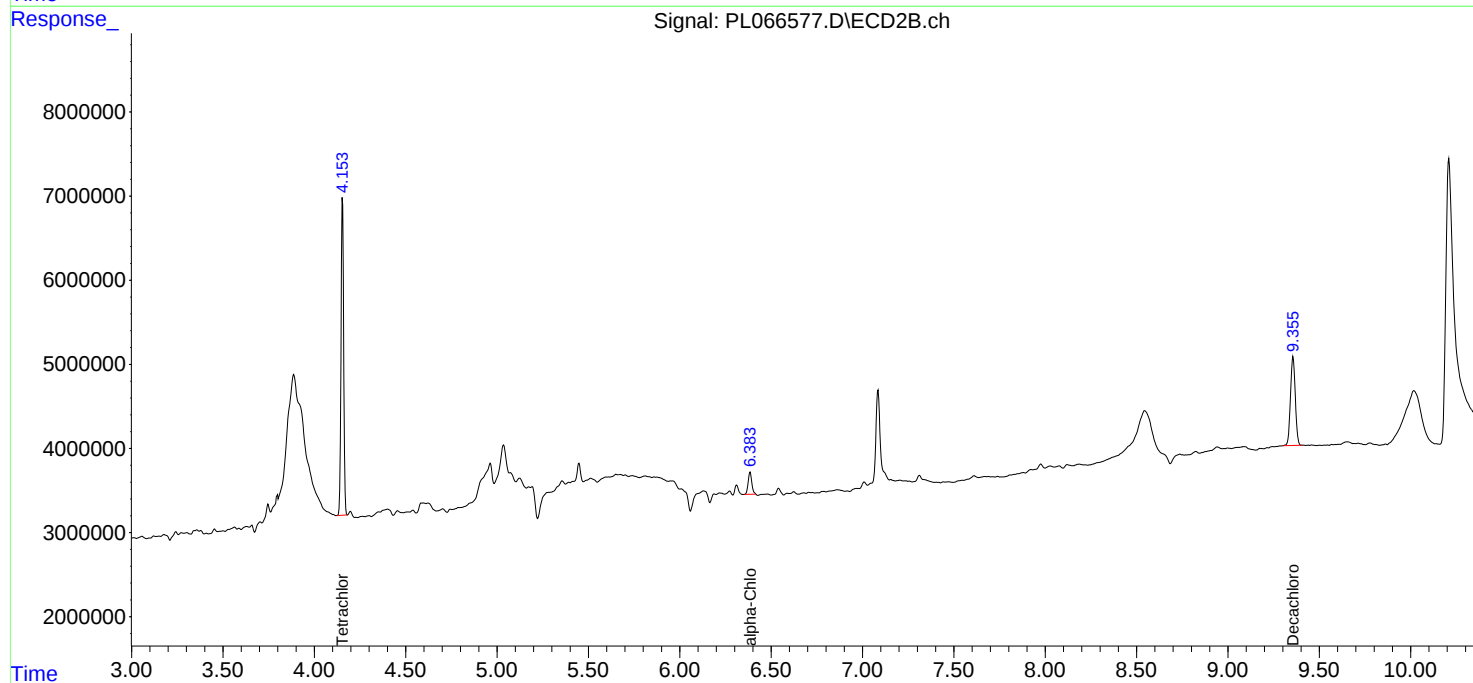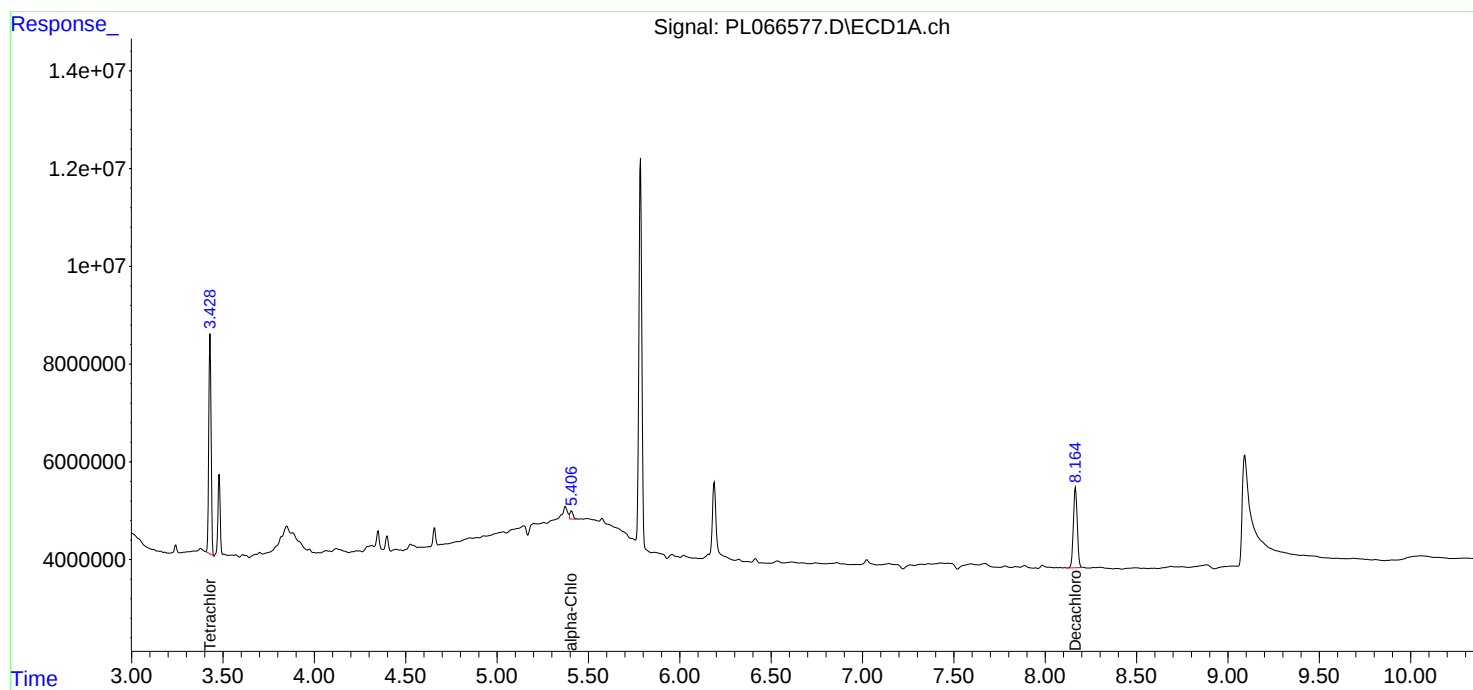

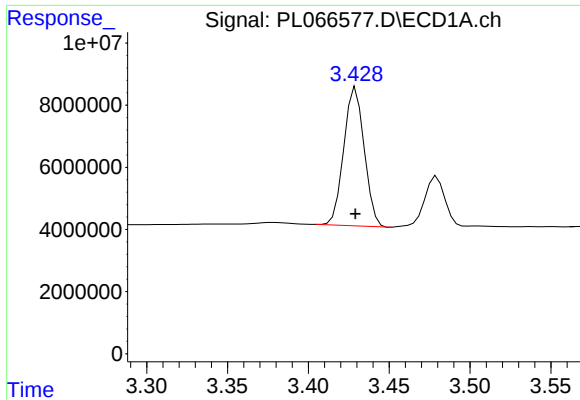


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 39181616
Conc: 10.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-071


Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:35 PM

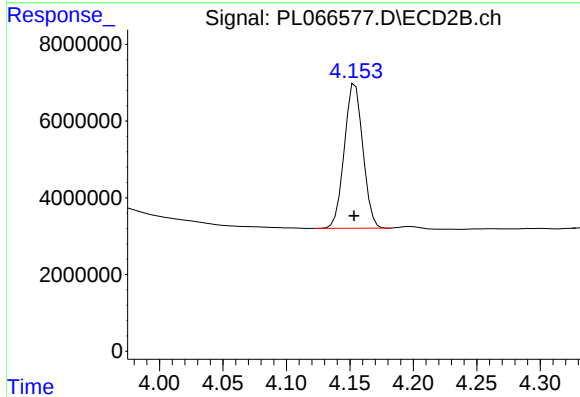


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 38230418
Conc: 10.89 ng/ml

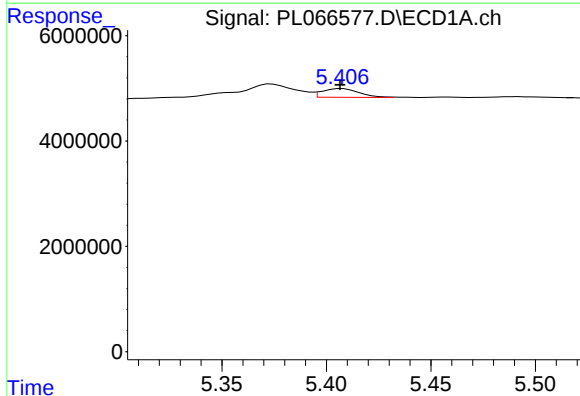


#11 alpha-Chlordane

R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 1959709
Conc: 0.40 ng/ml m

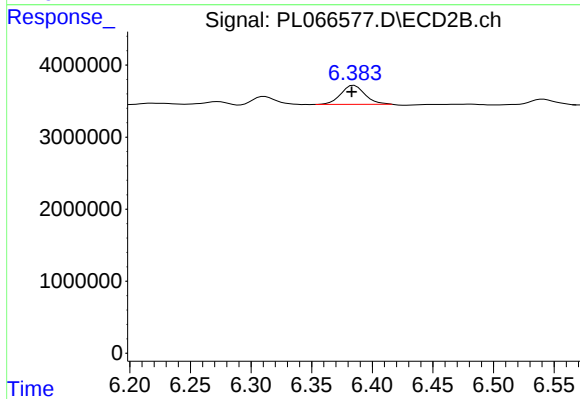

#11 alpha-Chlordane

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 3661505
Conc: 0.88 ng/ml m

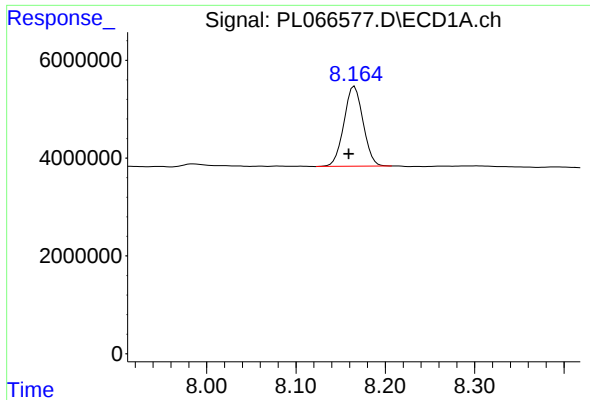


#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: 0.006 min
Response: 24355010
Conc: 6.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-071

Manual Integrations
APPROVED

Ankita
4/30/2021 2:26:35 PM

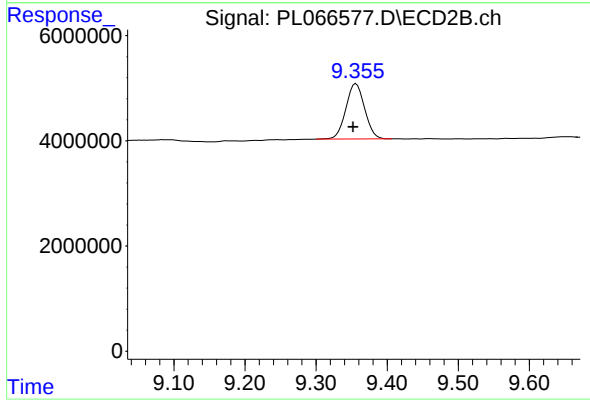

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.004 min
Response: 19291128
Conc: 6.24 ng/ml