

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
 Data File : PL048049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 21:56
 Operator : AJ\SJ
 Sample : K2598-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OIL-WATER-SEPERATOR-2(OWS-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:16:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	106.5E6	28412827	11.513	11.902
28)	SA Decachlor...	7.995	8.974	94581650	26640931	8.449	9.333
Target Compounds							
2)	A alpha-BHC	0.000	4.335	0	3666391	N.D.	1.105 #
3)	MA gamma-BHC...	4.051f	4.636f	2164440	2823966	0.163	0.900 #
4)	MA Heptachlor	0.000	5.123	0	694395	N.D.	0.207 #
6)	B beta-BHC	4.288	0.000	7379522	0	1.306	N.D. #
10)	B gamma-Chl...	5.240f	6.047	13737064	4409425	1.032	1.457 #
11)	B alpha-Chl...	5.274	0.000	44649139	0	3.422	N.D. #
25)	Chlordane-3	5.274	0.000	44649139	0	33.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
Data File : PL048049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 21:56
Operator : AJ\SJ
Sample : K2598-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2(OWS-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:16:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

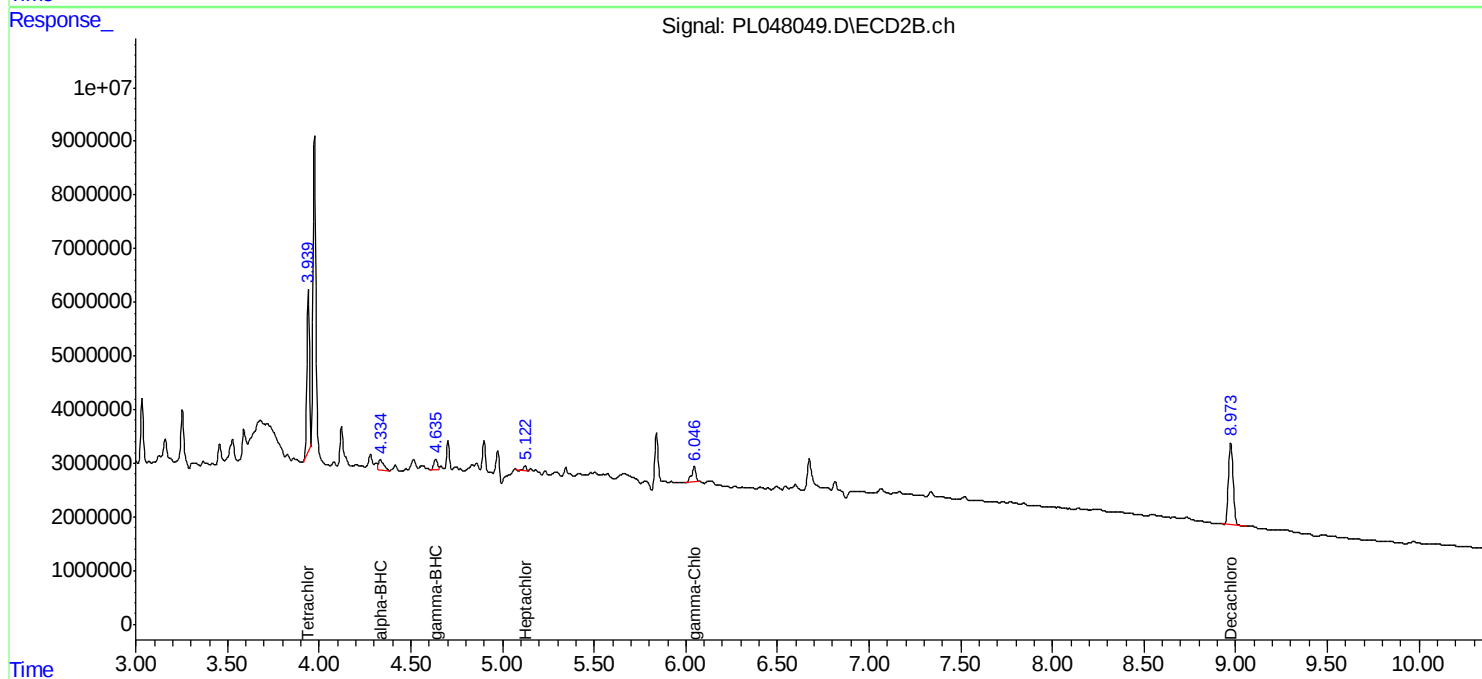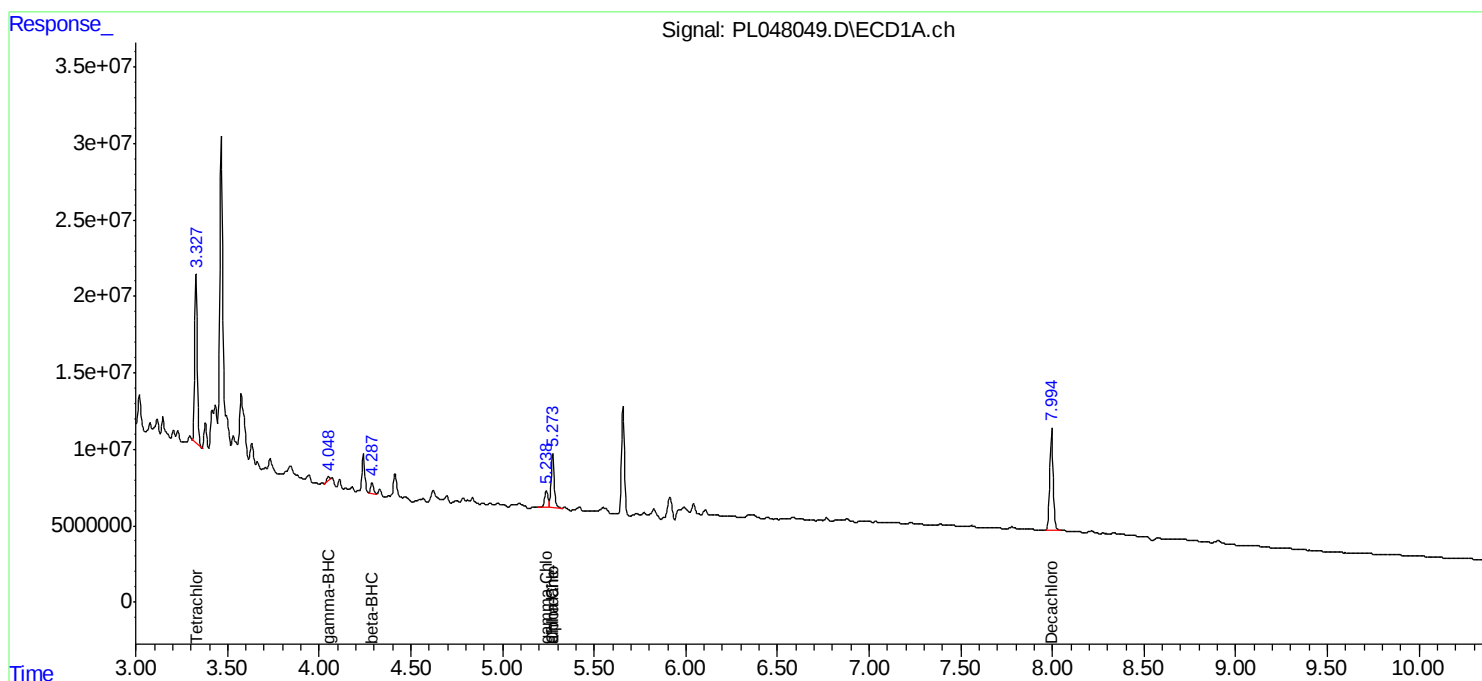


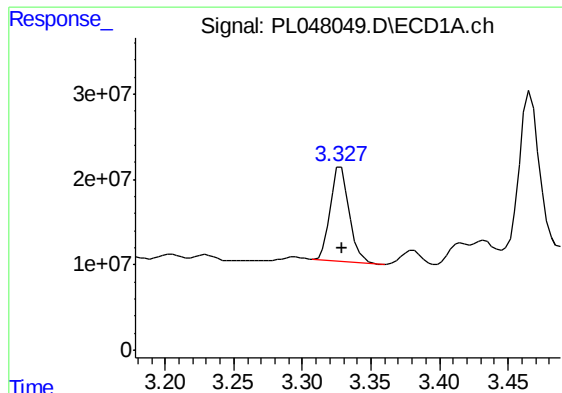

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: -0.001 min
Response: 106476408
Conc: 11.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2(OWS-2)

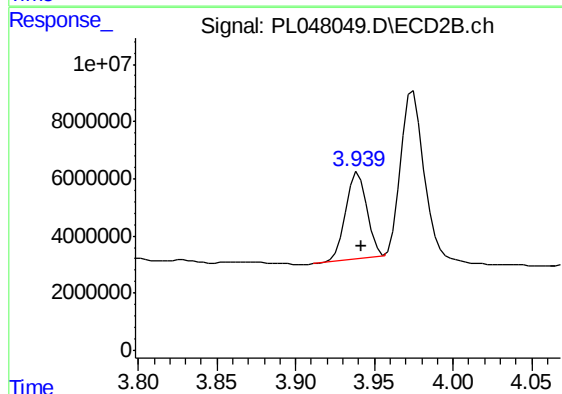


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.002 min
Response: 28412827
Conc: 11.90 ng/ml

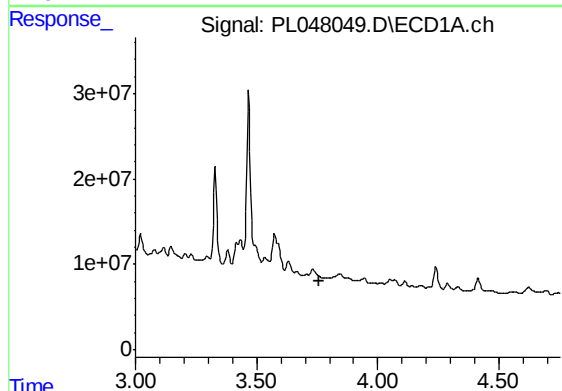


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.757 min
Response: 0
Conc: N.D.

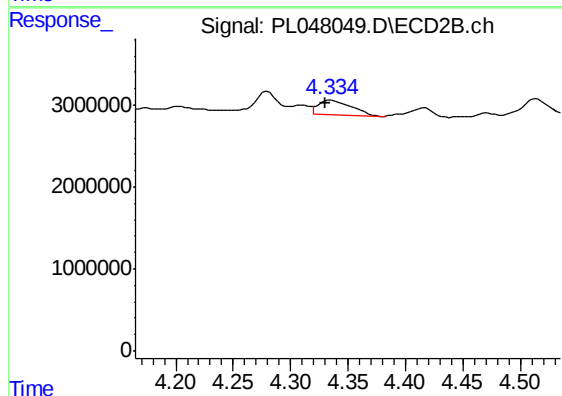

#2 alpha-BHC


R.T.: 4.335 min
Delta R.T.: 0.005 min
Response: 3666391
Conc: 1.10 ng/ml

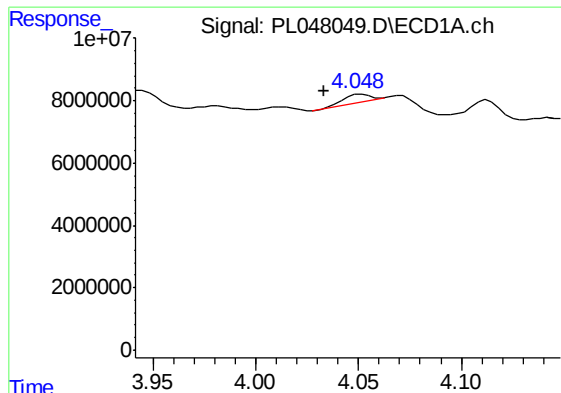

#3 gamma-BHC (Lindane)


R.T.: 4.051 min
Delta R.T.: 0.018 min
Response: 2164440
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPARATOR-2(OWS-2)

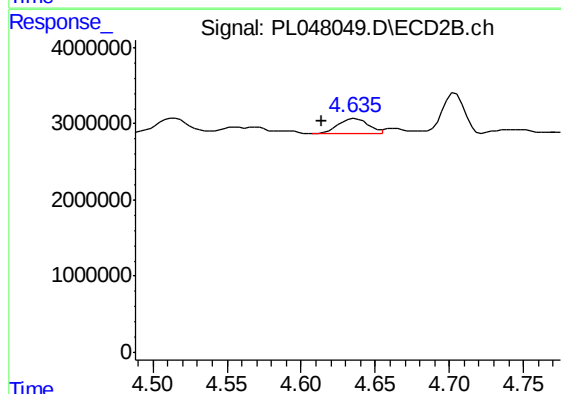


#3 gamma-BHC (Lindane)

R.T.: 4.636 min
Delta R.T.: 0.023 min
Response: 2823966
Conc: 0.90 ng/ml

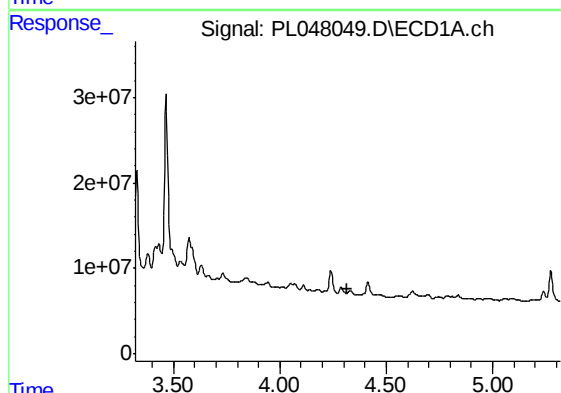


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

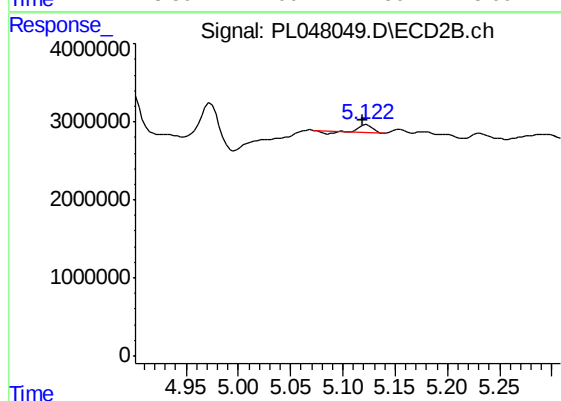

#4 Heptachlor


R.T.: 5.123 min
Delta R.T.: 0.005 min
Response: 694395
Conc: 0.21 ng/ml

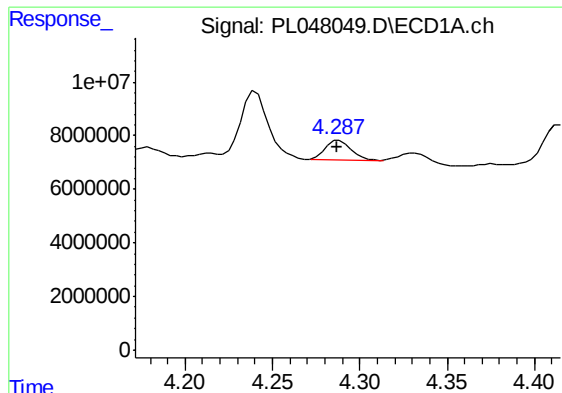

#6 beta-BHC


R.T.: 4.288 min
Delta R.T.: 0.001 min
Response: 7379522
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2(OWS-2)

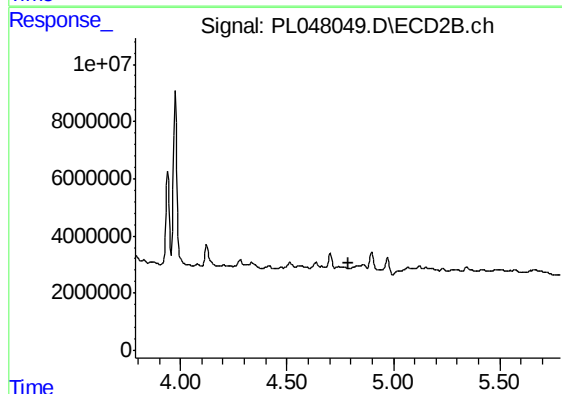


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.788 min
Response: 0
Conc: N.D.

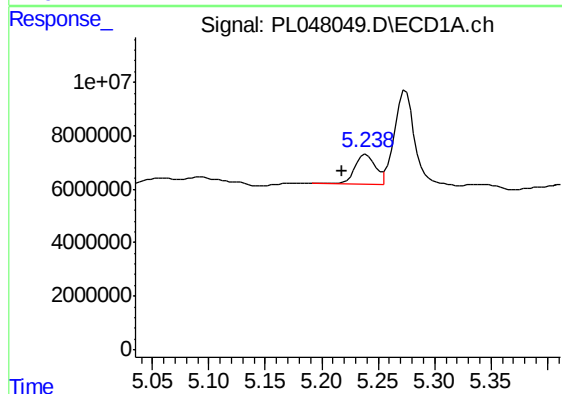


#10 gamma-Chlordane

R.T.: 5.240 min
Delta R.T.: 0.022 min
Response: 13737064
Conc: 1.03 ng/ml

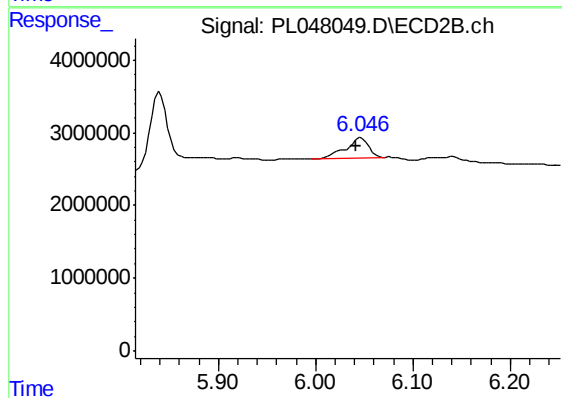

#10 gamma-Chlordane


R.T.: 6.047 min
Delta R.T.: 0.005 min
Response: 4409425
Conc: 1.46 ng/ml

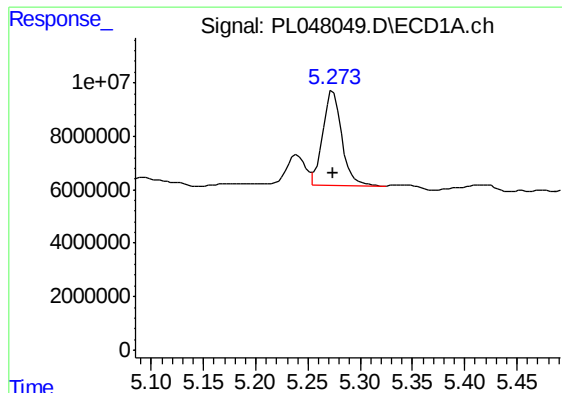

#11 alpha-Chlordane


R.T.: 5.274 min
Delta R.T.: 0.000 min
Response: 44649139
Conc: 3.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2(OWS-2)

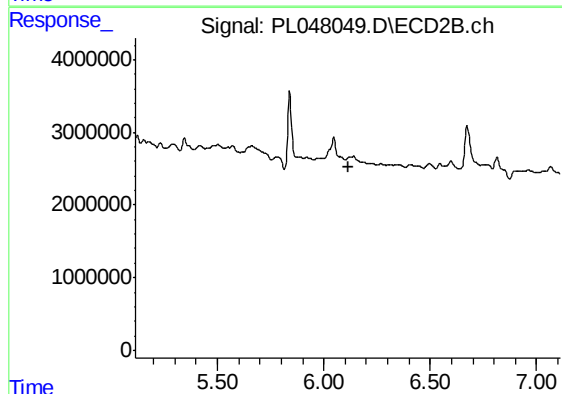


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

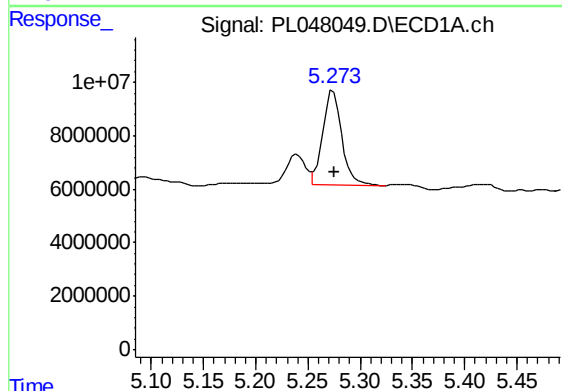


#25 Chlordane-3

R.T.: 5.274 min
Delta R.T.: -0.002 min
Response: 44649139
Conc: 33.87 ng/ml

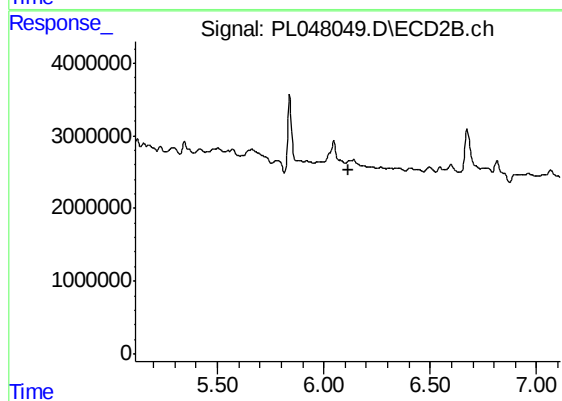

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

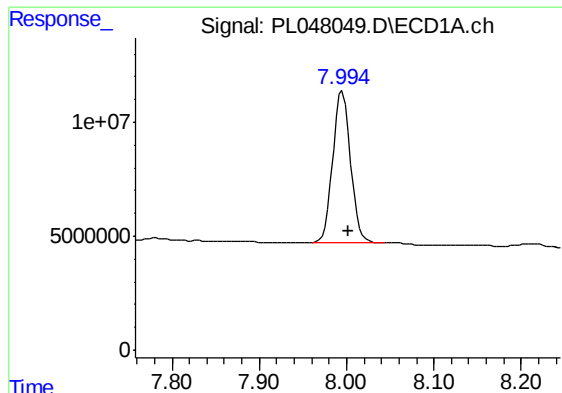

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.006 min
Response: 94581650
Conc: 8.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
OIL-WATER-SEPERATOR-2(OWS-2

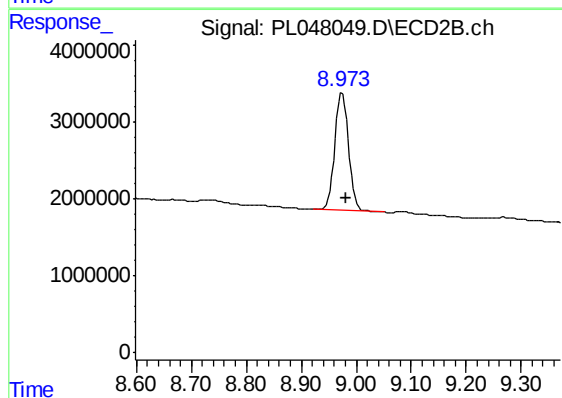

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.007 min
Response: 26640931
Conc: 9.33 ng/ml