

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
 Data File : PL048058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 May 2019 00:27
 Operator : AJ\SJ
 Sample : K2194-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-042919-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:18:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.939	123.9E6	31864916	13.401	13.348
28)	SA Decachlor...	7.995	8.974	121.7E6	40551197	10.876	14.206 #
Target Compounds							
6)	B beta-BHC	0.000	4.806f	0	3098827	N.D.	2.151 #
10)	B gamma-Chl...	5.215	6.037	6869152	4448072	0.516	1.470 #
11)	B alpha-Chl...	5.270	6.111	12989142	8628338	0.995	2.852 #
12)	B 4,4'-DDE	5.438	6.266	5979536	2329632	0.481	0.844 #
16)	A 4,4'-DDD	0.000	6.761	0	1541385	N.D.	0.687 #
17)	MA 4,4'-DDT	6.180	7.057	6730621	1895125	0.675	0.796
25)	Chlordane-3	5.270	6.111	12989142	8628338	9.852	29.128 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
Data File : PL048058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 May 2019 00:27
Operator : AJ\SJ
Sample : K2194-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:18:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

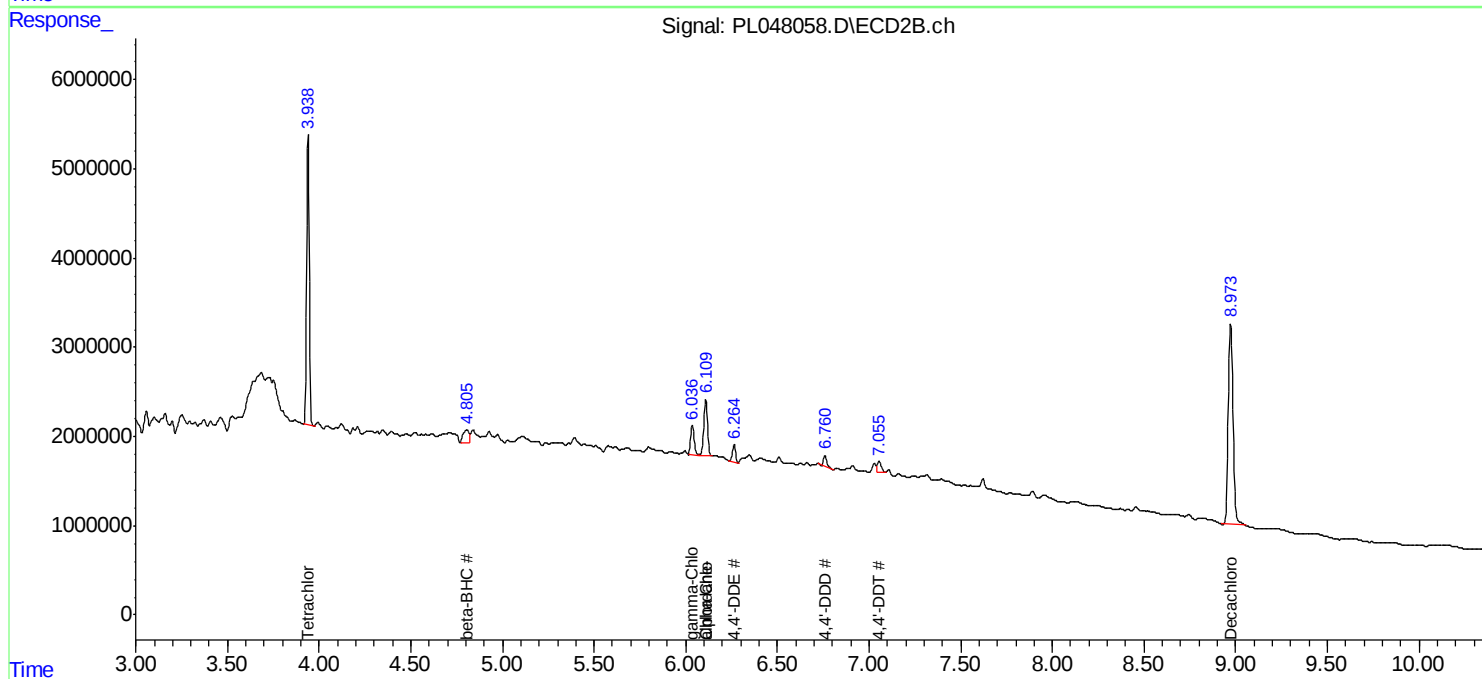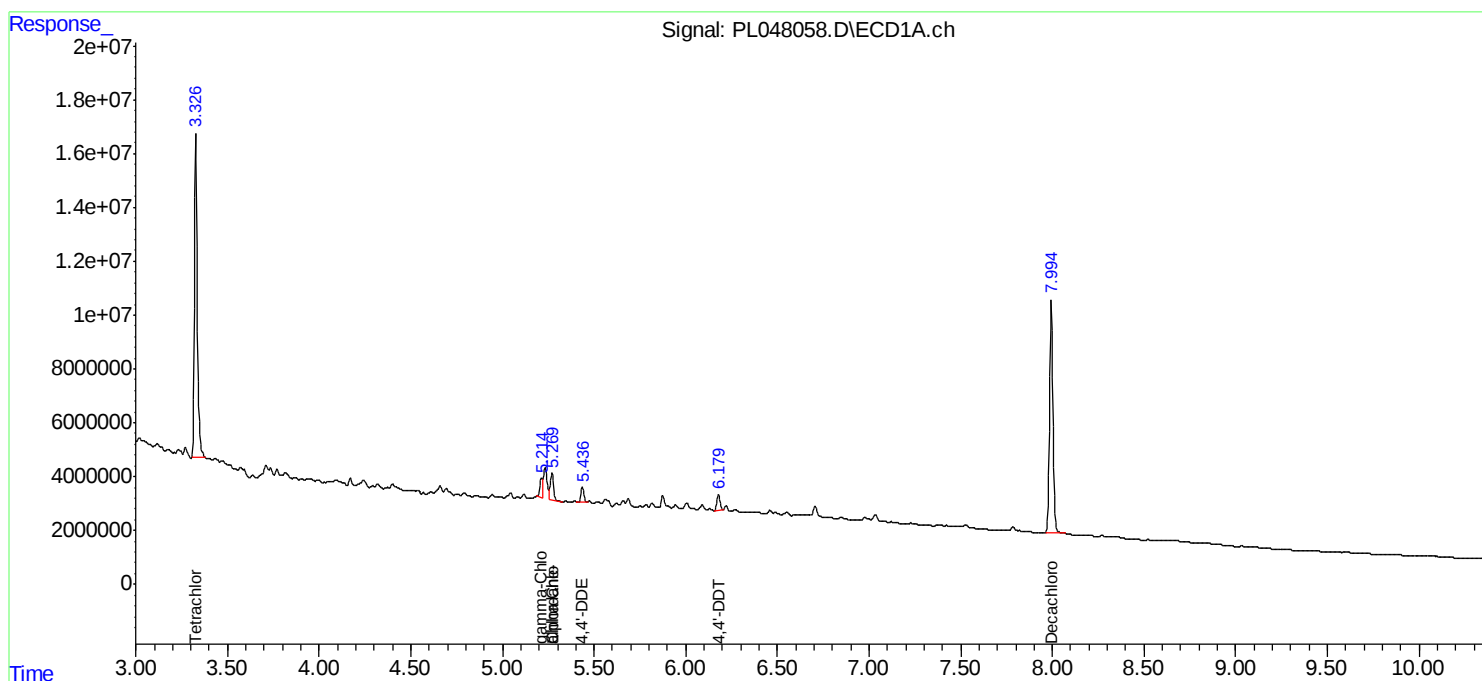


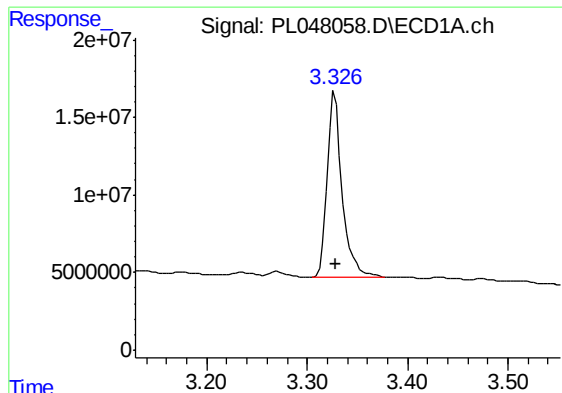

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: -0.001 min
Response: 123934579
Conc: 13.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

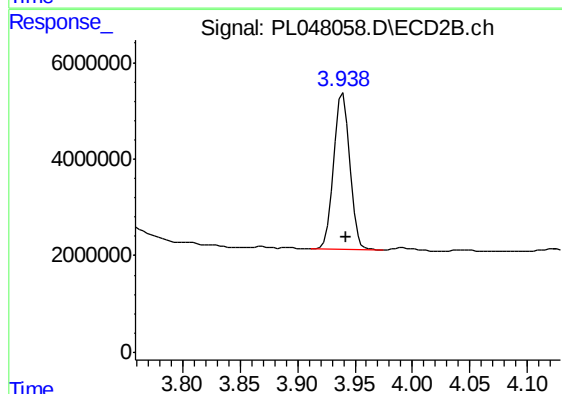


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.003 min
Response: 31864916
Conc: 13.35 ng/ml

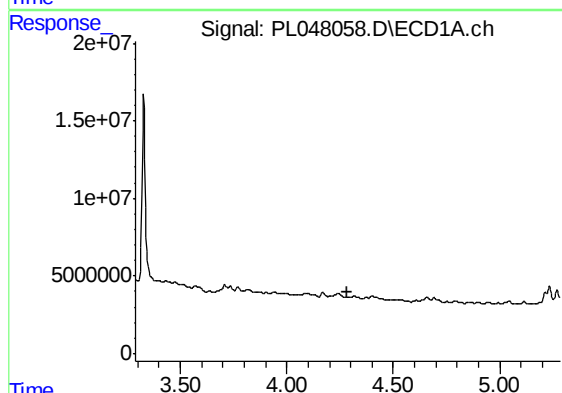


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.287 min
Response: 0
Conc: N.D.

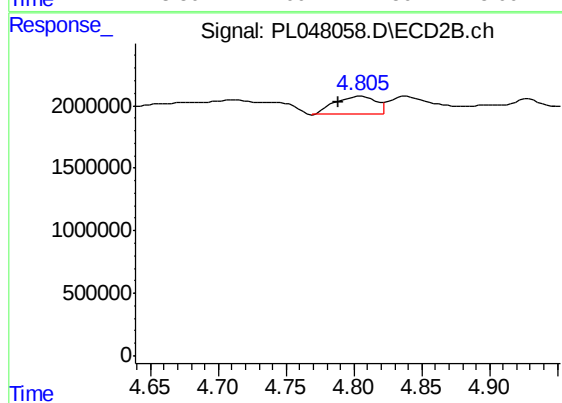

#6 beta-BHC


R.T.: 4.806 min
Delta R.T.: 0.018 min
Response: 3098827
Conc: 2.15 ng/ml

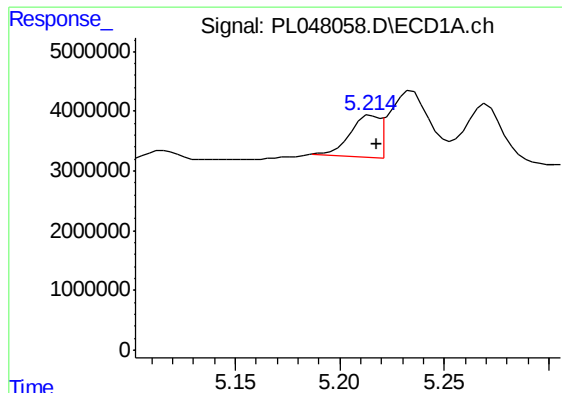

#10 gamma-Chlordane


R.T.: 5.215 min
Delta R.T.: -0.002 min
Response: 6869152
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

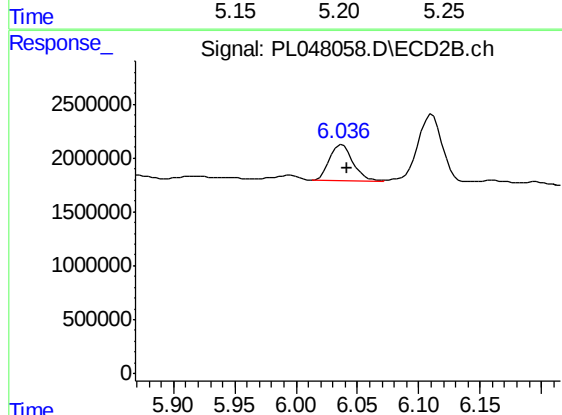


#10 gamma-Chlordane

R.T.: 6.037 min
Delta R.T.: -0.004 min
Response: 4448072
Conc: 1.47 ng/ml

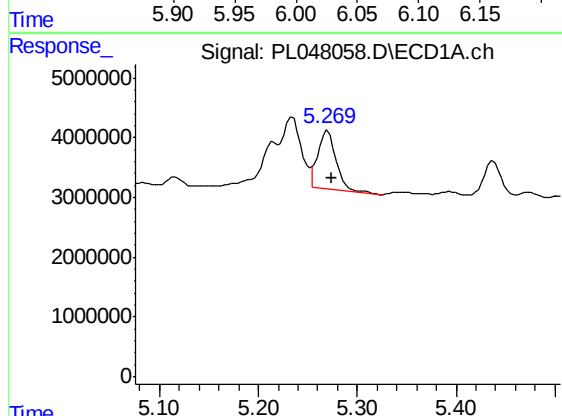


#11 alpha-Chlordane

R.T.: 5.270 min
Delta R.T.: -0.004 min
Response: 12989142
Conc: 1.00 ng/ml

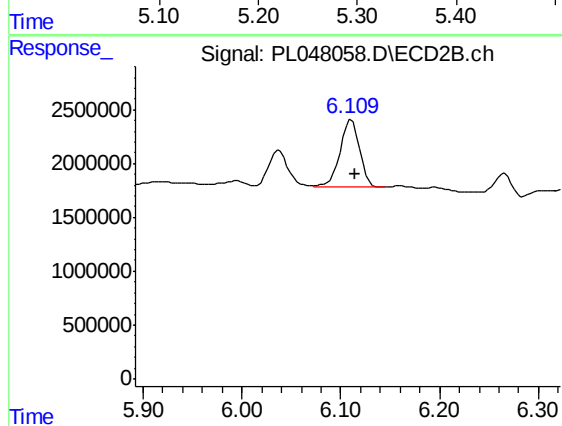

#11 alpha-Chlordane


R.T.: 6.111 min
Delta R.T.: -0.003 min
Response: 8628338
Conc: 2.85 ng/ml

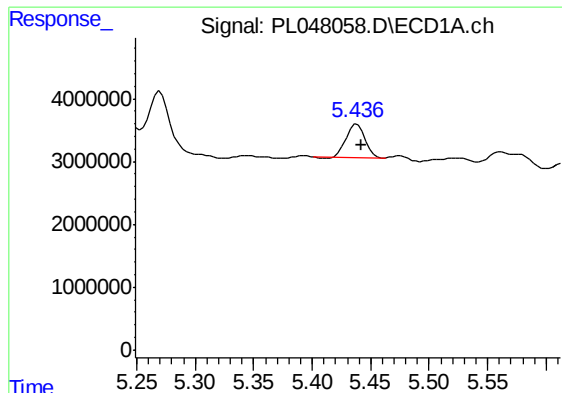

#12 4,4'-DDE


R.T.: 5.438 min
Delta R.T.: -0.004 min
Response: 5979536
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

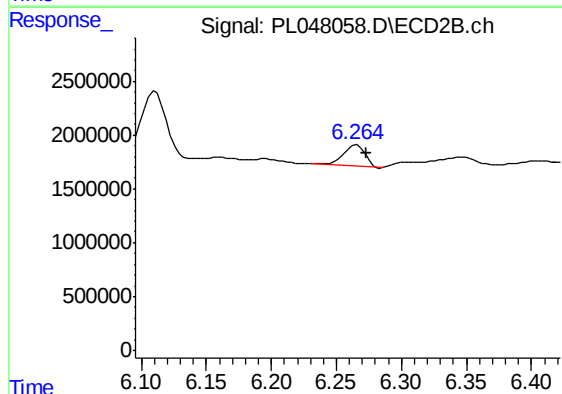


#12 4,4'-DDE

R.T.: 6.266 min
Delta R.T.: -0.007 min
Response: 2329632
Conc: 0.84 ng/ml

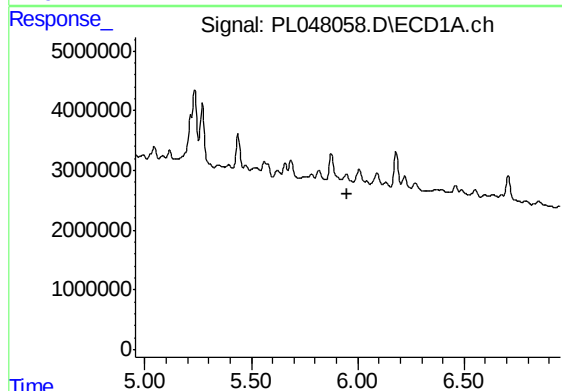


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

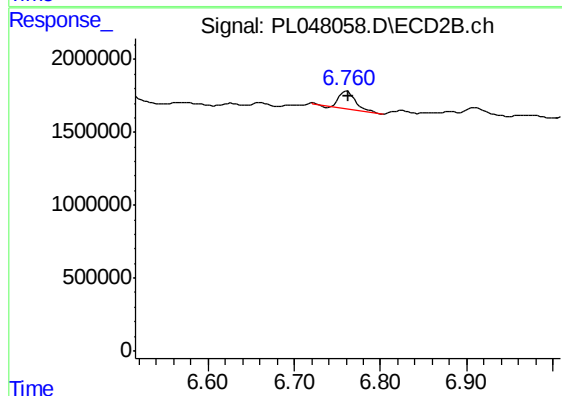

#16 4,4'-DDD


R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 1541385
Conc: 0.69 ng/ml

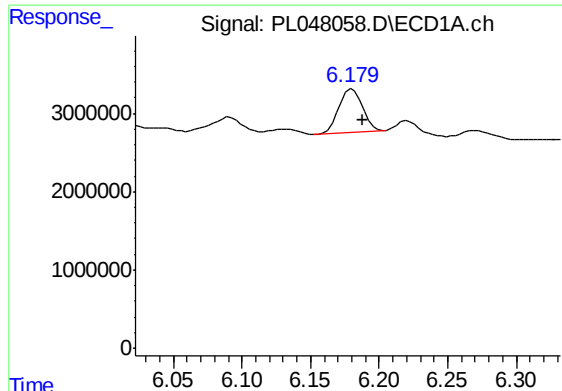

#17 4,4'-DDT


R.T.: 6.180 min
Delta R.T.: -0.008 min
Response: 6730621
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

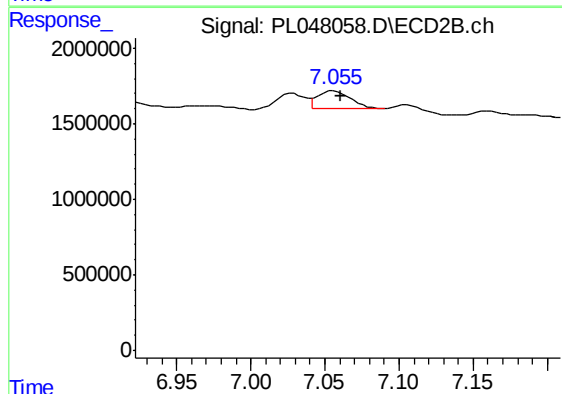


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: -0.004 min
Response: 1895125
Conc: 0.80 ng/ml

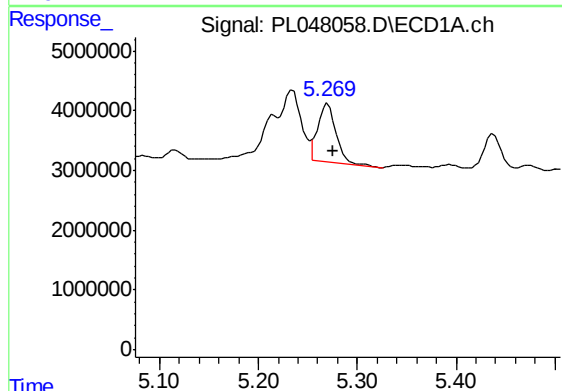


#25 Chlordane-3

R.T.: 5.270 min
Delta R.T.: -0.005 min
Response: 12989142
Conc: 9.85 ng/ml

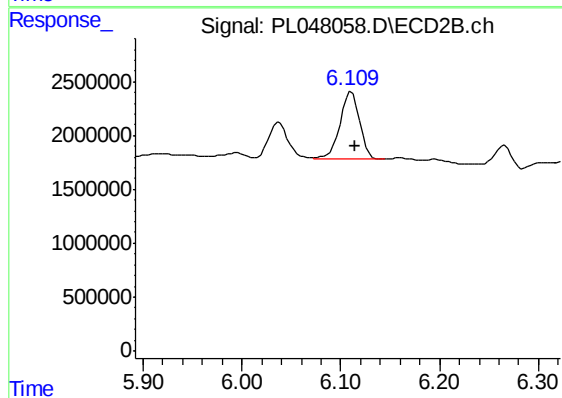

#25 Chlordane-3


R.T.: 6.111 min
Delta R.T.: -0.003 min
Response: 8628338
Conc: 29.13 ng/ml

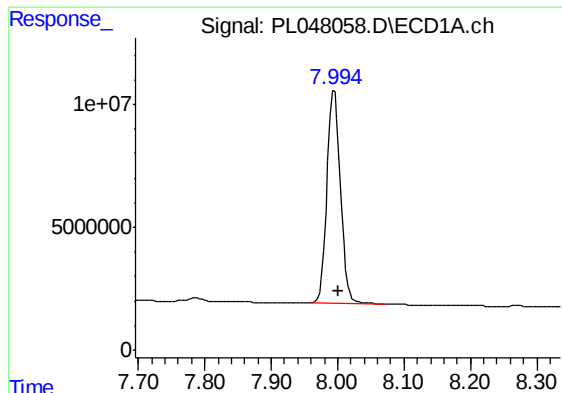

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: -0.007 min
Response: 121746111
Conc: 10.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-042919-C

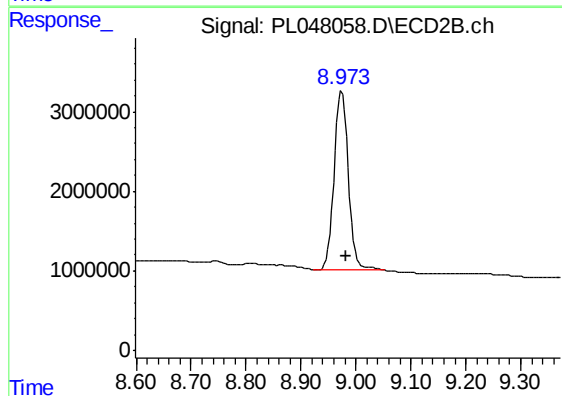

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.007 min
Response: 40551197
Conc: 14.21 ng/ml