

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
 Data File : PL048017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 11:51
 Operator : AJ\SJ
 Sample : K2578-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WATER-COMP

Manual Integrations
 APPROVED

mohammad
 5/1/2019 3:39:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 12:07:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	95375313	32832048	10.313m	13.753m#
28)	SA Decachlor...	7.999	8.978	50449913	15205844	4.507	5.327

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043019\
Data File : PL048017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 11:51
Operator : AJ\SJ
Sample : K2578-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

mohammad
5/1/2019 3:39:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 12:07:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

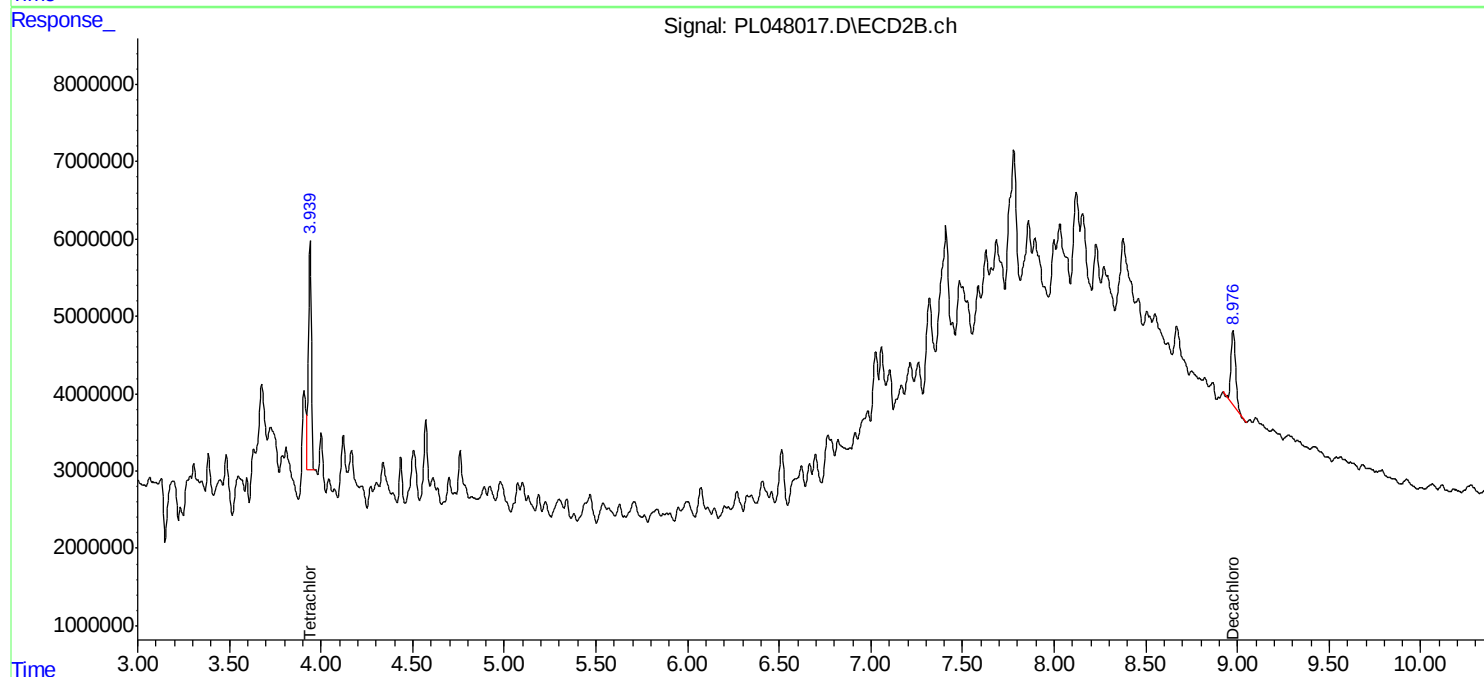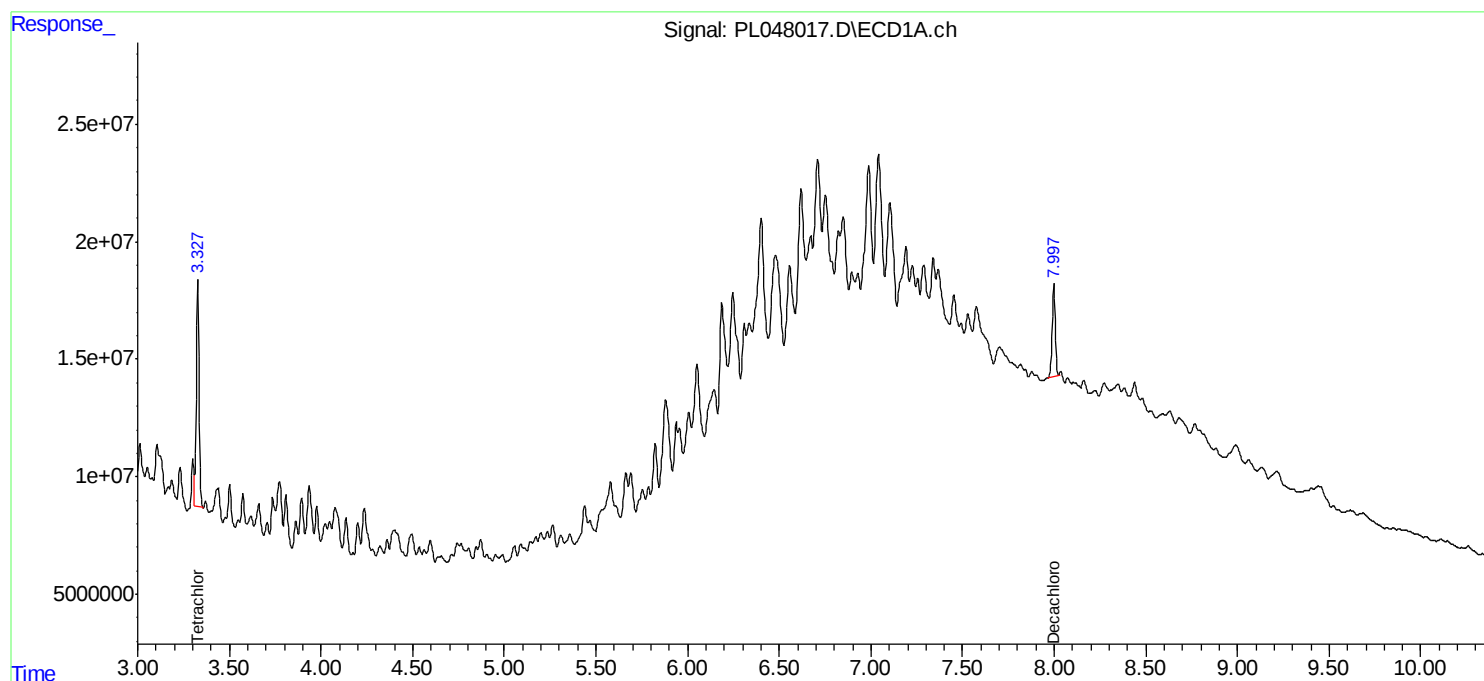

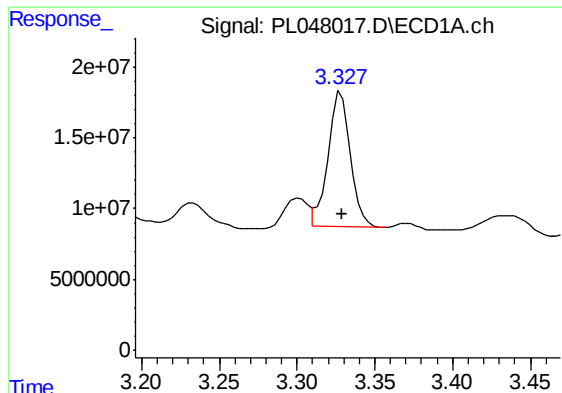


#1 Tetrachloro-m-xylene

R.T.: 3.327 min
Delta R.T.: -0.002 min
Response: 95375313
Conc: 10.31 ng/ml m

Instrument :
ECD_L
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

mohammad
5/1/2019 3:39:36 PM

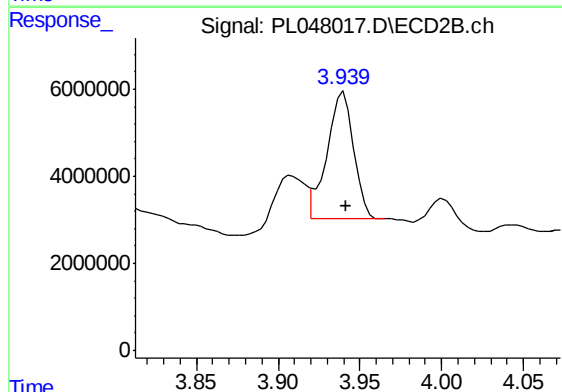


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.003 min
Response: 32832048
Conc: 13.75 ng/ml m

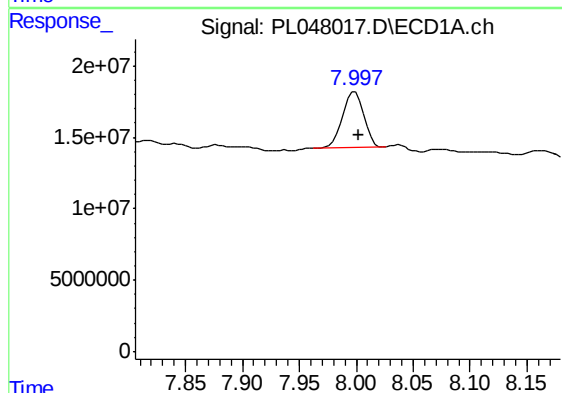

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: -0.003 min
Response: 50449913
Conc: 4.51 ng/ml

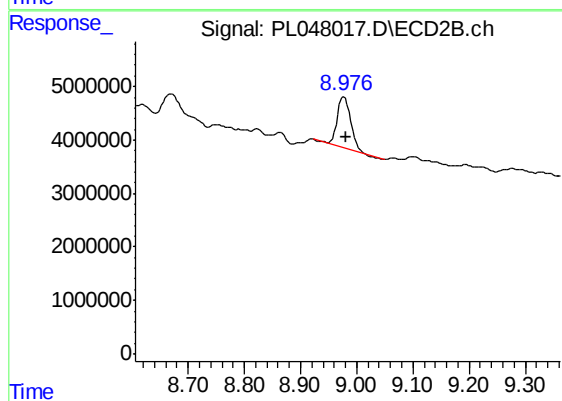

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.004 min
Response: 15205844
Conc: 5.33 ng/ml