

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
 Data File : PL066596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2021 11:15
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 01:06:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	6.078	0	2370305	N.D.	0.641 #
9) A	Endosulfan I	0.000	6.452	0	808172	N.D.	0.212 #
11) B	alpha-Chl...	0.000	6.367f	0	5448805	N.D.	1.314 #
14) MA	Endrin	5.972f	0.000	937605	0	0.215	N.D. #
15) B	Endosulfa...	6.201f	0.000	5077138	0	1.230	N.D. #
21) B	Endrin ke...	0.000	7.976	0	1708709	N.D.	0.481 #
26)	Chlordane-4	0.000	6.367f	0	5448805	N.D.	8.116 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL043021\
Data File : PL066596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2021 11:15
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 01:06:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

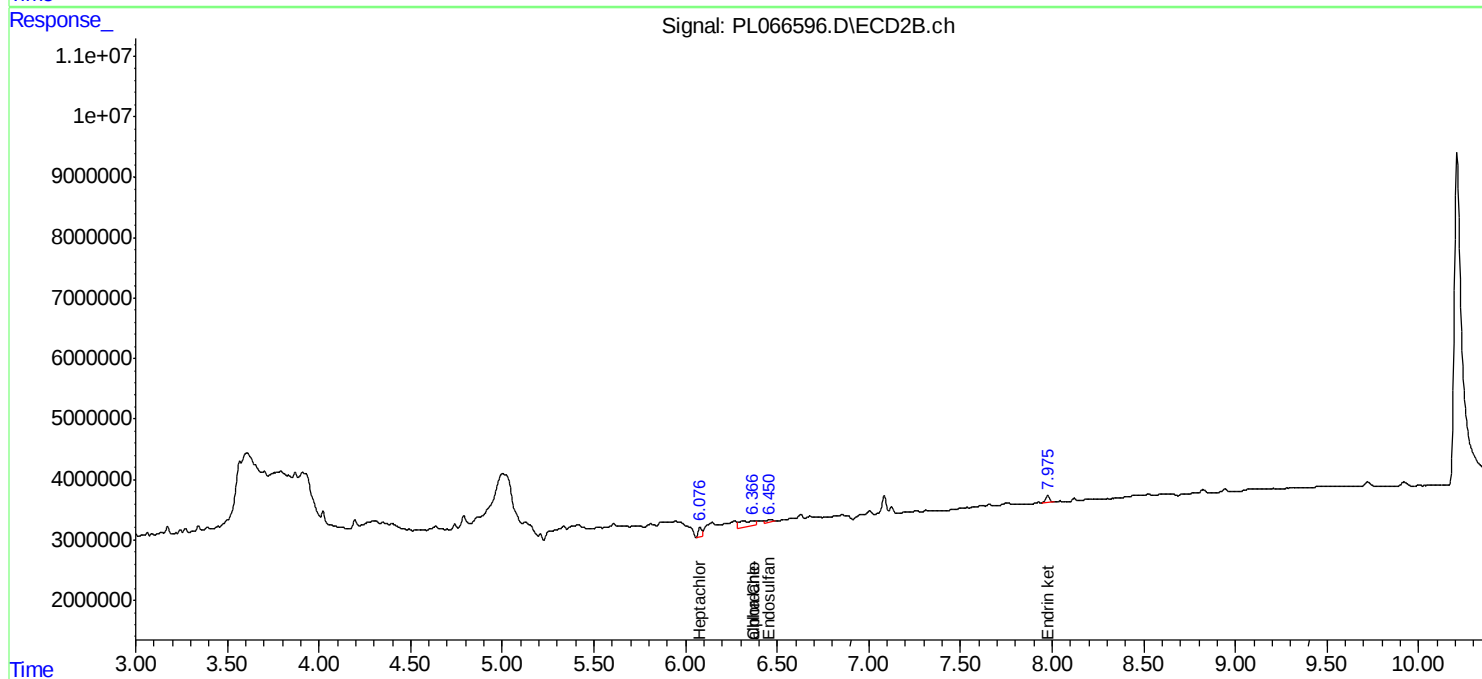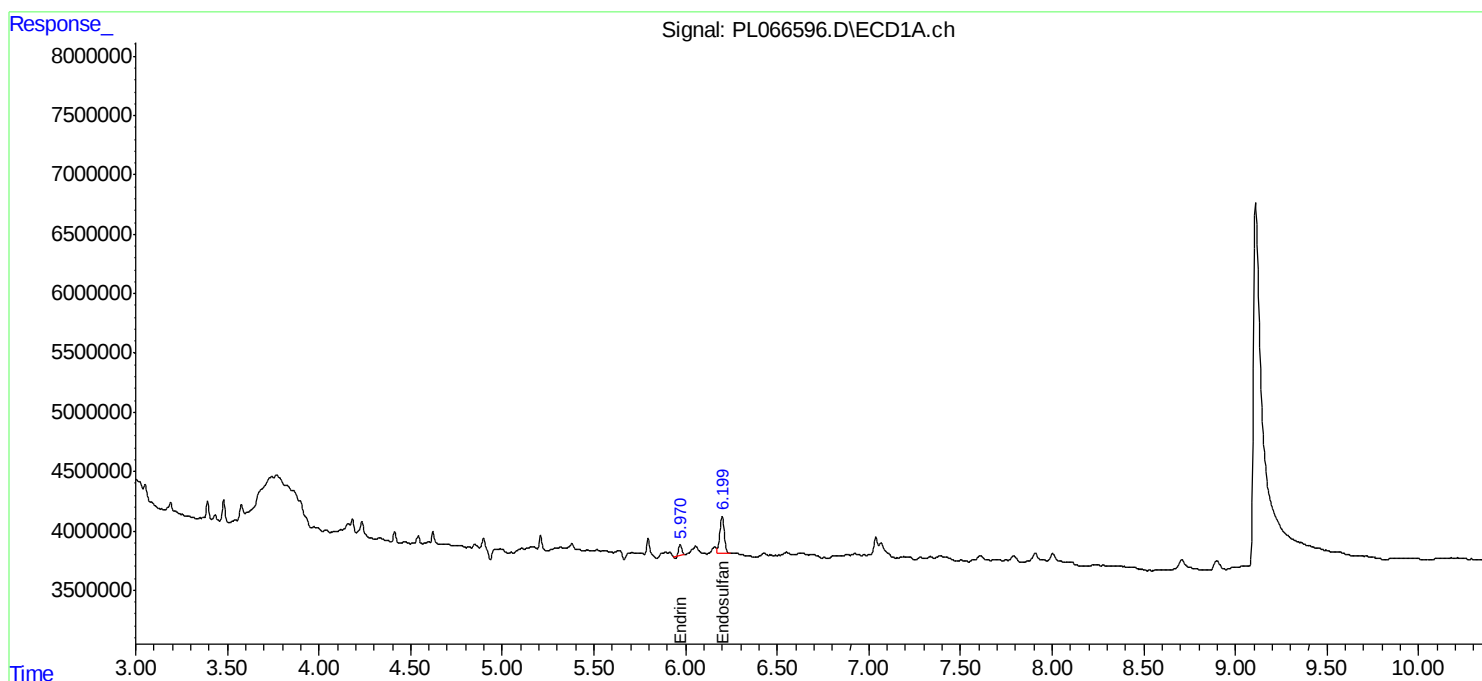


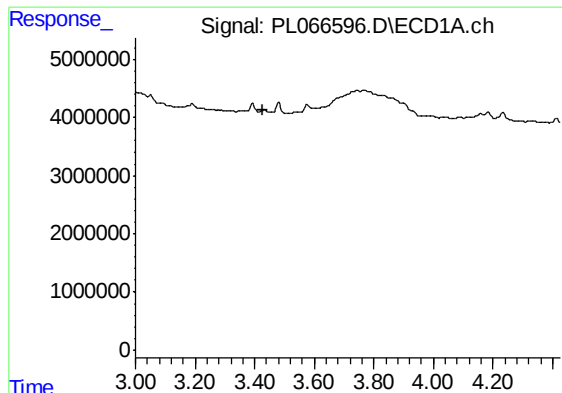

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

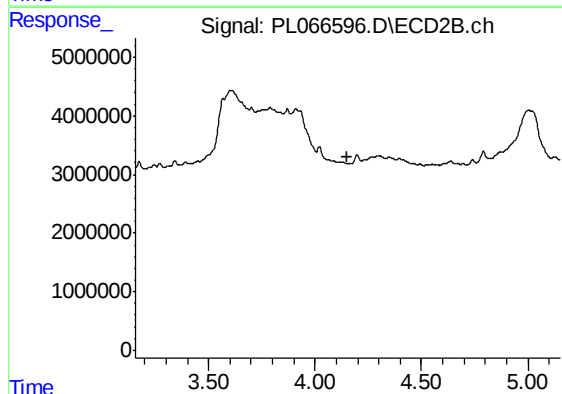


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

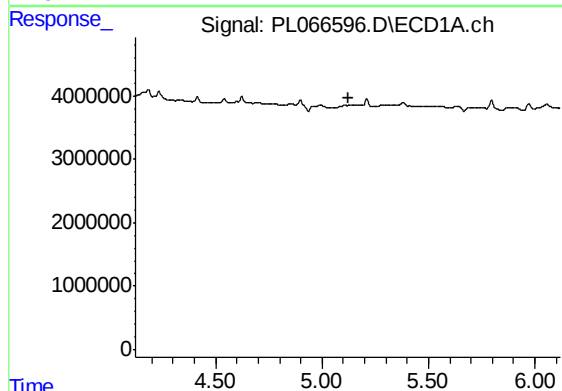


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.123 min
Response: 0
Conc: N.D.

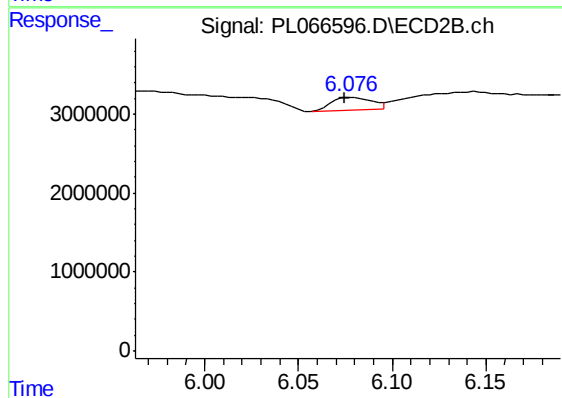

#8 Heptachlor epoxide


R.T.: 6.078 min
Delta R.T.: 0.004 min
Response: 2370305
Conc: 0.64 ng/ml

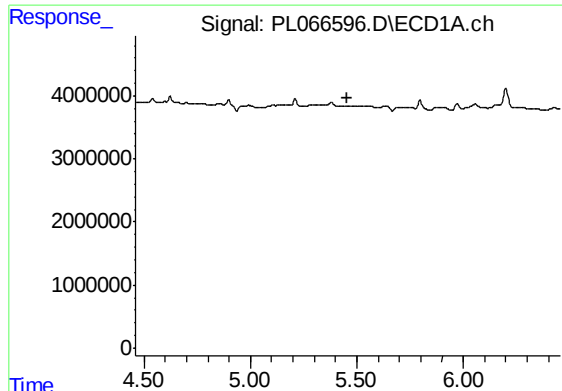

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

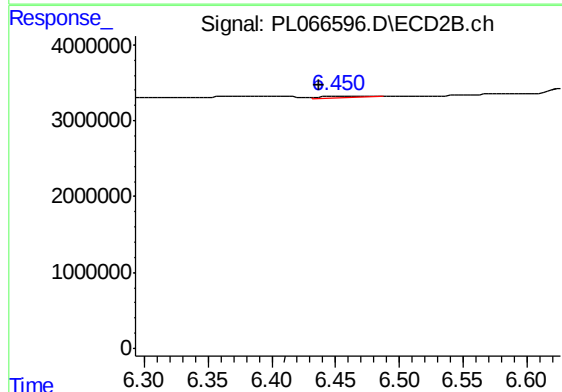


#9 Endosulfan I

R.T.: 6.452 min
Delta R.T.: 0.015 min
Response: 808172
Conc: 0.21 ng/ml

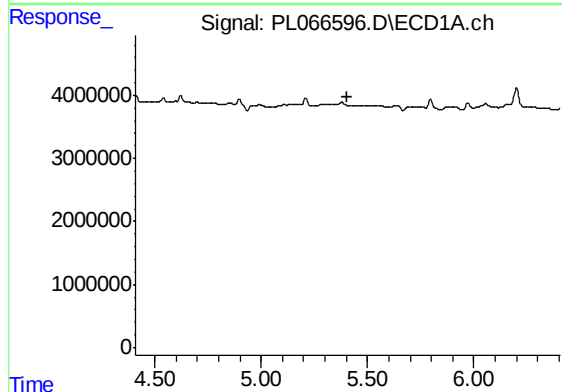


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

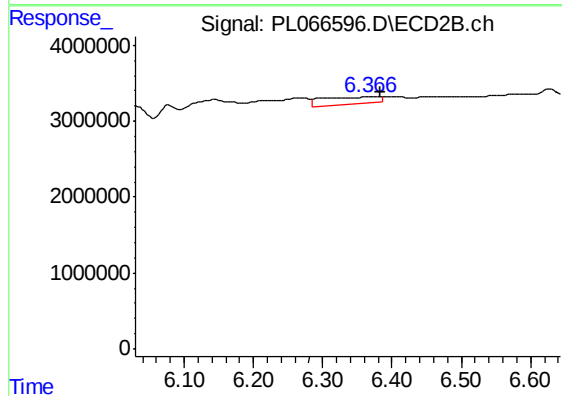

#11 alpha-Chlordane


R.T.: 6.367 min
Delta R.T.: -0.016 min
Response: 5448805
Conc: 1.31 ng/ml

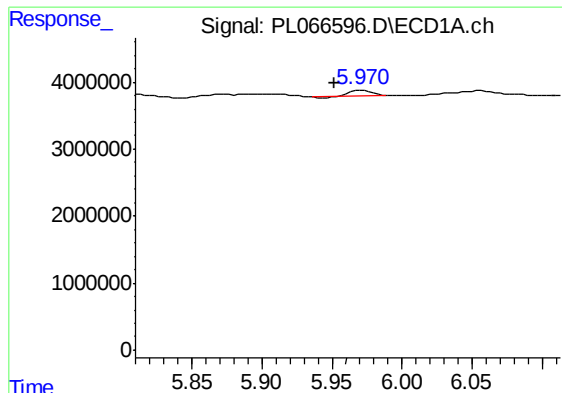

#14 Endrin


R.T.: 5.972 min
Delta R.T.: 0.020 min
Response: 937605
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

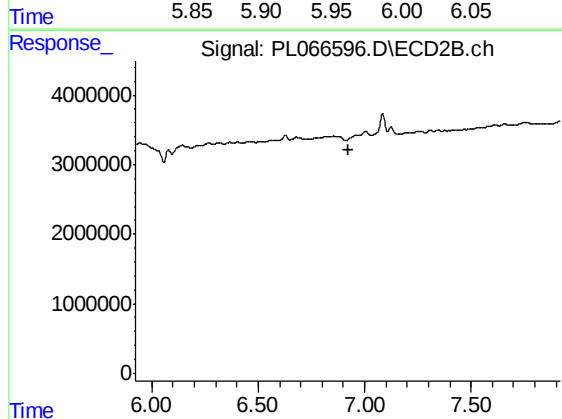


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

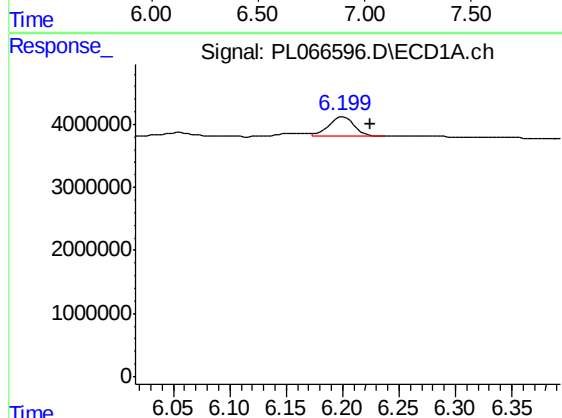


#15 Endosulfan II

R.T.: 6.201 min
Delta R.T.: -0.024 min
Response: 5077138
Conc: 1.23 ng/ml

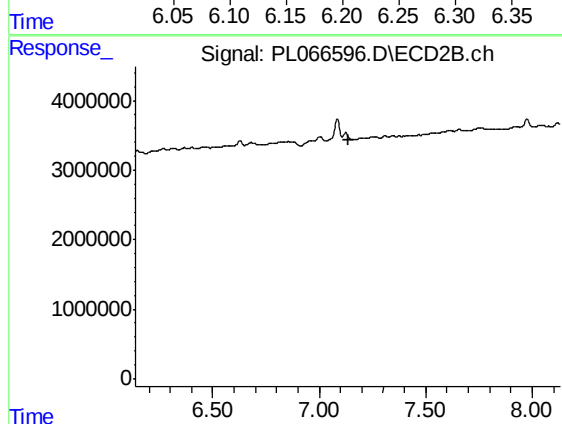

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

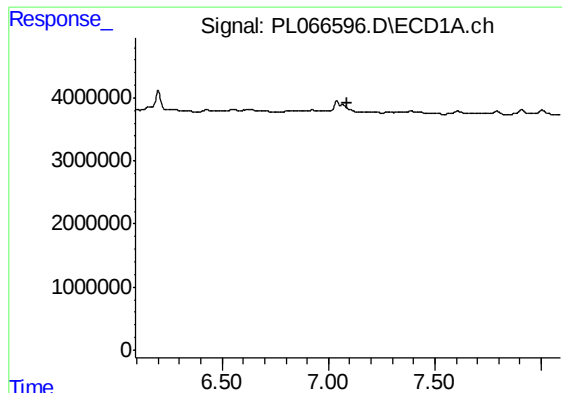

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

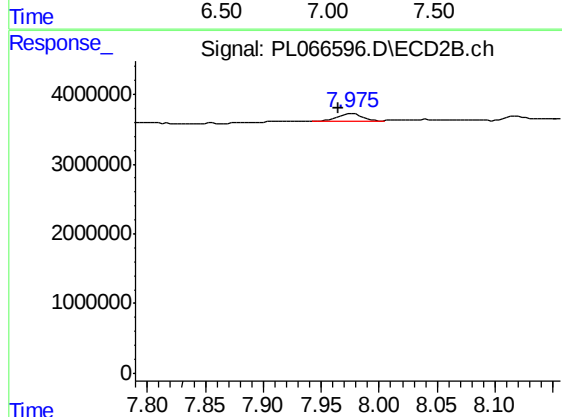


#21 Endrin ketone

R.T.: 7.976 min
Delta R.T.: 0.012 min
Response: 1708709
Conc: 0.48 ng/ml

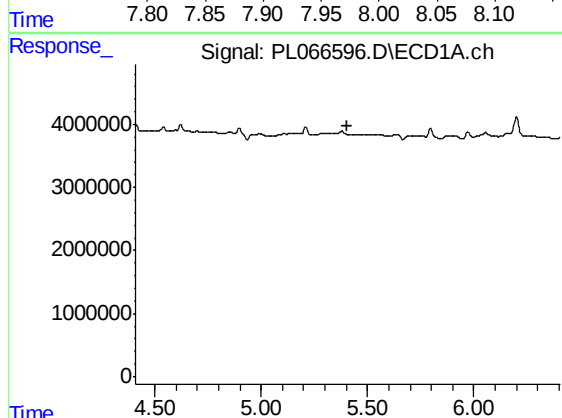


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

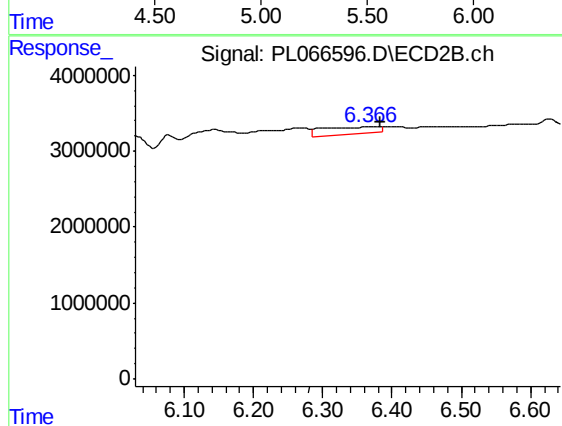

#26 Chlordane-4


R.T.: 6.367 min
Delta R.T.: -0.017 min
Response: 5448805
Conc: 8.12 ng/ml

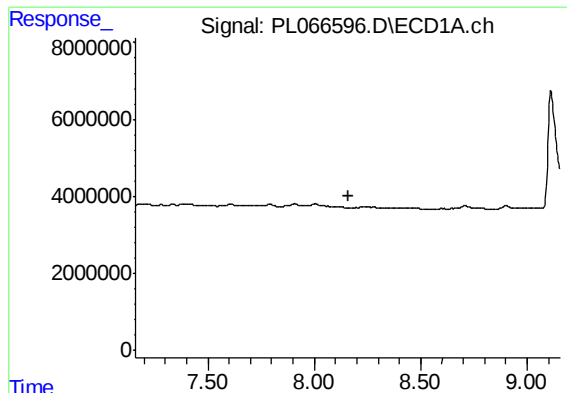

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

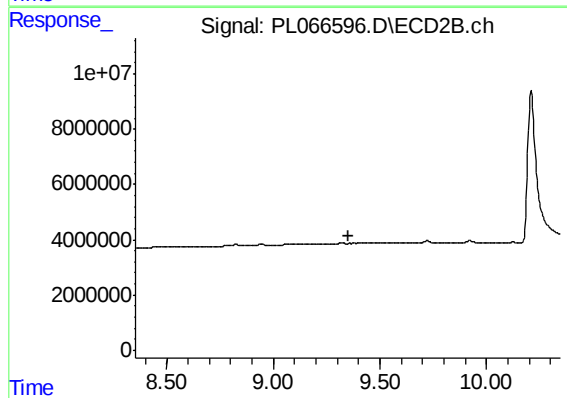

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.352 min
Response: 0
Conc: N.D.